

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014673.D
 Acq On : 12 Apr 2023 14:56
 Operator : CG/JU
 Sample : 02251-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014673.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	39	rVB	30144	41331	2.10%	0.175%
2	3.805	103	105	120	rBV	130701	235313	11.93%	0.997%
3	4.017	137	141	145	rVB4	4363	7462	0.38%	0.032%
4	4.117	154	158	167	rVB	34078	49189	2.49%	0.208%
5	4.458	214	216	219	rBV4	2126	2145	0.11%	0.009%
6	4.658	248	250	255	rVB6	3100	3529	0.18%	0.015%
7	5.070	313	320	328	rBV	31341	50426	2.56%	0.214%
8	5.240	345	349	350	rBV4	2201	2757	0.14%	0.012%
9	5.387	371	374	379	rBV7	1909	3570	0.18%	0.015%
10	5.522	393	397	401	rVB6	2365	3580	0.18%	0.015%
11	5.564	401	404	406	rBV3	2213	2608	0.13%	0.011%
12	7.164	670	676	689	rBV2	42188	104810	5.31%	0.444%
13	7.305	694	700	713	rBV	397639	646676	32.78%	2.739%
14	7.511	728	735	753	rBV	231394	422162	21.40%	1.788%
15	7.869	794	796	801	rVB6	1600	2183	0.11%	0.009%
16	7.975	806	814	829	rVV	465534	780537	39.56%	3.306%
17	8.075	829	831	834	rVV4	2427	3242	0.16%	0.014%
18	8.705	930	938	957	rBV2	192176	406256	20.59%	1.721%
19	8.846	960	962	965	rVB4	1877	2126	0.11%	0.009%
20	9.158	1006	1015	1036	rBV	498749	872296	44.22%	3.694%
21	9.516	1072	1076	1082	rVB4	7233	12331	0.63%	0.052%
22	9.610	1086	1092	1098	rBV10	3776	8109	0.41%	0.034%
23	9.881	1131	1138	1157	rBV	229364	439041	22.25%	1.859%
24	10.428	1224	1231	1252	rBV	248470	601097	30.47%	2.546%
25	10.593	1255	1259	1275	rVB6	14110	36567	1.85%	0.155%
26	10.799	1287	1294	1310	rVB	639170	1090615	55.28%	4.619%
27	10.952	1314	1320	1341	rBV	287473	667710	33.85%	2.828%
28	11.187	1354	1360	1367	rVB2	26603	47602	2.41%	0.202%
29	11.281	1374	1376	1384	rVB9	1847	3655	0.19%	0.015%
30	11.340	1384	1386	1390	rBV5	1680	2222	0.11%	0.009%
31	11.469	1405	1408	1410	rBV4	1996	2064	0.10%	0.009%
32	11.522	1414	1417	1422	rVB7	1163	2330	0.12%	0.010%
33	11.669	1432	1442	1450	rBV7	3282	11283	0.57%	0.048%
34	12.016	1499	1501	1507	rVB7	2151	2729	0.14%	0.012%
35	12.151	1518	1524	1526	rBV5	4029	6696	0.34%	0.028%
36	12.199	1529	1532	1538	rVB8	3920	7268	0.37%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014673.D
 Acq On : 12 Apr 2023 14:56
 Operator : CG/JU
 Sample : 02251-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	12.334	1549	1555	1562	rVV2	38313	77901	3.95%	0.330%
38	12.399	1562	1566	1573	rVV3	10268	22172	1.12%	0.094%
39	12.551	1588	1592	1594	rBV5	1762	2232	0.11%	0.009%
40	12.628	1598	1605	1614	rBV6	5872	14227	0.72%	0.060%
41	12.716	1619	1620	1627	rVB7	1537	2501	0.13%	0.011%
42	12.804	1627	1635	1637	rBV8	1794	3350	0.17%	0.014%
43	12.946	1656	1659	1664	rBV7	1586	2318	0.12%	0.010%
44	12.999	1666	1668	1674	rVB7	1897	2924	0.15%	0.012%
45	13.451	1735	1745	1754	rBV5	53797	114356	5.80%	0.484%
46	13.516	1754	1756	1763	rVB7	5247	8239	0.42%	0.035%
47	13.604	1768	1771	1774	rVV5	5537	8154	0.41%	0.035%
48	13.651	1774	1779	1785	rVV3	22308	37668	1.91%	0.160%
49	13.710	1785	1789	1802	rVV3	12026	33157	1.68%	0.140%
50	13.798	1802	1804	1806	rVV3	2241	2554	0.13%	0.011%
51	13.834	1806	1810	1813	rVB5	1706	2874	0.15%	0.012%
52	14.040	1835	1845	1858	rBV	1027994	1471554	74.59%	6.232%
53	14.140	1858	1862	1870	rVV9	9457	22131	1.12%	0.094%
54	14.322	1887	1893	1903	rBV	1050217	1583268	80.25%	6.705%
55	14.393	1903	1905	1914	rVB9	8522	13953	0.71%	0.059%
56	14.534	1928	1929	1933	rVB3	2113	2082	0.11%	0.009%
57	14.628	1937	1945	1958	rVV	834855	1266405	64.19%	5.363%
58	14.740	1962	1964	1968	rVV4	3068	4656	0.24%	0.020%
59	14.793	1971	1973	1977	rVB5	2062	2509	0.13%	0.011%
60	14.987	2003	2006	2010	rVV6	3649	7665	0.39%	0.032%
61	15.028	2012	2013	2020	rVV6	3421	6162	0.31%	0.026%
62	15.087	2020	2023	2026	rVB5	1841	2300	0.12%	0.010%
63	15.193	2039	2041	2047	rVB6	1578	2195	0.11%	0.009%
64	15.375	2066	2072	2082	rBV	303509	440591	22.33%	1.866%
65	15.457	2084	2086	2089	rVB4	5540	5652	0.29%	0.024%
66	15.563	2100	2104	2107	rBV5	2225	3417	0.17%	0.014%
67	15.628	2107	2115	2124	rBV	1343362	1923459	97.50%	8.146%
68	15.704	2124	2128	2133	rVV6	14357	32807	1.66%	0.139%
69	15.769	2133	2139	2152	rVV	118659	257961	13.08%	1.092%
70	15.869	2154	2156	2165	rVB10	9443	14201	0.72%	0.060%
71	15.998	2173	2178	2186	rVB	54229	84364	4.28%	0.357%
72	16.275	2221	2225	2228	rVB6	1788	2938	0.15%	0.012%
73	16.322	2228	2233	2241	rBV4	9305	18682	0.95%	0.079%
74	16.451	2251	2255	2259	rBV7	2355	4681	0.24%	0.020%
75	16.557	2271	2273	2277	rVB5	2384	2674	0.14%	0.011%
76	16.787	2311	2312	2315	rBV3	2659	2431	0.12%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014673.D
 Acq On : 12 Apr 2023 14:56
 Operator : CG/JU
 Sample : 02251-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

77	16.975	2341	2344	2345	rBV3	1771	2088	0.11%	0.009%
78	16.992	2345	2347	2349	rVB3	4213	3029	0.15%	0.013%
79	17.039	2349	2355	2358	rBV7	3951	8437	0.43%	0.036%
80	17.075	2358	2361	2365	rBV6	2967	3821	0.19%	0.016%
81	17.122	2365	2369	2372	rBV5	7872	9822	0.50%	0.042%
82	17.392	2408	2415	2424	rBV	906591	1280323	64.90%	5.422%
83	17.492	2426	2432	2448	rVV	1254588	1925555	97.60%	8.155%
84	17.786	2478	2482	2485	rBV6	2896	4975	0.25%	0.021%
85	17.863	2492	2495	2498	rBV5	4387	5229	0.27%	0.022%
86	18.269	2560	2564	2573	rBV5	29716	60827	3.08%	0.258%
87	19.304	2737	2740	2745	rVB6	12856	18205	0.92%	0.077%
88	19.381	2748	2753	2756	rBV3	15194	28337	1.44%	0.120%
89	19.504	2770	2774	2779	rBV5	18100	33936	1.72%	0.144%
90	19.728	2806	2812	2824	rBV	1267262	1745132	88.46%	7.391%
91	20.222	2893	2896	2901	rBV2	22637	25668	1.30%	0.109%
92	20.704	2976	2978	2983	rVB2	33617	29728	1.51%	0.126%
93	21.163	3053	3056	3064	rBV5	61664	135808	6.88%	0.575%
94	21.486	3106	3111	3122	rBV	653678	990900	50.23%	4.197%
95	23.827	3502	3509	3519	rBV2	960906	1972809	100.00%	8.355%
96	23.992	3530	3537	3551	rVB2	526675	1230720	62.38%	5.212%




Sum of corrected areas: 23612231

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014673.D
Acq On : 12 Apr 2023 14:56
Operator : CG/JU
Sample : 02251-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

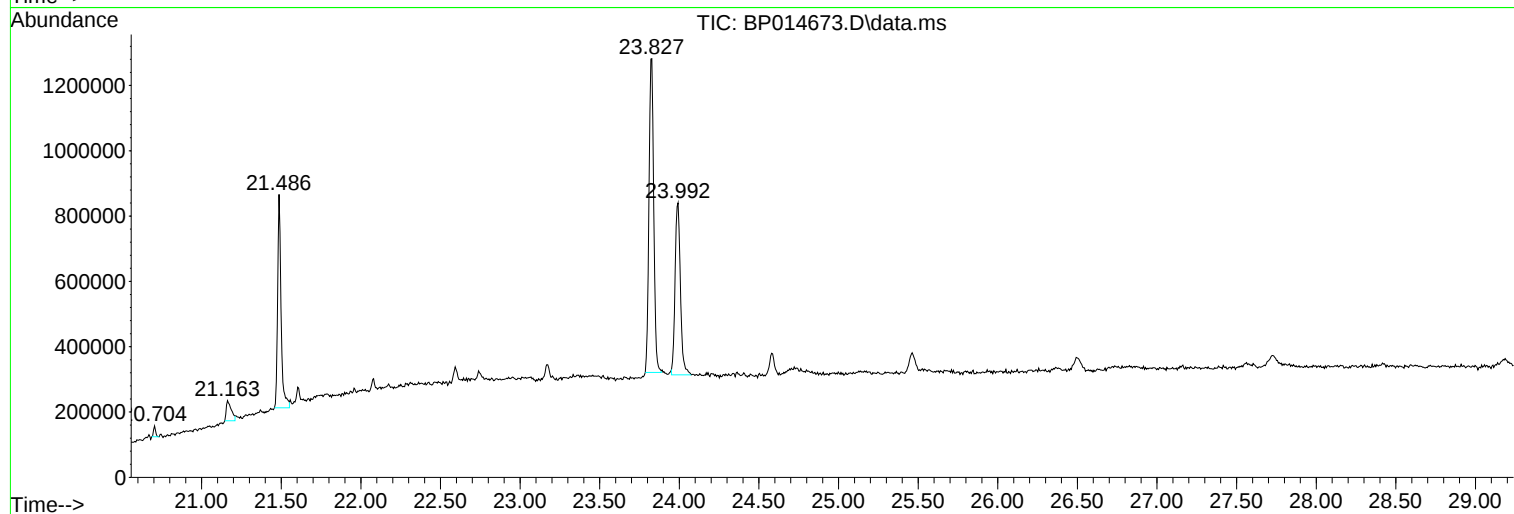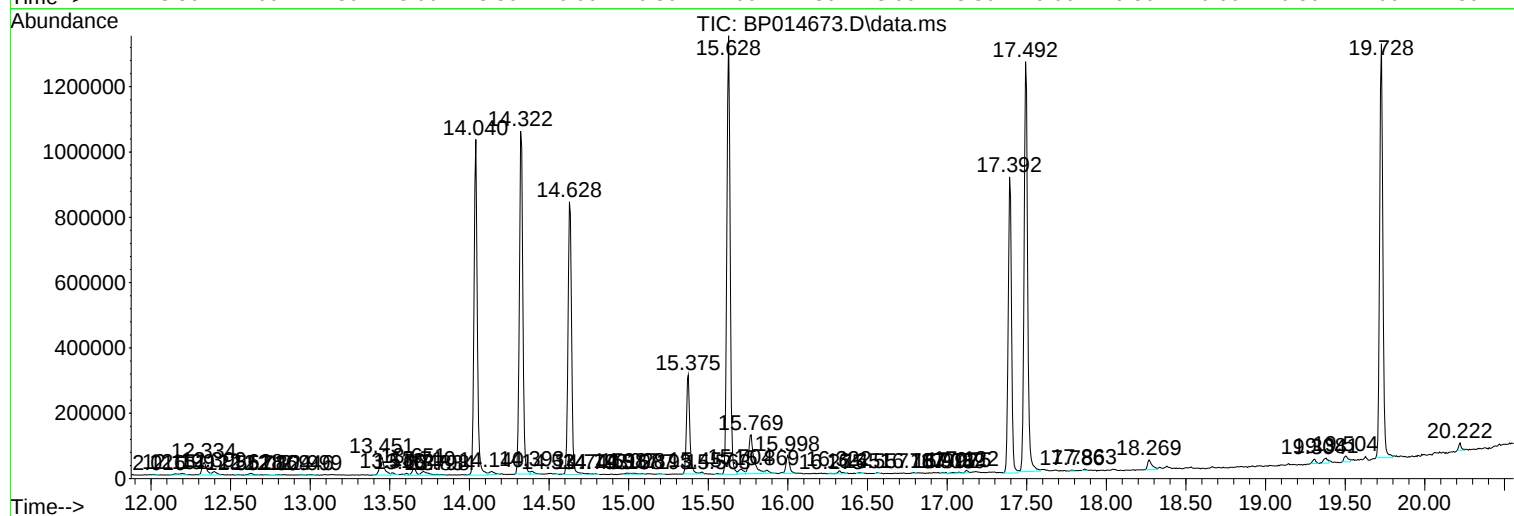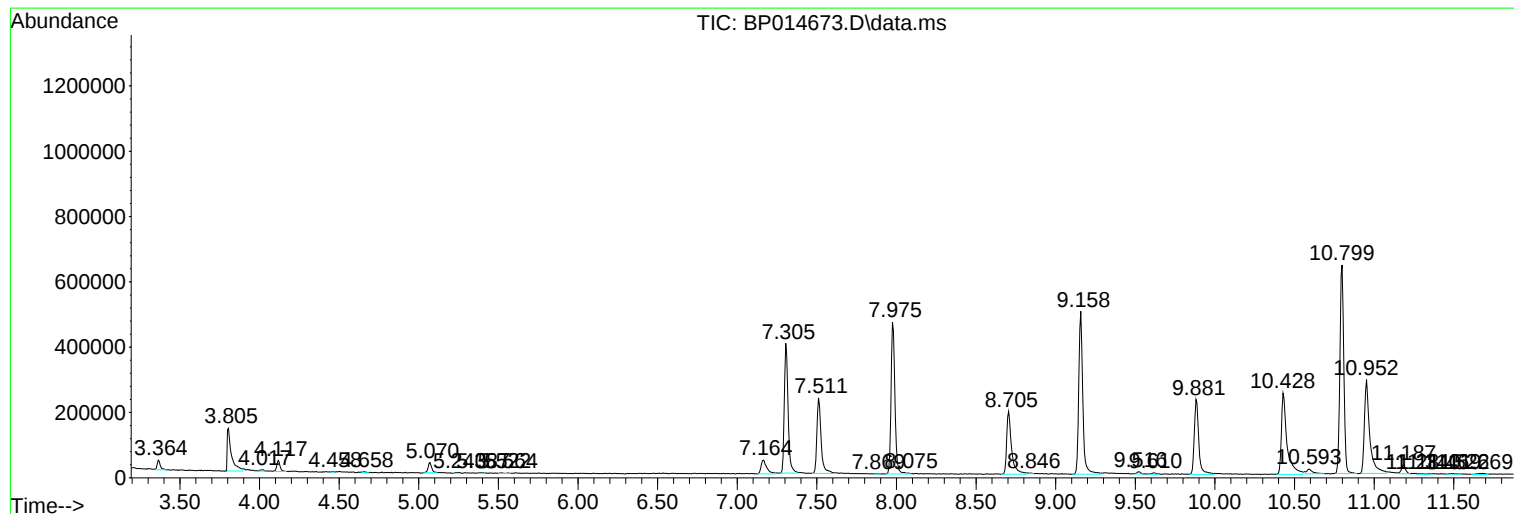

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014673.D
Acq On : 12 Apr 2023 14:56
Operator : CG/JU
Sample : 02251-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMD3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Diethyltoluamide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.375	6.96 ng/ul	440591	Acenaphthene-d10	14.628

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diethyltoluamide	191	C12H17NO	000134-62-3	97
2			Diethyltoluamide	191	C12H17NO	000134-62-3	94
3			Benzamide, 3-methyl-N-methyl-N-p...	191	C12H17NO	1000421-46-2	93
4			Diethyltoluamide	191	C12H17NO	000134-62-3	87
5			Benzamide, 2-methyl-N-methyl-N-p...	191	C12H17NO	1000421-44-4	74

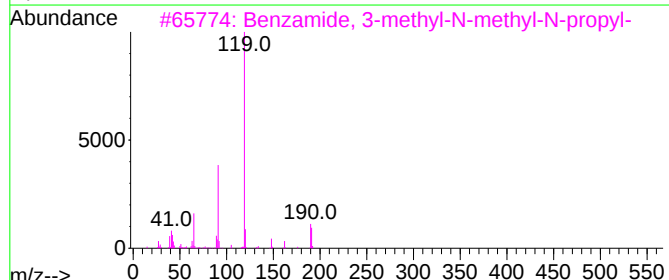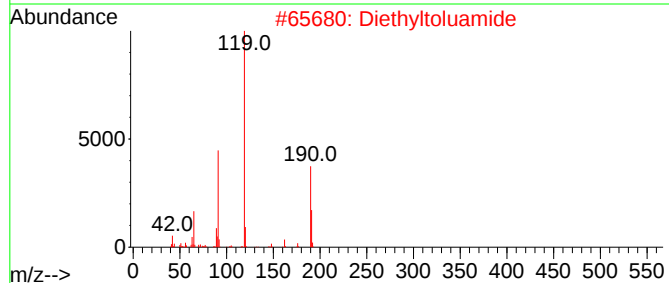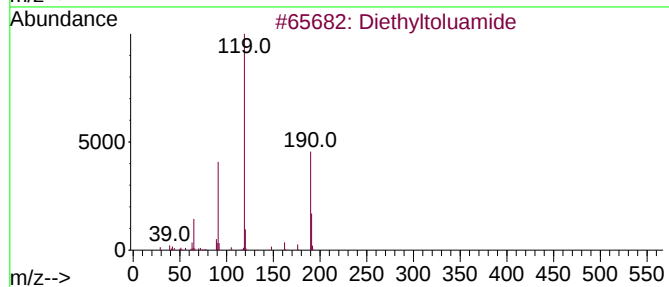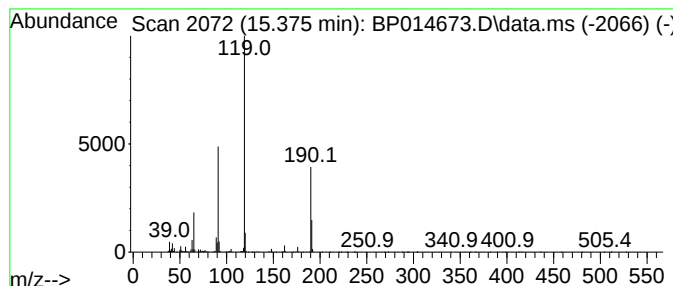

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014673.D
Acq On : 12 Apr 2023 14:56
Operator : CG/JU
Sample : 02251-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMD3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Cyclic21.163 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.163	2.74 ng/ul	135808	Chrysene-d12	21.486

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexadecane	224	C16H32	000295-65-8	86
2			E-15-Heptadecenal	252	C17H32O	1000130-97-9	83
3			1-Octadecene	252	C18H36	000112-88-9	80
4			Carbonic acid, eicosyl vinyl ester	368	C23H44O3	1000382-54-3	70
5			Carbonic acid, octadecyl prop-1-...	354	C22H42O3	1000383-11-5	70

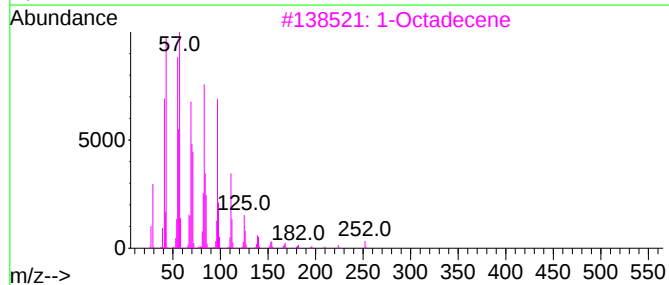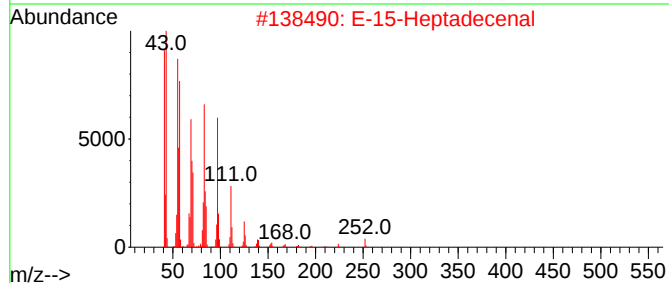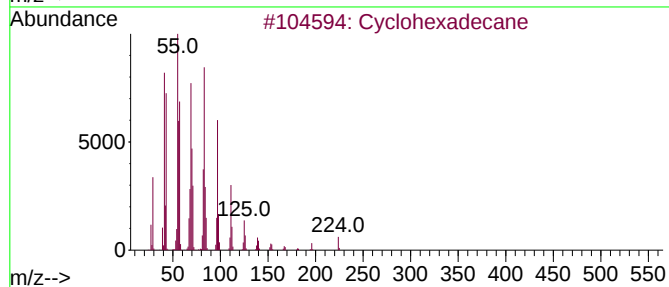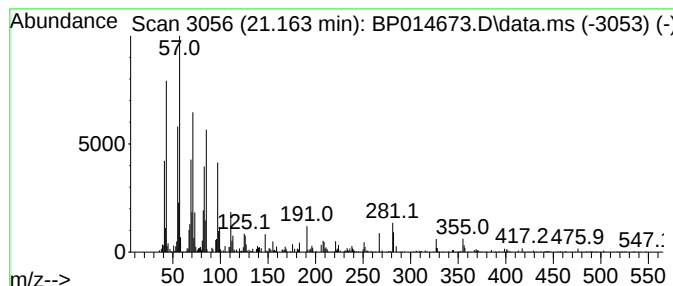

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014673.D
Acq On : 12 Apr 2023 14:56
Operator : CG/JU
Sample : 02251-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0MD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diethyltoluamide	15.375	7.0	ng/u1	440591	3	14.628	1266410	20.0
(DEL) Alkane: C...	21.163	2.7	ng/u1	135808	5	21.486	990900	20.0