

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014676.D
 Acq On : 12 Apr 2023 16:39
 Operator : CG/JU
 Sample : 02251-17
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014676.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	26	30	36	rBV	29537	39829	1.36%	0.149%
2	3.810	104	106	125	rBV	67997	150203	5.14%	0.561%
3	4.110	154	157	163	rVB2	9422	13462	0.46%	0.050%
4	5.263	348	353	360	rBV	18174	30368	1.04%	0.113%
5	6.210	509	514	517	rBV7	2839	4857	0.17%	0.018%
6	7.145	667	673	687	rBV	85008	191814	6.56%	0.716%
7	7.304	693	700	714	rBV	341496	580860	19.87%	2.168%
8	7.504	728	734	752	rVB	354060	627424	21.46%	2.342%
9	7.863	788	795	802	rBV2	19480	36917	1.26%	0.138%
10	7.975	807	814	818	rBV	412001	700957	23.97%	2.616%
11	8.328	868	874	882	rBV	80549	142400	4.87%	0.531%
12	8.698	930	937	949	rBV	249774	503768	17.23%	1.880%
13	9.151	1007	1014	1033	rBV	432864	776192	26.55%	2.897%
14	9.516	1071	1076	1080	rBV3	7396	12602	0.43%	0.047%
15	9.875	1131	1137	1156	rBV	347613	630517	21.57%	2.353%
16	10.422	1223	1230	1261	rVV	356321	845536	28.92%	3.156%
17	10.657	1264	1270	1276	rVB3	19689	37095	1.27%	0.138%
18	10.792	1285	1293	1306	rBV	567117	960973	32.87%	3.587%
19	10.945	1312	1319	1343	rBV	304127	729555	24.95%	2.723%
20	11.180	1354	1359	1364	rVB6	8697	15948	0.55%	0.060%
21	11.416	1396	1399	1405	rVB8	2021	3578	0.12%	0.013%
22	12.010	1494	1500	1507	rVB10	3383	6303	0.22%	0.024%
23	12.351	1554	1558	1560	rBV5	2422	3672	0.13%	0.014%
24	12.404	1562	1567	1574	rVV8	6636	15984	0.55%	0.060%
25	13.427	1738	1741	1746	rVB7	3837	6274	0.21%	0.023%
26	13.516	1751	1756	1759	rVV7	2464	3766	0.13%	0.014%
27	13.610	1768	1772	1776	rVB7	2074	3414	0.12%	0.013%
28	14.033	1836	1844	1860	rBV	908827	1341233	45.87%	5.006%
29	14.322	1886	1893	1902	rBV2	996247	1528014	52.26%	5.703%
30	14.627	1937	1945	1956	rBV	833137	1250128	42.76%	4.666%
31	14.933	1989	1997	2005	rBV10	14843	57078	1.95%	0.213%
32	15.621	2107	2114	2130	rBV	1269584	1920882	65.70%	7.169%
33	15.757	2131	2137	2152	rBV2	324971	588028	20.11%	2.195%
34	15.868	2154	2156	2157	rVB2	4723	3408	0.12%	0.013%
35	15.998	2173	2178	2184	rBV	25696	40871	1.40%	0.153%
36	17.180	2374	2379	2382	rBV7	3354	5196	0.18%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014676.D
 Acq On : 12 Apr 2023 16:39
 Operator : CG/JU
 Sample : 02251-17
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	17.386	2407	2414	2425	rVV	1001064	1483165	50.73%	5.536%
38	17.492	2425	2432	2447	rVV	1391419	2096617	71.71%	7.825%
39	17.721	2469	2471	2474	rVB4	3937	3061	0.10%	0.011%
40	17.768	2474	2479	2482	rBV7	4102	8729	0.30%	0.033%
41	18.039	2521	2525	2530	rBV7	4555	7892	0.27%	0.029%
42	18.262	2558	2563	2573	rBV4	33062	70679	2.42%	0.264%
43	18.468	2595	2598	2604	rBV5	11097	23031	0.79%	0.086%
44	18.974	2682	2684	2688	rVB5	5984	6574	0.22%	0.025%
45	19.298	2735	2739	2743	rBV4	20269	31395	1.07%	0.117%
46	19.374	2748	2752	2759	rBV	19258	39874	1.36%	0.149%
47	19.492	2770	2772	2780	rBV8	17429	30585	1.05%	0.114%
48	19.621	2792	2794	2800	rVB6	12939	13971	0.48%	0.052%
49	19.721	2805	2811	2820	rBV	1930945	2562567	87.65%	9.564%
50	20.662	2968	2971	2975	rVB	77041	81794	2.80%	0.305%
51	21.480	3105	3110	3122	rBV	1200683	1788774	61.18%	6.676%
52	23.821	3501	3508	3520	rVB2	1419239	2923777	100.00%	10.912%
53	23.980	3529	3535	3545	rVB2	814812	1811484	61.96%	6.761%




Sum of corrected areas: 26793075

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014676.D
Acq On : 12 Apr 2023 16:39
Operator : CG/JU
Sample : 02251-17
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMD5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

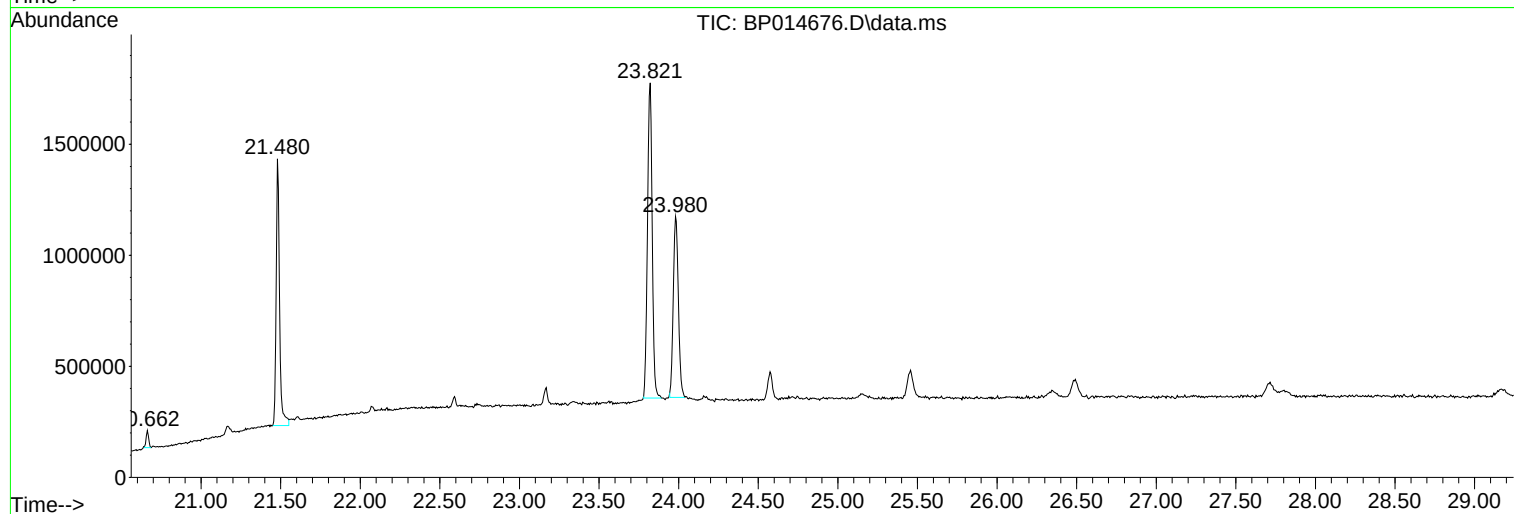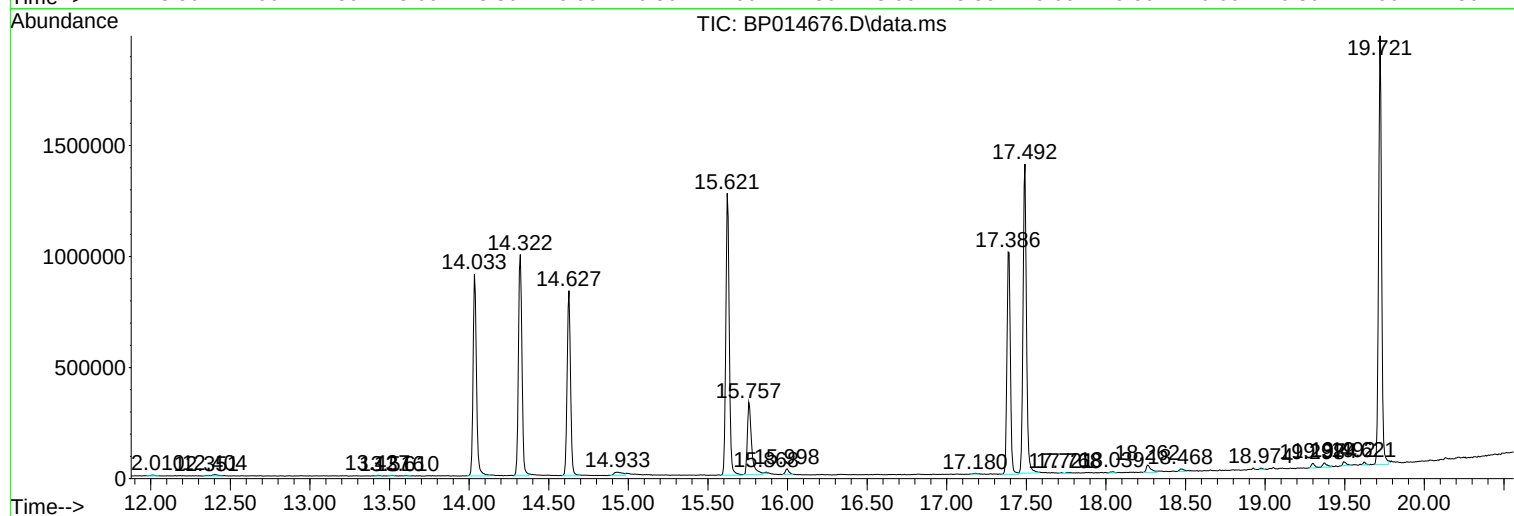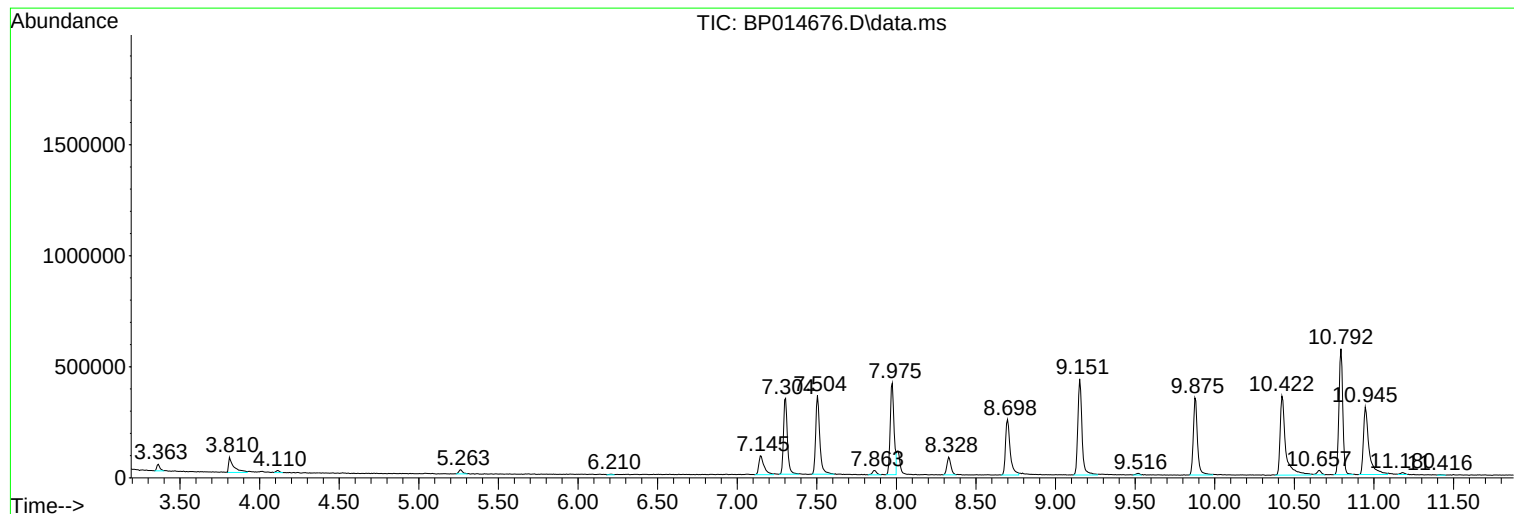

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014676.D
Acq On : 12 Apr 2023 16:39
Operator : CG/JU
Sample : 02251-17
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0MD5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014676.D
Acq On : 12 Apr 2023 16:39
Operator : CG/JU
Sample : 02251-17
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0MD5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------