

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014677.D
 Acq On : 12 Apr 2023 17:14
 Operator : CG/JU
 Sample : 02251-18
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014677.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	26	30	34	rVB	29387	37206	1.14%	0.117%
2	3.822	105	108	117	rBV	33077	73107	2.23%	0.229%
3	4.116	153	158	162	rBV3	11192	16700	0.51%	0.052%
4	5.040	312	315	318	rBV4	2629	3635	0.11%	0.011%
5	5.258	346	352	358	rBV4	10490	19592	0.60%	0.061%
6	6.940	634	638	641	rVB5	1898	3343	0.10%	0.010%
7	7.146	666	673	686	rBV	104557	230267	7.03%	0.723%
8	7.305	694	700	721	rVB	398840	685047	20.92%	2.149%
9	7.505	727	734	750	rBV	428481	746910	22.81%	2.344%
10	7.975	807	814	829	rBV	458535	789111	24.10%	2.476%
11	8.334	866	875	879	rBV9	4753	10759	0.33%	0.034%
12	8.699	930	937	958	rBV	329623	662548	20.24%	2.079%
13	9.152	1007	1014	1027	rBV	545366	951378	29.06%	2.985%
14	9.363	1044	1050	1053	rBV8	2335	3358	0.10%	0.011%
15	9.487	1064	1071	1073	rBV8	2358	4614	0.14%	0.014%
16	9.510	1073	1075	1084	rVB7	5095	8282	0.25%	0.026%
17	9.875	1130	1137	1154	rBV	440240	819146	25.02%	2.570%
18	10.422	1223	1230	1250	rBV	496579	1045074	31.92%	3.279%
19	10.793	1285	1293	1302	rBV	691269	1178750	36.00%	3.699%
20	10.946	1312	1319	1339	rBV	308130	733568	22.41%	2.302%
21	12.398	1561	1566	1574	rVB6	6771	16279	0.50%	0.051%
22	13.428	1737	1741	1745	rBV6	3532	5282	0.16%	0.017%
23	13.610	1767	1772	1775	rBV7	3275	4645	0.14%	0.015%
24	14.034	1832	1844	1860	rBV	1282253	1914901	58.49%	6.008%
25	14.145	1860	1863	1868	rVB6	4661	6904	0.21%	0.022%
26	14.322	1886	1893	1906	rBV	1454245	2094765	63.98%	6.573%
27	14.628	1938	1945	1959	rBV	1120495	1676973	51.22%	5.262%
28	14.910	1985	1993	2000	rBV7	25571	86631	2.65%	0.272%
29	15.381	2069	2073	2079	rVV6	4653	8115	0.25%	0.025%
30	15.622	2107	2114	2131	rBV	1817074	2738193	83.63%	8.592%
31	15.757	2131	2137	2152	rVV	585037	966910	29.53%	3.034%
32	15.869	2154	2156	2162	rVB3	10565	13611	0.42%	0.043%
33	15.998	2173	2178	2185	rVB	26297	42806	1.31%	0.134%
34	16.198	2210	2212	2217	rVB6	2534	3689	0.11%	0.012%
35	16.410	2246	2248	2253	rVB6	2942	4245	0.13%	0.013%
36	17.180	2376	2379	2383	rVB6	3677	5169	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014677.D
Acq On : 12 Apr 2023 17:14
Operator : CG/JU
Sample : 02251-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0MD6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION

37	17.386	2408	2414	2425	rBV	1376108	2013342	61.49%	6.317%
38	17.492	2425	2432	2451	rVV	2032587	3061355	93.50%	9.606%
39	18.263	2558	2563	2571	rBV3	61511	113901	3.48%	0.357%
40	19.298	2735	2739	2745	rBV3	27941	38867	1.19%	0.122%
41	19.369	2748	2751	2759	rVV4	24712	45510	1.39%	0.143%
42	19.492	2768	2772	2781	rBV9	38772	88455	2.70%	0.278%
43	19.722	2805	2811	2825	rBV	2468239	3274096	100.00%	10.273%
44	21.480	3105	3110	3121	rBV	1055650	1630156	49.79%	5.115%
45	23.815	3501	3507	3522	rVB2	1232569	2509503	76.65%	7.874%
46	23.986	3529	3536	3550	rVB2	671447	1483807	45.32%	4.656%




Sum of corrected areas: 31870505

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014677.D
Acq On : 12 Apr 2023 17:14
Operator : CG/JU
Sample : 02251-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

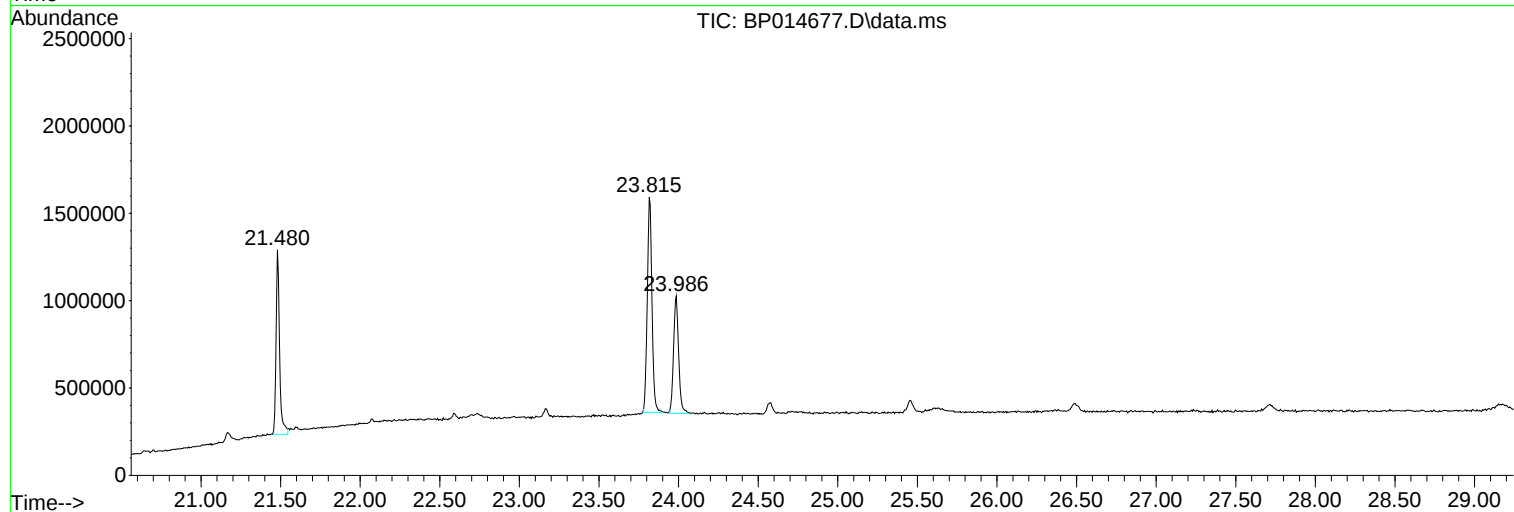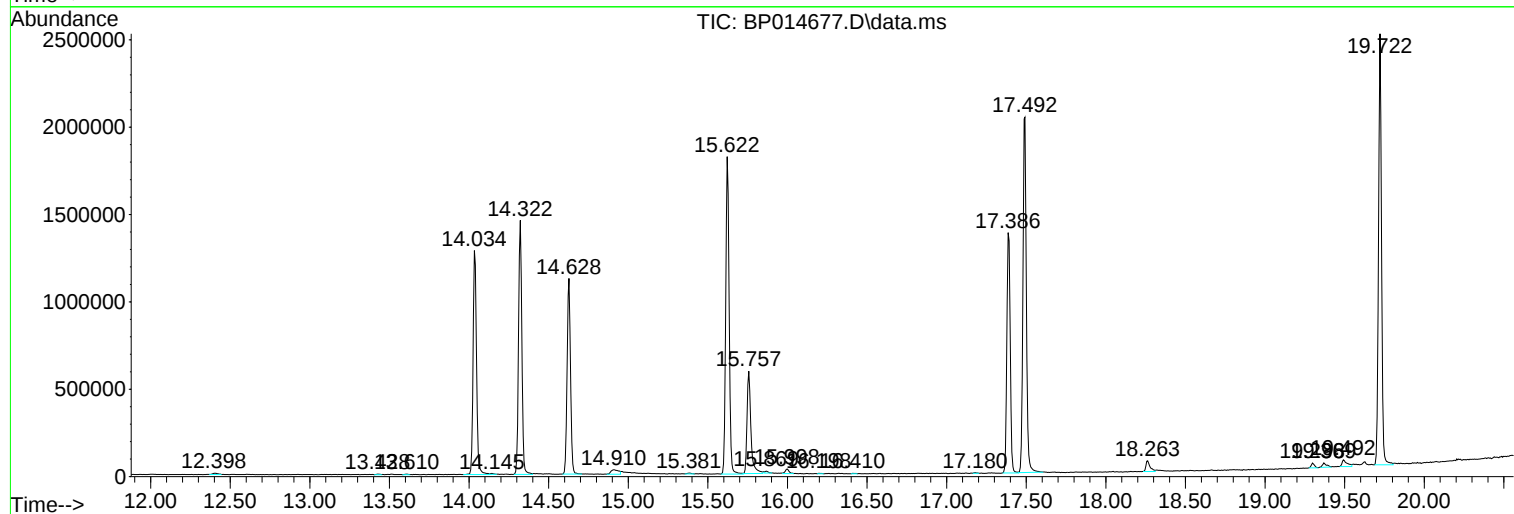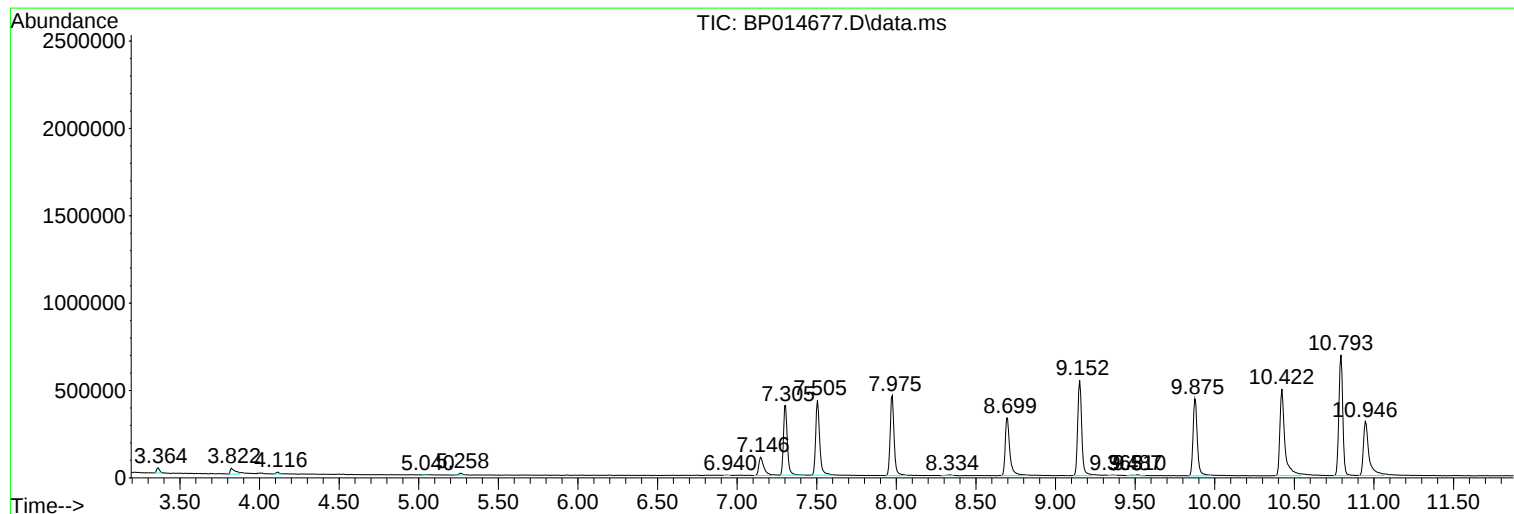

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014677.D
Acq On : 12 Apr 2023 17:14
Operator : CG/JU
Sample : 02251-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0MD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014677.D
Acq On : 12 Apr 2023 17:14
Operator : CG/JU
Sample : 02251-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0MD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc