

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014678.D
 Acq On : 12 Apr 2023 17:48
 Operator : CG/JU
 Sample : 02251-19
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014678.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	26	30	38	rVB	31588	42997	1.62%	0.139%
2	3.805	102	105	128	rBV	107898	238191	8.96%	0.768%
3	4.111	153	157	162	rVB3	9909	16313	0.61%	0.053%
4	5.046	311	316	317	rBV5	2540	4150	0.16%	0.013%
5	5.264	348	353	362	rBV2	13413	23378	0.88%	0.075%
6	6.234	516	518	523	rVB6	1921	2805	0.11%	0.009%
7	7.146	667	673	687	rBV	103381	220243	8.29%	0.711%
8	7.299	693	699	715	rBV	446950	747731	28.14%	2.412%
9	7.505	727	734	752	rBV	452278	789220	29.70%	2.546%
10	7.969	805	813	833	rBV	491543	859818	32.36%	2.774%
11	8.334	868	875	882	rVB	4310	8908	0.34%	0.029%
12	8.693	929	936	951	rBV	323770	638539	24.03%	2.060%
13	8.911	972	973	978	rVB5	2712	3012	0.11%	0.010%
14	9.152	1006	1014	1033	rBV	577867	998797	37.59%	3.222%
15	9.311	1036	1041	1048	rVB	2966	6067	0.23%	0.020%
16	9.516	1071	1076	1082	rVB6	4570	6619	0.25%	0.021%
17	9.875	1129	1137	1151	rBV	478328	847818	31.91%	2.735%
18	10.422	1222	1230	1256	rBV	496166	1102112	41.48%	3.556%
19	10.793	1285	1293	1303	rBV	731537	1253615	47.18%	4.045%
20	10.946	1311	1319	1341	rBV	382784	892149	33.58%	2.878%
21	12.399	1559	1566	1577	rBV5	7536	18148	0.68%	0.059%
22	13.146	1687	1693	1696	rVV8	1336	3344	0.13%	0.011%
23	13.434	1736	1742	1746	rBV9	4077	7717	0.29%	0.025%
24	13.510	1749	1755	1759	rVV9	5085	8848	0.33%	0.029%
25	13.604	1767	1771	1774	rBV6	2199	3941	0.15%	0.013%
26	13.869	1811	1816	1820	rVB8	1820	3294	0.12%	0.011%
27	14.034	1835	1844	1860	rBV	1231871	1807677	68.03%	5.832%
28	14.140	1860	1862	1868	rVB7	4748	7094	0.27%	0.023%
29	14.322	1885	1893	1903	rBV	1431187	2085113	78.47%	6.727%
30	14.504	1922	1924	1927	rVB4	2811	2689	0.10%	0.009%
31	14.628	1937	1945	1957	rBV	1181275	1711393	64.41%	5.521%
32	14.928	1989	1996	2006	rBV9	16451	67772	2.55%	0.219%
33	15.375	2069	2072	2075	rBV5	2104	3115	0.12%	0.010%
34	15.622	2107	2114	2129	rBV	1787984	2594654	97.65%	8.371%
35	15.757	2131	2137	2153	rVV	468550	818824	30.82%	2.642%
36	15.869	2153	2156	2161	rVB5	11693	18422	0.69%	0.059%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014678.D
 Acq On : 12 Apr 2023 17:48
 Operator : CG/JU
 Sample : 02251-19
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0MD7

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	15.998	2173	2178	2186	rBV	29267	49109	1.85%	0.158%
38	16.322	2231	2233	2239	rBV7	2524	4249	0.16%	0.014%
39	16.569	2271	2275	2278	rVV5	2428	3468	0.13%	0.011%
40	16.822	2316	2318	2322	rVB5	2871	4241	0.16%	0.014%
41	17.069	2357	2360	2363	rVB5	3396	4433	0.17%	0.014%
42	17.181	2377	2379	2385	rVB7	3529	5545	0.21%	0.018%
43	17.387	2408	2414	2425	rBV	1309310	1877782	70.67%	6.058%
44	17.492	2425	2432	2450	rVV	1775367	2657107	100.00%	8.573%
45	18.263	2559	2563	2573	rBV4	31969	66687	2.51%	0.215%
46	19.298	2736	2739	2746	rVB5	19784	28626	1.08%	0.092%
47	19.375	2747	2752	2759	rBV3	19920	42986	1.62%	0.139%
48	19.492	2769	2772	2777	rBV6	20761	37413	1.41%	0.121%
49	19.722	2805	2811	2825	rBV	1900169	2643847	99.50%	8.530%
50	21.480	3105	3110	3124	rBV	977171	1558252	58.64%	5.027%
51	23.822	3501	3508	3523	rVB	1201324	2482354	93.42%	8.009%
52	23.980	3529	3535	3550	rVB2	734011	1664546	62.65%	5.370%




Sum of corrected areas: 30995172

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014678.D
Acq On : 12 Apr 2023 17:48
Operator : CG/JU
Sample : 02251-19
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMD7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

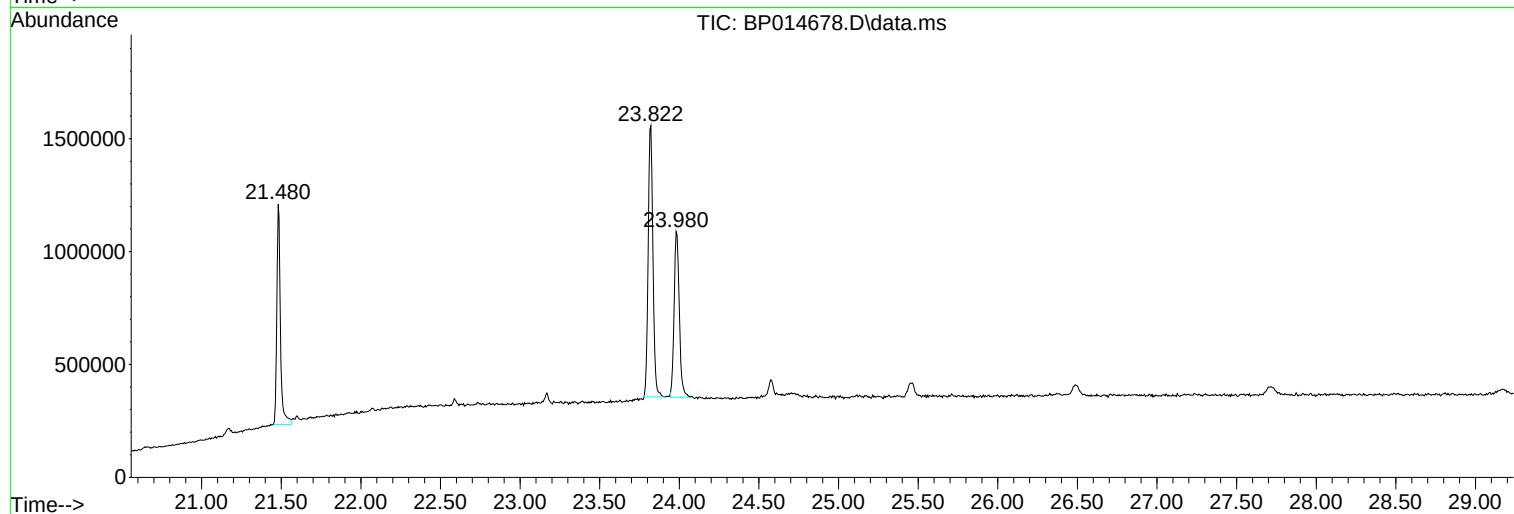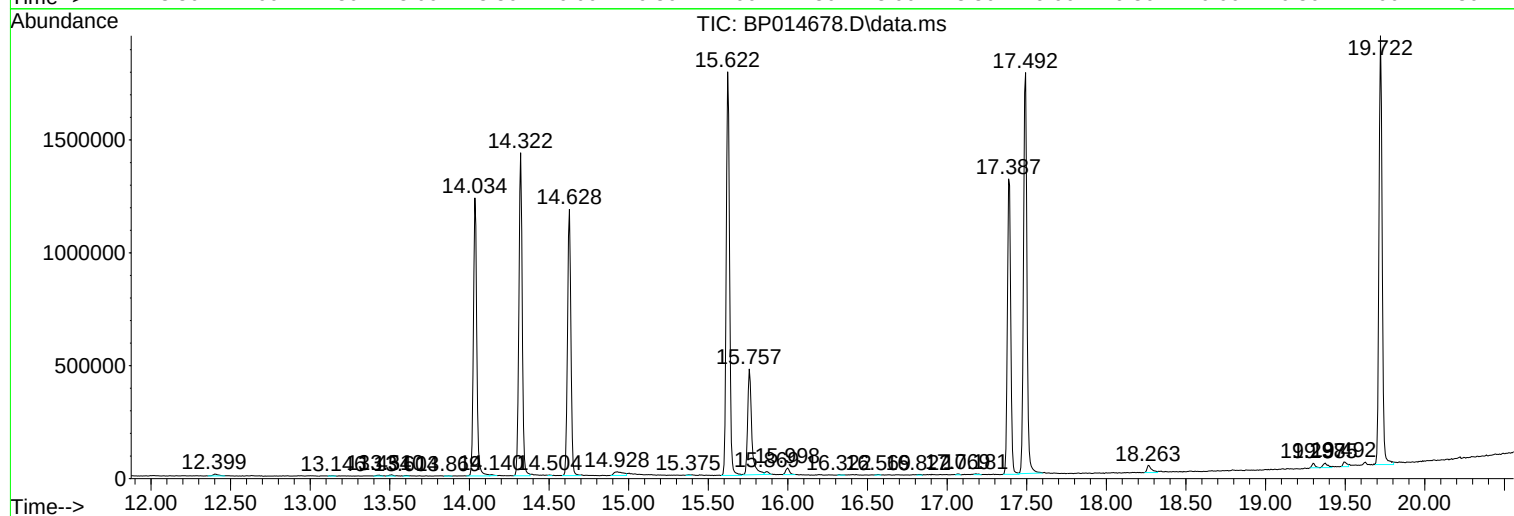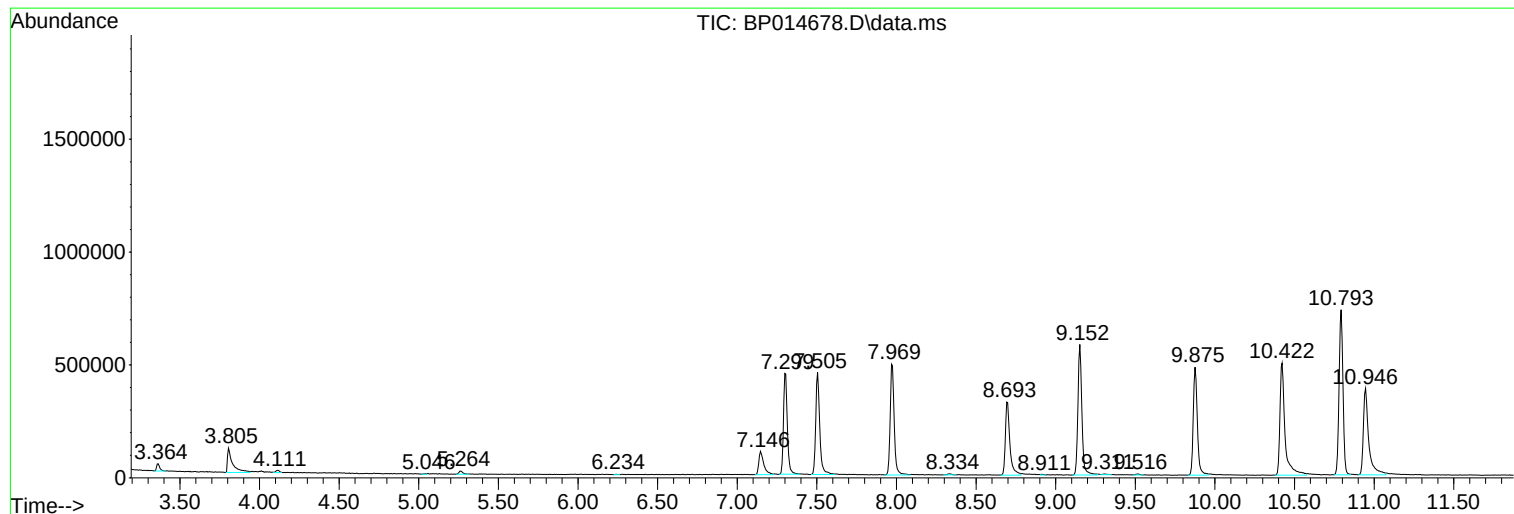

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014678.D
Acq On : 12 Apr 2023 17:48
Operator : CG/JU
Sample : 02251-19
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0MD7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014678.D
Acq On : 12 Apr 2023 17:48
Operator : CG/JU
Sample : 02251-19
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0MD7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc