

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014683.D
 Acq On : 12 Apr 2023 20:41
 Operator : CG/JU
 Sample : PB152055BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014683.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	25	29	35	rBV	30125	40874	1.83%	0.170%
2	3.793	100	103	125	rBV	256500	479617	21.45%	1.996%
3	4.111	154	157	164	rVB3	8374	12016	0.54%	0.050%
4	4.481	218	220	222	rBV2	2742	2340	0.10%	0.010%
5	6.569	571	575	578	rBV6	1571	2541	0.11%	0.011%
6	7.069	655	660	662	rVB6	1755	2608	0.12%	0.011%
7	7.140	665	672	693	rBV	356107	706461	31.60%	2.940%
8	7.299	693	699	712	rVV	328993	550140	24.60%	2.290%
9	7.387	712	714	717	rVB4	2131	2610	0.12%	0.011%
10	7.505	727	734	748	rBV	409766	730514	32.67%	3.040%
11	7.705	767	768	774	rVB6	2481	3031	0.14%	0.013%
12	7.969	807	813	827	rBV	378743	631933	28.26%	2.630%
13	8.581	913	917	920	rBV6	1452	2567	0.11%	0.011%
14	8.693	930	936	958	rBV	430107	851545	38.08%	3.544%
15	9.152	1006	1014	1027	rBV	386361	700558	31.33%	2.916%
16	9.875	1130	1137	1150	rBV	320383	594154	26.57%	2.473%
17	9.975	1153	1154	1160	rVB6	2746	4151	0.19%	0.017%
18	10.093	1172	1174	1180	rVB7	1718	3392	0.15%	0.014%
19	10.422	1222	1230	1254	rBV	330479	799767	35.77%	3.329%
20	10.569	1254	1255	1259	rVB4	4497	4363	0.20%	0.018%
21	10.793	1283	1293	1311	rBV	506361	897065	40.12%	3.734%
22	10.946	1311	1319	1339	rBV	277934	705330	31.55%	2.936%
23	11.263	1371	1373	1378	rVB6	2741	2898	0.13%	0.012%
24	11.528	1417	1418	1423	rVB5	1875	2413	0.11%	0.010%
25	12.410	1561	1568	1575	rBV10	5490	14307	0.64%	0.060%
26	12.828	1636	1639	1643	rBV5	2057	2269	0.10%	0.009%
27	13.510	1753	1755	1760	rVB6	3067	3665	0.16%	0.015%
28	13.598	1767	1770	1773	rBV5	2128	3167	0.14%	0.013%
29	14.034	1838	1844	1859	rBV	732134	1151531	51.50%	4.793%
30	14.322	1884	1893	1910	rBV	860341	1323596	59.20%	5.509%
31	14.628	1938	1945	1958	rBV	738614	1106331	49.48%	4.604%
32	14.881	1981	1988	2004	rBV2	87628	339564	15.19%	1.413%
33	15.451	2082	2085	2088	rBV5	1822	2249	0.10%	0.009%
34	15.622	2107	2114	2128	rBV	1112445	1635271	73.14%	6.806%
35	15.757	2131	2137	2152	rBV	311540	541381	24.21%	2.253%
36	15.951	2168	2170	2175	rVB5	1616	2532	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014683.D
 Acq On : 12 Apr 2023 20:41
 Operator : CG/JU
 Sample : PB152055BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	16.328	2230	2234	2235	rBV4	1849	2648	0.12%	0.011%
38	16.410	2245	2248	2254	rBV8	2439	4261	0.19%	0.018%
39	16.528	2265	2268	2269	rBV3	2072	2541	0.11%	0.011%
40	16.928	2332	2336	2337	rBV4	2183	2274	0.10%	0.009%
41	17.386	2408	2414	2424	rBV	887250	1268094	56.71%	5.278%
42	17.486	2425	2431	2447	rVV	1142087	1732669	77.49%	7.211%
43	17.739	2469	2474	2477	rBV7	2501	4381	0.20%	0.018%
44	18.510	2603	2605	2608	rBV4	2838	2870	0.13%	0.012%
45	19.298	2736	2739	2744	rBV5	12853	18922	0.85%	0.079%
46	19.722	2805	2811	2821	rBV	1433051	2011380	89.96%	8.371%
47	21.480	3105	3110	3122	rBV	874240	1430417	63.97%	5.953%
48	23.816	3500	3507	3518	rBV2	1062884	2235919	100.00%	9.306%
49	23.980	3529	3535	3547	rVB2	637195	1452124	64.95%	6.044%




Sum of corrected areas: 24027251

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014683.D
Acq On : 12 Apr 2023 20:41
Operator : CG/JU
Sample : PB152055BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

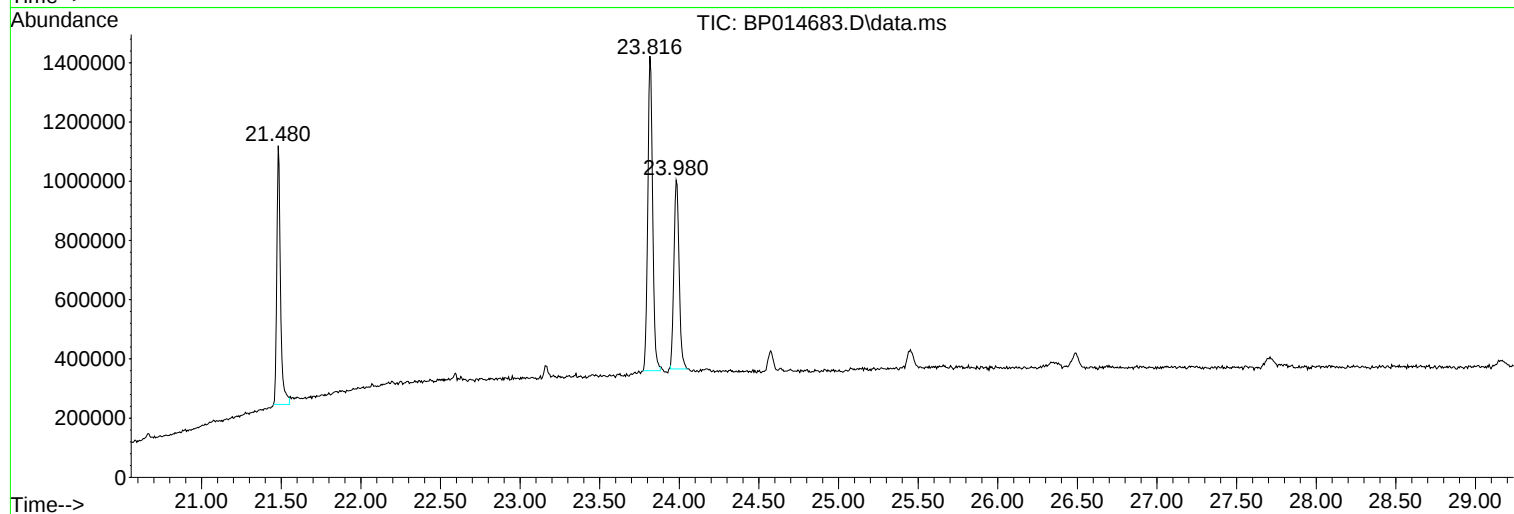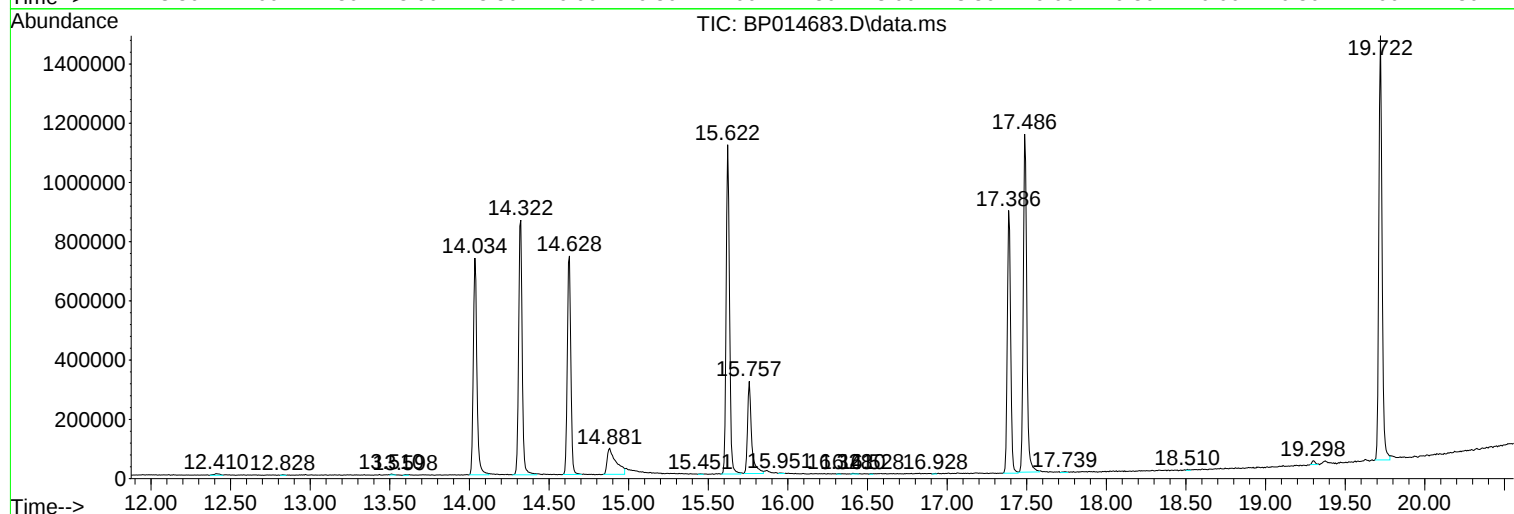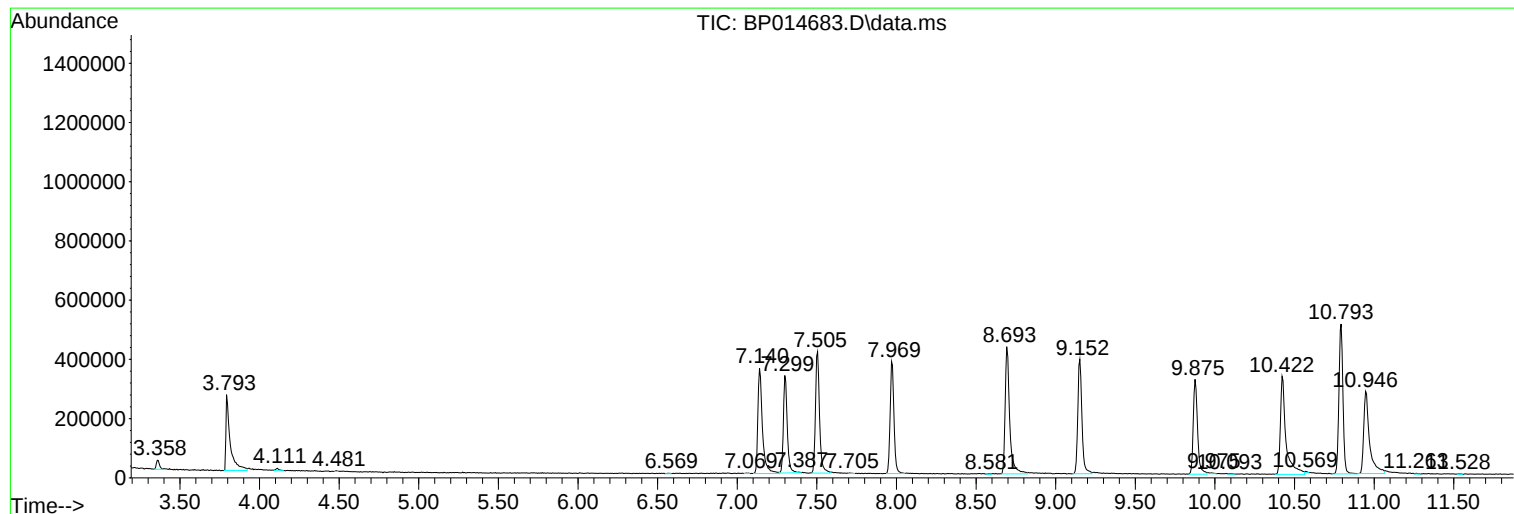

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014683.D
Acq On : 12 Apr 2023 20:41
Operator : CG/JU
Sample : PB152055BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014683.D
Acq On : 12 Apr 2023 20:41
Operator : CG/JU
Sample : PB152055BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc