

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014685.D
 Acq On : 12 Apr 2023 22:24
 Operator : CG/JU
 Sample : PB152042BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK042

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014685.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	26	29	36	rVB	34902	45643	2.00%	0.172%
2	3.793	101	103	120	rBV	295179	524562	22.97%	1.979%
3	4.105	154	156	163	rVB2	8010	12612	0.55%	0.048%
4	5.105	322	326	329	rBV5	2440	4102	0.18%	0.015%
5	5.269	352	354	357	rBV4	2313	2500	0.11%	0.009%
6	7.140	665	672	690	rBV	432208	810809	35.50%	3.058%
7	7.299	693	699	717	rVB	382825	633525	27.74%	2.390%
8	7.499	727	733	749	rBV	475175	831881	36.42%	3.138%
9	7.969	806	813	824	rBV	449115	741959	32.49%	2.799%
10	8.693	929	936	958	rBV	511500	975605	42.72%	3.680%
11	9.152	1006	1014	1030	rBV	452241	816444	35.75%	3.079%
12	9.875	1128	1137	1156	rBV	409825	729143	31.93%	2.750%
13	10.422	1223	1230	1255	rBV	398829	933891	40.89%	3.522%
14	10.640	1265	1267	1272	rVB6	2324	3511	0.15%	0.013%
15	10.787	1285	1292	1304	rBV	623572	1081650	47.36%	4.080%
16	10.946	1312	1319	1341	rBV	344969	838610	36.72%	3.163%
17	12.316	1546	1552	1553	rBV6	1478	2550	0.11%	0.010%
18	12.416	1561	1569	1574	rBV9	6165	15829	0.69%	0.060%
19	13.510	1752	1755	1759	rVB4	3349	4130	0.18%	0.016%
20	13.598	1768	1770	1774	rBV5	2464	3987	0.17%	0.015%
21	14.034	1837	1844	1859	rBV	841015	1272694	55.73%	4.800%
22	14.322	1885	1893	1909	rBV	953170	1464627	64.13%	5.524%
23	14.628	1938	1945	1957	rVB	805382	1239347	54.27%	4.675%
24	14.875	1980	1987	2015	rBV2	101379	448402	19.63%	1.691%
25	15.192	2038	2041	2043	rBV4	1994	2411	0.11%	0.009%
26	15.457	2081	2086	2090	rVB8	1645	2670	0.12%	0.010%
27	15.622	2107	2114	2126	rBV	1156445	1760116	77.07%	6.639%
28	15.757	2130	2137	2153	rBV	324182	594774	26.04%	2.243%
29	15.863	2153	2155	2160	rVB6	6277	8269	0.36%	0.031%
30	16.428	2244	2251	2254	rBV9	2528	5465	0.24%	0.021%
31	17.028	2350	2353	2356	rBV5	2356	3065	0.13%	0.012%
32	17.063	2356	2359	2361	rBV3	3285	4391	0.19%	0.017%
33	17.175	2375	2378	2383	rBV6	3100	4804	0.21%	0.018%
34	17.386	2408	2414	2425	rBV	975734	1401546	61.37%	5.286%
35	17.486	2425	2431	2446	rVV	1159185	1813346	79.40%	6.840%
36	17.757	2475	2477	2480	rBV4	2193	2375	0.10%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014685.D
Acq On : 12 Apr 2023 22:24
Operator : CG/JU
Sample : PB152042BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK042

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION

37	19.304	2736	2740	2743	rVB4	16483	20295	0.89%	0.077%
38	19.375	2748	2752	2760	rVB3	12526	25720	1.13%	0.097%
39	19.722	2805	2811	2822	rBV	1434298	2040949	89.36%	7.698%
40	21.480	3105	3110	3119	rBV	931637	1509312	66.09%	5.693%
41	23.816	3500	3507	3517	rVB2	1116920	2283853	100.00%	8.614%
42	23.980	3528	3535	3550	rVB2	679381	1591316	69.68%	6.002%




Sum of corrected areas: 26512690

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014685.D
Acq On : 12 Apr 2023 22:24
Operator : CG/JU
Sample : PB152042BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK042

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

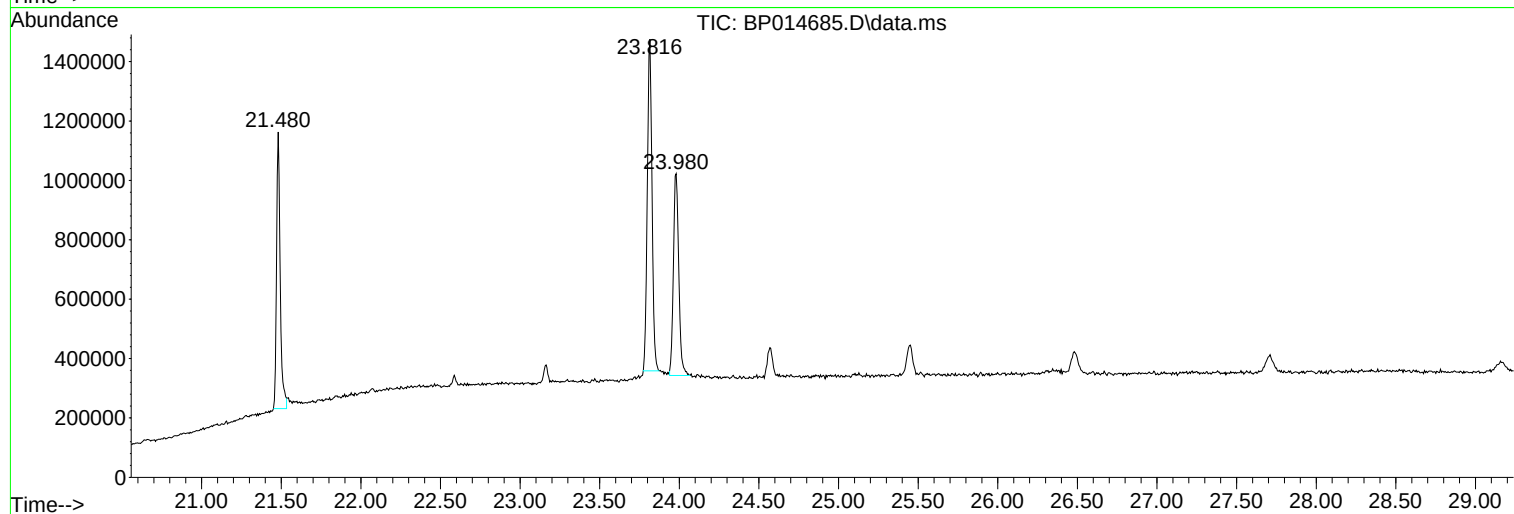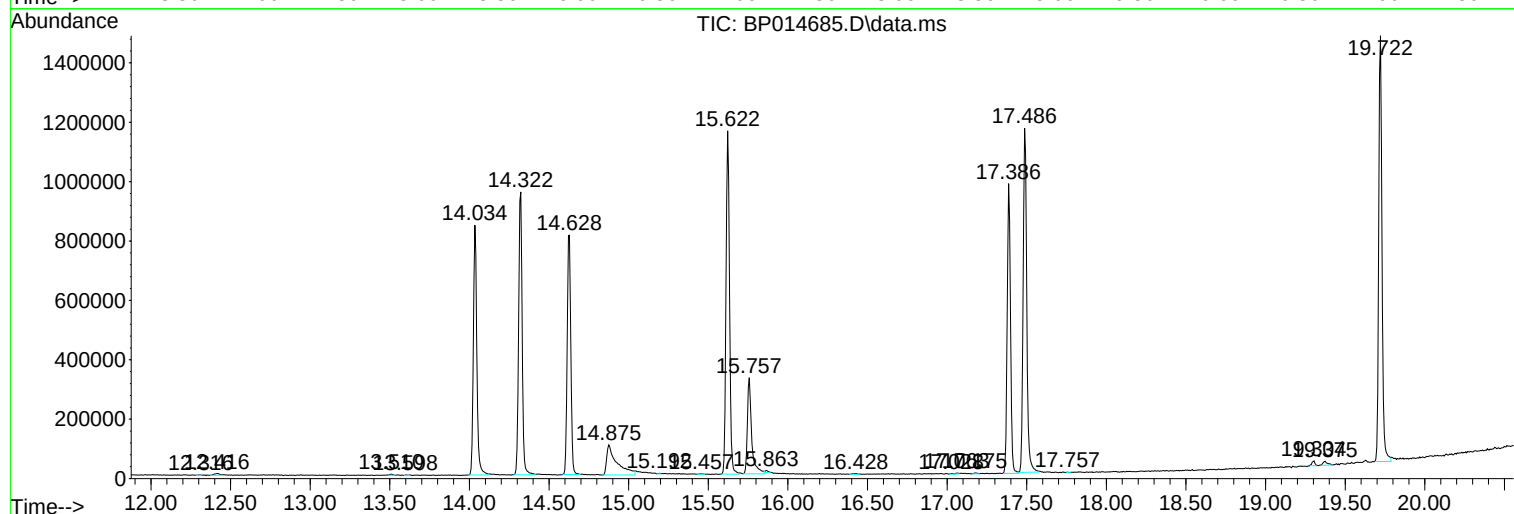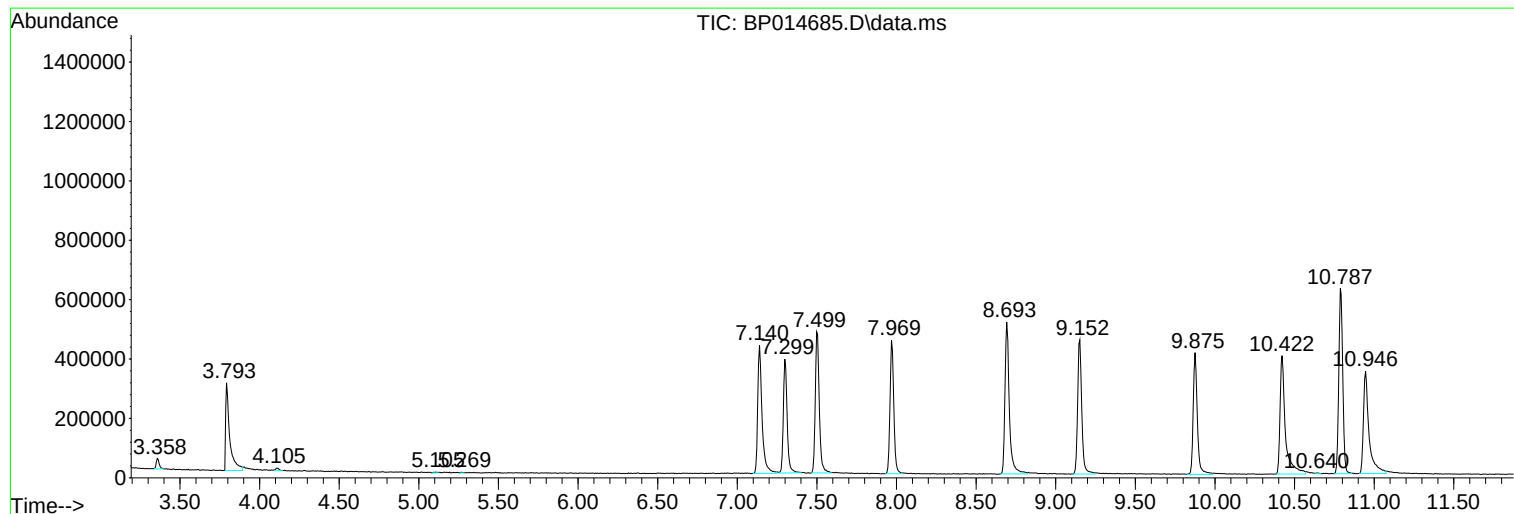

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014685.D
Acq On : 12 Apr 2023 22:24
Operator : CG/JU
Sample : PB152042BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK042

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014685.D
Acq On : 12 Apr 2023 22:24
Operator : CG/JU
Sample : PB152042BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK042

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------