

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014686.D
 Acq On : 12 Apr 2023 22:58
 Operator : CG/JU
 Sample : 02250-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014686.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	26	29	38	rBV	26365	36974	1.52%	0.153%
2	3.828	107	109	118	rBV	19761	46075	1.90%	0.191%
3	4.111	153	157	163	rVB	20549	31038	1.28%	0.128%
4	4.893	286	290	291	rBV3	3065	3176	0.13%	0.013%
5	5.899	459	461	466	rVB6	2713	2695	0.11%	0.011%
6	6.064	486	489	492	rBV5	2226	2995	0.12%	0.012%
7	7.152	666	674	686	rBV	70580	169660	6.98%	0.702%
8	7.299	693	699	713	rBV	361413	601862	24.76%	2.491%
9	7.416	718	719	723	rVB4	2327	2448	0.10%	0.010%
10	7.505	727	734	753	rBV	350327	654029	26.90%	2.707%
11	7.969	806	813	823	rBV	406643	679082	27.93%	2.811%
12	8.693	930	936	951	rBV	246463	486097	20.00%	2.012%
13	9.152	1007	1014	1028	rBV	435687	795800	32.73%	3.294%
14	9.287	1032	1037	1051	rVV10	12638	48680	2.00%	0.202%
15	9.510	1072	1075	1079	rVB6	2249	3257	0.13%	0.013%
16	9.875	1130	1137	1151	rBV	390384	692674	28.49%	2.867%
17	10.422	1223	1230	1261	rBV	363776	881353	36.25%	3.648%
18	10.787	1283	1292	1301	rBV	550748	935525	38.48%	3.872%
19	10.952	1312	1320	1345	rBV	131619	376568	15.49%	1.559%
20	11.140	1348	1352	1354	rVB5	1994	2829	0.12%	0.012%
21	11.352	1386	1388	1392	rBV5	1611	2832	0.12%	0.012%
22	12.116	1513	1518	1519	rBV5	2088	2729	0.11%	0.011%
23	12.157	1519	1525	1526	rBV5	2021	4150	0.17%	0.017%
24	12.404	1561	1567	1573	rVV7	5354	12210	0.50%	0.051%
25	12.722	1617	1621	1624	rBV6	1628	2787	0.11%	0.012%
26	12.910	1648	1653	1656	rBV6	2579	3600	0.15%	0.015%
27	12.975	1661	1664	1667	rBV5	2386	3424	0.14%	0.014%
28	13.122	1684	1689	1692	rVB6	1506	2436	0.10%	0.010%
29	13.228	1702	1707	1710	rVB7	3275	5380	0.22%	0.022%
30	14.034	1836	1844	1861	rBV	976156	1435117	59.03%	5.940%
31	14.181	1867	1869	1874	rVB6	2027	3018	0.12%	0.012%
32	14.275	1880	1885	1886	rBV5	2015	3568	0.15%	0.015%
33	14.316	1886	1892	1905	rVV2	1061817	1560856	64.20%	6.461%
34	14.622	1937	1944	1953	rBV	785333	1160737	47.75%	4.805%
35	14.698	1953	1957	1964	rVB6	11854	18058	0.74%	0.075%
36	14.875	1981	1987	1989	rBV6	2504	4388	0.18%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014686.D
 Acq On : 12 Apr 2023 22:58
 Operator : CG/JU
 Sample : 02250-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	14.928	1989	1996	1999	rBV7	11908	27304	1.12%	0.113%
38	15.034	2011	2014	2017	rVB4	4214	5129	0.21%	0.021%
39	15.075	2019	2021	2027	rVB7	2173	2759	0.11%	0.011%
40	15.298	2056	2059	2061	rBV4	4059	4907	0.20%	0.020%
41	15.404	2072	2077	2081	rBV6	4206	6624	0.27%	0.027%
42	15.440	2081	2083	2088	rVB4	4257	5561	0.23%	0.023%
43	15.622	2107	2114	2131	rBV	1321692	1936617	79.66%	8.016%
44	15.757	2131	2137	2153	rBV	376781	691245	28.43%	2.861%
45	16.687	2292	2295	2298	rBV5	2197	3514	0.14%	0.015%
46	16.975	2339	2344	2348	rBV7	4970	7967	0.33%	0.033%
47	17.386	2408	2414	2425	rVV	837359	1192778	49.06%	4.937%
48	17.486	2425	2431	2449	rVV	1431378	2165301	89.07%	8.963%
49	18.039	2520	2525	2532	rVB2	137798	169818	6.99%	0.703%
50	18.269	2560	2564	2571	rBV8	14035	29427	1.21%	0.122%
51	18.328	2571	2574	2577	rVV2	8379	9686	0.40%	0.040%
52	18.492	2600	2602	2607	rBV6	3208	5486	0.23%	0.023%
53	18.692	2634	2636	2638	rBV3	3442	3993	0.16%	0.017%
54	19.298	2735	2739	2742	rBV3	20065	25482	1.05%	0.105%
55	19.369	2747	2751	2756	rBV	16981	28542	1.17%	0.118%
56	19.498	2769	2773	2778	rBV7	15602	27918	1.15%	0.116%
57	19.716	2805	2810	2818	rBV	1619645	2277744	93.69%	9.428%
58	21.480	3105	3110	3122	rBV	755597	1202428	49.46%	4.977%
59	23.810	3500	3506	3518	rVB2	1183311	2431055	100.00%	10.063%
60	23.980	3529	3535	3544	rVB2	544832	1218931	50.14%	5.046%




Sum of corrected areas: 24158323

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014686.D
Acq On : 12 Apr 2023 22:58
Operator : CG/JU
Sample : 02250-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

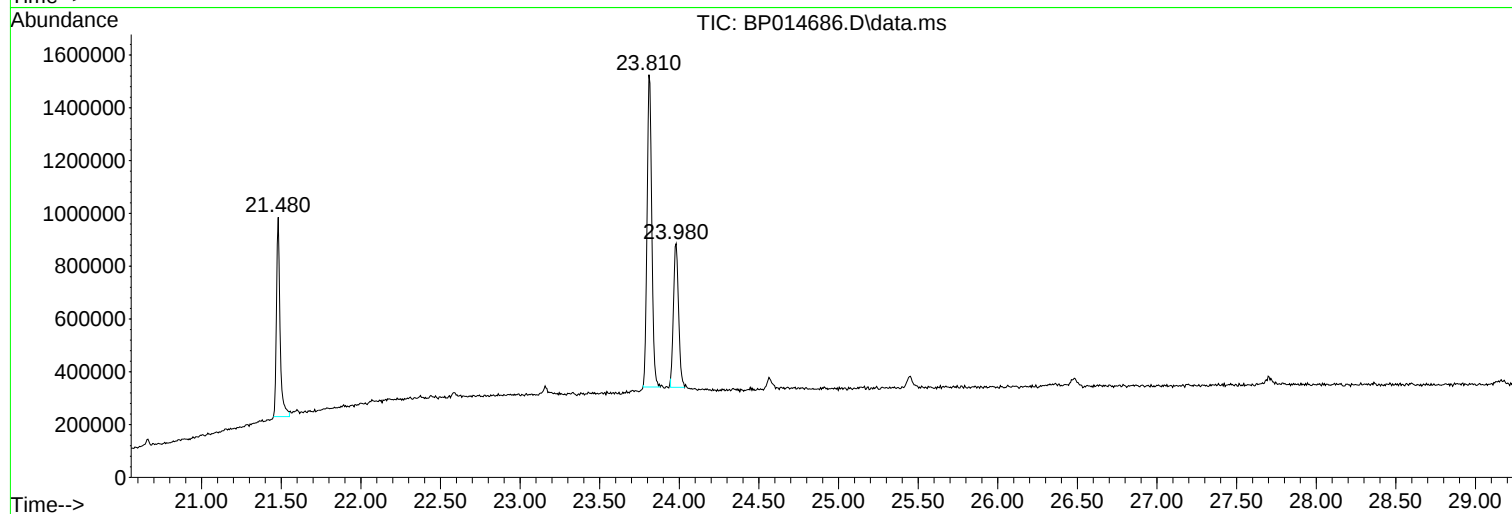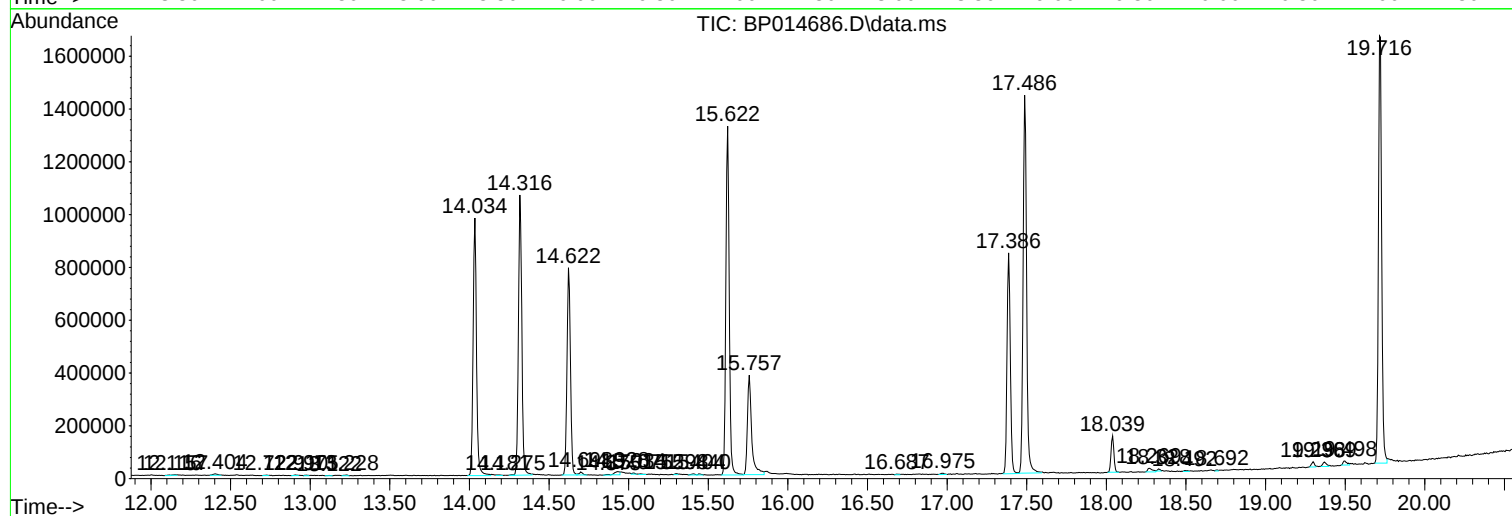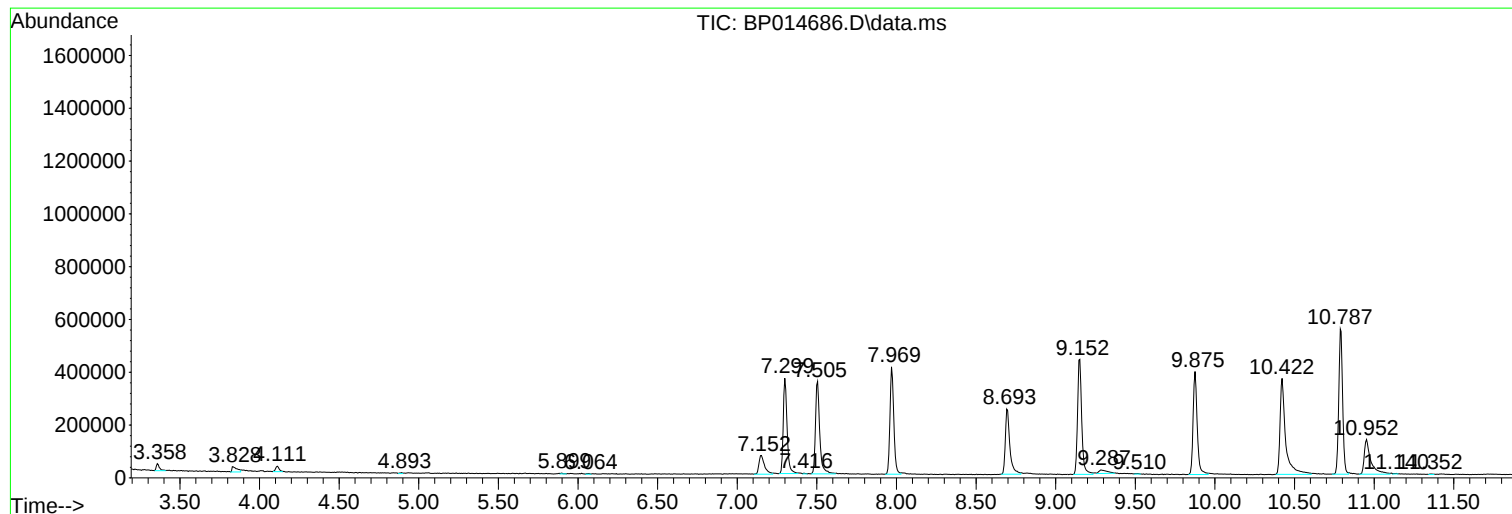

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014686.D
Acq On : 12 Apr 2023 22:58
Operator : CG/JU
Sample : 02250-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 7,9-Di-tert-butyl-1-oxaspiro... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
18.039	2.85 ng/ul	169818	Phenanthrene-d10	17.387

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	95		
2	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	87		
3	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	60		
4	2,5-Cyclohexadien-1-one, 2,6-bis...	232	C16H24O	006738-27-8	47		
5	Butylated Hydroxytoluene	220	C15H24O	000128-37-0	46		

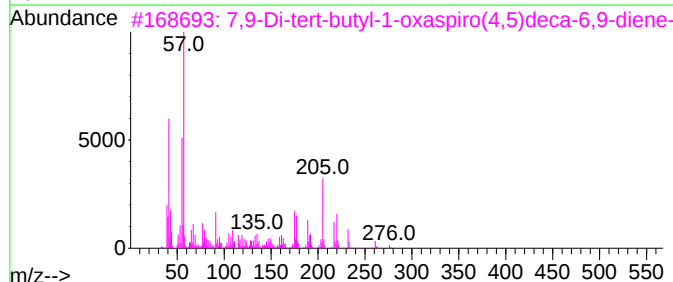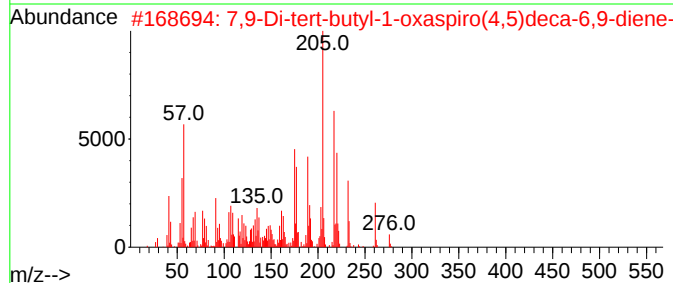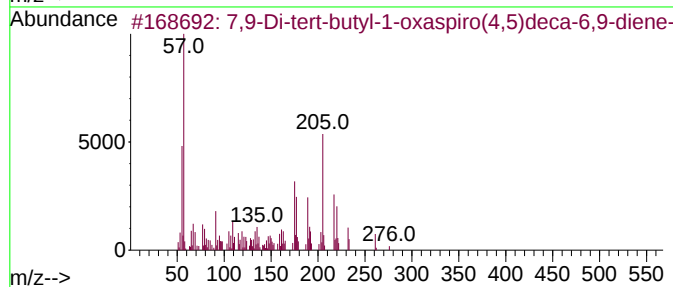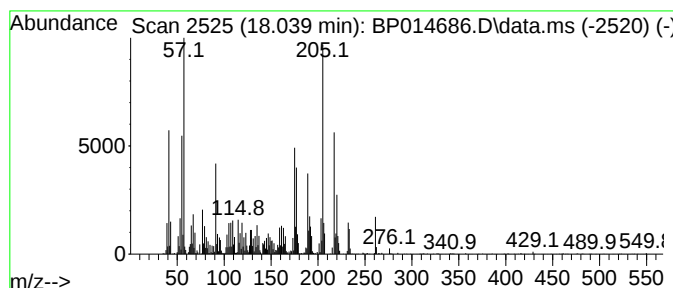

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014686.D
Acq On : 12 Apr 2023 22:58
Operator : CG/JU
Sample : 02250-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
7,9-Di-tert-but...	18.039	2.9	ng/u1	169818	4	17.387	1192780	20.0