

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014688.D
 Acq On : 13 Apr 2023 00:07
 Operator : CG/JU
 Sample : 02250-13
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014688.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	26	29	34	rBV	26539	33047	1.26%	0.141%
2	3.811	105	106	123	rBV	42865	107172	4.09%	0.457%
3	3.923	123	125	129	rVB5	4180	4390	0.17%	0.019%
4	4.111	153	157	162	rVB3	7778	11755	0.45%	0.050%
5	6.158	502	505	511	rBV6	2619	4548	0.17%	0.019%
6	7.152	668	674	689	rBV	72728	174855	6.68%	0.745%
7	7.299	693	699	717	rVV	366708	611196	23.33%	2.604%
8	7.505	726	734	750	rBV	348632	649046	24.78%	2.765%
9	7.969	804	813	826	rBV	364507	622347	23.76%	2.651%
10	8.693	928	936	952	rBV	229561	479233	18.30%	2.042%
11	9.152	1005	1014	1030	rBV	428950	791987	30.23%	3.374%
12	9.316	1037	1042	1052	rBV	3543	10219	0.39%	0.044%
13	9.511	1071	1075	1081	rVB8	3401	5490	0.21%	0.023%
14	9.875	1130	1137	1153	rBV	357518	663135	25.32%	2.825%
15	10.152	1180	1184	1187	rVB5	1667	2771	0.11%	0.012%
16	10.422	1223	1230	1259	rBV	349482	844867	32.25%	3.599%
17	10.787	1285	1292	1301	rBV	466244	816052	31.15%	3.476%
18	10.946	1312	1319	1342	rBV	264813	677483	25.86%	2.886%
19	11.093	1342	1344	1347	rVB4	3681	4114	0.16%	0.018%
20	11.722	1446	1451	1452	rBV4	1887	2845	0.11%	0.012%
21	12.010	1497	1500	1503	rBV4	2087	2879	0.11%	0.012%
22	12.410	1562	1568	1575	rBV9	6709	15534	0.59%	0.066%
23	13.428	1734	1741	1744	rBV7	3095	3728	0.14%	0.016%
24	14.034	1833	1844	1855	rBV	885794	1318248	50.32%	5.616%
25	14.140	1860	1862	1865	rVB4	4129	4239	0.16%	0.018%
26	14.316	1886	1892	1907	rBV	941747	1461452	55.79%	6.226%
27	14.416	1907	1909	1913	rVV5	3454	4734	0.18%	0.020%
28	14.622	1935	1944	1952	rBV	642496	941362	35.94%	4.010%
29	14.934	1989	1997	2000	rBV5	12441	34027	1.30%	0.145%
30	15.104	2025	2026	2036	rVB10	2758	6271	0.24%	0.027%
31	15.404	2073	2077	2080	rBV4	3613	5343	0.20%	0.023%
32	15.446	2081	2084	2089	rVB5	4961	7535	0.29%	0.032%
33	15.622	2107	2114	2130	rBV	1206479	1858163	70.94%	7.916%
34	15.757	2130	2137	2152	rBV	339770	627790	23.97%	2.674%
35	15.998	2172	2178	2183	rBV	24251	45639	1.74%	0.194%
36	16.116	2194	2198	2200	rVB5	2128	3056	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014688.D
 Acq On : 13 Apr 2023 00:07
 Operator : CG/JU
 Sample : 02250-13
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	16.157	2200	2205	2206	rBV5	1620	2851	0.11%	0.012%
38	16.381	2240	2243	2246	rBV5	1589	2871	0.11%	0.012%
39	16.410	2246	2248	2253	rVB6	2709	3112	0.12%	0.013%
40	16.510	2262	2265	2267	rBV4	2215	2843	0.11%	0.012%
41	16.716	2296	2300	2302	rBV4	2750	4461	0.17%	0.019%
42	16.816	2315	2317	2320	rBV3	2086	2747	0.10%	0.012%
43	16.934	2335	2337	2341	rVB4	2457	3747	0.14%	0.016%
44	17.281	2394	2396	2400	rBV5	2744	3281	0.13%	0.014%
45	17.387	2407	2414	2425	rBV	738224	1049642	40.07%	4.472%
46	17.487	2425	2431	2449	rVV	1360701	2018434	77.06%	8.599%
47	17.669	2458	2462	2463	rBV3	3682	3683	0.14%	0.016%
48	18.039	2523	2525	2530	rVB6	5261	6160	0.24%	0.026%
49	18.263	2559	2563	2571	rBV7	19863	41530	1.59%	0.177%
50	18.334	2572	2575	2578	rVB3	9893	12592	0.48%	0.054%
51	19.298	2736	2739	2746	rVB6	18604	25267	0.96%	0.108%
52	19.375	2748	2752	2757	rVV5	16421	26261	1.00%	0.112%
53	19.722	2805	2811	2821	rBV	1626848	2295886	87.65%	9.781%
54	21.480	3105	3110	3122	rBV2	743499	1198520	45.75%	5.106%
55	23.816	3500	3507	3520	rVB2	1272053	2619471	100.00%	11.159%
56	23.974	3528	3534	3549	rVB2	592652	1293987	49.40%	5.512%




Sum of corrected areas: 23473898

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014688.D
Acq On : 13 Apr 2023 00:07
Operator : CG/JU
Sample : 02250-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

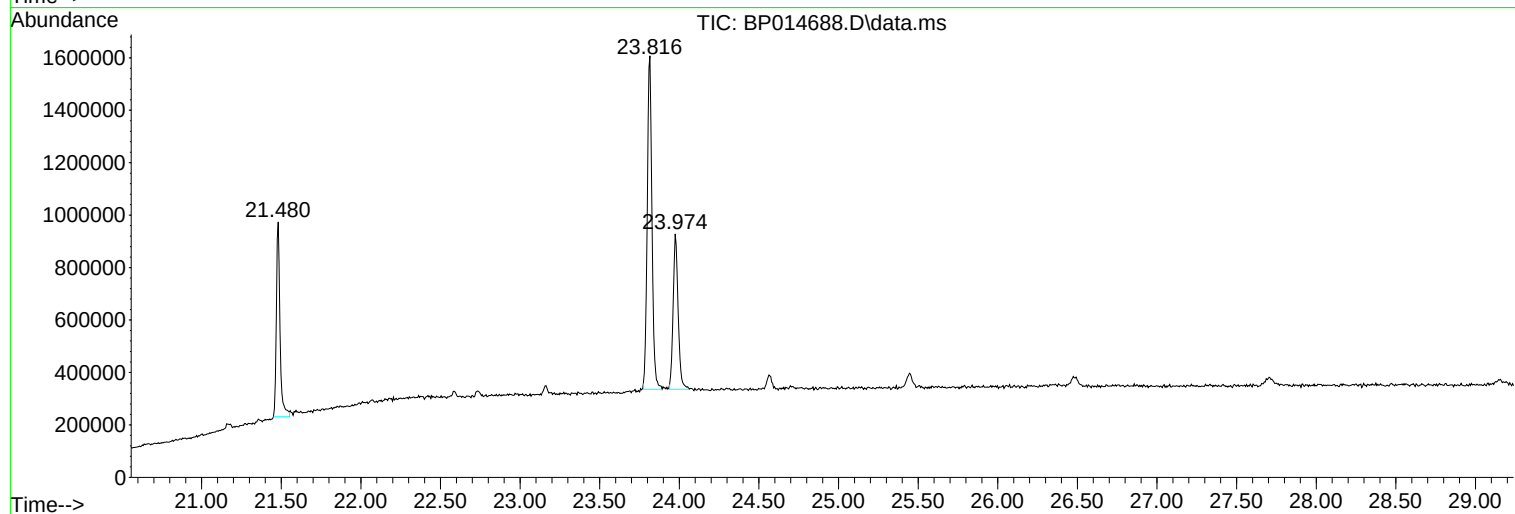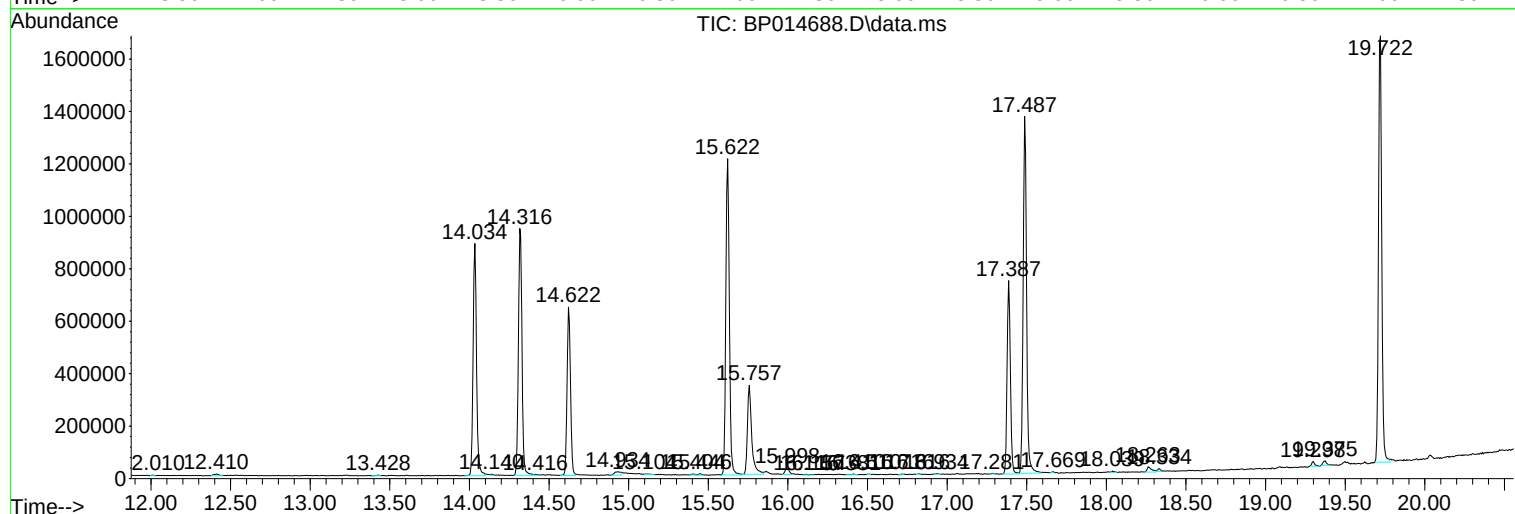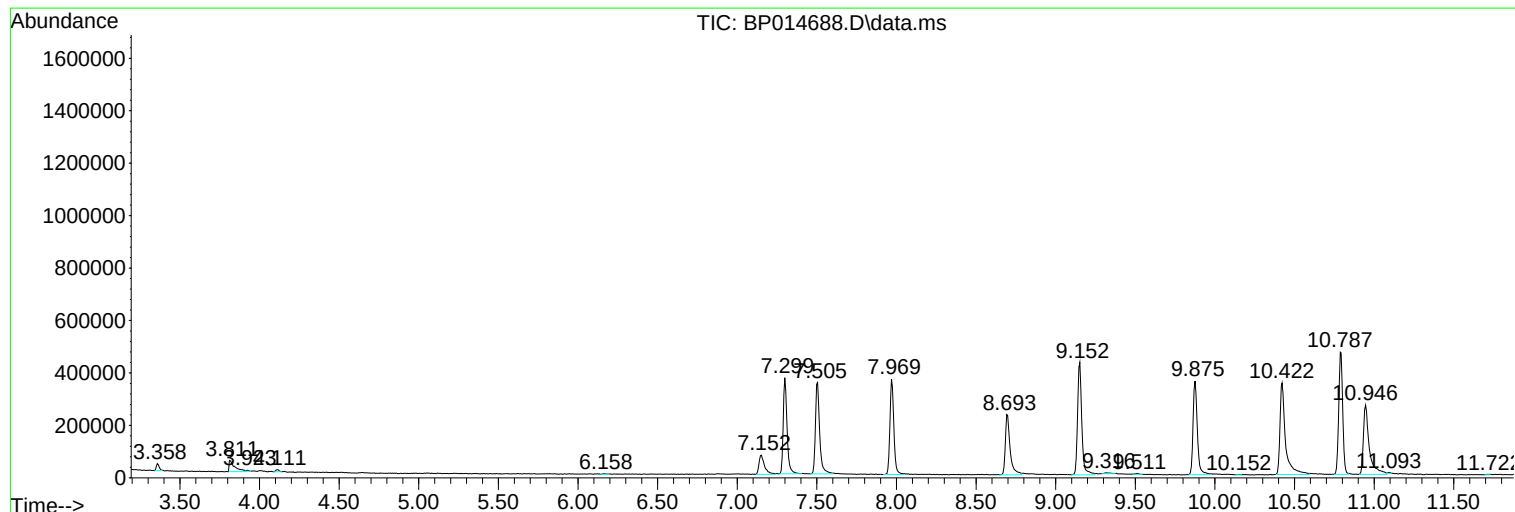

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014688.D
Acq On : 13 Apr 2023 00:07
Operator : CG/JU
Sample : 02250-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014688.D
Acq On : 13 Apr 2023 00:07
Operator : CG/JU
Sample : 02250-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
