

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014689.D
 Acq On : 13 Apr 2023 00:41
 Operator : CG/JU
 Sample : 02250-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014689.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	19	23	27	rBV	130710	169533	6.94%	0.755%
2	3.358	27	29	33	rVV	26504	34105	1.40%	0.152%
3	3.393	33	35	41	rVB5	8703	12147	0.50%	0.054%
4	3.634	74	76	80	rVB4	6457	8772	0.36%	0.039%
5	3.817	104	107	119	rBV	39142	85617	3.51%	0.381%
6	3.999	136	138	141	rBV4	3366	3930	0.16%	0.018%
7	4.111	154	157	160	rVB3	6824	8891	0.36%	0.040%
8	4.223	174	176	179	rVB4	2893	2795	0.11%	0.012%
9	4.646	241	248	265	rBV	535685	805495	32.98%	3.587%
10	5.775	435	440	443	rBV7	1307	2458	0.10%	0.011%
11	7.152	665	674	687	rBV2	57091	139795	5.72%	0.623%
12	7.299	693	699	712	rBV	298228	497899	20.39%	2.217%
13	7.505	727	734	750	rBV	284483	550017	22.52%	2.450%
14	7.969	806	813	825	rBV	338984	567015	23.22%	2.525%
15	8.122	837	839	845	rVB7	1882	3119	0.13%	0.014%
16	8.346	874	877	883	rBV7	1984	2732	0.11%	0.012%
17	8.699	931	937	948	rBV	187654	378061	15.48%	1.684%
18	9.152	1006	1014	1033	rBV	376377	709830	29.07%	3.161%
19	9.510	1072	1075	1081	rVB3	5264	7630	0.31%	0.034%
20	9.875	1130	1137	1152	rBV	310389	570784	23.37%	2.542%
21	10.422	1221	1230	1253	rBV	301889	729089	29.86%	3.247%
22	10.787	1285	1292	1304	rBV	447824	779655	31.93%	3.472%
23	10.946	1312	1319	1337	rBV	212324	528918	21.66%	2.356%
24	12.210	1531	1534	1538	rVB5	2115	2693	0.11%	0.012%
25	12.404	1561	1567	1577	rBV7	4872	12860	0.53%	0.057%
26	13.428	1738	1741	1744	rVB4	3532	3789	0.16%	0.017%
27	14.034	1837	1844	1858	rBV	802791	1211096	49.59%	5.394%
28	14.316	1884	1892	1907	rBV2	844340	1317446	53.95%	5.867%
29	14.504	1920	1924	1928	rVB6	2973	5522	0.23%	0.025%
30	14.622	1936	1944	1955	rBV	616912	935578	38.31%	4.167%
31	14.934	1991	1997	1999	rBV3	10349	19251	0.79%	0.086%
32	15.622	2107	2114	2131	rBV	1093995	1670821	68.42%	7.441%
33	15.757	2131	2137	2152	rVV	314705	582487	23.85%	2.594%
34	15.869	2152	2156	2161	rVB8	8735	16376	0.67%	0.073%
35	15.992	2172	2177	2187	rVB	37821	62482	2.56%	0.278%
36	16.410	2246	2248	2251	rVB4	3104	2699	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014689.D
 Acq On : 13 Apr 2023 00:41
 Operator : CG/JU
 Sample : 02250-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	16.540	2264	2270	2275	rBV10	2098	4652	0.19%	0.021%
38	16.628	2283	2285	2288	rBV4	2100	2542	0.10%	0.011%
39	16.781	2307	2311	2312	rBV4	2156	2793	0.11%	0.012%
40	16.804	2312	2315	2316	rBV2	2934	2658	0.11%	0.012%
41	17.116	2366	2368	2370	rBV3	2675	2537	0.10%	0.011%
42	17.169	2376	2377	2384	rVB6	4258	6301	0.26%	0.028%
43	17.387	2407	2414	2424	rBV	721763	1032806	42.29%	4.600%
44	17.486	2424	2431	2443	rBV	1250865	1849587	75.74%	8.237%
45	18.257	2558	2562	2571	rBV5	29308	60721	2.49%	0.270%
46	18.328	2571	2574	2580	rVB2	9610	13781	0.56%	0.061%
47	19.292	2735	2738	2745	rBV5	15872	25879	1.06%	0.115%
48	19.369	2748	2751	2759	rVV3	17121	30445	1.25%	0.136%
49	19.716	2805	2810	2819	rBV	1620990	2154153	88.21%	9.594%
50	21.480	3105	3110	3119	rBV	705570	1125230	46.08%	5.011%
51	23.810	3500	3506	3520	rVB2	1179241	2442042	100.00%	10.876%
52	23.974	3528	3534	3548	rVB2	547503	1256489	51.45%	5.596%




Sum of corrected areas: 22454003

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014689.D
Acq On : 13 Apr 2023 00:41
Operator : CG/JU
Sample : 02250-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

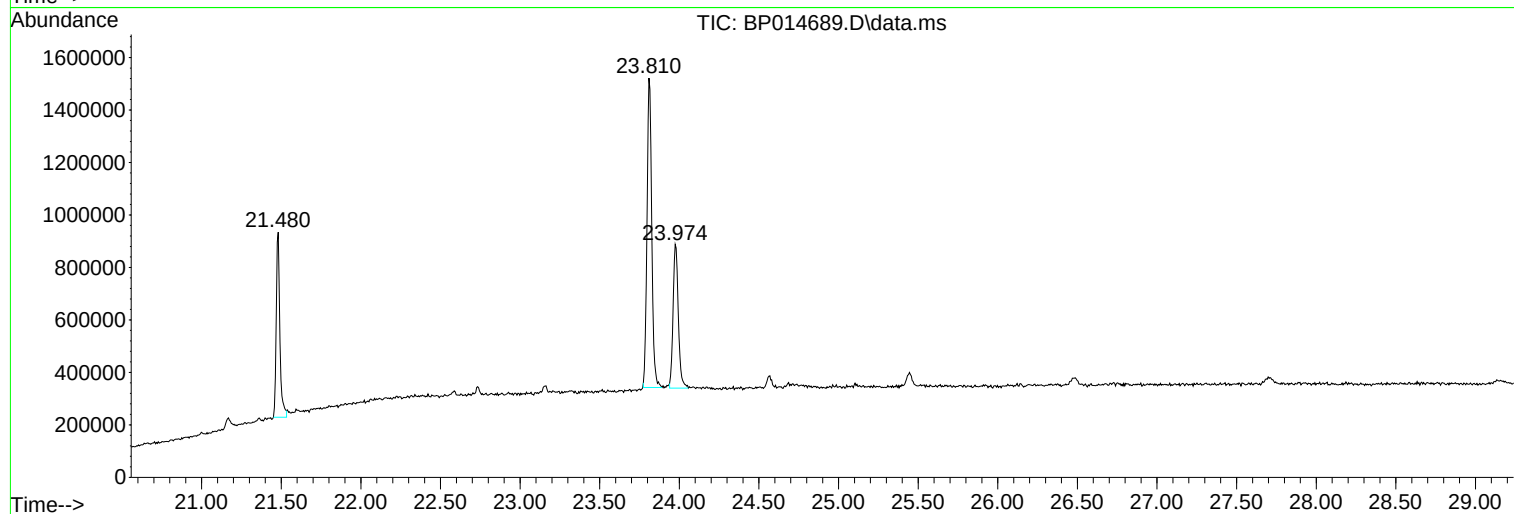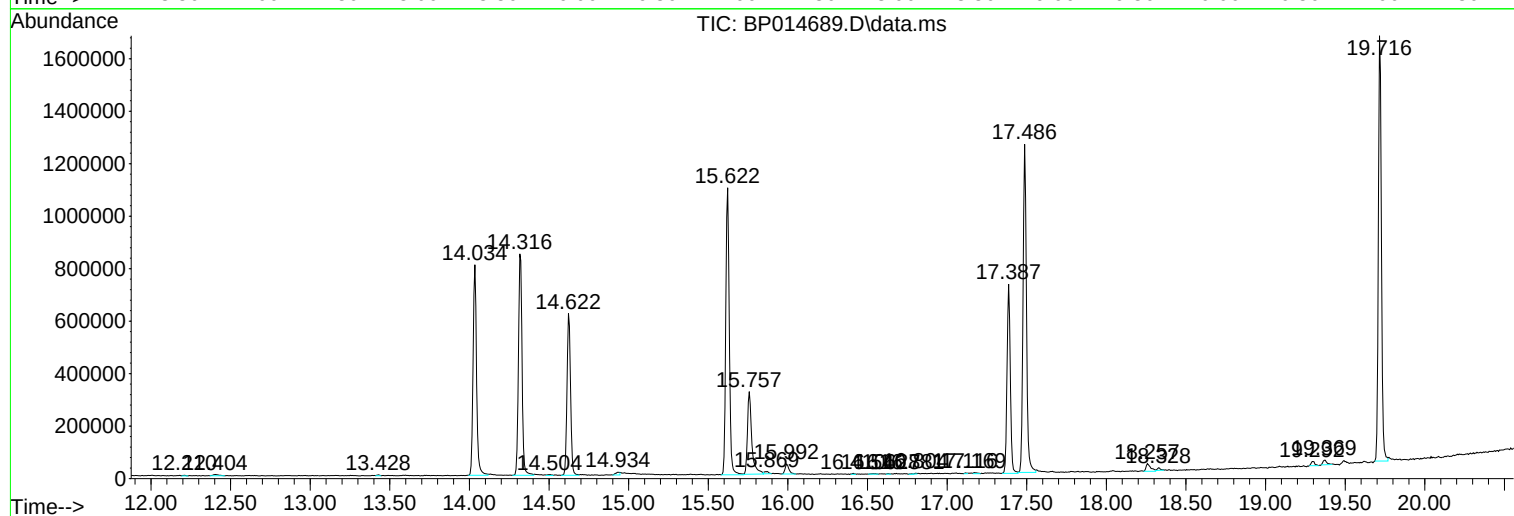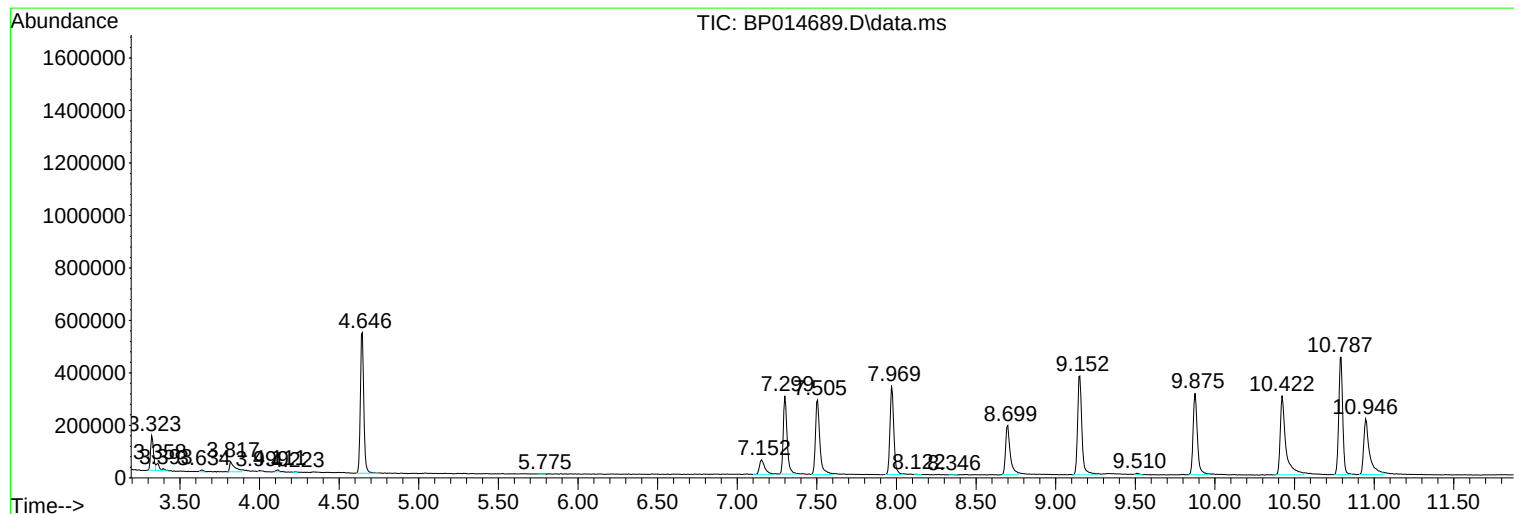

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014689.D
Acq On : 13 Apr 2023 00:41
Operator : CG/JU
Sample : 02250-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014689.D
Acq On : 13 Apr 2023 00:41
Operator : CG/JU
Sample : 02250-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
