

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014690.D
 Acq On : 13 Apr 2023 01:15
 Operator : CG/JU
 Sample : 02250-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014690.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	26	29	37	rVB	28322	40521	1.48%	0.154%
2	3.811	104	106	119	rBV	55176	100311	3.67%	0.380%
3	4.111	153	157	161	rVB4	8366	11827	0.43%	0.045%
4	4.487	218	221	227	rVB3	11975	16685	0.61%	0.063%
5	4.646	244	248	252	rBV7	3713	5063	0.19%	0.019%
6	7.146	668	673	686	rBV2	76175	174956	6.40%	0.664%
7	7.299	693	699	712	rBV	380839	616468	22.55%	2.338%
8	7.452	721	725	727	rBV5	3463	3527	0.13%	0.013%
9	7.505	727	734	749	rBV	361783	654646	23.95%	2.483%
10	7.969	806	813	824	rBV	405786	670476	24.53%	2.543%
11	8.693	930	936	956	rBV	244926	485641	17.77%	1.842%
12	8.816	956	957	963	rVB6	2403	3051	0.11%	0.012%
13	9.152	1007	1014	1029	rBV	469690	854317	31.25%	3.240%
14	9.322	1038	1043	1045	rBV6	3064	6263	0.23%	0.024%
15	9.510	1070	1075	1081	rVV2	8156	13726	0.50%	0.052%
16	9.875	1130	1137	1152	rBV	405656	739231	27.04%	2.804%
17	10.416	1222	1229	1250	rBV	410999	933603	34.15%	3.541%
18	10.787	1283	1292	1307	rBV	552738	948999	34.72%	3.599%
19	10.946	1312	1319	1339	rBV	260722	636976	23.30%	2.416%
20	11.687	1441	1445	1446	rBV3	2709	2879	0.11%	0.011%
21	12.193	1528	1531	1535	rBV6	2468	3789	0.14%	0.014%
22	12.399	1559	1566	1572	rBV3	7548	15060	0.55%	0.057%
23	12.975	1661	1664	1671	rBV9	1439	3710	0.14%	0.014%
24	13.075	1676	1681	1683	rBV6	1651	2819	0.10%	0.011%
25	13.222	1703	1706	1713	rVB9	1941	3779	0.14%	0.014%
26	13.422	1736	1740	1744	rBV4	4964	7196	0.26%	0.027%
27	13.516	1751	1756	1759	rBV7	2257	3749	0.14%	0.014%
28	14.034	1836	1844	1856	rBV	1049103	1525518	55.81%	5.786%
29	14.128	1859	1860	1866	rVB6	3528	5307	0.19%	0.020%
30	14.269	1881	1884	1886	rBV4	2985	3874	0.14%	0.015%
31	14.316	1886	1892	1904	rVV2	1145783	1715134	62.74%	6.505%
32	14.622	1937	1944	1954	rBV	771679	1159790	42.43%	4.399%
33	14.863	1979	1985	1986	rBV6	2825	3722	0.14%	0.014%
34	14.928	1989	1996	2001	rBV8	14561	45059	1.65%	0.171%
35	15.251	2049	2051	2055	rVB5	2173	2742	0.10%	0.010%
36	15.404	2074	2077	2079	rVV3	2936	3079	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014690.D
 Acq On : 13 Apr 2023 01:15
 Operator : CG/JU
 Sample : 02250-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	15.445	2081	2084	2090	rVB4	6643	8785	0.32%	0.033%
38	15.569	2101	2105	2107	rBV5	2994	4543	0.17%	0.017%
39	15.622	2107	2114	2130	rVV	1455881	2123938	77.70%	8.055%
40	15.757	2130	2137	2152	rVV	397602	709842	25.97%	2.692%
41	15.857	2152	2154	2161	rVB8	8591	16725	0.61%	0.063%
42	15.992	2171	2177	2184	rBV	67921	105913	3.87%	0.402%
43	16.675	2288	2293	2297	rBV7	4509	6467	0.24%	0.025%
44	16.863	2323	2325	2328	rVB3	3020	3409	0.12%	0.013%
45	16.928	2328	2336	2341	rBV3	7980	17806	0.65%	0.068%
46	17.063	2355	2359	2364	rVB8	2558	4518	0.17%	0.017%
47	17.122	2365	2369	2372	rBV5	3228	4212	0.15%	0.016%
48	17.157	2372	2375	2377	rBV4	2123	2776	0.10%	0.011%
49	17.387	2408	2414	2424	rBV	924651	1272514	46.55%	4.826%
50	17.486	2425	2431	2451	rVB	1482379	2235698	81.79%	8.479%
51	17.669	2458	2462	2464	rBV4	4833	6714	0.25%	0.025%
52	18.257	2558	2562	2569	rBV3	62983	108386	3.96%	0.411%
53	18.334	2572	2575	2582	rVB	12268	19515	0.71%	0.074%
54	19.092	2700	2704	2708	rBV7	7614	15129	0.55%	0.057%
55	19.298	2736	2739	2746	rBV5	19705	26189	0.96%	0.099%
56	19.369	2748	2751	2757	rVV4	17360	30910	1.13%	0.117%
57	19.492	2768	2772	2781	rBV8	33049	68152	2.49%	0.258%
58	19.722	2805	2811	2825	rBV	1834447	2506925	91.71%	9.508%
59	21.163	3053	3056	3065	rBV4	61729	127730	4.67%	0.484%
60	21.480	3105	3110	3122	rBV	850578	1317251	48.19%	4.996%
61	23.816	3500	3507	3521	rBV2	1314605	2733608	100.00%	10.368%
62	23.974	3529	3534	3551	rVB2	673643	1465604	53.61%	5.559%




Sum of corrected areas: 26366752

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014690.D
Acq On : 13 Apr 2023 01:15
Operator : CG/JU
Sample : 02250-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

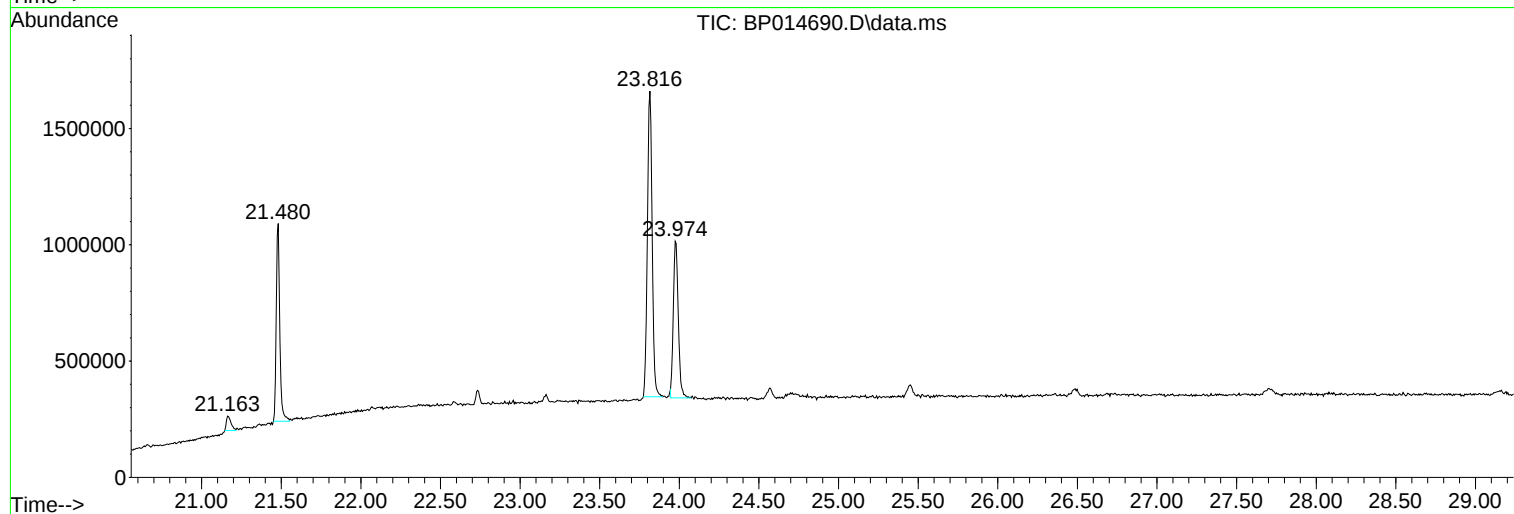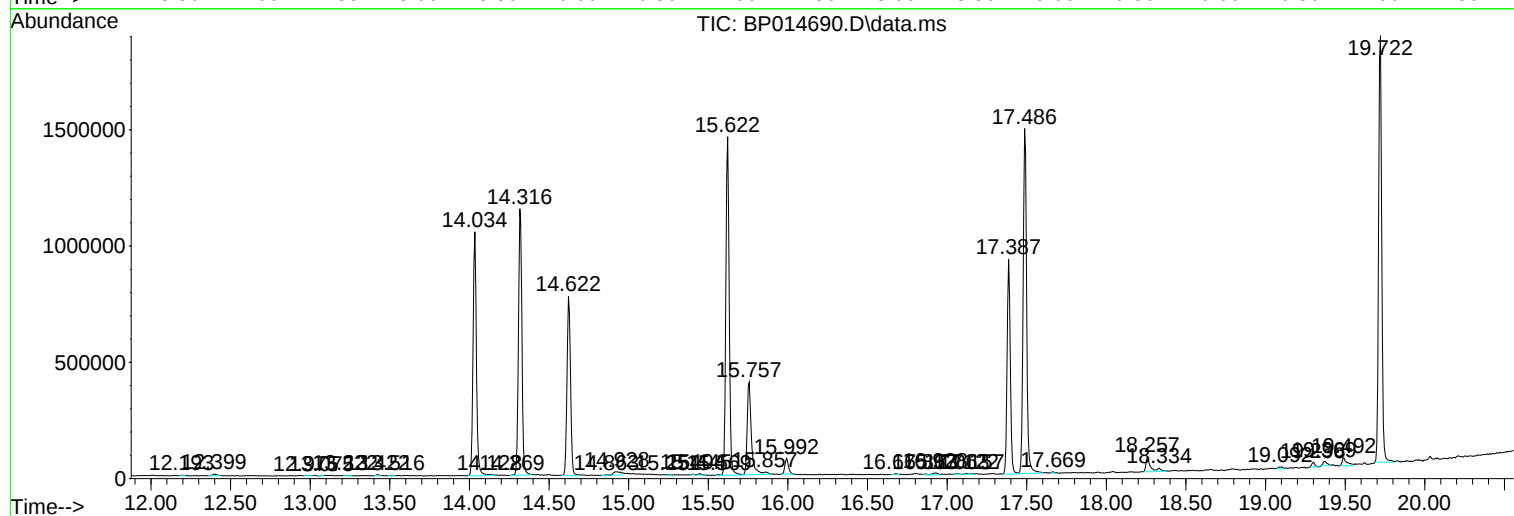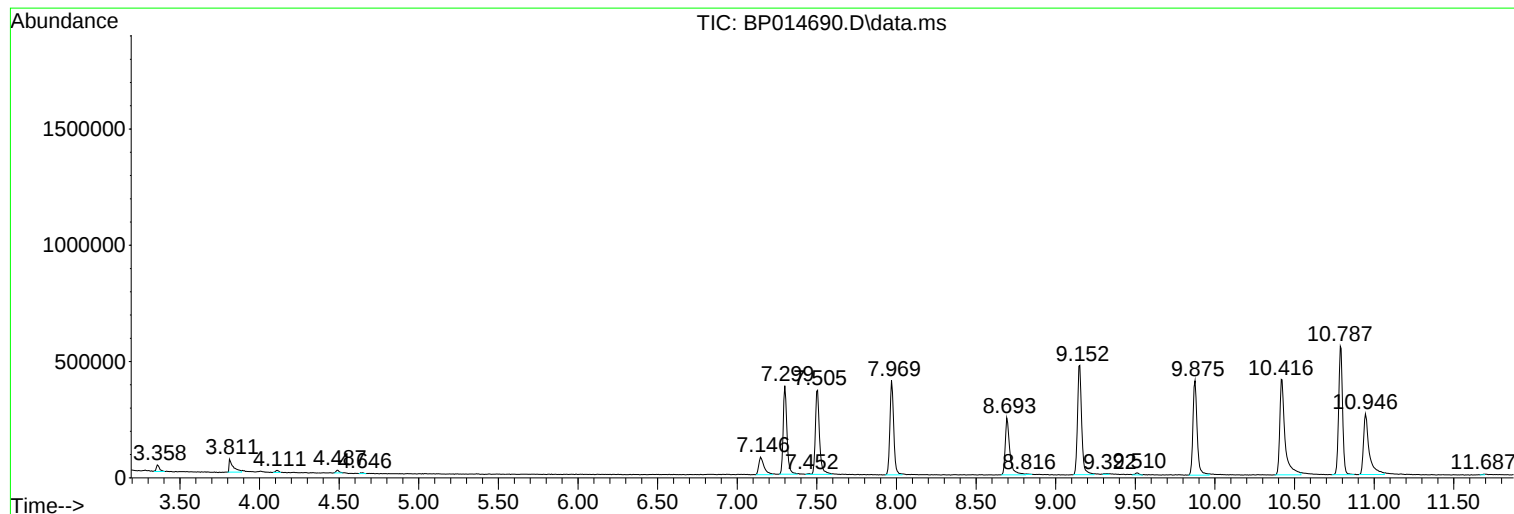

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014690.D
Acq On : 13 Apr 2023 01:15
Operator : CG/JU
Sample : 02250-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014690.D
Acq On : 13 Apr 2023 01:15
Operator : CG/JU
Sample : 02250-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc