

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014695.D
 Acq On : 13 Apr 2023 04:39
 Operator : CG/JU
 Sample : PB152057BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK057

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014695.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	25	29	38	rVB	38654	56988	2.31%	0.184%
2	3.793	100	103	123	rBV	318508	568438	23.05%	1.831%
3	4.111	154	157	166	rVB4	9678	16927	0.69%	0.055%
4	4.440	211	213	218	rVB6	2976	3364	0.14%	0.011%
5	4.511	223	225	228	rBV4	3082	2674	0.11%	0.009%
6	5.858	452	454	458	rVB4	2273	3091	0.13%	0.010%
7	6.463	554	557	561	rBV6	1992	2786	0.11%	0.009%
8	7.134	665	671	691	rBV	444856	878246	35.62%	2.829%
9	7.299	693	699	712	rVB	416725	671975	27.25%	2.164%
10	7.499	725	733	750	rBV	518183	890499	36.11%	2.868%
11	7.757	775	777	781	rVB5	2583	2542	0.10%	0.008%
12	7.969	806	813	824	rBV	481051	798026	32.36%	2.570%
13	8.187	847	850	853	rBV4	2310	2741	0.11%	0.009%
14	8.687	929	935	959	rBV	557194	1080795	43.83%	3.481%
15	9.146	1003	1013	1025	rBV	527529	907311	36.80%	2.922%
16	9.869	1126	1136	1152	rBV	440072	818353	33.19%	2.636%
17	10.416	1221	1229	1252	rBV	490717	1067859	43.31%	3.439%
18	10.787	1284	1292	1303	rBV	662319	1121236	45.47%	3.611%
19	10.940	1311	1318	1348	rBV	418325	992914	40.27%	3.198%
20	12.410	1563	1568	1573	rBV7	6573	14579	0.59%	0.047%
21	12.934	1654	1657	1659	rBV3	1800	2501	0.10%	0.008%
22	13.516	1749	1756	1759	rBV8	1963	3351	0.14%	0.011%
23	13.604	1767	1771	1775	rVB7	2263	3058	0.12%	0.010%
24	13.828	1805	1809	1814	rBV6	1654	2830	0.11%	0.009%
25	14.034	1836	1844	1860	rBV	1176524	1785831	72.43%	5.752%
26	14.316	1885	1892	1910	rBV	1347613	1963530	79.63%	6.324%
27	14.622	1937	1944	1956	rBV	1040797	1545345	62.67%	4.977%
28	14.869	1978	1986	2009	rBV	137077	567191	23.00%	1.827%
29	15.622	2107	2114	2128	rBV	1576762	2394438	97.11%	7.712%
30	15.751	2130	2136	2151	rVV	455261	792060	32.12%	2.551%
31	15.863	2153	2155	2161	rVB7	11087	16243	0.66%	0.052%
32	16.310	2229	2231	2234	rBV4	2366	2515	0.10%	0.008%
33	16.410	2245	2248	2253	rVB7	2561	3640	0.15%	0.012%
34	17.122	2366	2369	2372	rBV5	1723	2716	0.11%	0.009%
35	17.175	2375	2378	2380	rBV4	2428	2920	0.12%	0.009%
36	17.275	2391	2395	2399	rBV6	1800	3738	0.15%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014695.D
 Acq On : 13 Apr 2023 04:39
 Operator : CG/JU
 Sample : PB152057BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK057

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	17.386	2407	2414	2424	rBV	1182626	1666766	67.60%	5.368%
38	17.486	2424	2431	2444	rBV	1600100	2396199	97.18%	7.718%
39	18.345	2575	2577	2579	rBV3	2868	3139	0.13%	0.010%
40	19.298	2735	2739	2745	rVB7	18392	28074	1.14%	0.090%
41	19.369	2748	2751	2755	rBV2	13464	20480	0.83%	0.066%
42	19.716	2805	2810	2822	rBV	1684551	2418522	98.08%	7.790%
43	21.480	3105	3110	3123	rBV	904557	1522956	61.76%	4.905%
44	23.810	3500	3506	3521	rVB2	1163094	2465758	100.00%	7.942%
45	23.974	3528	3534	3547	rVB2	716804	1533045	62.17%	4.938%




Sum of corrected areas: 31048190

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014695.D
Acq On : 13 Apr 2023 04:39
Operator : CG/JU
Sample : PB152057BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK057

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

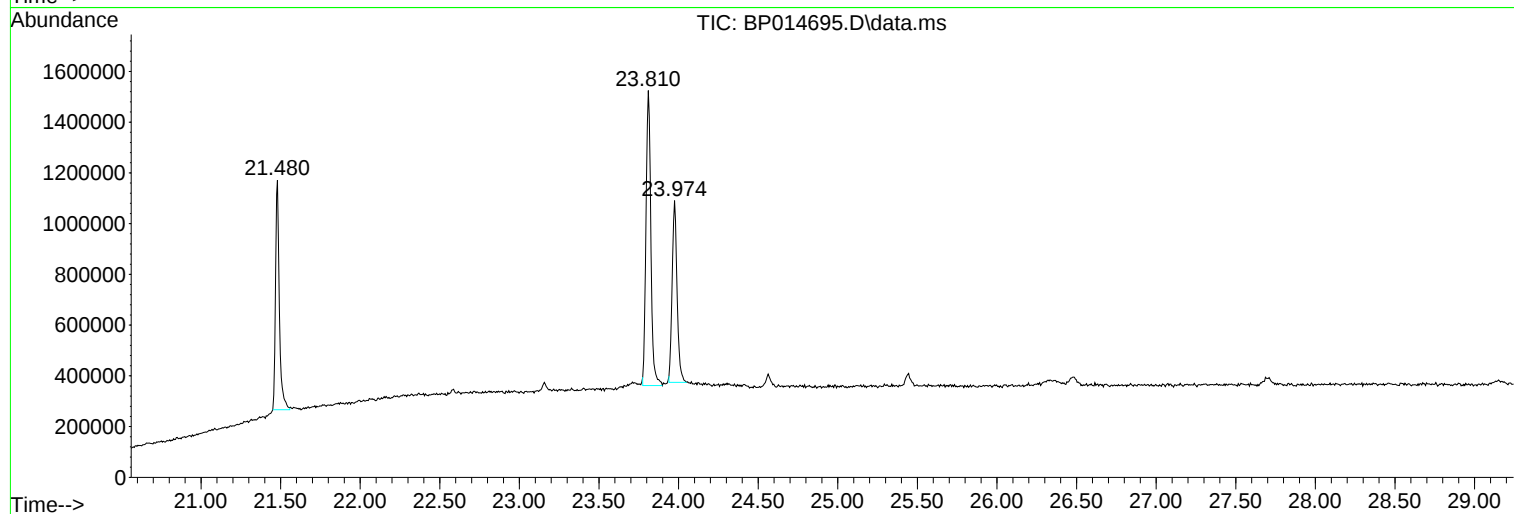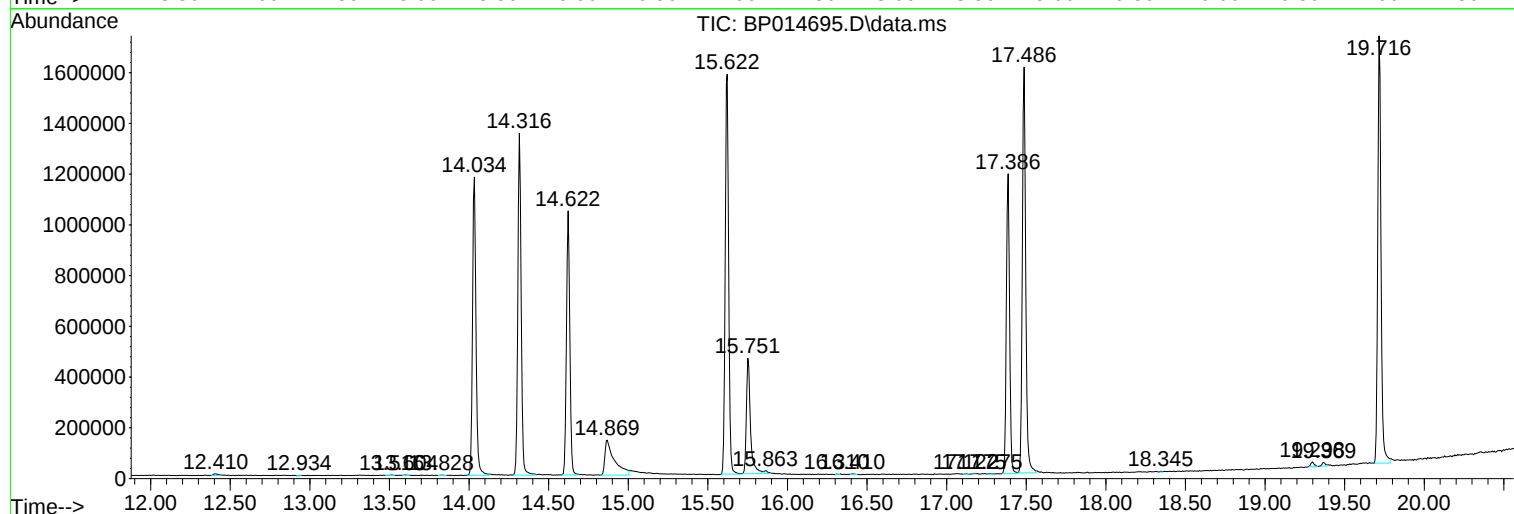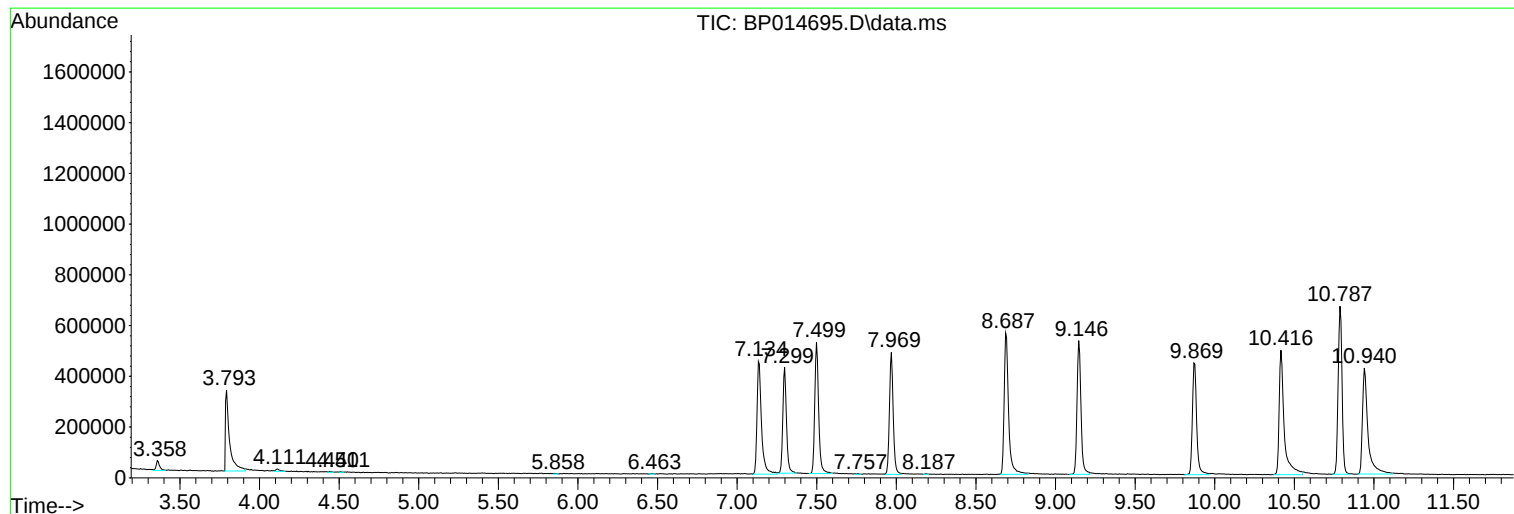

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014695.D
Acq On : 13 Apr 2023 04:39
Operator : CG/JU
Sample : PB152057BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK057

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014695.D
Acq On : 13 Apr 2023 04:39
Operator : CG/JU
Sample : PB152057BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK057

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc