

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014702.D
 Acq On : 13 Apr 2023 08:36
 Operator : CG/JU
 Sample : 02254-01
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014702.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	26	29	32	rBV	36637	40869	1.35%	0.139%
2	3.393	32	35	40	rVB	43599	54953	1.81%	0.187%
3	3.787	100	102	122	rBV	326133	568597	18.74%	1.932%
4	4.111	153	157	161	rBV4	10454	14678	0.48%	0.050%
5	5.040	311	315	316	rBV4	3113	3630	0.12%	0.012%
6	7.134	665	671	689	rBV	437997	825112	27.19%	2.804%
7	7.299	692	699	714	rVB	375250	622660	20.52%	2.116%
8	7.499	725	733	748	rBV	480683	838286	27.63%	2.849%
9	7.963	806	812	827	rVB	373059	632764	20.85%	2.150%
10	8.687	927	935	955	rBV	524788	996300	32.83%	3.386%
11	9.146	1006	1013	1030	rBV	464897	832490	27.43%	2.829%
12	9.869	1125	1136	1148	rBV	415326	734965	24.22%	2.497%
13	10.416	1222	1229	1247	rBV	451760	968530	31.92%	3.291%
14	10.652	1268	1269	1274	rVB5	2477	3058	0.10%	0.010%
15	10.787	1285	1292	1300	rBV	501956	846691	27.90%	2.877%
16	10.940	1311	1318	1344	rBV	394391	961656	31.69%	3.268%
17	12.393	1560	1565	1574	rBV6	6508	16488	0.54%	0.056%
18	14.034	1836	1844	1860	rBV	948465	1487349	49.01%	5.054%
19	14.316	1885	1892	1903	rBV	1134544	1679392	55.34%	5.707%
20	14.622	1937	1944	1957	rBV	724845	1088363	35.87%	3.698%
21	14.863	1979	1985	2004	rBV2	158144	557235	18.36%	1.894%
22	15.616	2107	2113	2129	rBV	1376357	2104405	69.35%	7.151%
23	15.751	2130	2136	2149	rVV	487536	782461	25.79%	2.659%
24	15.863	2153	2155	2160	rVB5	8581	11414	0.38%	0.039%
25	16.198	2208	2212	2218	rVB9	2215	5207	0.17%	0.018%
26	16.251	2218	2221	2224	rBV5	2015	3152	0.10%	0.011%
27	16.316	2229	2232	2238	rBV8	2345	3804	0.13%	0.013%
28	16.928	2331	2336	2341	rVV9	2957	7174	0.24%	0.024%
29	17.063	2356	2359	2364	rVB7	3409	4358	0.14%	0.015%
30	17.181	2375	2379	2380	rBV3	4606	5172	0.17%	0.018%
31	17.386	2407	2414	2424	rBV	899161	1324494	43.65%	4.501%
32	17.486	2424	2431	2449	rVV	1550364	2340351	77.12%	7.953%
33	18.034	2522	2524	2526	rBV3	3985	3599	0.12%	0.012%
34	19.292	2735	2738	2743	rVB4	20502	25633	0.84%	0.087%
35	19.363	2748	2750	2756	rVB4	16522	24692	0.81%	0.084%
36	19.716	2804	2810	2823	rBV	2012453	2814887	92.76%	9.565%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014702.D
Acq On : 13 Apr 2023 08:36
Operator : CG/JU
Sample : 02254-01
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION

37	21.475	3104	3109	3121	rBV	1003217	1571089	51.77%	5.339%
38	23.810	3499	3506	3519	rVB2	1486553	3034517	100.00%	10.312%
39	23.974	3527	3534	3545	rVB2	719552	1587626	52.32%	5.395%




Sum of corrected areas: 29428101

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014702.D
Acq On : 13 Apr 2023 08:36
Operator : CG/JU
Sample : 02254-01
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

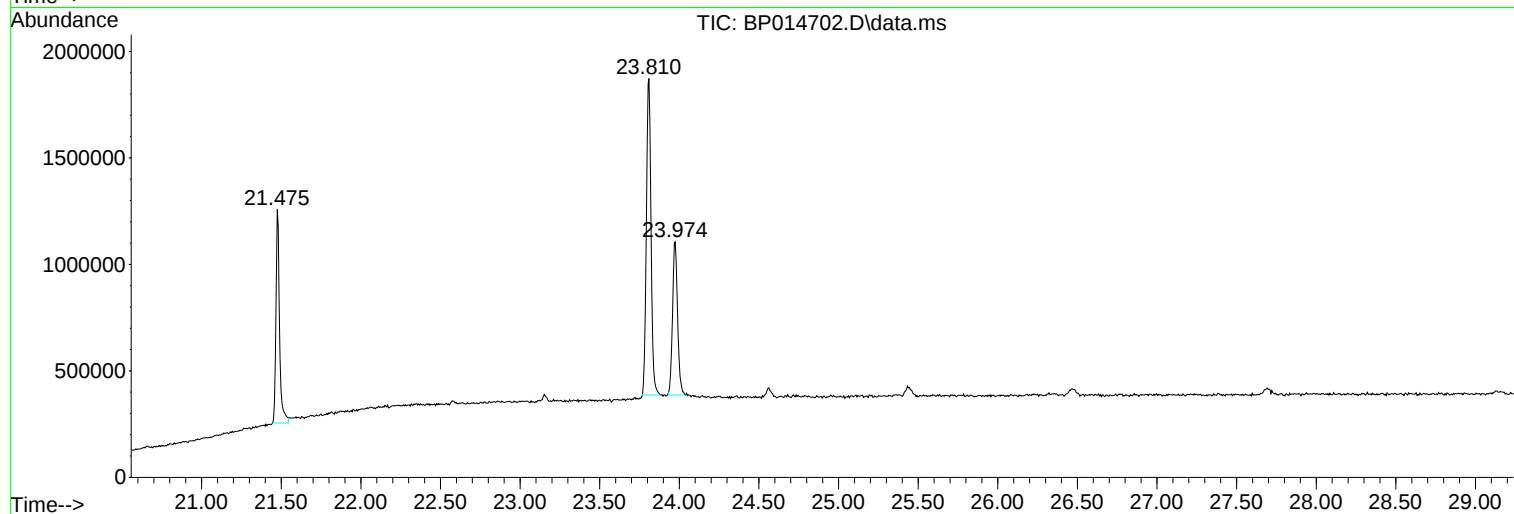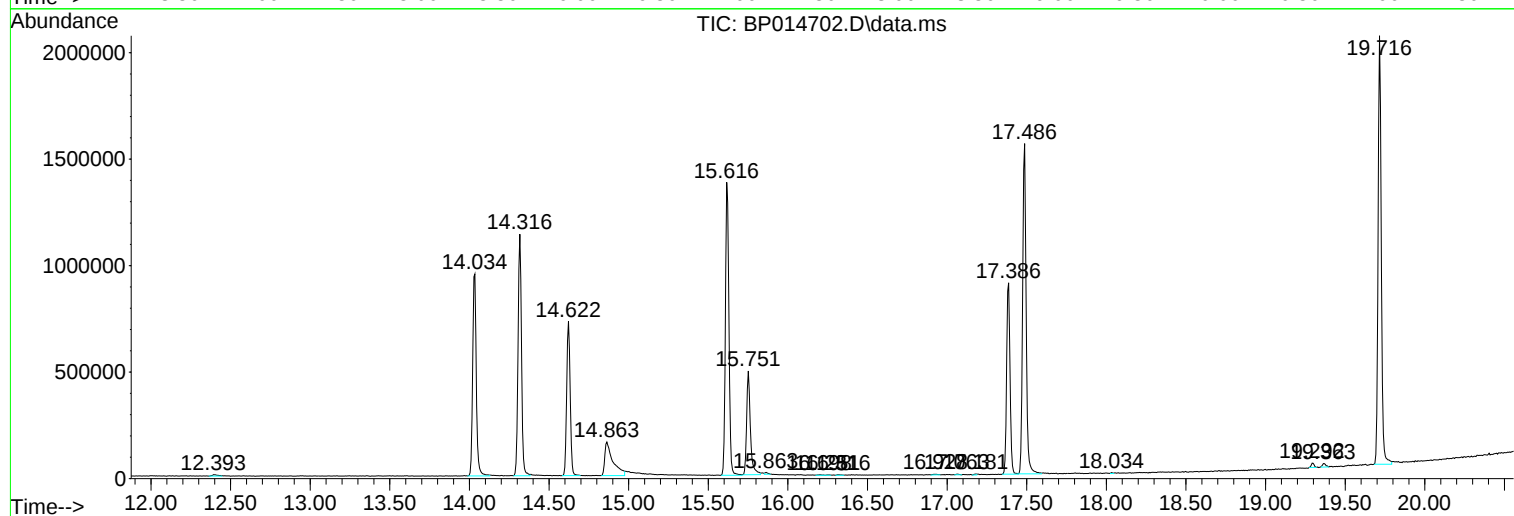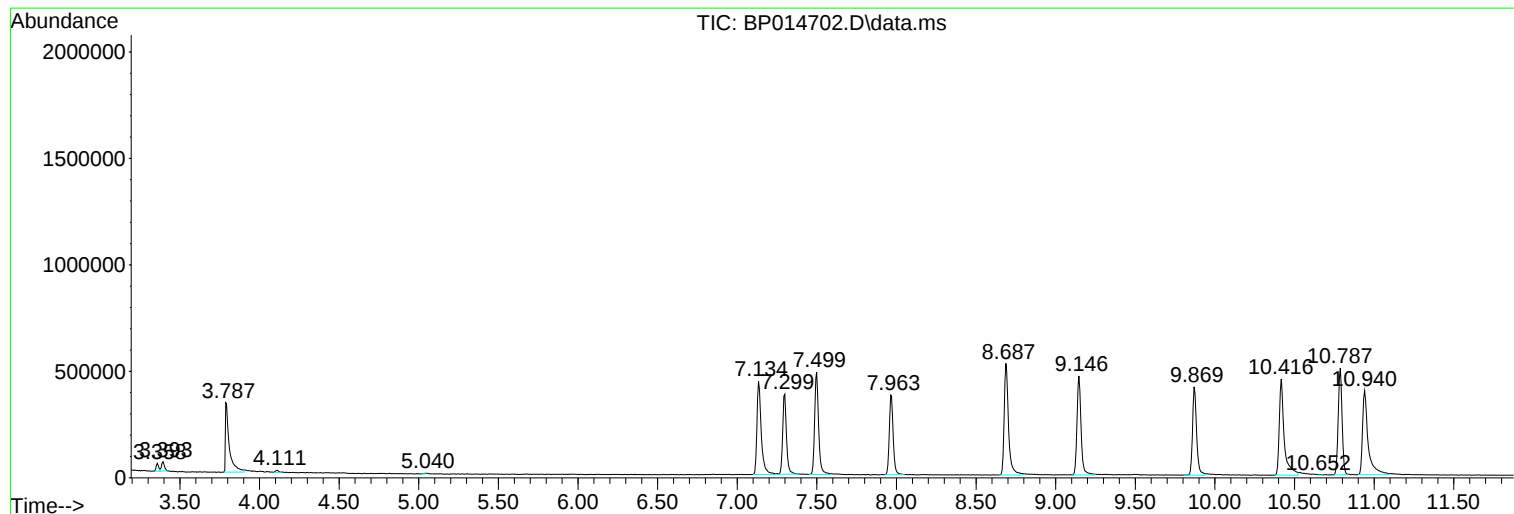

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014702.D
Acq On : 13 Apr 2023 08:36
Operator : CG/JU
Sample : 02254-01
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014702.D
Acq On : 13 Apr 2023 08:36
Operator : CG/JU
Sample : 02254-01
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc