

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014704.D
 Acq On : 13 Apr 2023 09:52
 Operator : CG/JU
 Sample : 02282-01DL2 50X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG3DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.876	115	117	120	rBV4	1730	1476	0.11%	0.019%
2	4.111	153	157	162	rBV3	10445	14413	1.10%	0.183%
3	4.499	222	223	226	rBV3	2418	2167	0.17%	0.028%
4	4.634	244	246	250	rVB5	1545	1458	0.11%	0.019%
5	4.693	255	256	259	rBV3	1387	1713	0.13%	0.022%
6	4.923	293	295	298	rBV4	1562	1595	0.12%	0.020%
7	5.364	367	370	372	rBV3	1758	2022	0.15%	0.026%
8	5.834	446	450	455	rBV7	2075	3682	0.28%	0.047%
9	5.887	457	459	462	rVB4	1899	1768	0.14%	0.022%
10	5.922	462	465	466	rBV3	1351	1598	0.12%	0.020%
11	5.958	466	471	475	rVV7	3226	5580	0.43%	0.071%
12	5.993	475	477	482	rVB6	1666	1661	0.13%	0.021%
13	6.246	519	520	525	rVB5	1476	1526	0.12%	0.019%
14	6.299	526	529	533	rVB6	1836	2380	0.18%	0.030%
15	6.593	576	579	581	rVB4	1866	1645	0.13%	0.021%
16	7.046	651	656	659	rBV6	3201	6140	0.47%	0.078%
17	7.075	659	661	663	rVB3	1558	1507	0.12%	0.019%
18	7.187	678	680	685	rVB5	2850	2641	0.20%	0.034%
19	7.322	699	703	704	rBV4	2694	2801	0.21%	0.036%
20	7.546	737	741	742	rVV3	2543	3265	0.25%	0.042%
21	7.569	742	745	746	rVV3	2908	3375	0.26%	0.043%
22	7.611	746	752	760	rVV2	12800	26630	2.04%	0.339%
23	7.687	763	765	771	rBV7	2249	4098	0.31%	0.052%
24	7.781	777	781	782	rVB3	1422	1575	0.12%	0.020%
25	7.799	782	784	787	rBV4	1107	1748	0.13%	0.022%
26	7.969	805	813	827	rBV	335322	618966	47.42%	7.875%
27	8.081	829	832	838	rVV4	10215	17784	1.36%	0.226%
28	8.158	841	845	848	rVV6	1053	1709	0.13%	0.022%
29	8.346	873	877	882	rVB7	3353	6710	0.51%	0.085%
30	8.522	901	907	911	rBV7	6928	14376	1.10%	0.183%
31	8.622	917	924	928	rBV9	2982	4867	0.37%	0.062%
32	8.669	931	932	937	rVB4	1247	1646	0.13%	0.021%
33	8.711	937	939	942	rBV4	1593	1574	0.12%	0.020%
34	8.899	968	971	975	rVV6	1693	2595	0.20%	0.033%
35	8.934	975	977	980	rVV3	2226	2515	0.19%	0.032%
36	8.987	983	986	992	rBV7	2246	4012	0.31%	0.051%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014704.D
 Acq On : 13 Apr 2023 09:52
 Operator : CG/JU
 Sample : 02282-01DL2 50X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG3DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	9.093	998	1004	1009	rBV10	2764	5042	0.39%	0.064%
38	9.164	1013	1016	1019	rBV4	1831	2400	0.18%	0.031%
39	9.452	1063	1065	1066	rBV2	2044	1480	0.11%	0.019%
40	9.599	1087	1090	1091	rBV3	1521	1659	0.13%	0.021%
41	9.616	1091	1093	1097	rVB5	3458	3961	0.30%	0.050%
42	9.669	1097	1102	1106	rBV6	5029	8834	0.68%	0.112%
43	9.905	1140	1142	1144	rBV3	1716	1462	0.11%	0.019%
44	9.934	1144	1147	1148	rVV3	1788	2084	0.16%	0.027%
45	9.969	1151	1153	1156	rVV4	1709	2328	0.18%	0.030%
46	10.034	1159	1164	1167	rVV7	2761	5619	0.43%	0.071%
47	10.181	1185	1189	1195	rBV7	5683	11673	0.89%	0.149%
48	10.416	1225	1229	1231	rBV5	2294	3202	0.25%	0.041%
49	10.487	1237	1241	1247	rBV8	2313	5348	0.41%	0.068%
50	10.693	1273	1276	1278	rBV4	1442	1583	0.12%	0.020%
51	10.787	1285	1292	1297	rBV	434451	786960	60.30%	10.013%
52	10.840	1297	1301	1318	rVB	131297	291076	22.30%	3.704%
53	11.181	1357	1359	1362	rVB4	1374	1471	0.11%	0.019%
54	11.240	1365	1369	1370	rBV4	1667	2034	0.16%	0.026%
55	11.346	1385	1387	1391	rBV5	1639	2460	0.19%	0.031%
56	11.481	1408	1410	1413	rVB4	2282	1744	0.13%	0.022%
57	11.957	1488	1491	1493	rVB4	1237	1514	0.12%	0.019%
58	12.057	1504	1508	1509	rBV4	1532	2074	0.16%	0.026%
59	12.116	1514	1518	1520	rBV5	1351	1985	0.15%	0.025%
60	12.199	1530	1532	1534	rBV3	1452	1466	0.11%	0.019%
61	12.257	1537	1542	1545	rVV6	1249	1766	0.14%	0.022%
62	12.310	1548	1551	1554	rBV5	1549	2216	0.17%	0.028%
63	12.387	1561	1564	1568	rVB6	1273	1479	0.11%	0.019%
64	12.481	1570	1580	1592	rVV3	10505	29355	2.25%	0.373%
65	12.610	1600	1602	1608	rVB7	1049	1673	0.13%	0.021%
66	12.687	1608	1615	1625	rBV2	13324	31961	2.45%	0.407%
67	12.946	1657	1659	1661	rBV3	1553	1475	0.11%	0.019%
68	13.163	1694	1696	1699	rVB4	2035	1706	0.13%	0.022%
69	13.675	1781	1783	1784	rBV2	1645	1612	0.12%	0.021%
70	13.804	1800	1805	1806	rBV5	1769	2101	0.16%	0.027%
71	13.951	1823	1830	1834	rBV7	4779	9043	0.69%	0.115%
72	14.004	1834	1839	1843	rVV7	3564	6332	0.49%	0.081%
73	14.063	1843	1849	1860	rVV2	9740	21214	1.63%	0.270%
74	14.187	1865	1870	1871	rVV5	2526	3785	0.29%	0.048%
75	14.216	1873	1875	1878	rVV4	2623	2837	0.22%	0.036%
76	14.322	1886	1893	1905	rVB	13399	29117	2.23%	0.370%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014704.D
 Acq On : 13 Apr 2023 09:52
 Operator : CG/JU
 Sample : 02282-01DL2 50X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG3DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

77	14.551	1930	1932	1934	rBV3	1492	1476	0.11%	0.019%
78	14.622	1937	1944	1955	rBV	648120	1047614	80.27%	13.329%
79	15.110	2022	2027	2028	rBV5	2153	3324	0.25%	0.042%
80	15.175	2036	2038	2040	rVB3	1624	1534	0.12%	0.020%
81	15.222	2040	2046	2047	rBV6	3049	4083	0.31%	0.052%
82	15.293	2052	2058	2071	rVV8	16824	43432	3.33%	0.553%
83	15.469	2085	2088	2091	rVB5	1409	2042	0.16%	0.026%
84	15.634	2111	2116	2124	rBV	17360	35281	2.70%	0.449%
85	15.881	2156	2158	2161	rBV3	1217	1557	0.12%	0.020%
86	16.140	2199	2202	2206	rVB5	2302	2698	0.21%	0.034%
87	16.181	2206	2209	2212	rBV4	1191	1771	0.14%	0.023%
88	16.304	2228	2230	2234	rVV5	1736	1678	0.13%	0.021%
89	16.375	2239	2242	2245	rBV5	1805	2417	0.19%	0.031%
90	16.634	2282	2286	2288	rBV5	1329	1703	0.13%	0.022%
91	16.657	2288	2290	2292	rBV3	1671	1801	0.14%	0.023%
92	16.810	2314	2316	2318	rBV3	2200	1950	0.15%	0.025%
93	17.040	2348	2355	2373	rBV	454502	880954	67.50%	11.209%
94	17.387	2408	2414	2427	rBV	696594	1122087	85.97%	14.277%
95	17.498	2429	2433	2446	rVB5	16279	45925	3.52%	0.584%
96	18.339	2574	2576	2578	rBV3	2547	1857	0.14%	0.024%
97	18.375	2580	2582	2586	rVB5	3911	3159	0.24%	0.040%
98	19.734	2809	2813	2819	rBV3	23288	40695	3.12%	0.518%
99	21.475	3105	3109	3121	rBV	750923	1232878	94.46%	15.687%
100	23.974	3528	3534	3547	rVB2	593788	1305182	100.00%	16.607%




Sum of corrected areas: 7859447

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014704.D
Acq On : 13 Apr 2023 09:52
Operator : CG/JU
Sample : 02282-01DL2 50X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG3DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

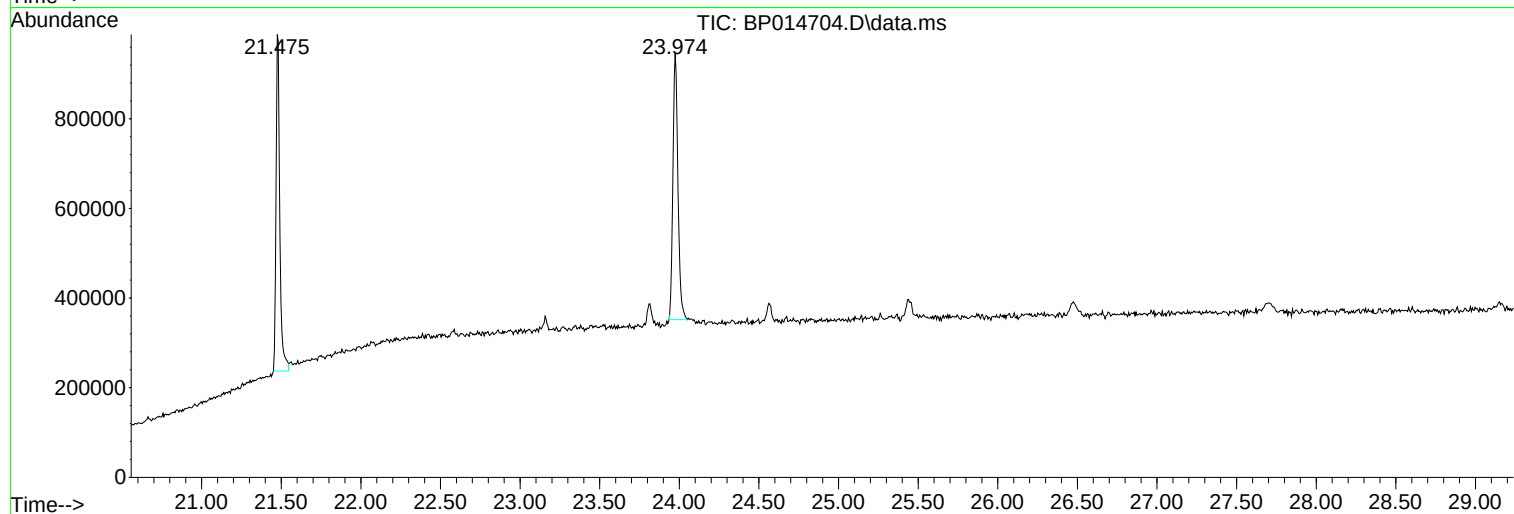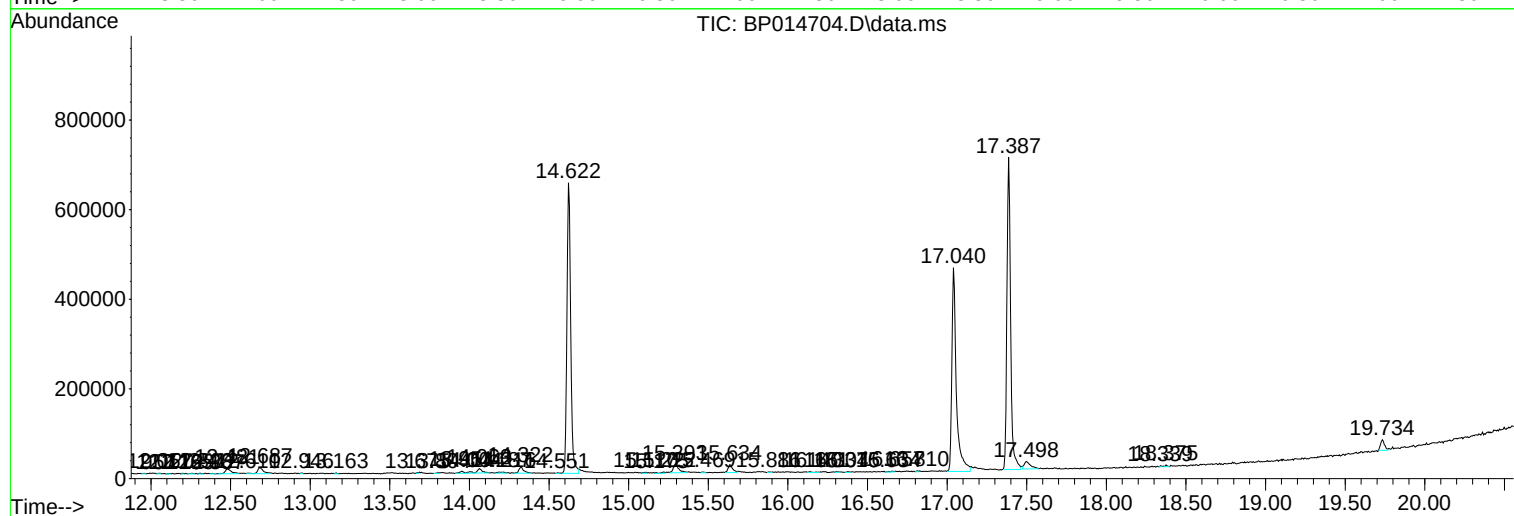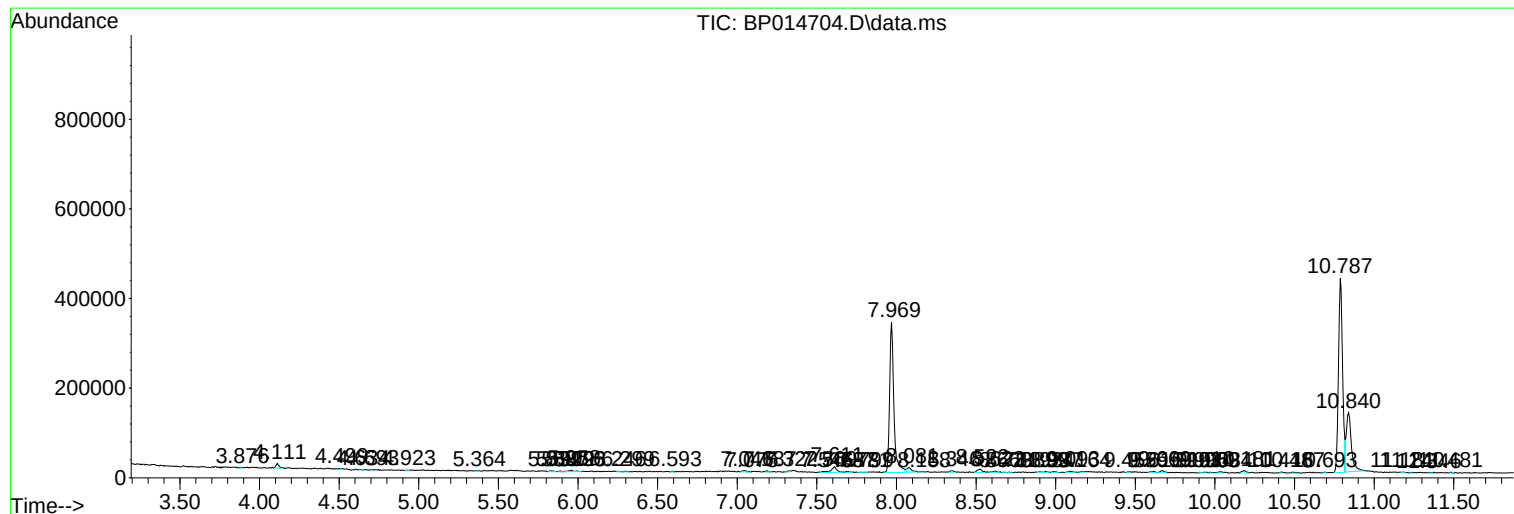

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014704.D
Acq On : 13 Apr 2023 09:52
Operator : CG/JU
Sample : 02282-01DL2 50X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG3DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014704.D
Acq On : 13 Apr 2023 09:52
Operator : CG/JU
Sample : 02282-01DL2 50X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG3DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc