

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014710.D
 Acq On : 13 Apr 2023 13:21
 Operator : CG/JU
 Sample : PB152052TB 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014710.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	26	30	36	rVB	33229	42182	1.74%	0.171%
2	3.805	103	105	129	rVV	92789	209727	8.66%	0.852%
3	4.116	154	158	162	rBV2	7643	12578	0.52%	0.051%
4	4.446	212	214	218	rBV5	2499	2427	0.10%	0.010%
5	4.905	291	292	296	rBV4	1936	2659	0.11%	0.011%
6	6.469	556	558	562	rVB5	1923	2683	0.11%	0.011%
7	7.140	666	672	688	rBV	393379	764185	31.57%	3.104%
8	7.299	693	699	715	rVV	351624	592887	24.49%	2.408%
9	7.504	727	734	748	rBV	445259	781669	32.29%	3.175%
10	7.969	806	813	830	rVV	366009	624582	25.80%	2.537%
11	8.075	830	831	837	rVV6	1950	2784	0.11%	0.011%
12	8.140	840	842	844	rVB3	2694	2567	0.11%	0.010%
13	8.375	878	882	885	rBV6	2312	2798	0.12%	0.011%
14	8.693	930	936	956	rBV	478173	926444	38.27%	3.763%
15	9.151	1007	1014	1029	rBV	428091	777814	32.13%	3.160%
16	9.875	1130	1137	1153	rBV	360760	670385	27.69%	2.723%
17	9.975	1153	1154	1159	rVB5	2473	2831	0.12%	0.011%
18	10.040	1164	1165	1171	rVB6	2308	3084	0.13%	0.013%
19	10.422	1223	1230	1268	rVV	323286	919139	37.97%	3.734%
20	10.792	1285	1293	1308	rVB	484052	849113	35.07%	3.449%
21	10.963	1315	1322	1339	rBV2	71948	238177	9.84%	0.967%
22	11.657	1437	1440	1443	rBV5	1771	2648	0.11%	0.011%
23	11.763	1456	1458	1465	rVB8	1466	2885	0.12%	0.012%
24	12.422	1564	1570	1577	rVV9	5252	11345	0.47%	0.046%
25	14.033	1838	1844	1859	rBV	816252	1313632	54.26%	5.336%
26	14.322	1885	1893	1908	rBV	973984	1515916	62.62%	6.158%
27	14.622	1935	1944	1957	rBV	668000	1045402	43.18%	4.246%
28	14.875	1979	1987	2011	rBV2	99026	436286	18.02%	1.772%
29	15.504	2091	2094	2098	rVB6	2632	3785	0.16%	0.015%
30	15.622	2107	2114	2126	rBV	1258439	1847590	76.32%	7.505%
31	15.757	2131	2137	2150	rVV	332833	596482	24.64%	2.423%
32	15.863	2153	2155	2161	rVB6	8577	13121	0.54%	0.053%
33	16.198	2207	2212	2216	rBV7	1888	2979	0.12%	0.012%
34	16.322	2230	2233	2235	rBV4	1960	2586	0.11%	0.011%
35	16.410	2245	2248	2251	rBV5	2115	2568	0.11%	0.010%
36	17.386	2405	2414	2423	rBV	826818	1154695	47.70%	4.690%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014710.D
 Acq On : 13 Apr 2023 13:21
 Operator : CG/JU
 Sample : PB152052TB 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	17.486	2425	2431	2448	rVV2	1285328	1970250	81.38%	8.003%
38	18.569	2613	2615	2617	rBV2	4086	3690	0.15%	0.015%
39	19.298	2736	2739	2743	rBV4	15454	20980	0.87%	0.085%
40	19.369	2748	2751	2757	rBV4	13921	21631	0.89%	0.088%
41	19.721	2805	2811	2821	rBV	1532321	2249870	92.93%	9.139%
42	21.480	3105	3110	3122	rBV2	773981	1252273	51.73%	5.087%
43	23.809	3500	3506	3521	rVB2	1164973	2420952	100.00%	9.834%
44	23.974	3528	3534	3546	rVB	575593	1295944	53.53%	5.264%




Sum of corrected areas: 24618225

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014710.D
Acq On : 13 Apr 2023 13:21
Operator : CG/JU
Sample : PB152052TB 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB052

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

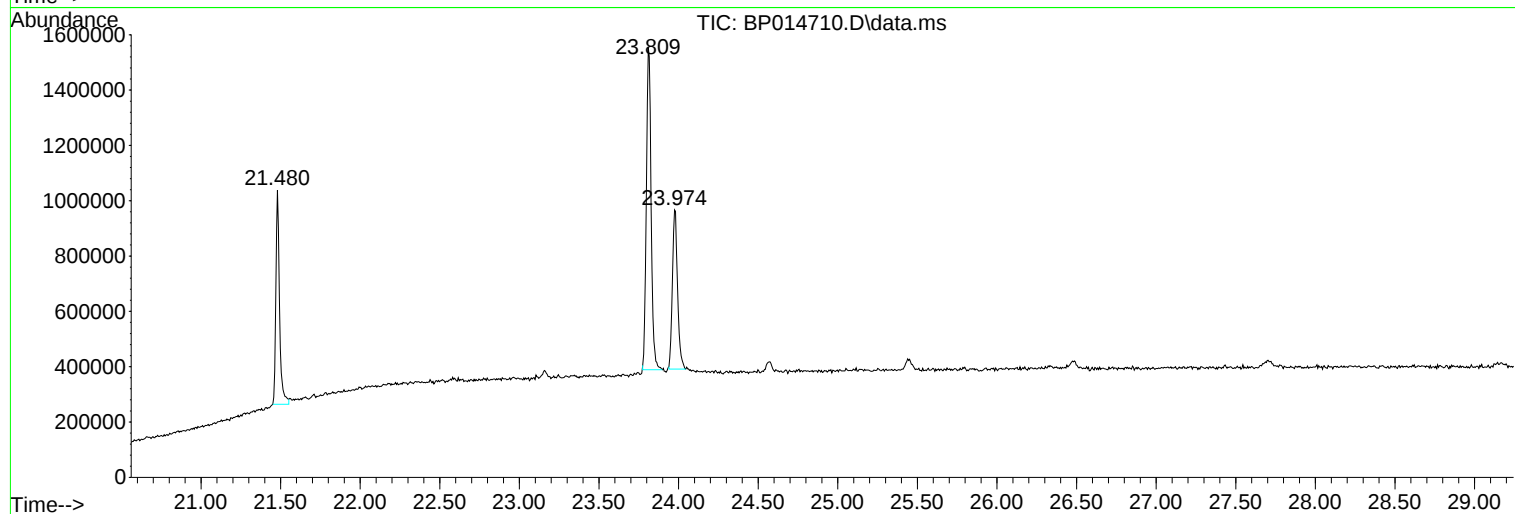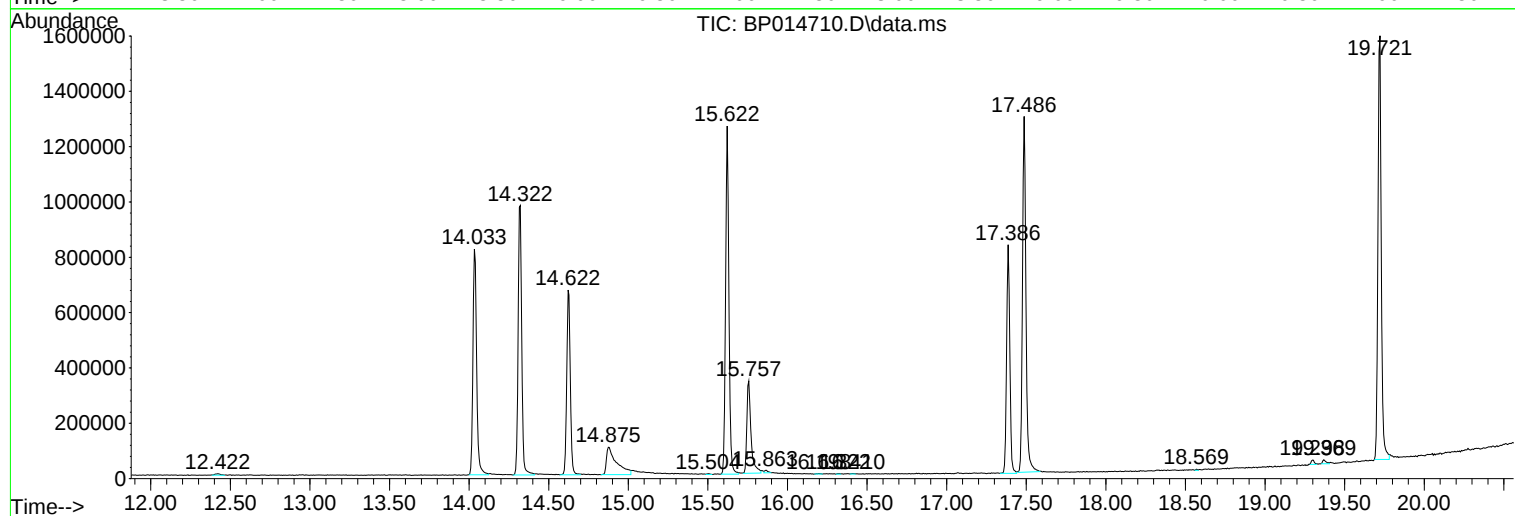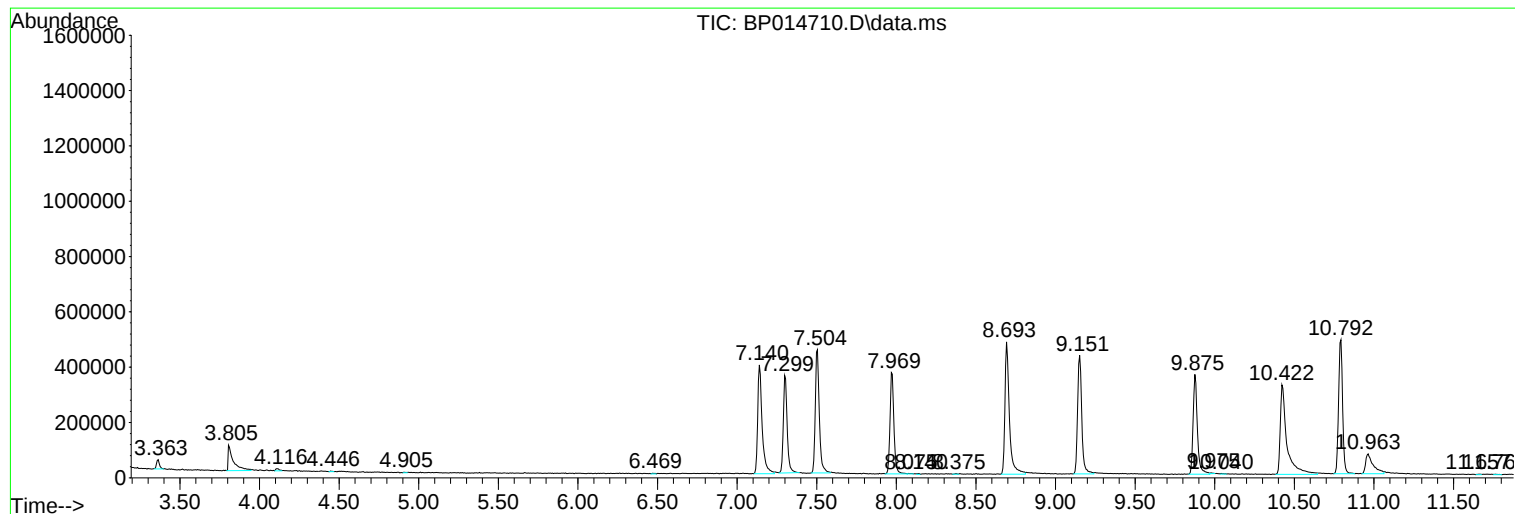

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014710.D
Acq On : 13 Apr 2023 13:21
Operator : CG/JU
Sample : PB152052TB 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB052

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014710.D
Acq On : 13 Apr 2023 13:21
Operator : CG/JU
Sample : PB152052TB 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB052

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------