
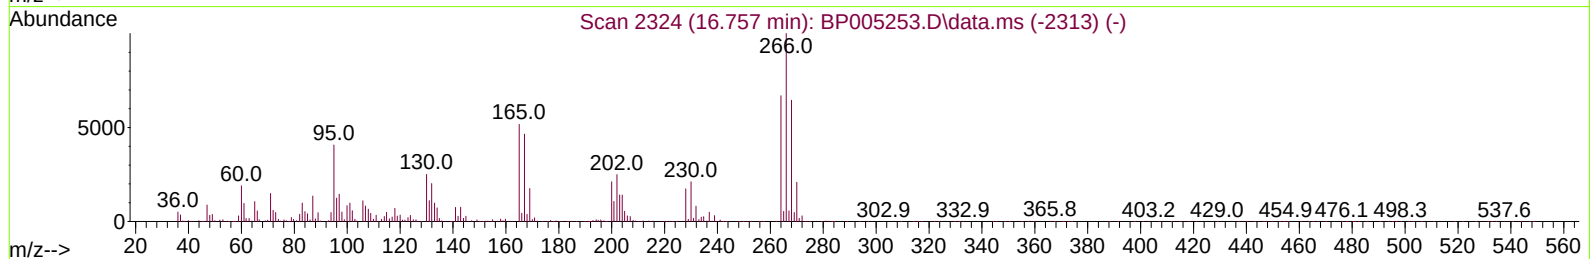
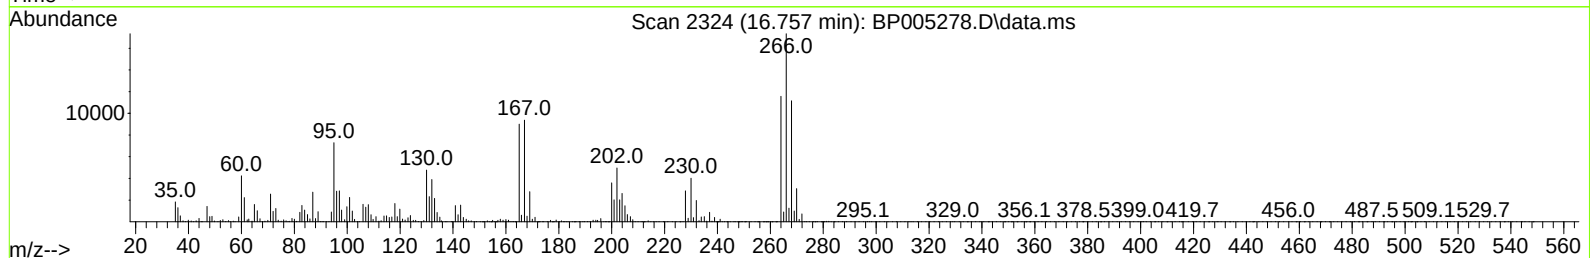


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041321\
Data File : BP005278.D
Acq On : 13 Apr 2021 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 05:37:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP040921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 18:44:11 2021
Response via : Initial Calibration

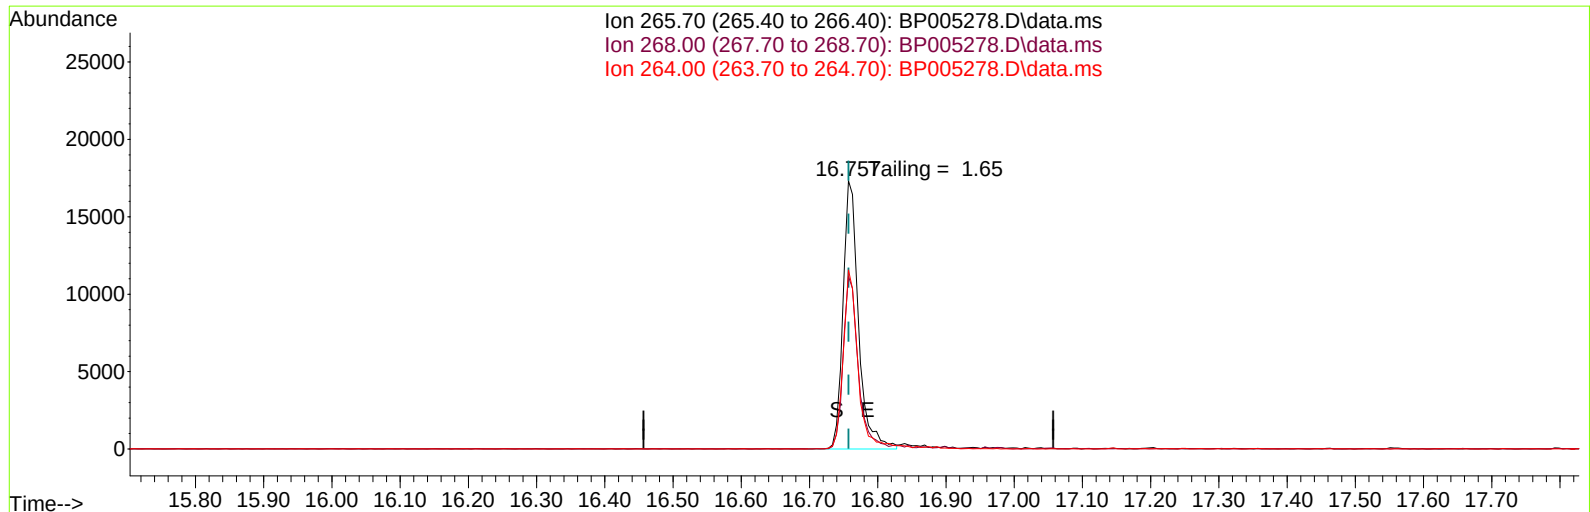

TIC: BP005278.D\data.ms

(70) Pentachlorophenol (C)




16.757min (-0.000) 466388.78 ng

response 27494

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.32
264.00	63.30	66.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041321\
 Data File : BP005278.D
 Acq On : 13 Apr 2021 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 05:37:22 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP040921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 09 18:44:11 2021
 Response via : Initial Calibration

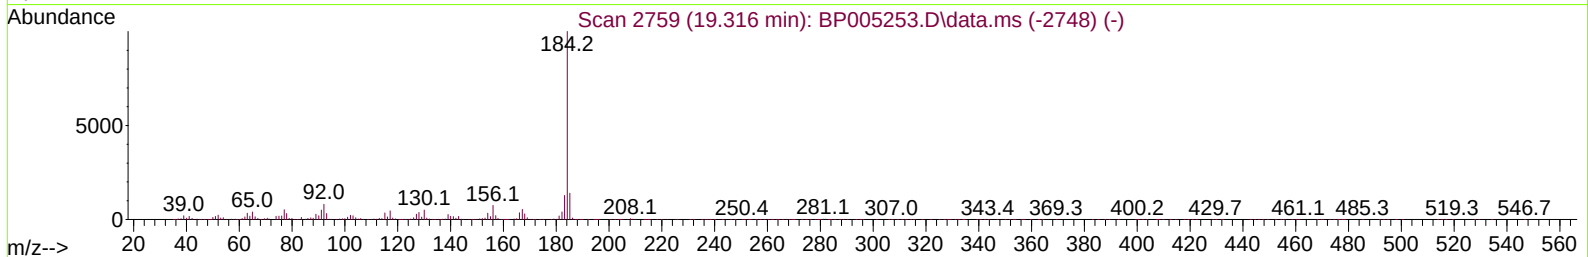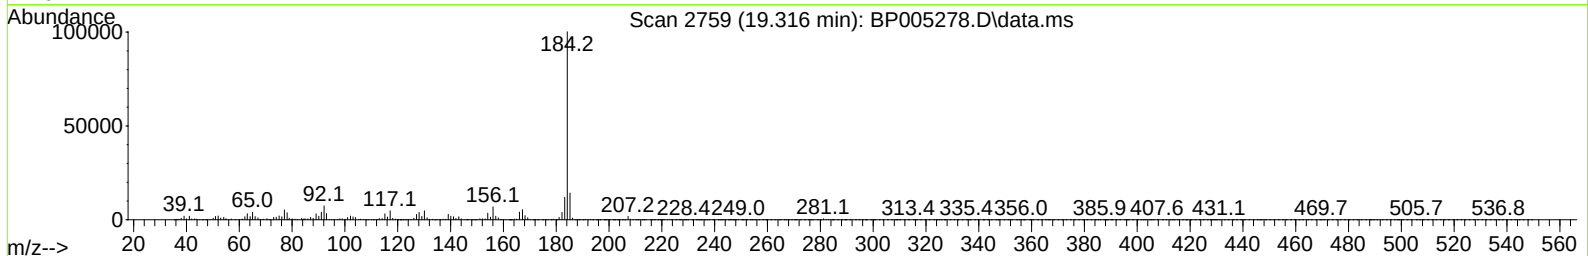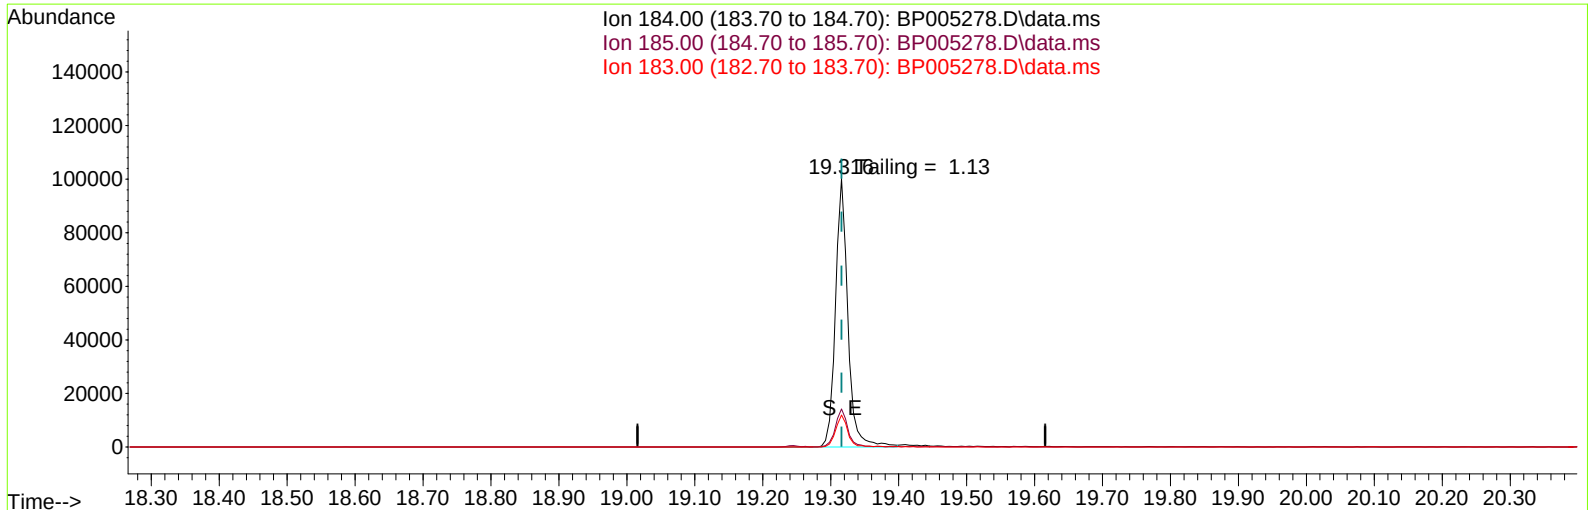

TIC: BP005278.D\data.ms

(77) Benzidine**19.316min (-0.000) 496539.88 ng****response 127223**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.23
183.00	12.00	11.96
0.00	0.00	0.00