
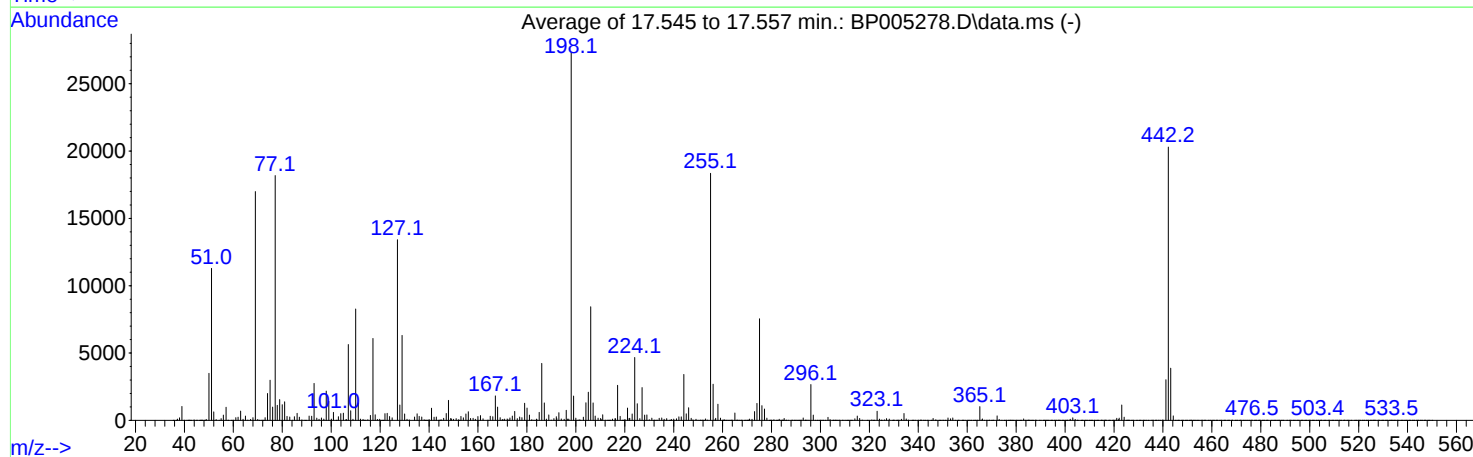


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041321\
 Data File : BP005278.D
 Acq On : 13 Apr 2021 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP040921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 09 18:44:11 2021

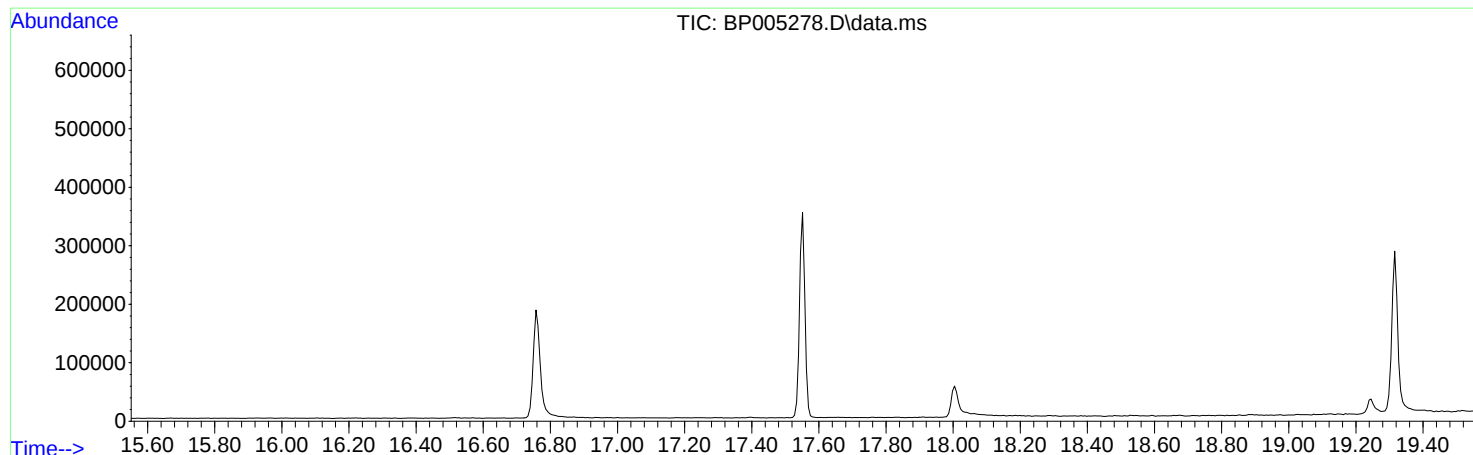




AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	11287	PASS
68	69	0.00	2	1.2	203	PASS
69	198	0.00	100	62.2	16988	PASS
70	69	0.00	2	0.4	74	PASS
127	198	10	80	49.1	13419	PASS
197	198	0.00	2	0.4	99	PASS
198	198	100	100	100.0	27320	PASS
199	198	5	9	6.6	1812	PASS
275	198	10	60	27.6	7547	PASS
365	198	1	100	3.7	1021	PASS
441	198	0.01	100	11.1	3024	PASS
442	442	100	100	100.0	20297	PASS
443	442	15	24	19.1	3871	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041321\
Data File : BP005278.D
Acq On : 13 Apr 2021 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 14 05:37:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP040921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 18:44:11 2021
Response via : Initial Calibration

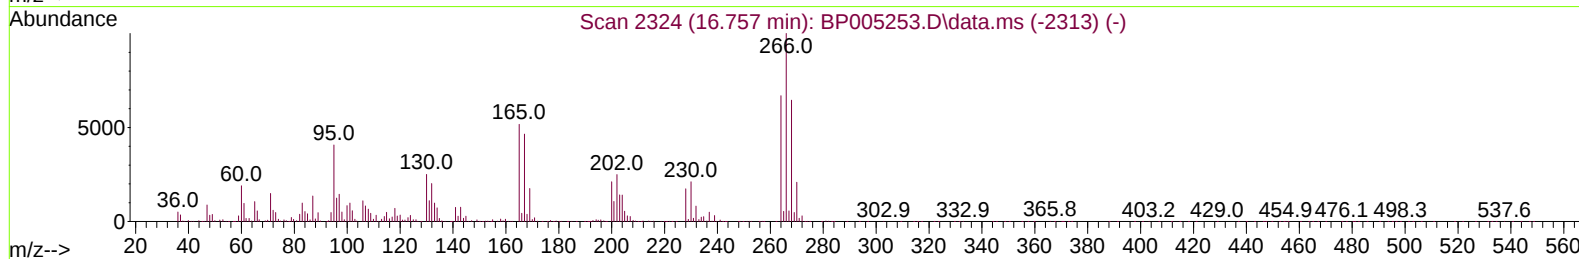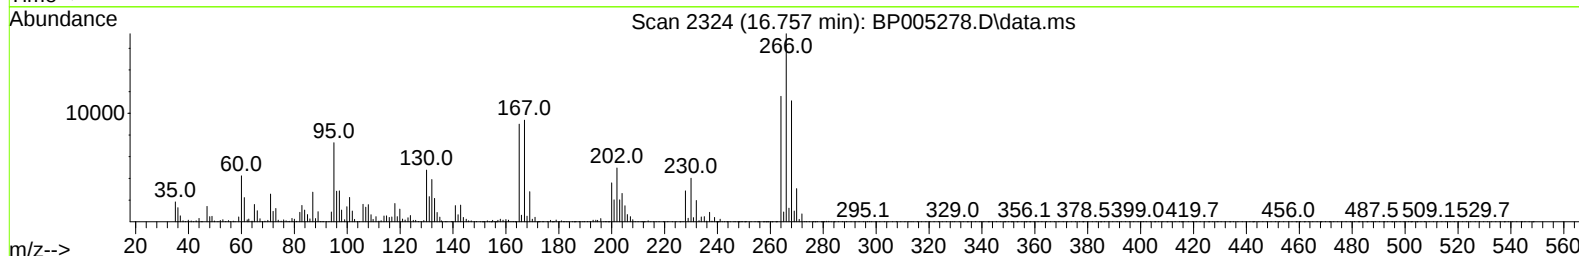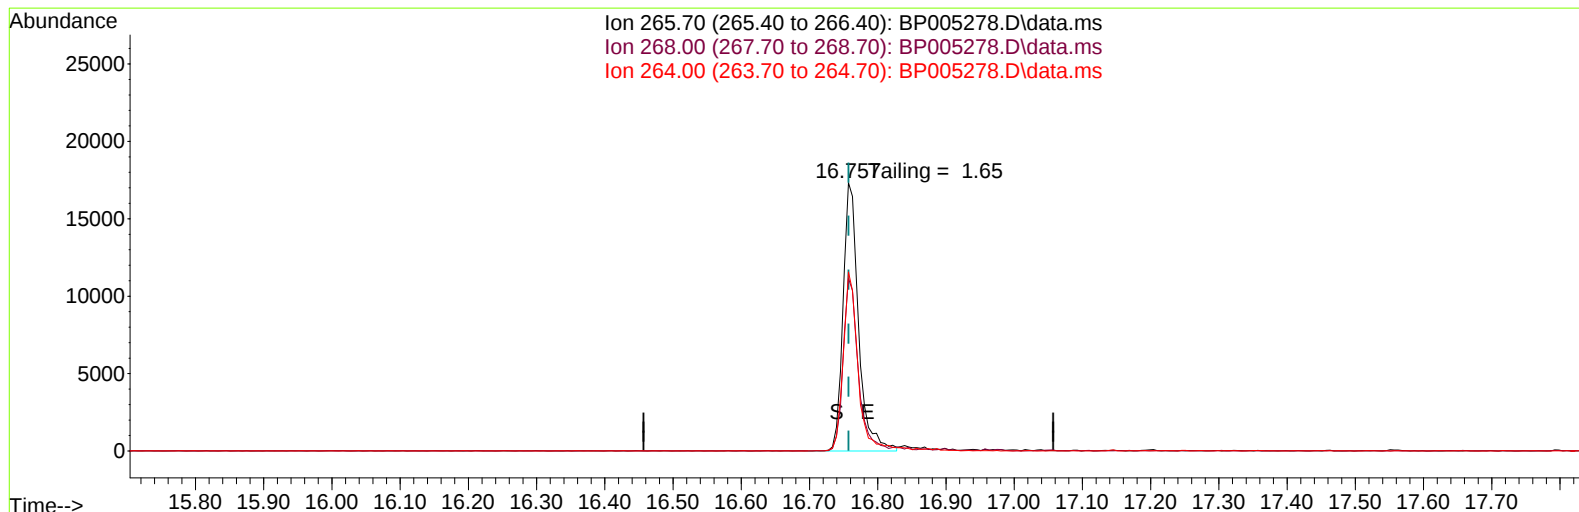

TIC: BP005278.D\data.ms

(70) Pentachlorophenol (C)

16.757min (-0.000) 466388.78 ng




response 27494

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.32
264.00	63.30	66.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041321\
 Data File : BP005278.D
 Acq On : 13 Apr 2021 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 14 05:37:22 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP040921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 09 18:44:11 2021
 Response via : Initial Calibration

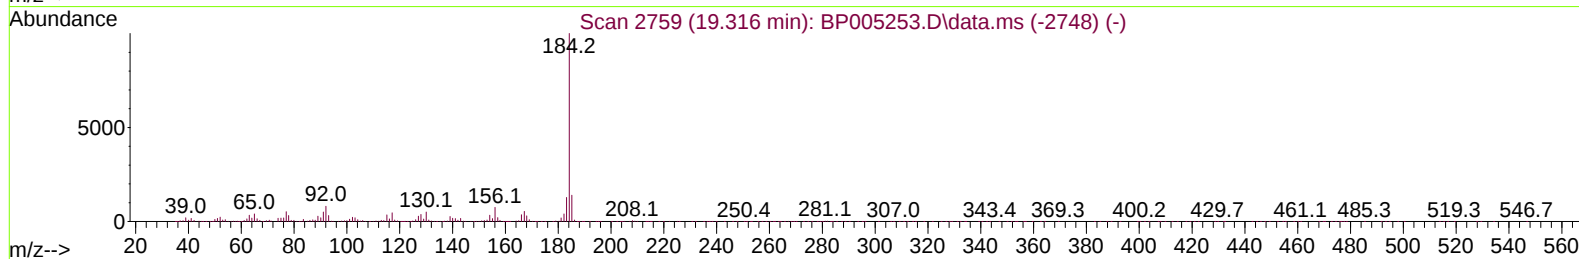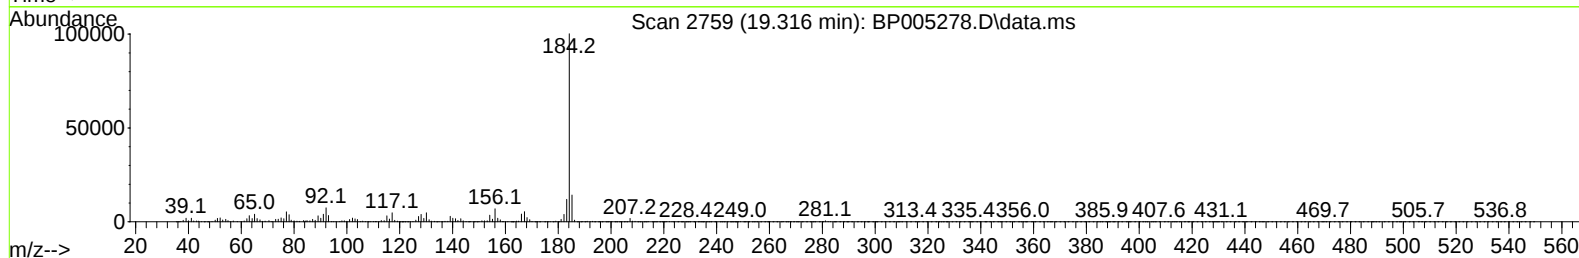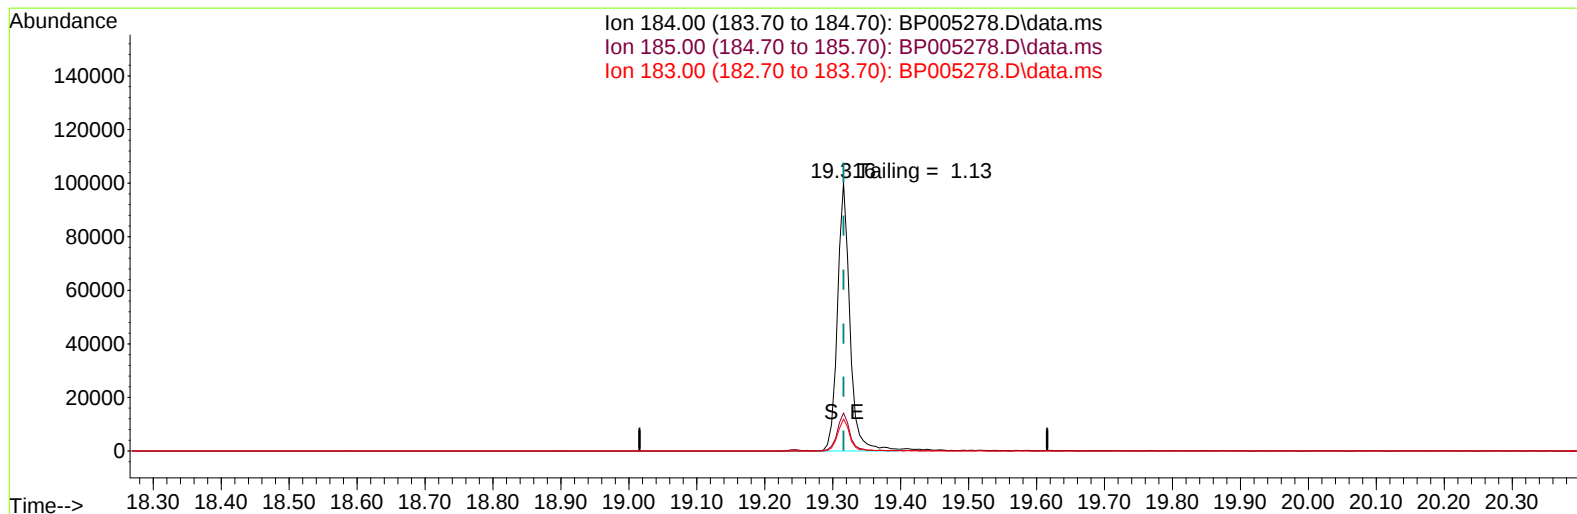

TIC: BP005278.D\data.ms

(77) Benzidine

19.316min (-0.000) 496539.88 ng

response 127223

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.23
183.00	12.00	11.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/13/2021	BNA_P	BP005078.D
Compound Name	Response	Retention Time
DDT	93112	20.51
DDD	1220	20.08
DDE	172	19.592
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1392	94504	1.47