




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
 Data File : BP009833.D
 Acq On : 14 Apr 2022 18:05
 Operator : CG/JU
 Sample : N2293-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETNN6

Manual IntegrationsAPPROVED

Quant Time: Apr 14 21:47:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/22/2022

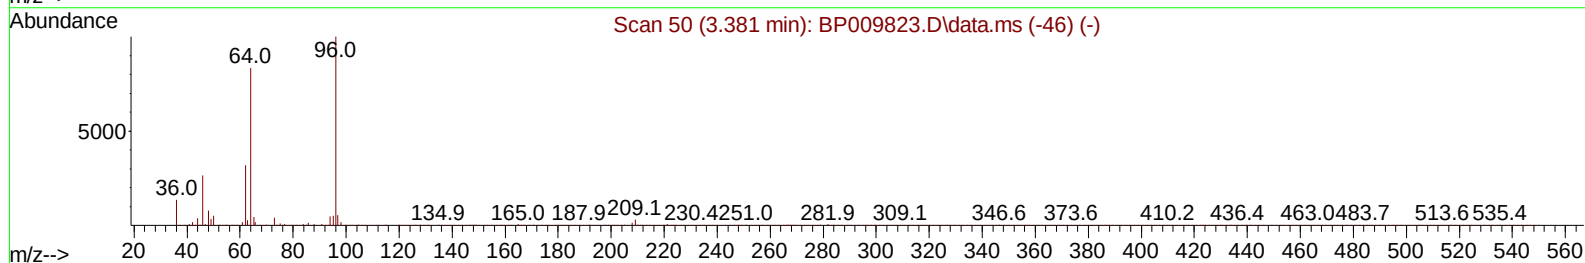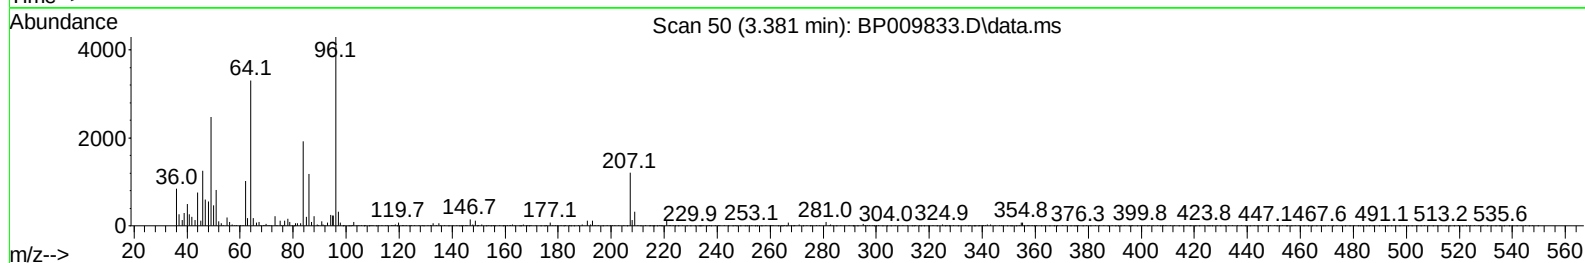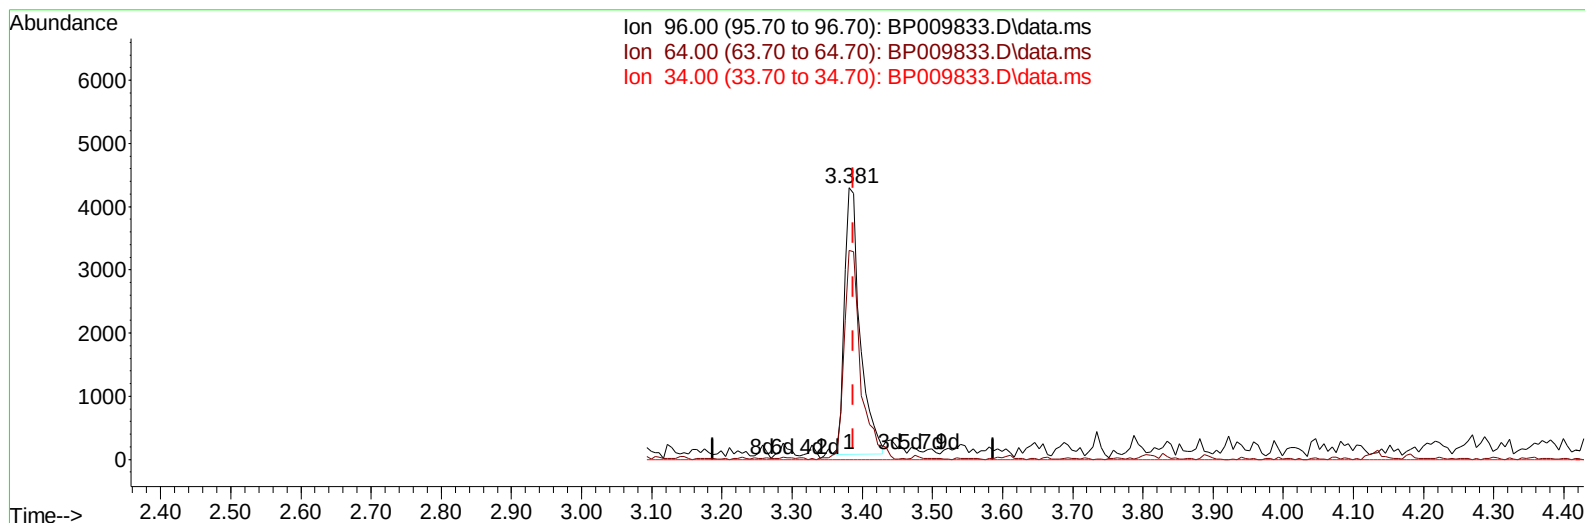

TIC: BP009833.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.381min (-0.006) 2.57 ng/uL

response 6536

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	76.96#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
 Data File : BP009833.D
 Acq On : 14 Apr 2022 18:05
 Operator : CG/JU
 Sample : N2293-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETNN6

Manual IntegrationsAPPROVED

Quant Time: Apr 14 21:47:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/22/2022

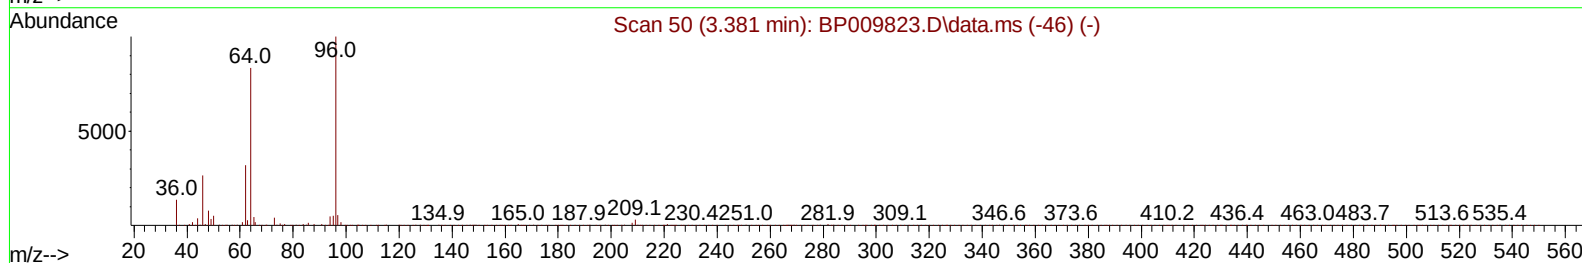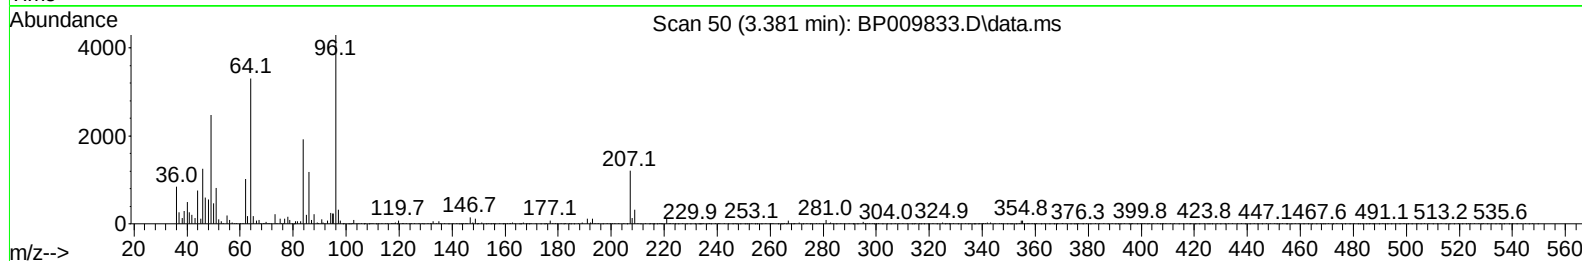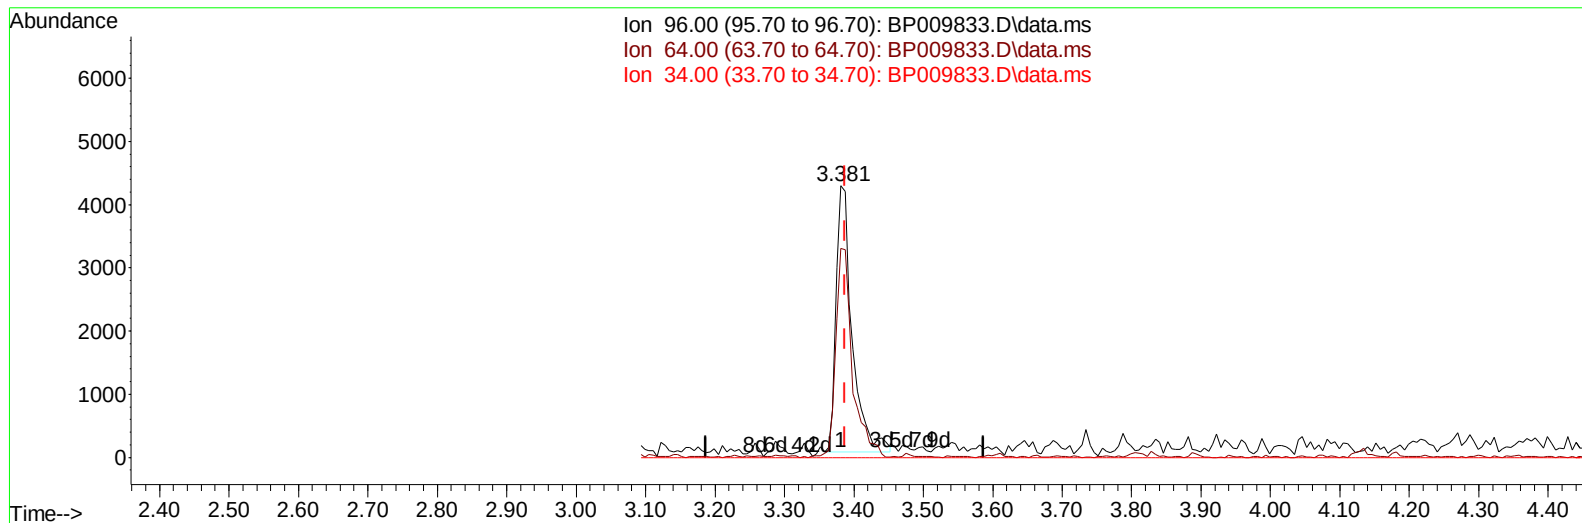

TIC: BP009833.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.381min (-0.006) 2.65 ng/uL m

response 6750

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	76.96#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
 Data File : BP009833.D
 Acq On : 14 Apr 2022 18:05
 Operator : CG/JU
 Sample : N2293-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETNN6

Manual IntegrationsAPPROVED

Quant Time: Apr 14 21:47:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/22/2022

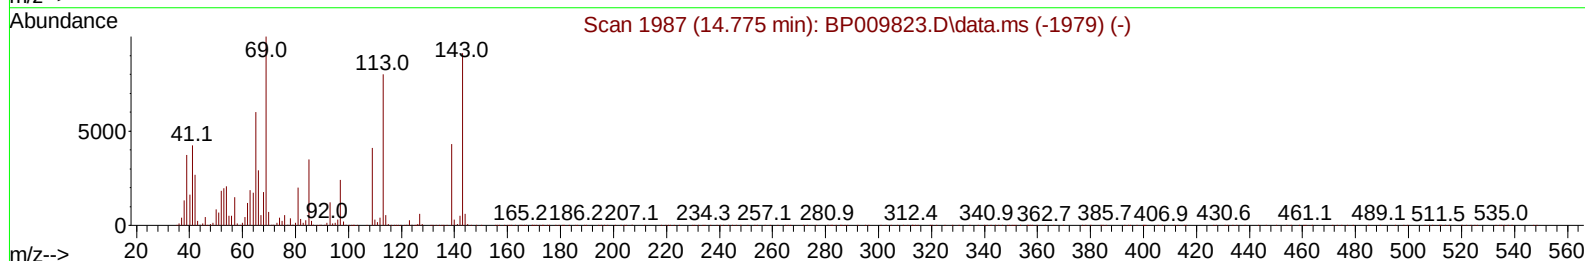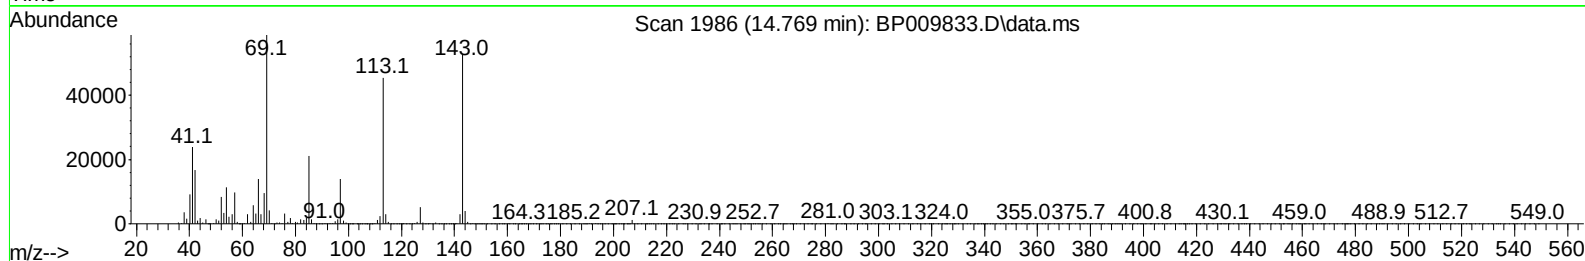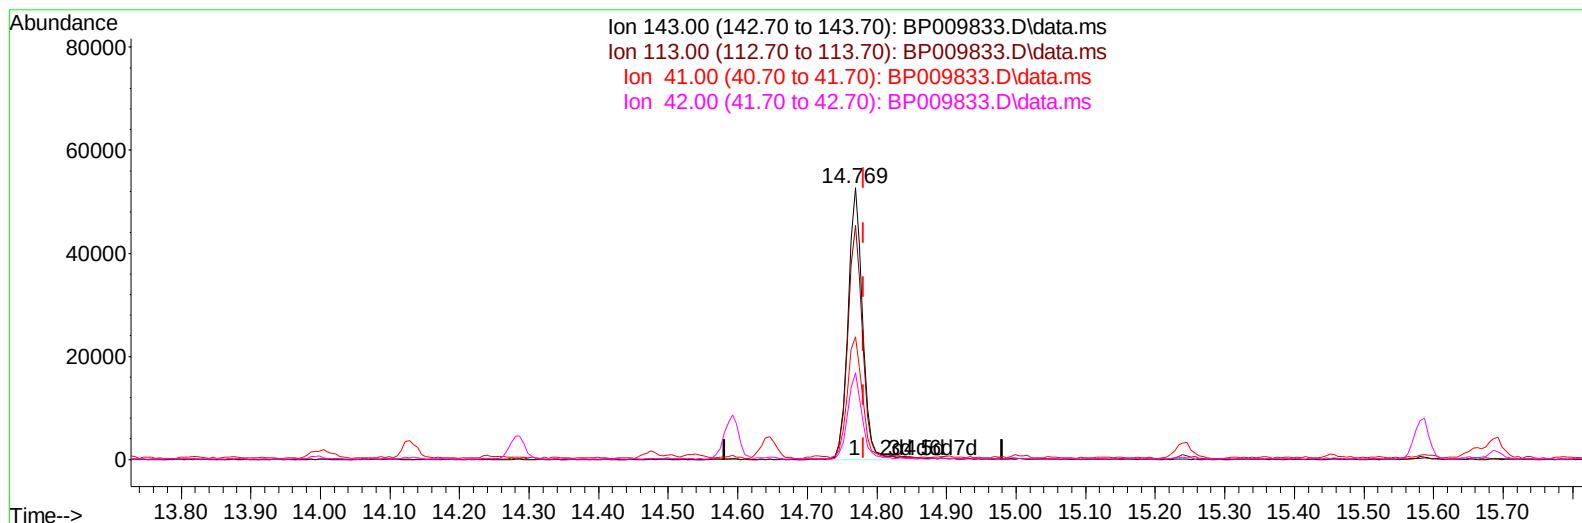

TIC: BP009833.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.769min (-0.012) 13.98 ng/ul

response 75014

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	86.24#
41.00	23.20	45.16#
42.00	18.00	31.89#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
Data File : BP009833.D
Acq On : 14 Apr 2022 18:05
Operator : CG/JU
Sample : N2293-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ETNN6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/22/2022

Quant Time: Apr 14 21:47:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 13 02:15:22 2022
Response via : Initial Calibration

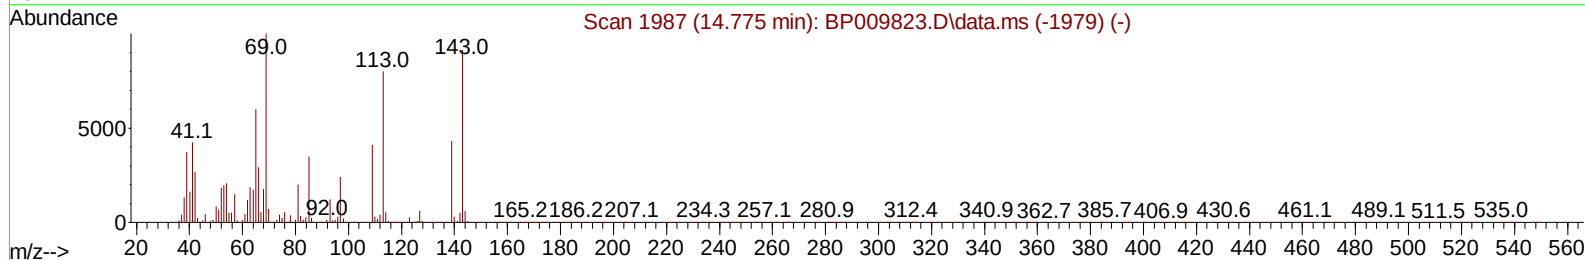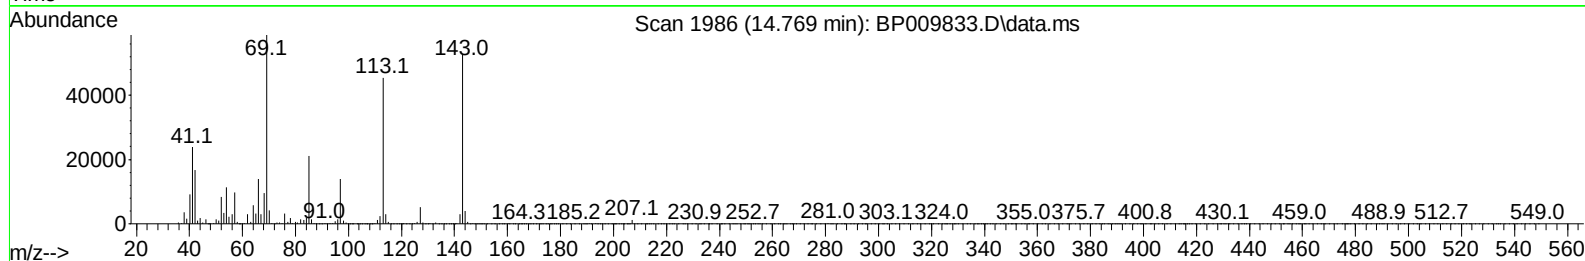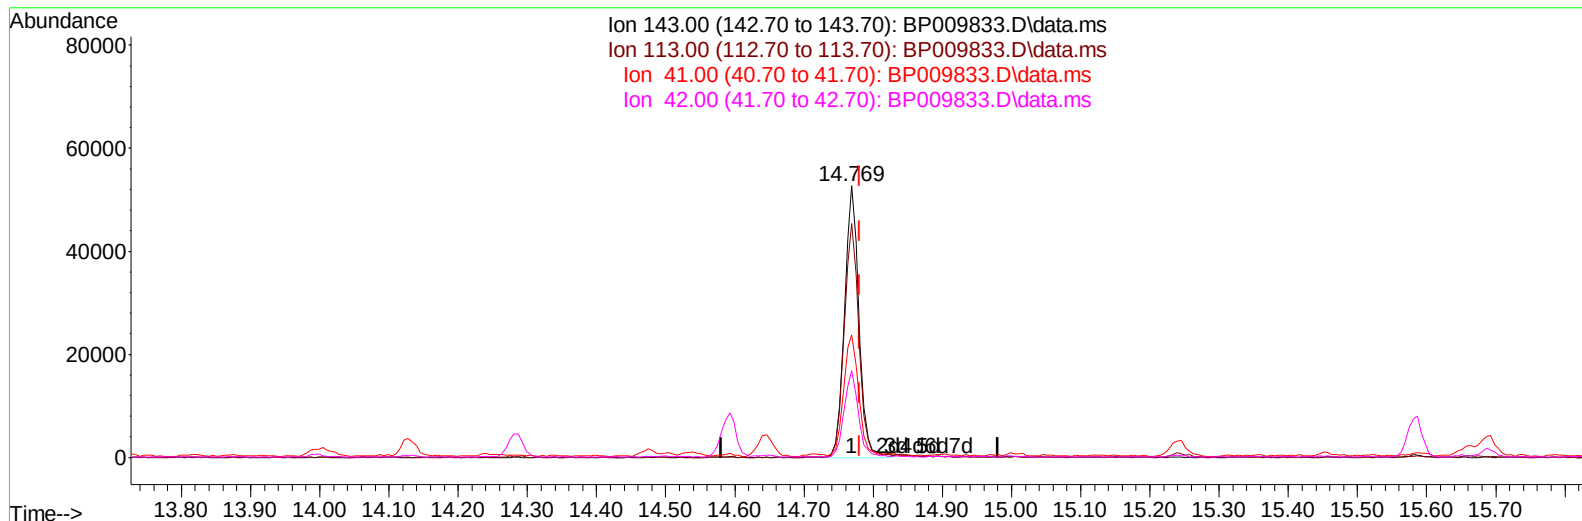

TIC: BP009833.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.769min (-0.012) 14.07 ng/ul m

response 75469

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	86.24#
41.00	23.20	45.16#
42.00	18.00	31.89#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
 Data File : BP009833.D
 Acq On : 14 Apr 2022 18:05
 Operator : CG/JU
 Sample : N2293-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETNN6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/22/2022

Quant Time: Apr 14 21:47:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.963	152		113718	20.000	ng/ul	0.00
20) Naphthalene-d8	10.769	136		516930	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.592	164		376547	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188		847517	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.422	240		889511	20.000	ng/ul	-0.01
88) Perylene-d12	23.886	264		854362	20.000	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.381	96		6750m	2.649	ng/uL	0.00
4) Pyridine-d5	3.805	84		48750	6.939	ng/ul	0.00
7) Phenol-d5	7.111	99		137136	13.736	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.287	67		93245	15.688	ng/ul	0.00
11) 2-Chlorophenol-d4	7.487	132		109687	14.565	ng/ul	-0.01
15) 4-Methylphenol-d8	8.663	113		120736	14.487	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128		59822	16.048	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.846	143		63149	15.452	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165		119206	13.939	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.899	131		171473	14.078	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166		501346	16.950	ng/ul	0.00
49) Acenaphthylene-d8	14.287	160		503072	14.356	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143		75469m	14.069	ng/ul	-0.01
60) Fluorene-d10	15.587	176		416886	16.754	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200		65555	13.057	ng/ul	0.00
73) Anthracene-d10	17.439	188		727262	17.922	ng/ul	-0.01
81) Pyrene-d10	19.669	212		992468	20.429	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.721	264		895620	20.130	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
Data File : BP009833.D
Acq On : 14 Apr 2022 18:05
Operator : CG/JU
Sample : N2293-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ETNN6

Manual IntegrationsAPPROVED

Quant Time: Apr 14 21:47:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 13 02:15:22 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/22/2022

