




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
 Data File : BP009842.D
 Acq On : 14 Apr 2022 23:44
 Operator : CG/JU
 Sample : N2293-22
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETNQ5

Manual IntegrationsAPPROVED

Quant Time: Apr 15 01:46:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/22/2022

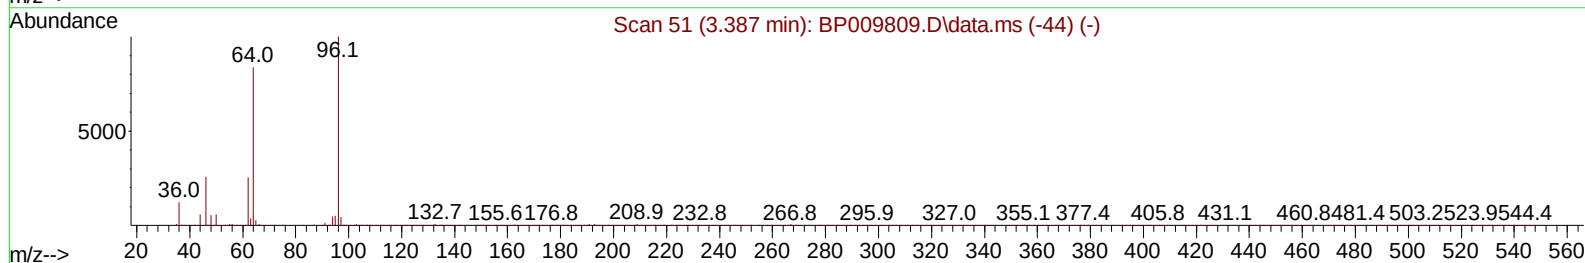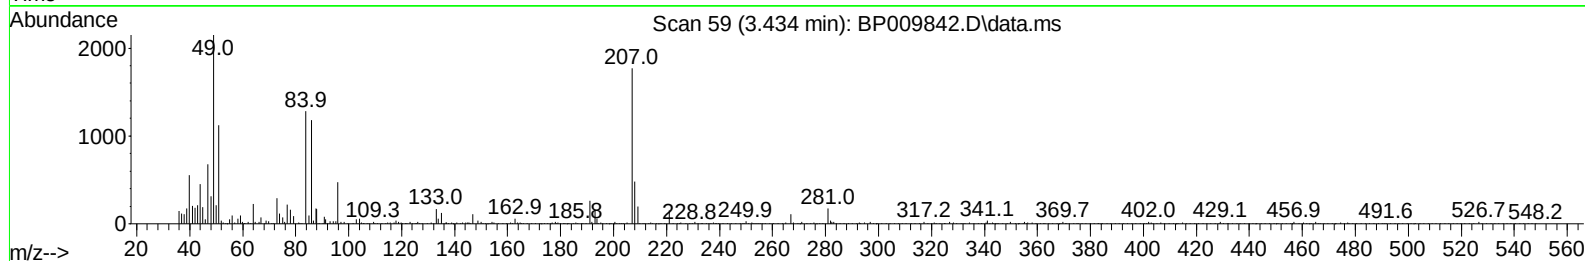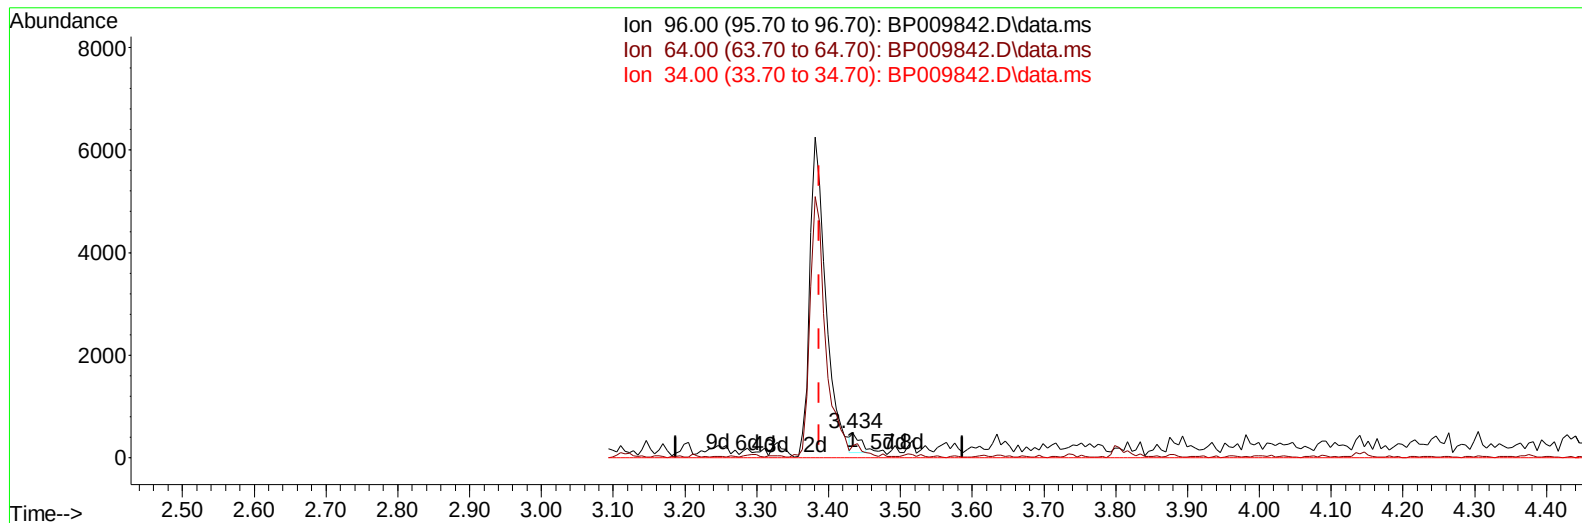

TIC: BP009842.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.434min (+ 0.047) 0.14 ng/uL

response 326

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	48.41
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
 Data File : BP009842.D
 Acq On : 14 Apr 2022 23:44
 Operator : CG/JU
 Sample : N2293-22
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETNQ5

Manual IntegrationsAPPROVED

Quant Time: Apr 15 01:46:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/22/2022

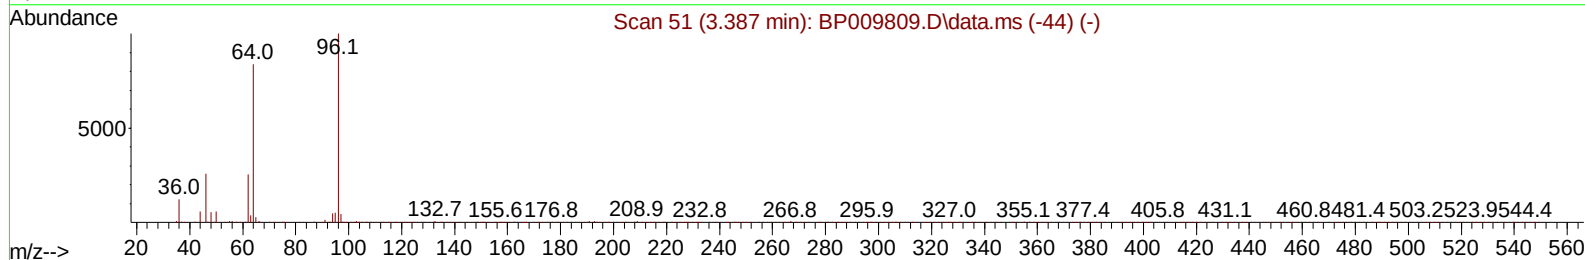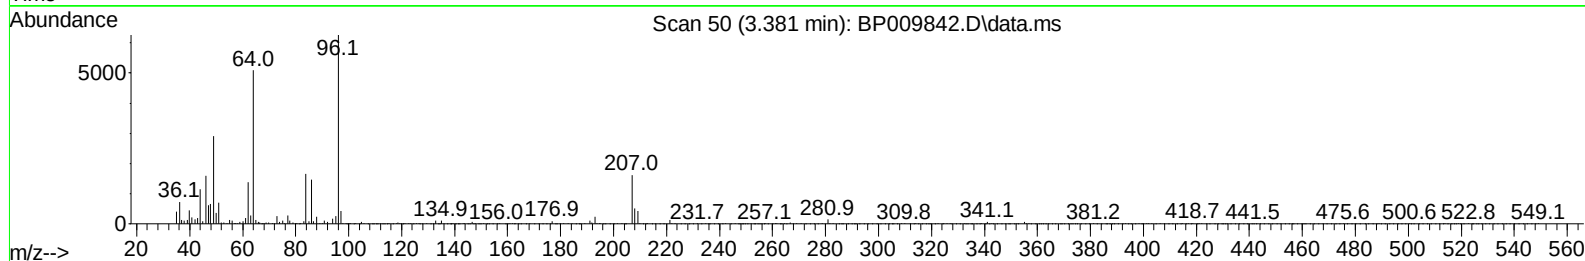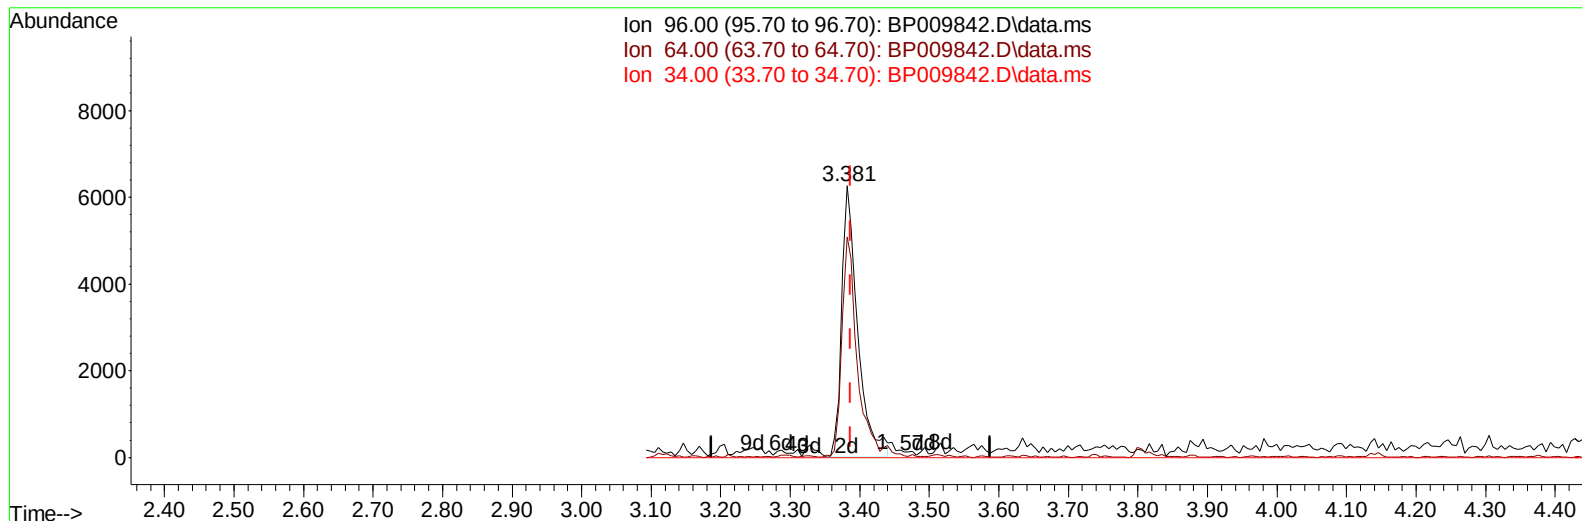

TIC: BP009842.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.381min (-0.006) 4.22 ng/uL m

response 10104

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	81.26#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
 Data File : BP009842.D
 Acq On : 14 Apr 2022 23:44
 Operator : CG/JU
 Sample : N2293-22
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETNQ5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/22/2022

Quant Time: Apr 15 01:46:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.963	152		106956	20.000	ng/ul	0.00
20) Naphthalene-d8	10.769	136		489283	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.593	164		354589	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188		822864	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.422	240		898396	20.000	ng/ul	-0.01
88) Perylene-d12	23.880	264		883182	20.000	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.381	96		10104m	4.216	ng/uL	0.00
4) Pyridine-d5	3.805	84		84493	12.787	ng/ul	0.00
7) Phenol-d5	7.116	99		193012	20.555	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67		127332	22.778	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.487	132		153926	21.732	ng/ul	-0.01
15) 4-Methylphenol-d8	8.658	113		171128	21.831	ng/ul	-0.01
21) Nitrobenzene-d5	9.116	128		81391	23.068	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.840	143		86934	22.473	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.381	165		164091	20.271	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.899	131		214710	18.623	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166		634132	22.767	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160		681040	20.639	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.769	143		88526	17.525	ng/ul	-0.01
60) Fluorene-d10	15.581	176		543060	23.177	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.687	200		56282	11.546	ng/ul	-0.01
73) Anthracene-d10	17.439	188		904691	22.963	ng/ul	-0.01
81) Pyrene-d10	19.669	212		1154395	23.527	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.721	264		1099292	23.901	ng/ul	-0.02
Target Compounds							
37) 1-Methylnaphthalene	12.640	142		30396	1.638	ng/ul#	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
Data File : BP009842.D
Acq On : 14 Apr 2022 23:44
Operator : CG/JU
Sample : N2293-22
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ETNQ5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/22/2022

Quant Time: Apr 15 01:46:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 13 02:15:22 2022
Response via : Initial Calibration

