

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
 Data File : BP009827.D
 Acq On : 14 Apr 2022 14:42
 Operator : CG/JU
 Sample : N2293-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETNN8

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/22/2022

Quant Time: Apr 14 21:45:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	123454	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	541636	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.592	164	390335	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.345	188	897344	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.421	240	963288	20.000	ng/u1	#-0.01
88) Perylene-d12	23.892	264	960052	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	6830	2.469	ng/uL	0.00
4) Pyridine-d5	3.805	84	43664	5.725	ng/u1	0.00
7) Phenol-d5	7.116	99	124421	11.480	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	86037	13.334	ng/u1	0.00
11) 2-Chlorophenol-d4	7.493	132	102766	12.570	ng/u1	0.00
15) 4-Methylphenol-d8	8.663	113	108315	11.971	ng/u1	0.00
21) Nitrobenzene-d5	9.116	128	52483	13.437	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.846	143	51537	12.035	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	102060	11.390	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.898	131	146285	11.462	ng/u1	0.00
46) Dimethylphthalate-d6	13.998	166	396170	12.921	ng/u1	0.00
49) Acenaphthylene-d8	14.287	160	433939	11.946	ng/u1	0.00
54) 4-Nitrophenol-d4	14.769	143	39656m	7.132	ng/u1	-0.01
60) Fluorene-d10	15.581	176	355148	13.769	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.692	200	31928	6.006	ng/u1	0.00
73) Anthracene-d10	17.439	188	577794	13.448	ng/u1	-0.01
81) Pyrene-d10	19.669	212	744675	14.155	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.727	264	702388	14.049	ng/u1	-0.01
Target Compounds						
16) Acetophenone	8.781	105	17092	1.199	ng/u1#	Qvalue 76

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
Data File : BP009827.D
Acq On : 14 Apr 2022 14:42
Operator : CG/JU
Sample : N2293-08
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
ETNN8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/22/2022


Quant Time: Apr 14 21:45:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 13 02:15:22 2022
Response via : Initial Calibration

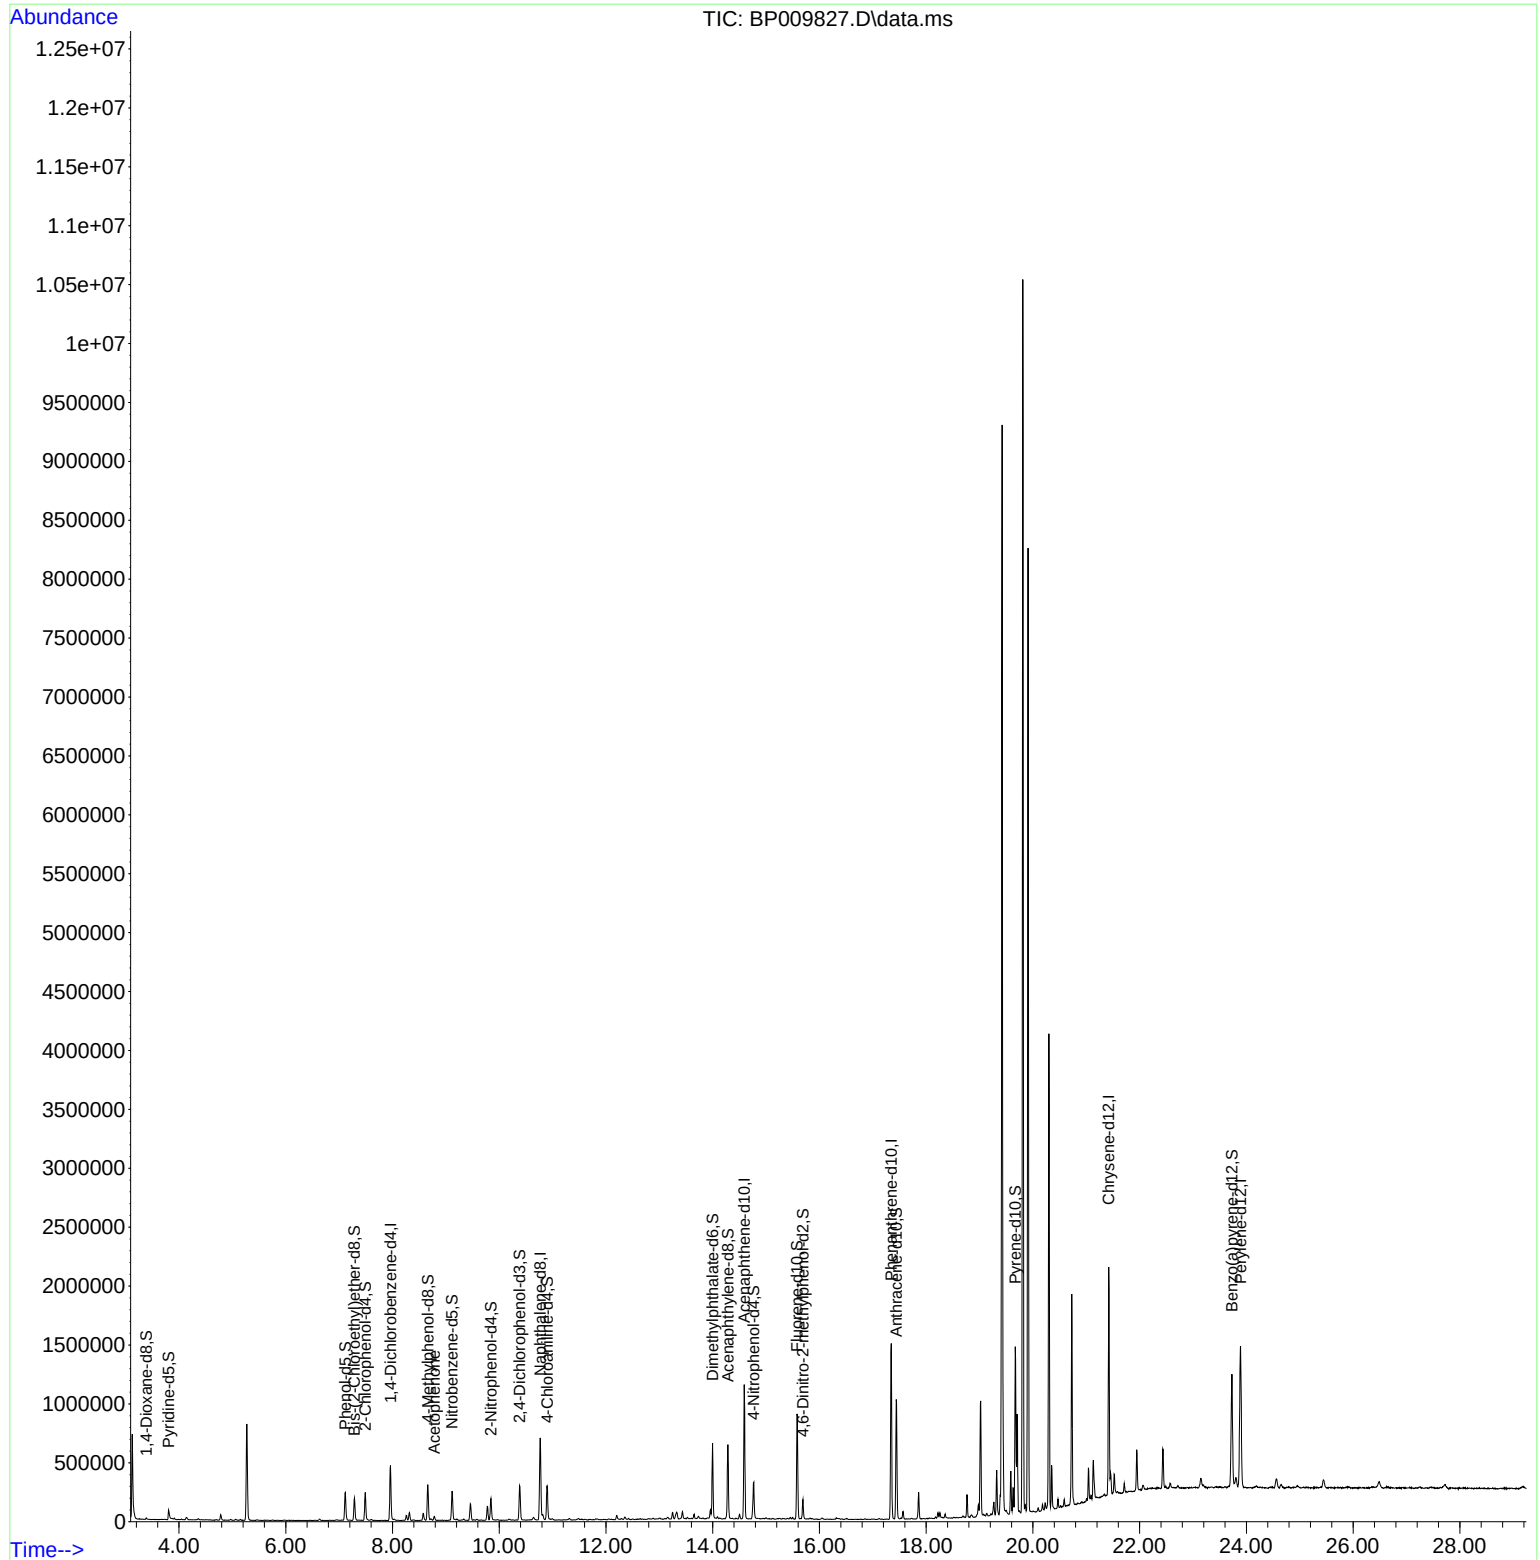

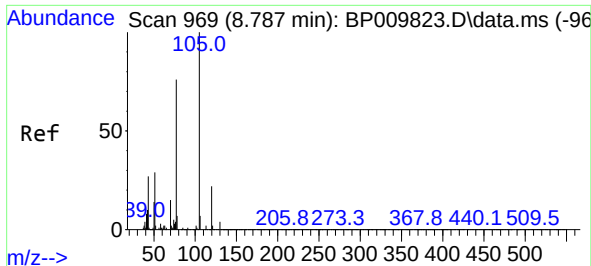

#16
Acetophenone
Concen: 1.199 ng/ul
RT: 8.781 min Scan# 90
Delta R.T. -0.006 min
Lab File: BP009827.D
Acq: 14 Apr 2022 14:42

Instrument :
BNA_P
ClientSampleId :
ETNN8

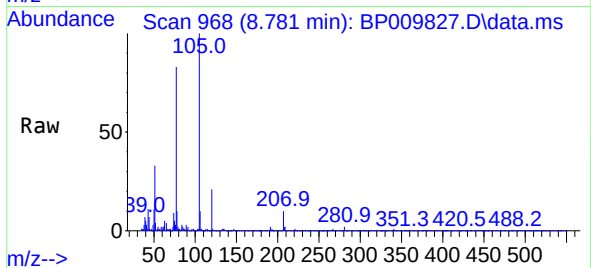

Tgt Ion:105 Resp: 17092
Ion Ratio Lower Upper
105 100
77 83.2 53.4 80.2
51 32.6 13.8 20.8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/22/2022

