

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
 Data File : BP009835.D
 Acq On : 14 Apr 2022 19:13
 Operator : CG/JU
 Sample : N2293-16
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETNP4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/22/2022

Quant Time: Apr 15 02:31:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	97977	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	437585	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.592	164	314772	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.339	188	729812	20.000	ng/u1	#-0.01
79) Chrysene-d12	21.422	240	836737	20.000	ng/u1	#-0.01
88) Perylene-d12	23.880	264	867723	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	11922m	5.431	ng/uL	0.00
4) Pyridine-d5	3.799	84	157179	25.968	ng/u1	0.00
7) Phenol-d5	7.116	99	237821	27.648	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	154194	30.111	ng/u1	0.00
11) 2-Chlorophenol-d4	7.493	132	186223	28.701	ng/u1	0.00
15) 4-Methylphenol-d8	8.663	113	212571	29.603	ng/u1	0.00
21) Nitrobenzene-d5	9.116	128	99903	31.659	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.846	143	107963	31.207	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	205705	28.415	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.899	131	298100m	28.911	ng/u1	0.00
46) Dimethylphthalate-d6	13.998	166	757143	30.622	ng/u1	0.00
49) Acenaphthylene-d8	14.281	160	840125	28.680	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.769	143	124304	27.721	ng/u1	-0.01
60) Fluorene-d10	15.581	176	653875	31.436	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.692	200	100796	23.314	ng/u1	0.00
73) Anthracene-d10	17.439	188	1053946	30.162	ng/u1	-0.01
81) Pyrene-d10	19.669	212	1329068	29.083	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.727	264	1384485	30.638	ng/u1	-0.01
Target Compounds						
29) 2,4-Dichlorophenol	10.410	162	22329	3.181	ng/u1#	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
Data File : BP009835.D
Acq On : 14 Apr 2022 19:13
Operator : CG/JU
Sample : N2293-16
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
ETNP4

Quant Time: Apr 15 02:31:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 13 02:15:22 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/22/2022

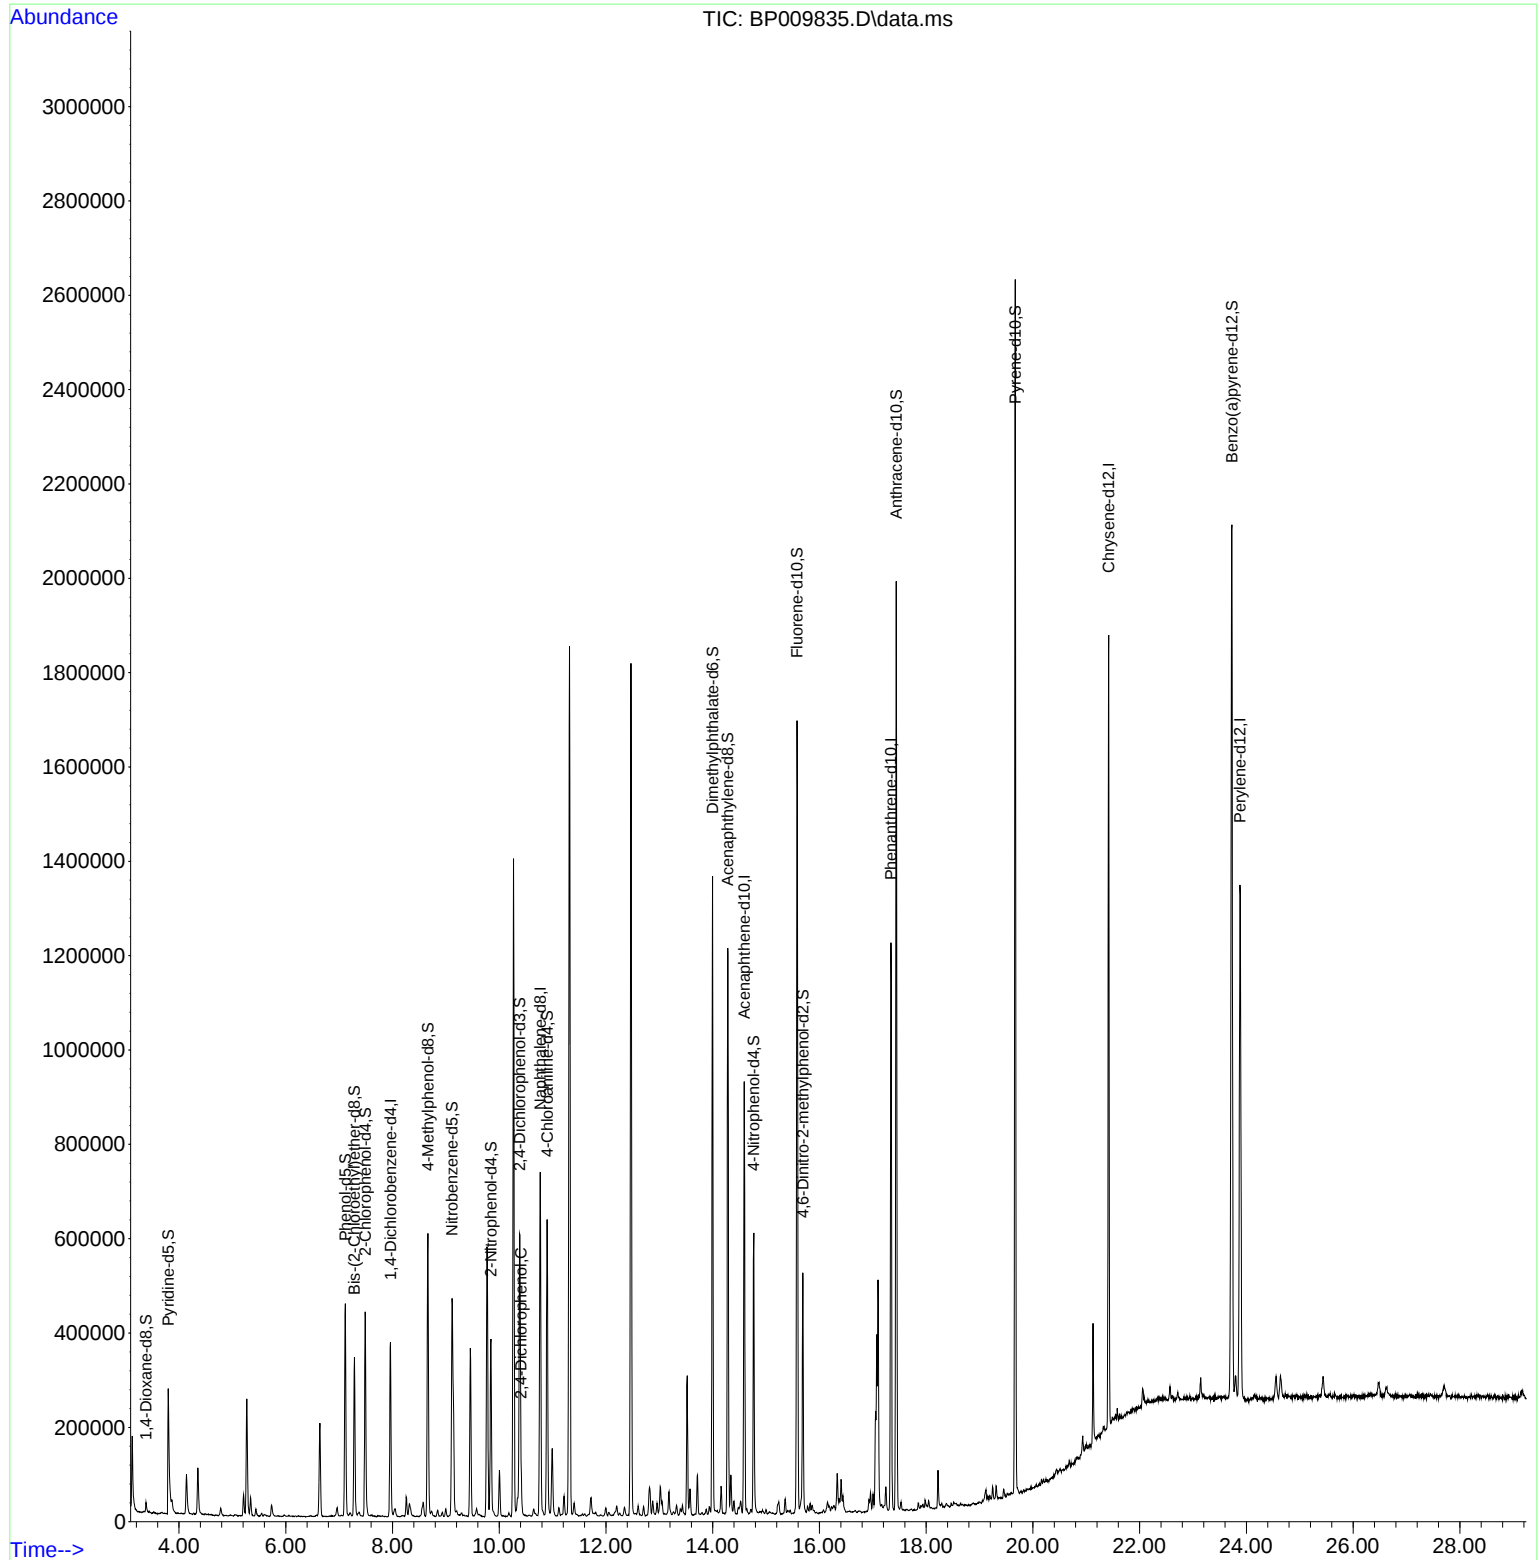

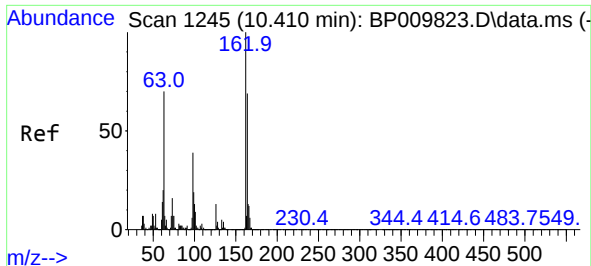

#29
2,4-Dichlorophenol
Concen: 3.181 ng/ul
RT: 10.410 min Scan# 10
Delta R.T. -0.012 min
Lab File: BP009835.D
Acq: 14 Apr 2022 19:13

Instrument :
BNA_P
ClientSampleId :
ETNP4

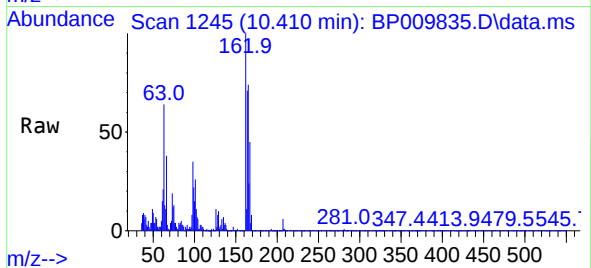

Tgt Ion:162 Resp: 22329
Ion Ratio Lower Upper
162 100
164 70.9 37.0 55.6
98 35.3 31.0 46.6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/22/2022

