

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
 Data File : BP009831.D
 Acq On : 14 Apr 2022 16:57
 Operator : CG/JU
 Sample : N2293-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETNN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009831.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	3	6	25	rVB	707244	986754	34.24%	3.095%
2	3.387	47	51	56	rBV2	13781	21409	0.74%	0.067%
3	3.805	119	122	136	rBV	81807	146854	5.10%	0.461%
4	4.040	158	162	167	rBV6	4647	7980	0.28%	0.025%
5	4.134	174	178	185	rBV2	10095	17019	0.59%	0.053%
6	4.781	282	288	297	rVB3	9086	18289	0.63%	0.057%
7	5.063	331	336	343	rBV4	11675	20855	0.72%	0.065%
8	5.269	365	371	378	rBV	53888	86796	3.01%	0.272%
9	6.640	601	604	608	rVB6	2321	3964	0.14%	0.012%
10	6.934	649	654	656	rBV6	2330	3362	0.12%	0.011%
11	7.116	677	685	696	rBV	269041	459114	15.93%	1.440%
12	7.287	706	714	723	rBV	211060	343840	11.93%	1.078%
13	7.363	723	727	732	rVB2	3533	6519	0.23%	0.020%
14	7.493	737	749	760	rBV	272844	464259	16.11%	1.456%
15	7.598	763	767	775	rVB9	4404	6997	0.24%	0.022%
16	7.963	822	829	837	rBV	528024	874498	30.34%	2.743%
17	8.034	837	841	847	rVB2	6744	10640	0.37%	0.033%
18	8.181	858	866	869	rBV9	2478	4401	0.15%	0.014%
19	8.322	886	890	896	rVB9	2032	3381	0.12%	0.011%
20	8.422	902	907	914	rVB9	5522	11821	0.41%	0.037%
21	8.663	935	948	954	rBV	370343	646775	22.44%	2.029%
22	8.781	965	968	980	rVB2	26440	50033	1.74%	0.157%
23	9.116	1018	1025	1036	rBV	274465	477243	16.56%	1.497%
24	9.228	1039	1044	1048	rVV7	2120	4222	0.15%	0.013%
25	9.292	1051	1055	1059	rVB6	4390	7386	0.26%	0.023%
26	9.457	1077	1083	1090	rVB2	28161	50943	1.77%	0.160%
27	9.575	1097	1103	1109	rBV5	8971	16909	0.59%	0.053%
28	9.787	1134	1139	1141	rVV6	5594	9444	0.33%	0.030%
29	9.845	1141	1149	1161	rVB	217955	374569	13.00%	1.175%
30	9.975	1167	1171	1176	rBV7	3416	5718	0.20%	0.018%
31	10.210	1205	1211	1215	rVB8	2974	6168	0.21%	0.019%
32	10.269	1215	1221	1227	rBV10	4703	8790	0.31%	0.028%
33	10.381	1233	1240	1260	rVB	338756	595068	20.65%	1.866%
34	10.645	1279	1285	1291	rBV10	3975	6835	0.24%	0.021%
35	10.769	1298	1306	1318	rBV	781160	1303355	45.23%	4.088%
36	10.898	1320	1328	1338	rBV	355043	618214	21.45%	1.939%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
 Data File : BP009831.D
 Acq On : 14 Apr 2022 16:57
 Operator : CG/JU
 Sample : N2293-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETNN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

37	11.169	1371	1374	1379	rBV7	2761	4554	0.16%	0.014%
38	11.234	1379	1385	1394	rVV	33685	88569	3.07%	0.278%
39	11.310	1395	1398	1405	rVB8	13794	25711	0.89%	0.081%
40	11.557	1433	1440	1445	rBV10	5594	9609	0.33%	0.030%
41	11.739	1462	1471	1476	rBV10	4221	9014	0.31%	0.028%
42	11.916	1496	1501	1505	rBV7	2985	4970	0.17%	0.016%
43	12.204	1545	1550	1553	rBV5	5569	8209	0.28%	0.026%
44	12.351	1570	1575	1581	rBV4	7090	13577	0.47%	0.043%
45	12.481	1592	1597	1599	rBV6	5060	9436	0.33%	0.030%
46	12.598	1614	1617	1621	rVB6	2625	3309	0.11%	0.010%
47	12.963	1676	1679	1683	rVB6	3302	4053	0.14%	0.013%
48	13.051	1692	1694	1697	rVB4	2802	3142	0.11%	0.010%
49	13.104	1697	1703	1708	rBV10	3378	8760	0.30%	0.027%
50	13.157	1708	1712	1716	rVB7	2369	4144	0.14%	0.013%
51	13.210	1718	1721	1726	rVV6	2300	3702	0.13%	0.012%
52	13.269	1726	1731	1734	rVV7	3223	5559	0.19%	0.017%
53	13.322	1735	1740	1747	rVB7	3422	7099	0.25%	0.022%
54	13.433	1754	1759	1764	rVB7	9768	14588	0.51%	0.046%
55	13.522	1769	1774	1778	rBV8	3390	6052	0.21%	0.019%
56	13.563	1778	1781	1788	rVB8	2540	5268	0.18%	0.017%
57	13.957	1845	1848	1849	rBV3	2563	3113	0.11%	0.010%
58	13.998	1849	1855	1863	rVV	758030	1054167	36.58%	3.306%
59	14.145	1877	1880	1885	rVB7	5346	7525	0.26%	0.024%
60	14.286	1892	1904	1915	rBV	695928	1093997	37.96%	3.431%
61	14.486	1935	1938	1943	rBV4	4454	7864	0.27%	0.025%
62	14.592	1948	1956	1966	rBV	1286983	1884286	65.38%	5.910%
63	14.680	1968	1971	1976	rVB2	4105	6312	0.22%	0.020%
64	14.769	1980	1986	1998	rVV	245570	373163	12.95%	1.170%
65	14.857	1998	2001	2005	rVV6	4580	7035	0.24%	0.022%
66	14.922	2008	2012	2016	rBV7	3479	5726	0.20%	0.018%
67	15.004	2021	2026	2032	rBV9	15767	22062	0.77%	0.069%
68	15.251	2064	2068	2072	rVB7	3964	6441	0.22%	0.020%
69	15.404	2089	2094	2099	rVB6	7094	11732	0.41%	0.037%
70	15.580	2117	2124	2136	rBV	1011741	1531741	53.15%	4.804%
71	15.692	2136	2143	2156	rVV	226183	340330	11.81%	1.067%
72	15.822	2160	2165	2169	rVV4	15549	27731	0.96%	0.087%
73	15.863	2170	2172	2178	rVB3	8944	11106	0.39%	0.035%
74	16.374	2255	2259	2264	rVB7	6825	9634	0.33%	0.030%
75	16.639	2300	2304	2307	rVB6	3679	4703	0.16%	0.015%
76	16.769	2324	2326	2330	rVB3	4092	4290	0.15%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
 Data File : BP009831.D
 Acq On : 14 Apr 2022 16:57
 Operator : CG/JU
 Sample : N2293-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETNN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

77	17.016	2367	2368	2374	rVB6	3137	4648	0.16%	0.015%
78	17.104	2378	2383	2384	rVV5	3771	5237	0.18%	0.016%
79	17.116	2384	2385	2390	rVB3	4621	5500	0.19%	0.017%
80	17.269	2408	2411	2415	rBV6	2359	4217	0.15%	0.013%
81	17.345	2417	2424	2432	rVV	1614036	2379563	82.57%	7.463%
82	17.439	2434	2440	2447	rVV	1316571	1910532	66.29%	5.992%
83	17.492	2447	2449	2452	rVV4	13941	19985	0.69%	0.063%
84	17.527	2452	2455	2462	rVB5	14220	23319	0.81%	0.073%
85	17.710	2483	2486	2487	rBV3	3193	3232	0.11%	0.010%
86	17.868	2510	2513	2517	rBV6	3844	4957	0.17%	0.016%
87	18.016	2535	2538	2542	rVB6	5094	6210	0.22%	0.019%
88	18.227	2569	2574	2579	rBV	62671	89626	3.11%	0.281%
89	18.692	2649	2653	2655	rBV4	4491	6166	0.21%	0.019%
90	19.245	2745	2747	2752	rVB5	20528	23376	0.81%	0.073%
91	19.310	2754	2758	2762	rBV	28744	44465	1.54%	0.139%
92	19.457	2780	2783	2786	rBV5	13548	13617	0.47%	0.043%
93	19.668	2813	2819	2822	rBV	1974287	2531345	87.84%	7.939%
94	19.704	2822	2825	2838	rVV	2422803	2881927	100.00%	9.039%
95	19.804	2840	2842	2847	rVB5	14202	17520	0.61%	0.055%
96	20.174	2903	2905	2910	rVB2	21970	24965	0.87%	0.078%
97	21.127	3064	3067	3074	rBV2	143689	199368	6.92%	0.625%
98	21.421	3112	3117	3124	rBV	2016360	2658841	92.26%	8.339%
99	23.727	3502	3509	3518	rVB2	1120565	2230921	77.41%	6.997%
100	23.886	3529	3536	3546	rVB	1207492	2461941	85.43%	7.722%




Sum of corrected areas: 31884185

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
Data File : BP009831.D
Acq On : 14 Apr 2022 16:57
Operator : CG/JU
Sample : N2293-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ETNN5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

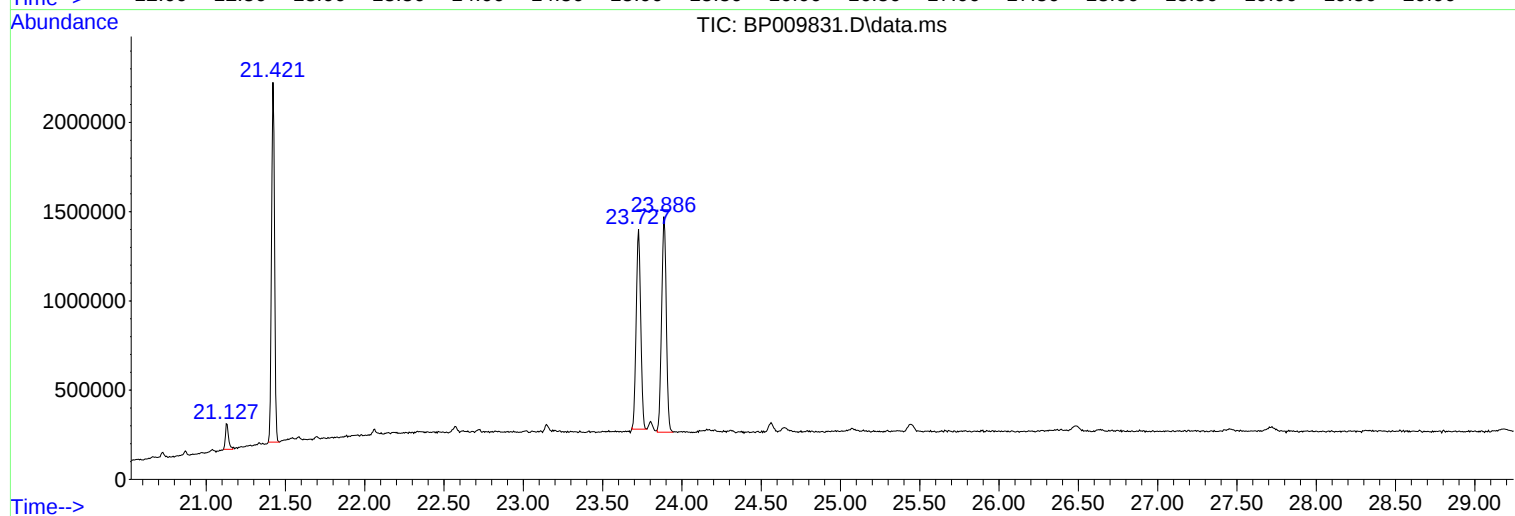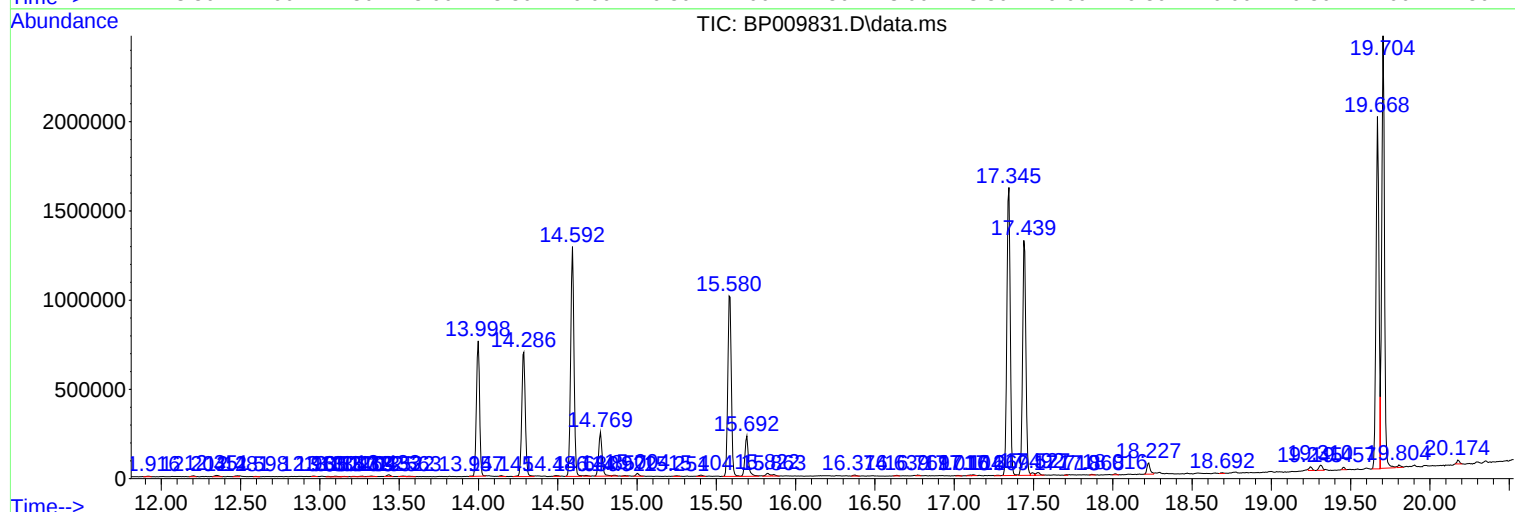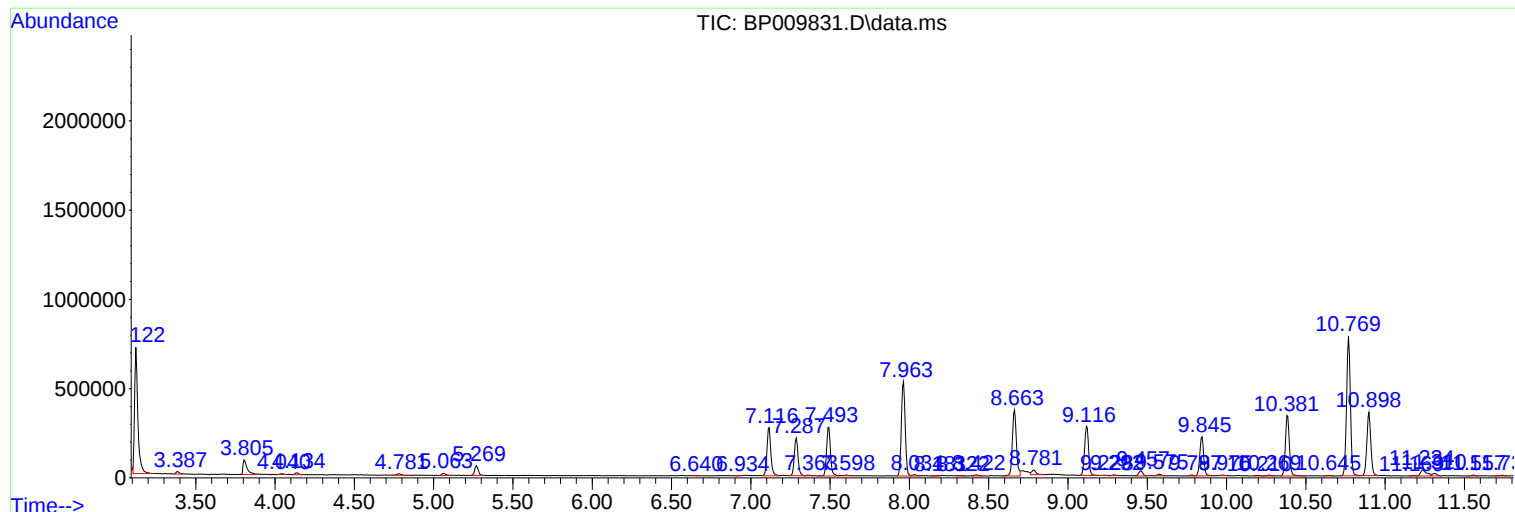

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
Data File : BP009831.D
Acq On : 14 Apr 2022 16:57
Operator : CG/JU
Sample : N2293-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ETNN5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.122	22.57 ng/ul	986754	1,4-Dichlorobenzene-d4	7.963

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	56
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
4			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	37
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	27

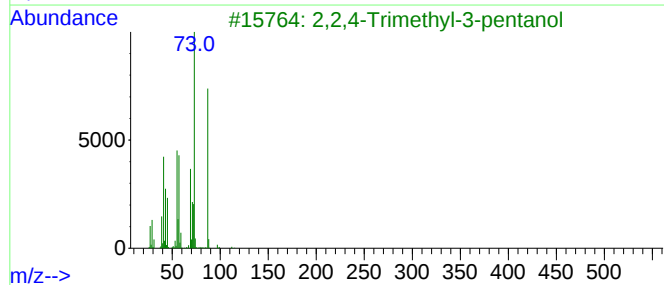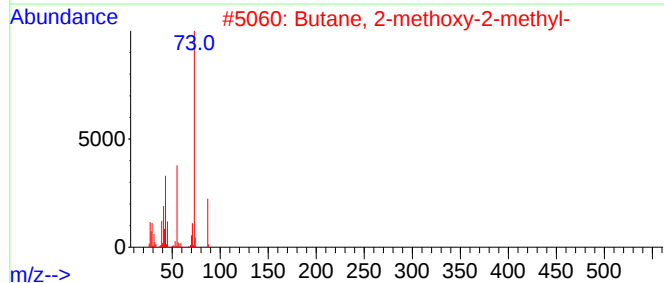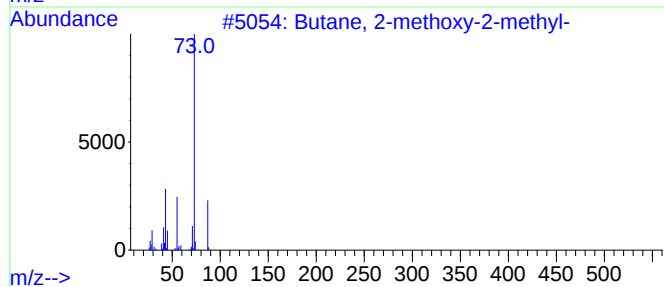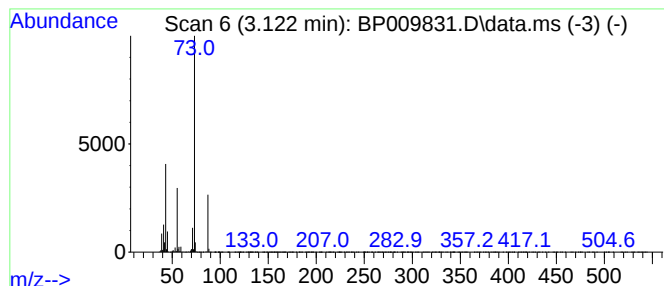

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041422\
Data File : BP009831.D
Acq On : 14 Apr 2022 16:57
Operator : CG/JU
Sample : N2293-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ETNN5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.122	22.6	ng/ul	986754	1	7.963	874498	20.0