
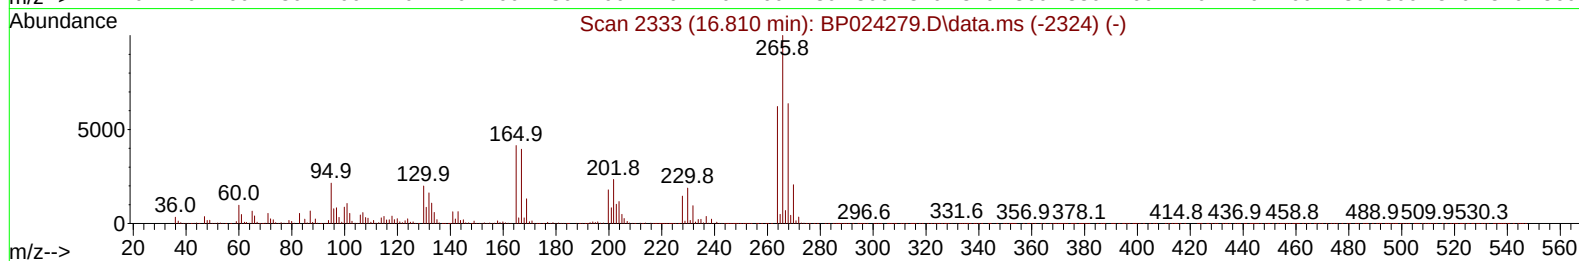
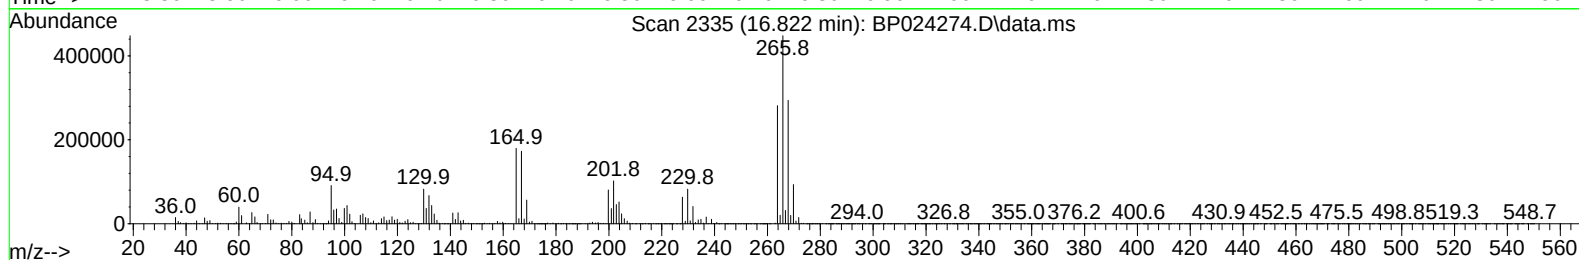


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041425\
Data File : BP024274.D
Acq On : 14 Apr 2025 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 15:07:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 14 15:04:09 2025
Response via : Initial Calibration

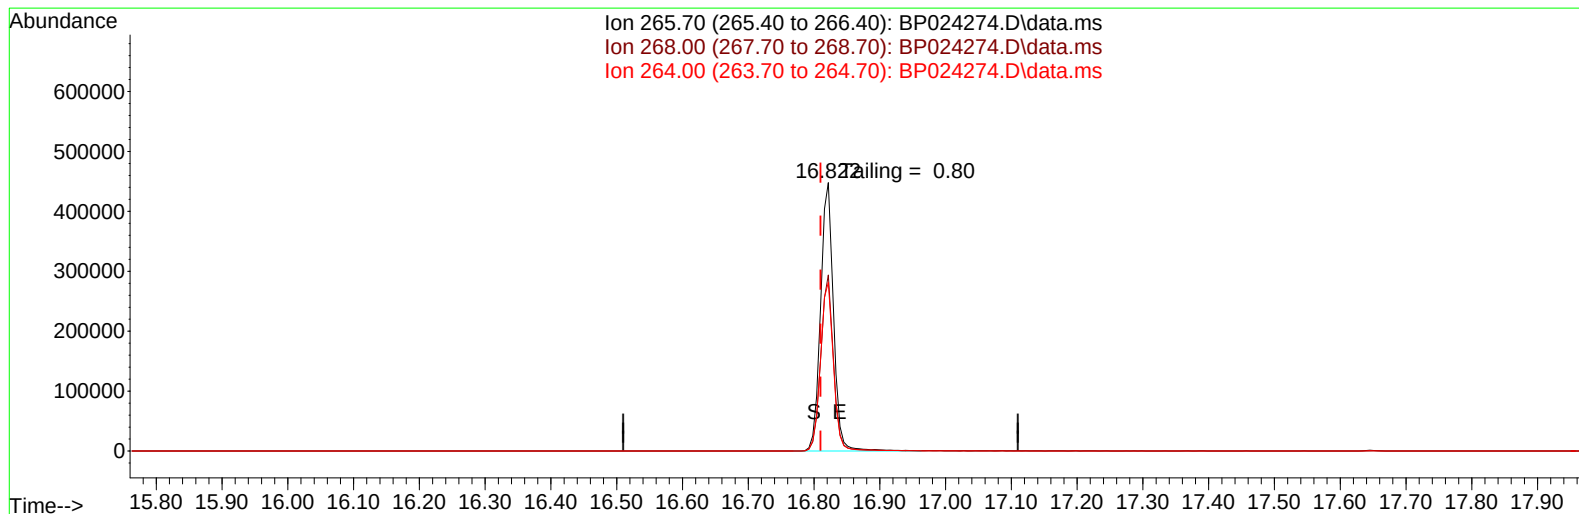

TIC: BP024274.D\data.ms

(70) Pentachlorophenol (C)




16.822min (+ 0.012) 3117222.42 ng

response 611847

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.61
264.00	62.20	62.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041425\
Data File : BP024274.D
Acq On : 14 Apr 2025 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 15:07:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 14 15:04:09 2025
Response via : Initial Calibration

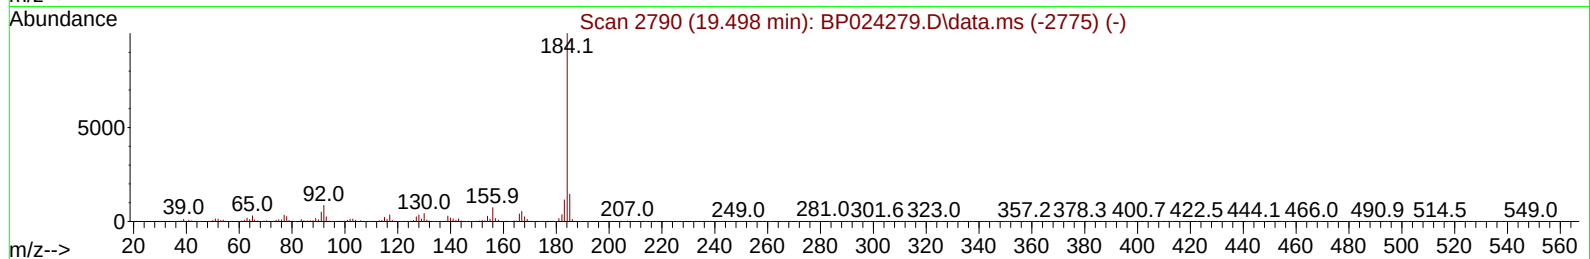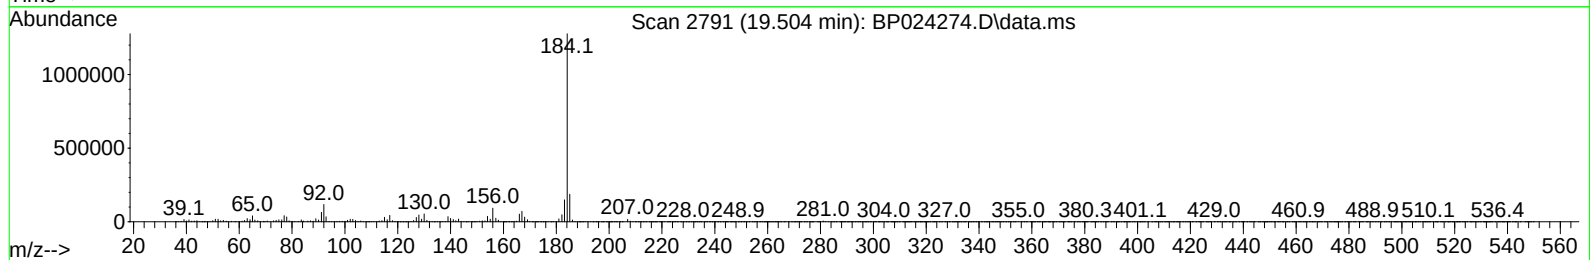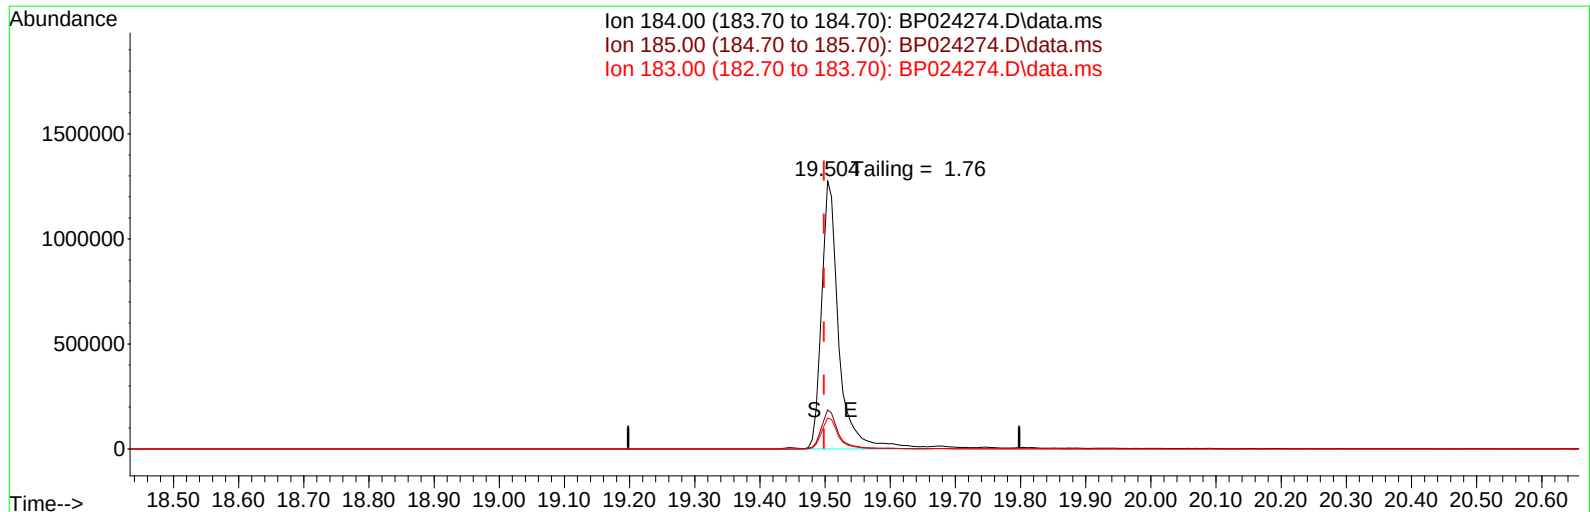

TIC: BP024274.D\data.ms

(77) Benzidine

19.504min (+ 0.006) 7415471.13 ng

response 2354373

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.60
183.00	11.50	11.64
0.00	0.00	0.00