
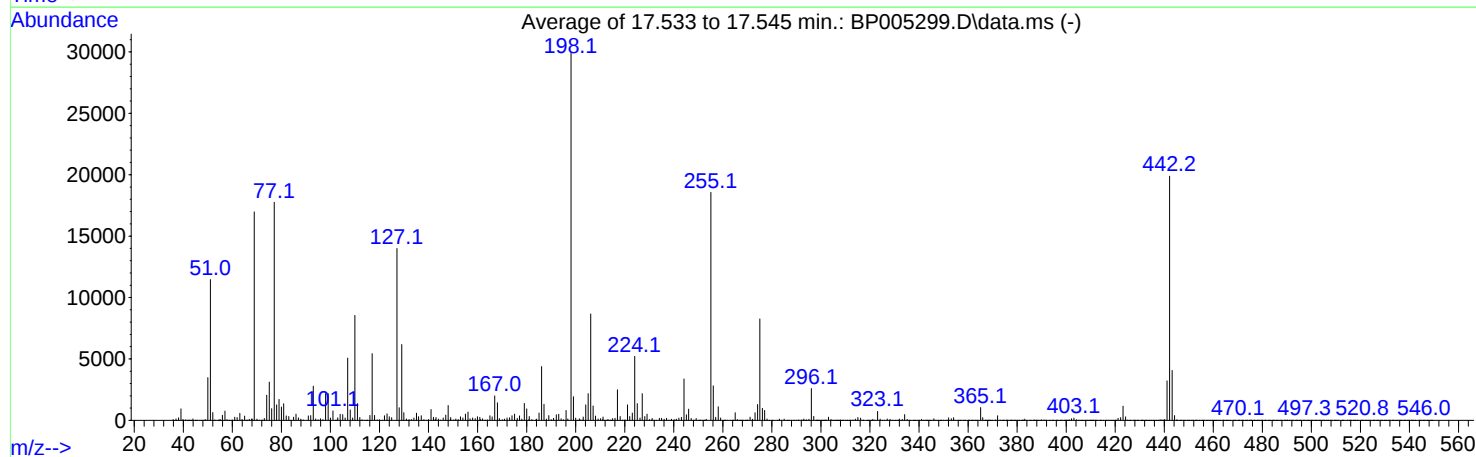


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041521\
 Data File : BP005299.D
 Acq On : 15 Apr 2021 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 16 11:02:58 2021

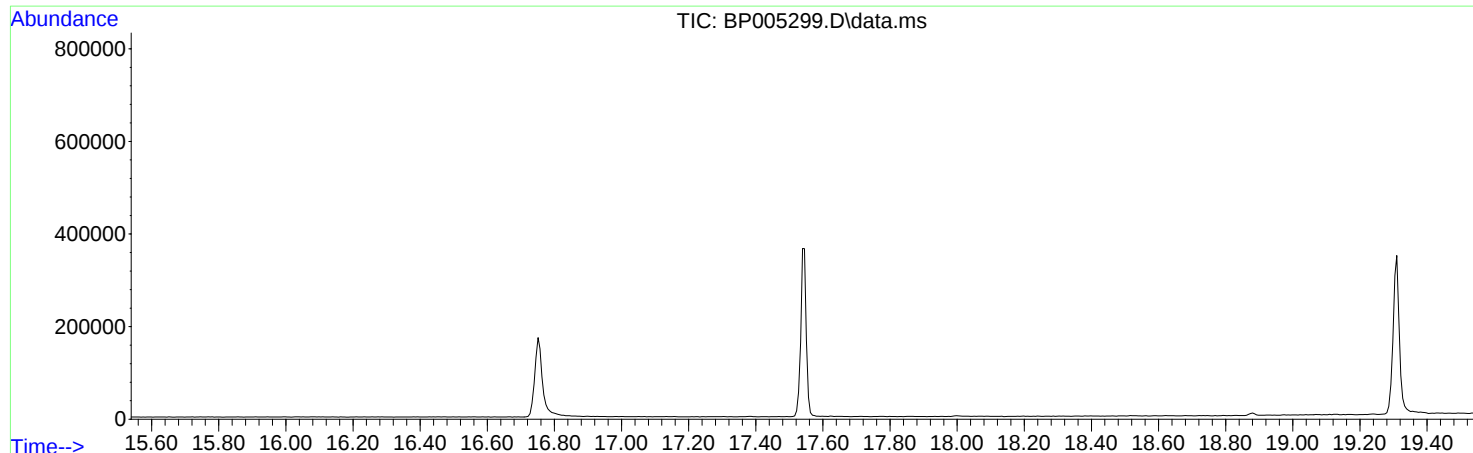




AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	11466	PASS
68	69	0.00	2	0.7	114	PASS
69	198	0.00	100	56.7	16972	PASS
70	69	0.00	2	0.6	104	PASS
127	198	10	80	46.7	13996	PASS
197	198	0.00	2	0.4	113	PASS
198	198	100	100	100.0	29952	PASS
199	198	5	9	6.4	1930	PASS
275	198	10	60	27.6	8264	PASS
365	198	1	100	3.5	1039	PASS
441	198	0.01	100	10.7	3219	PASS
442	442	100	100	100.0	19878	PASS
443	442	15	24	20.5	4067	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041521\
 Data File : BP005299.D
 Acq On : 15 Apr 2021 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 16 05:53:03 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 03:03:58 2021
 Response via : Initial Calibration

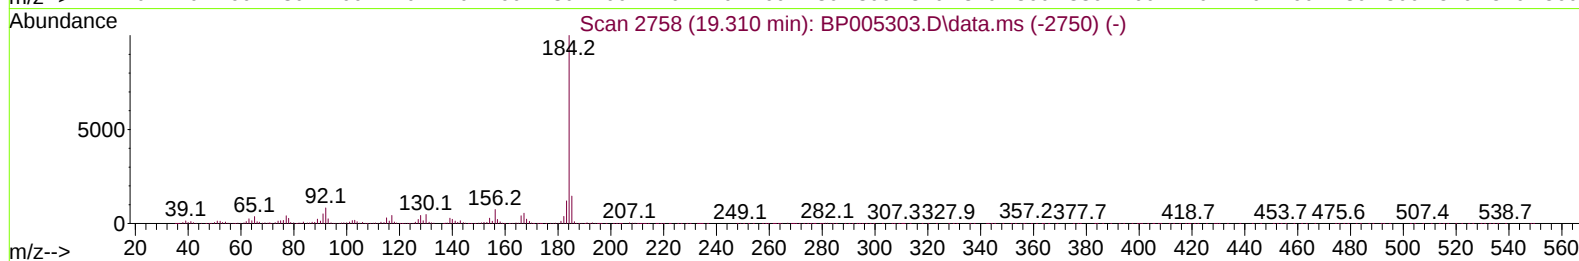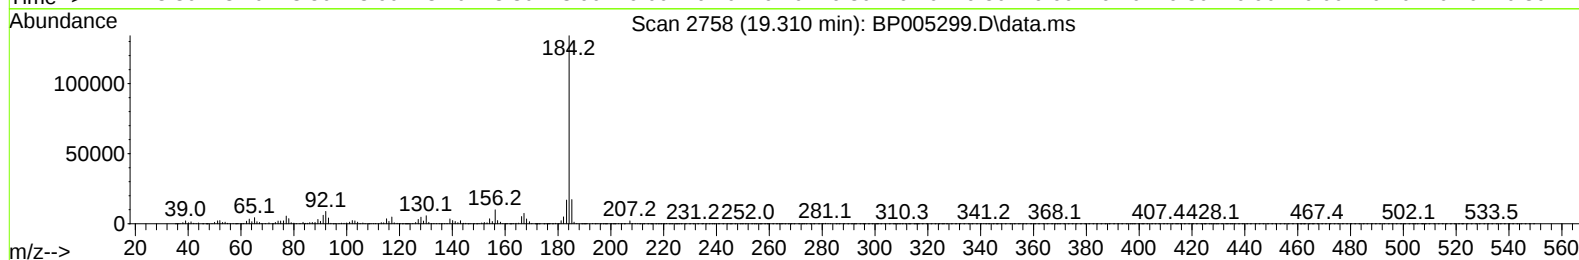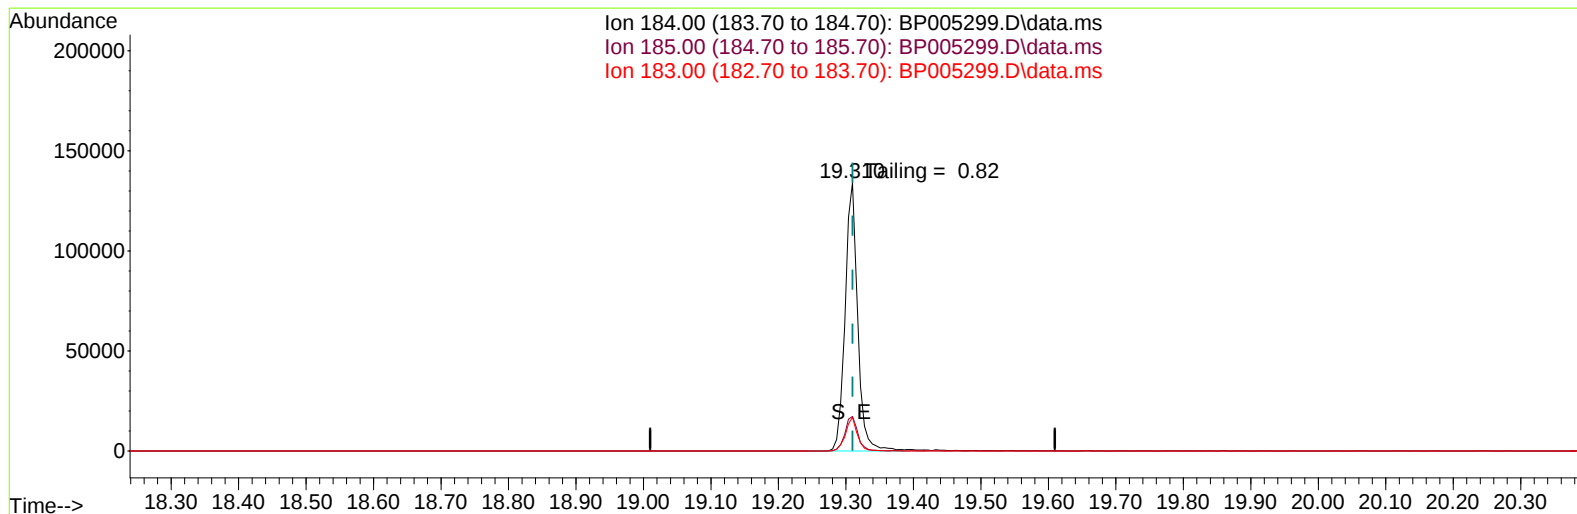

TIC: BP005299.D\data.ms

(77) Benzidine

19.310min (-0.000) 192230.66 ng




response 173551

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	12.89
183.00	12.10	12.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041521\
Data File : BP005299.D
Acq On : 15 Apr 2021 09:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 16 05:53:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 03:03:58 2021
Response via : Initial Calibration

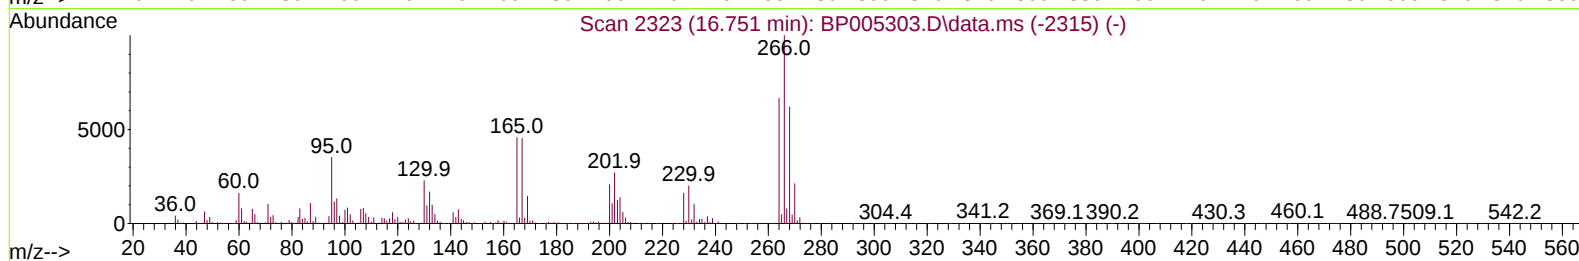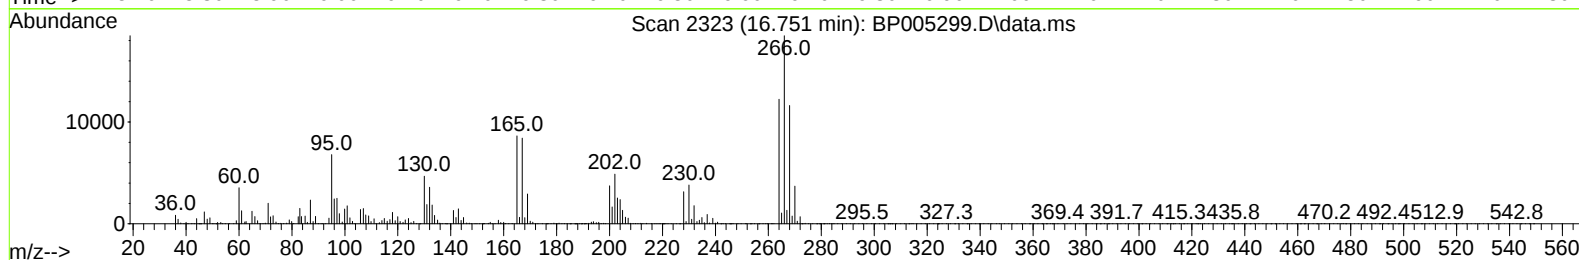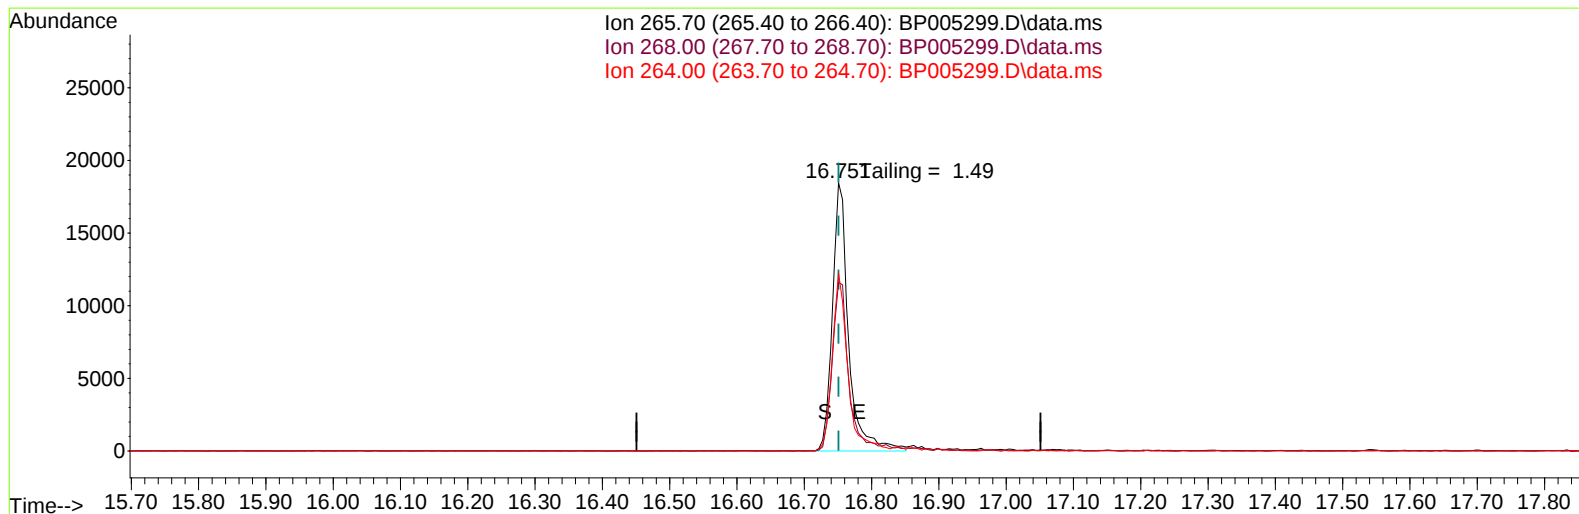

TIC: BP005299.D\data.ms

(70) Pentachlorophenol (C)

16.751min (0.000) 276101.75 ng

response 30764

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	62.90
264.00	66.60	66.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/15/2021	BNA_P	<u>BP005299.D</u>
Compound Name	Response	Retention Time
DDT	137473	20.504
DDD	1616	20.08
DDE	213	19.574
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1829	139302	1.31