
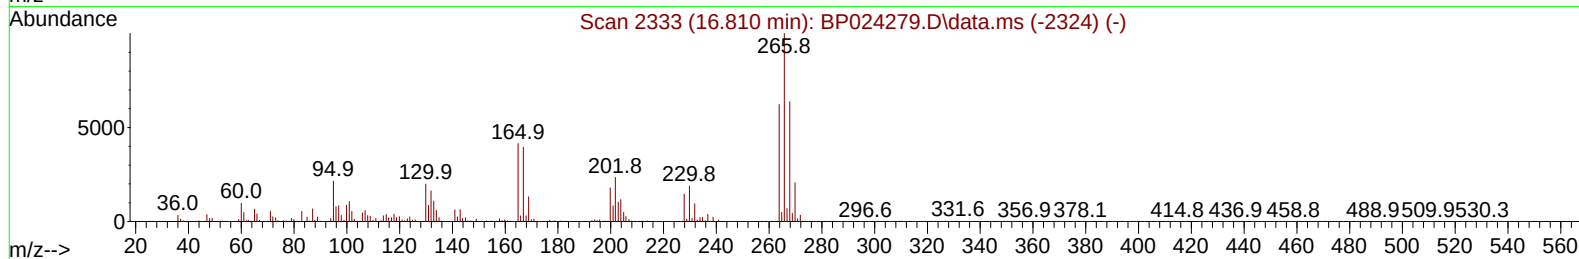
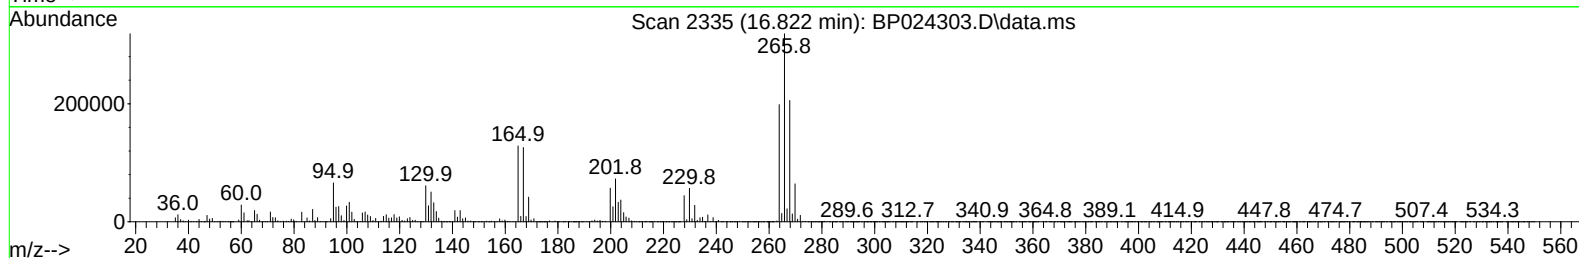


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041625\
Data File : BP024303.D
Acq On : 16 Apr 2025 09:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 11:22:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 15 04:48:42 2025
Response via : Initial Calibration

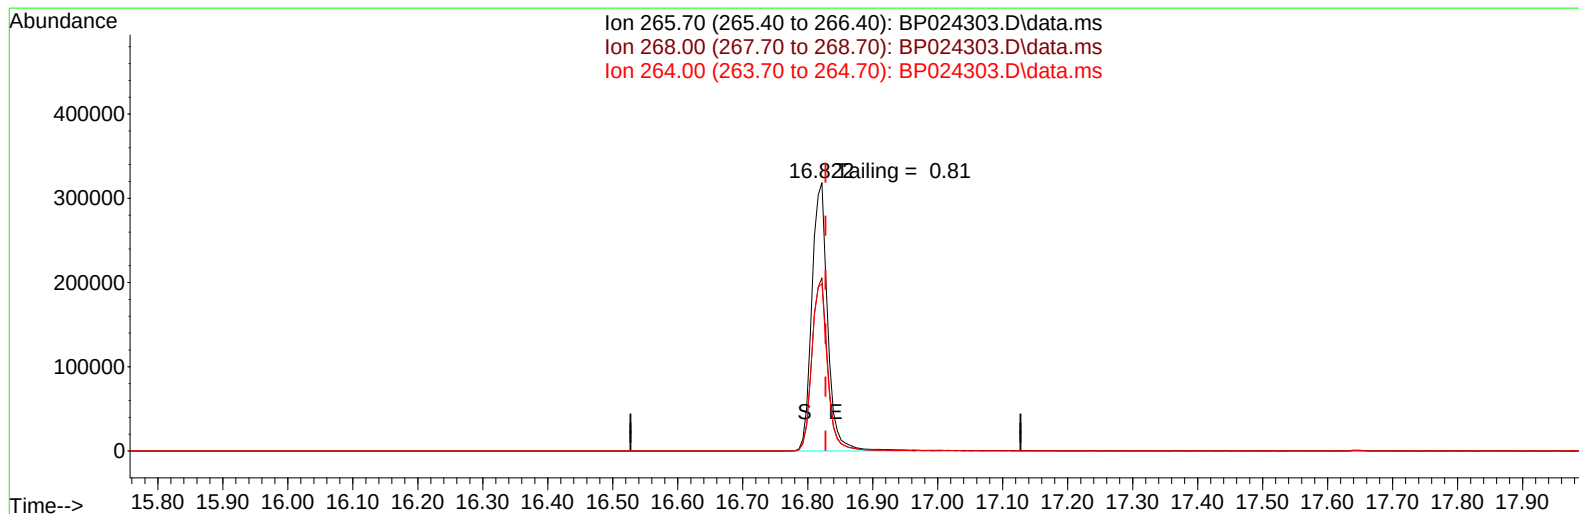

TIC: BP024303.D\data.ms

(70) Pentachlorophenol (C)




16.822min (-0.006) 63083.83 ng

response 543342

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.53
264.00	62.20	62.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041625\
 Data File : BP024303.D
 Acq On : 16 Apr 2025 09:02
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 11:22:11 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 15 04:48:42 2025
 Response via : Initial Calibration

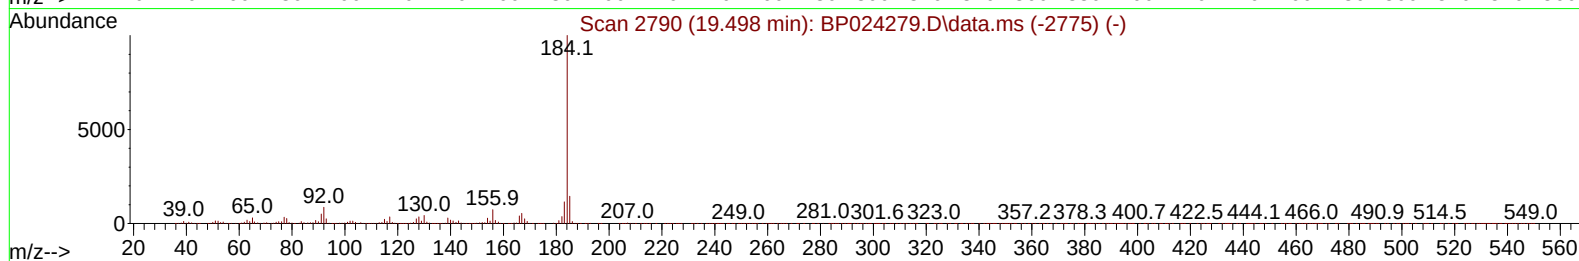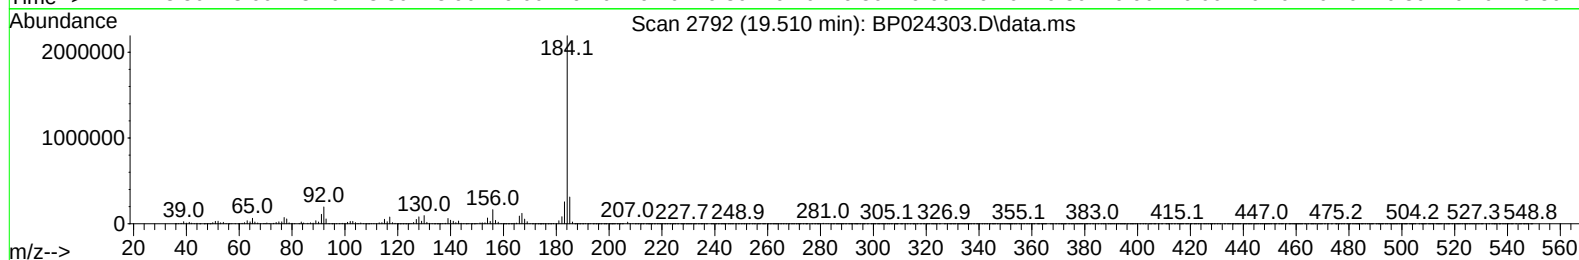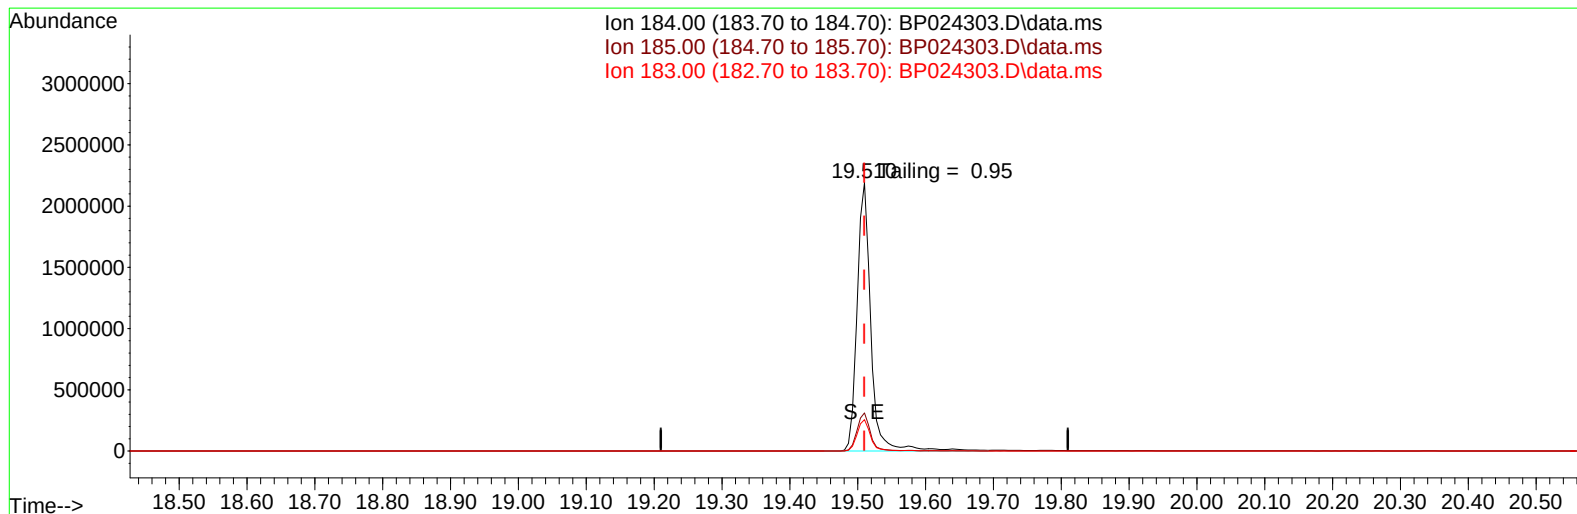

TIC: BP024303.D\data.ms

(77) Benzidine

19.510min (+ 0.000) 173060.25 ng

response 2961475

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.19
183.00	11.50	11.69
0.00	0.00	0.00