




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009912.D
Acq On : 18 Apr 2022 13:20
Operator : CG/JU
Sample : N2422-07DL 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J54DL

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:54:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/22/2022

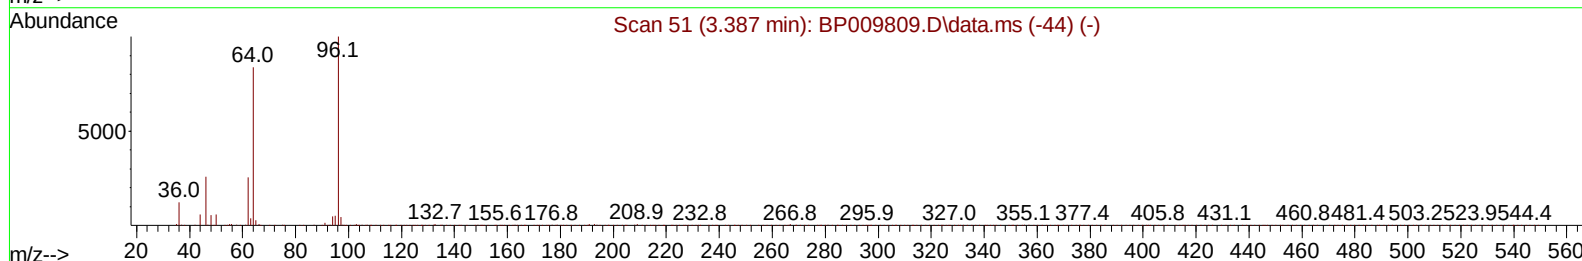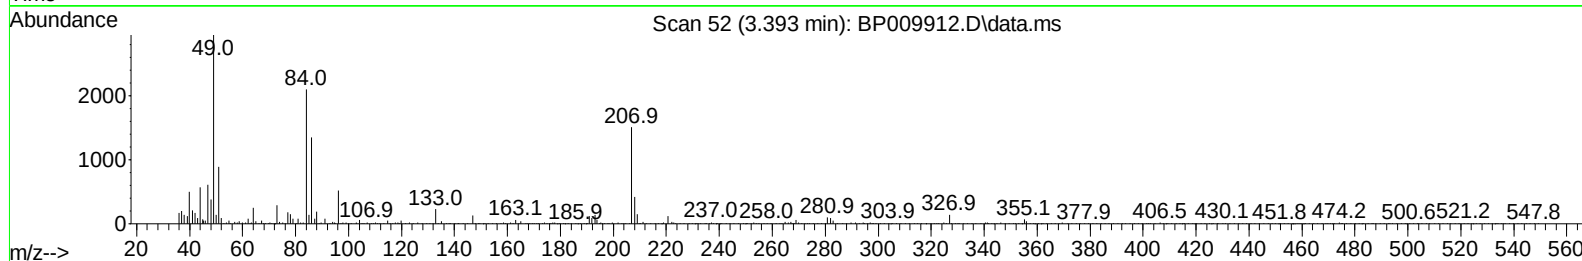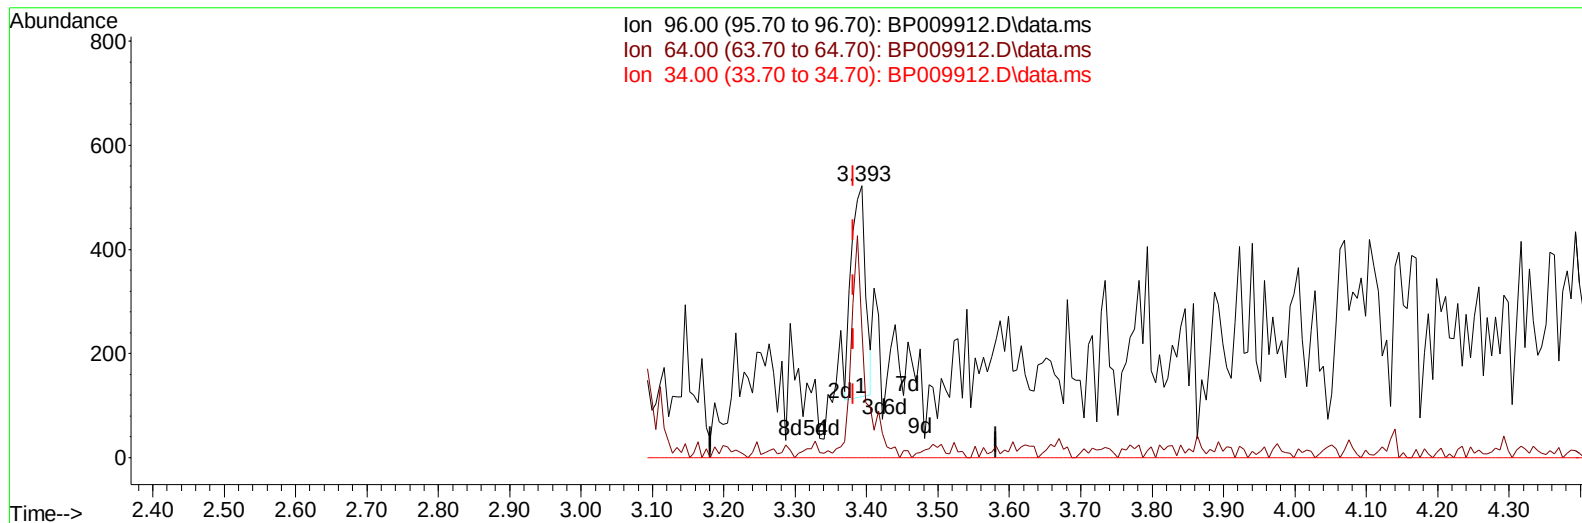

TIC: BP009912.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.393min (+ 0.012) 0.22 ng/uL

response 565

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	47.13
34.00	0.00	0.00
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009912.D
 Acq On : 18 Apr 2022 13:20
 Operator : CG/JU
 Sample : N2422-07DL 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J54DL

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:54:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/22/2022

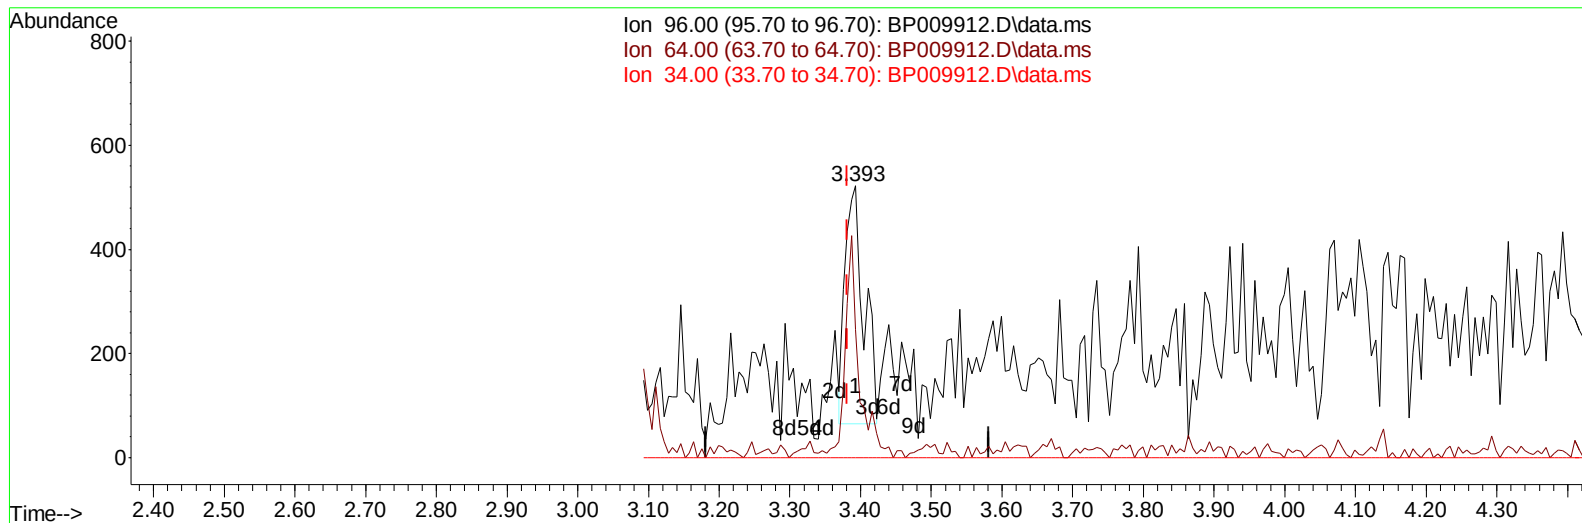




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009912.D
 Acq On : 18 Apr 2022 13:20
 Operator : CG/JU
 Sample : N2422-07DL 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J54DL

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:54:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/22/2022

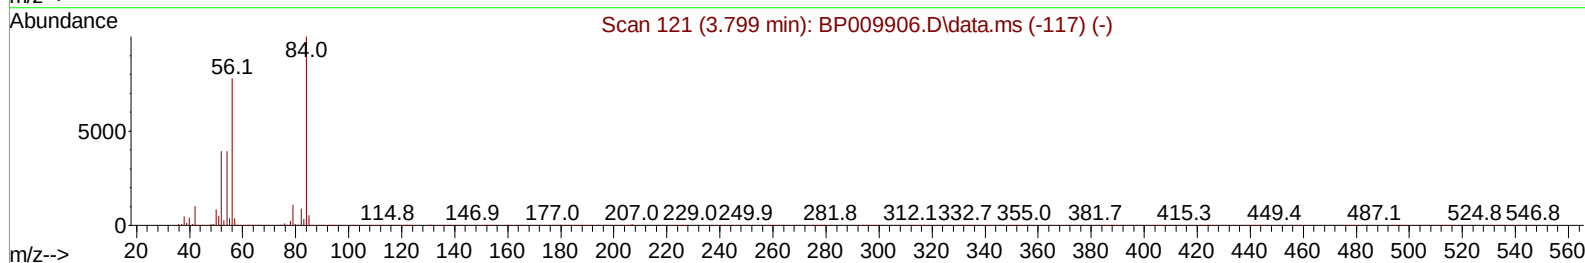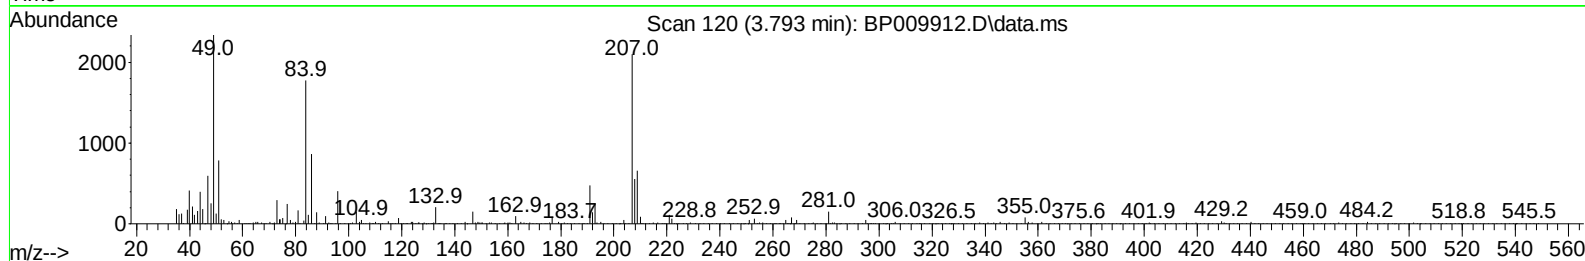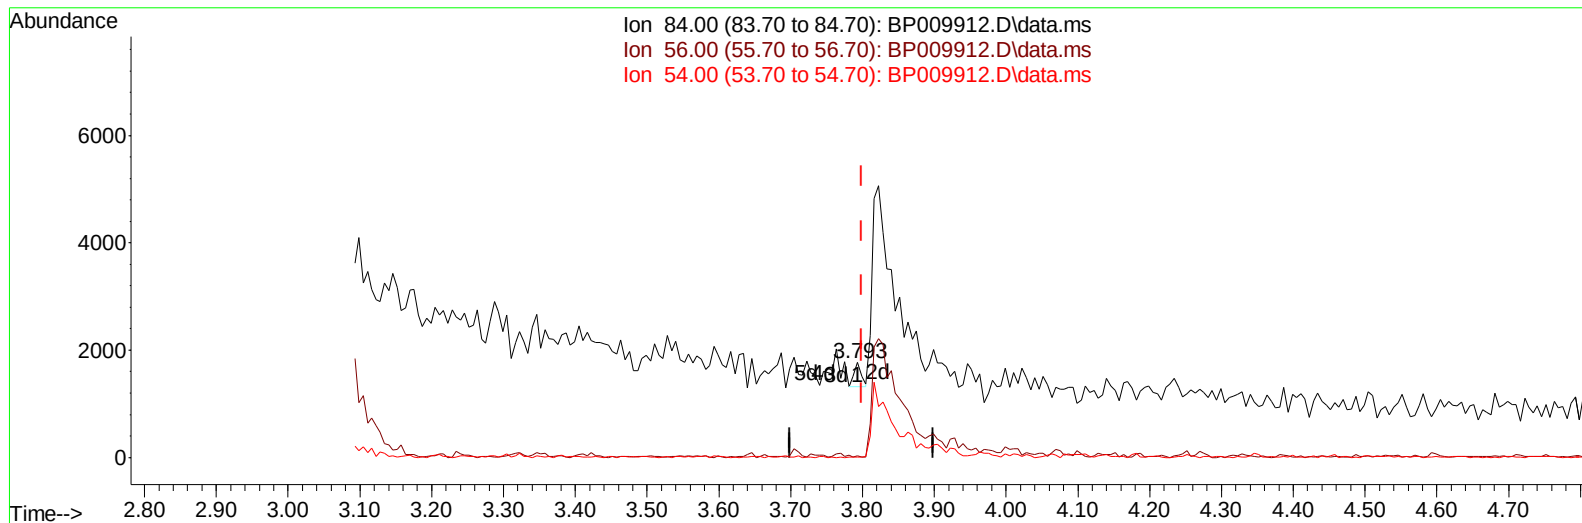

TIC: BP009912.D\data.ms

(4) Pyridine-d5 (S)

3.793min (-0.006) 0.04 ng/uI

response 320

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	1.86#
54.00	24.80	0.11#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009912.D
 Acq On : 18 Apr 2022 13:20
 Operator : CG/JU
 Sample : N2422-07DL 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J54DL

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:54:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/22/2022

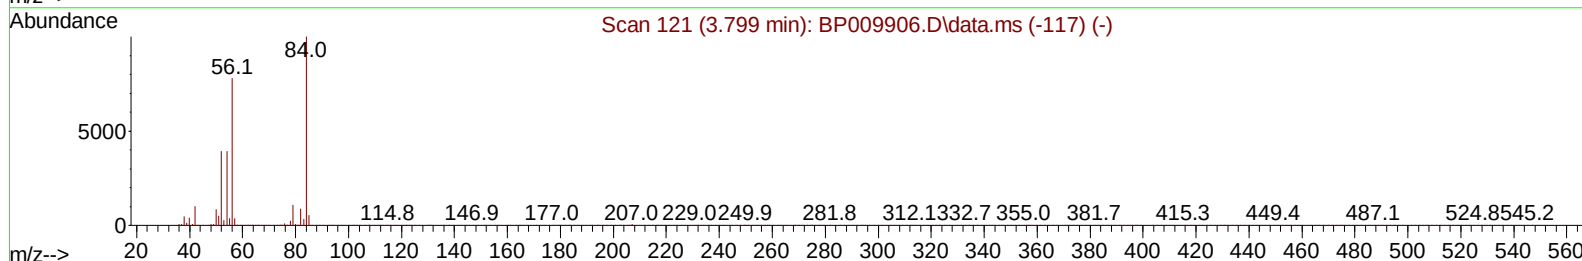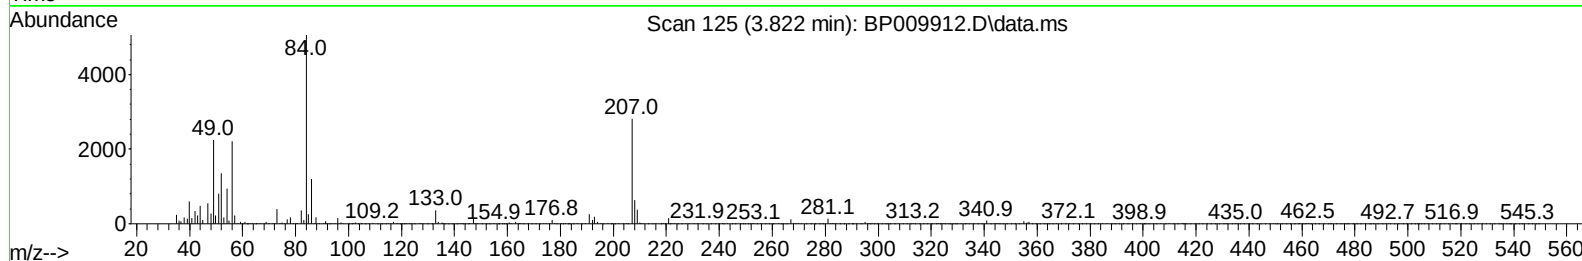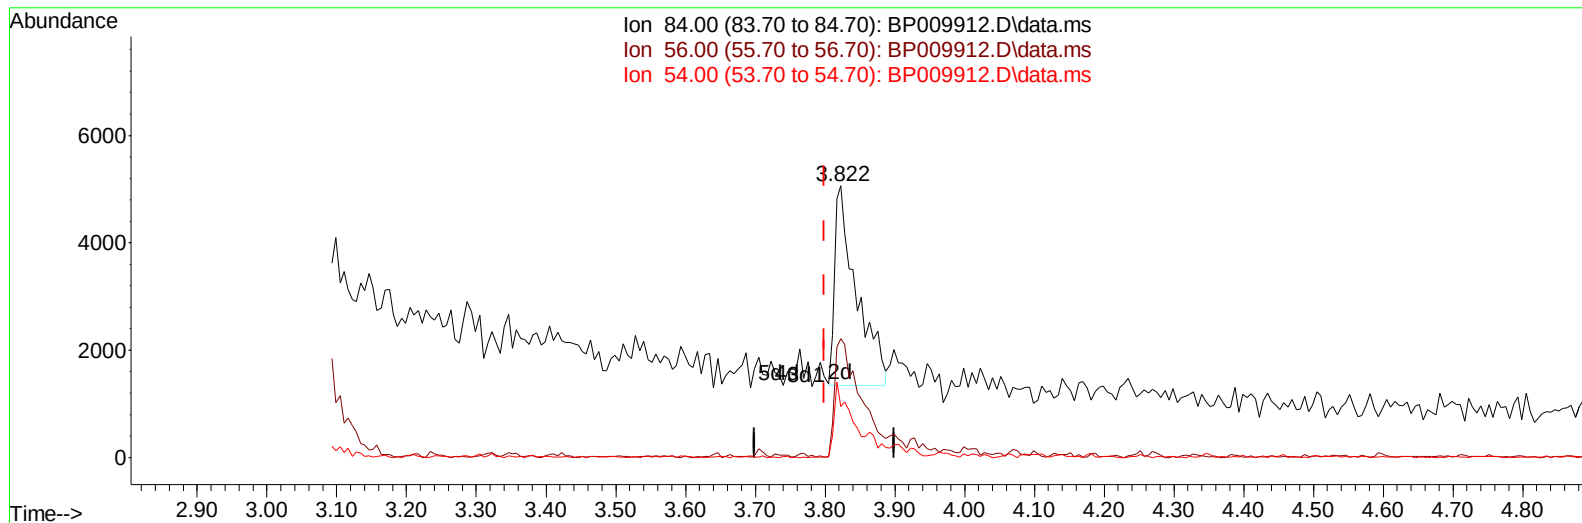

TIC: BP009912.D\data.ms

(4) Pyridine-d5 (S)

3.822min (+ 0.023) 1.14 ng/ul m

response 8121

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	43.83#
54.00	24.80	18.79#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009912.D
 Acq On : 18 Apr 2022 13:20
 Operator : CG/JU
 Sample : N2422-07DL 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J54DL

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:54:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/22/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	115248	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	508019	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.586	164	389742	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.333	188	904464	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.416	240	833747	20.000	ng/ul	# 0.00
88) Perylene-d12	23.874	264	731443	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	840m	0.325	ng/uL	0.01
4) Pyridine-d5	3.822	84	8121m	1.141	ng/ul	0.02
7) Phenol-d5	7.105	99	7193	0.711	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	42377	7.035	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	19310	2.530	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	13672	1.619	ng/ul	-0.01
21) Nitrobenzene-d5	9.110	128	12369	3.376	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	11177	2.783	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	21664	2.578	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	38685	3.232	ng/ul	0.00
46) Dimethylphthalate-d6	13.992	166	101470	3.314	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	101892	2.809	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.575	176	92111	3.577	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	9274	1.731	ng/ul	0.00
73) Anthracene-d10	17.433	188	151875	3.507	ng/ul	0.00
81) Pyrene-d10	19.663	212	183253	4.024	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.710	264	132033	3.466	ng/ul	-0.02
Target Compounds						
					Qvalue	
22) Nitrobenzene	9.152	77	381215	40.540	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009912.D
Acq On : 18 Apr 2022 13:20
Operator : CG/JU
Sample : N2422-07DL 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J54DL

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:54:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/22/2022

