




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009924.D
 Acq On : 18 Apr 2022 20:03
 Operator : CG/JU
 Sample : N2421-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J74

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:58:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/22/2022

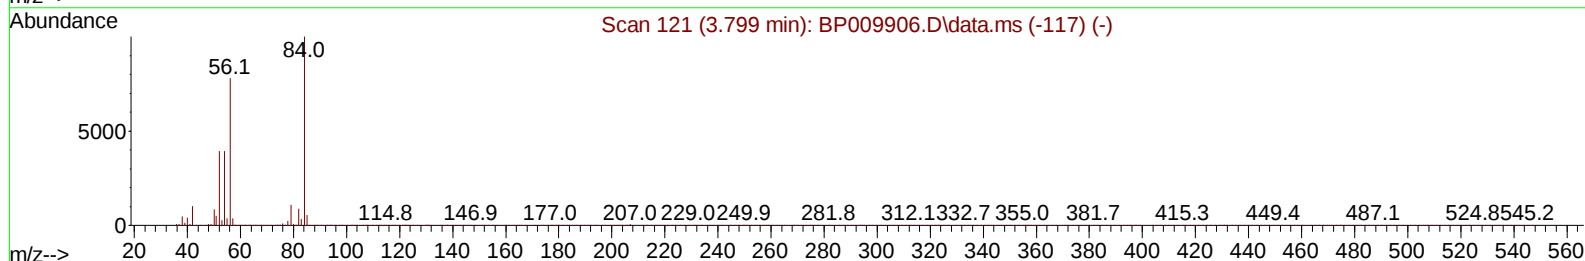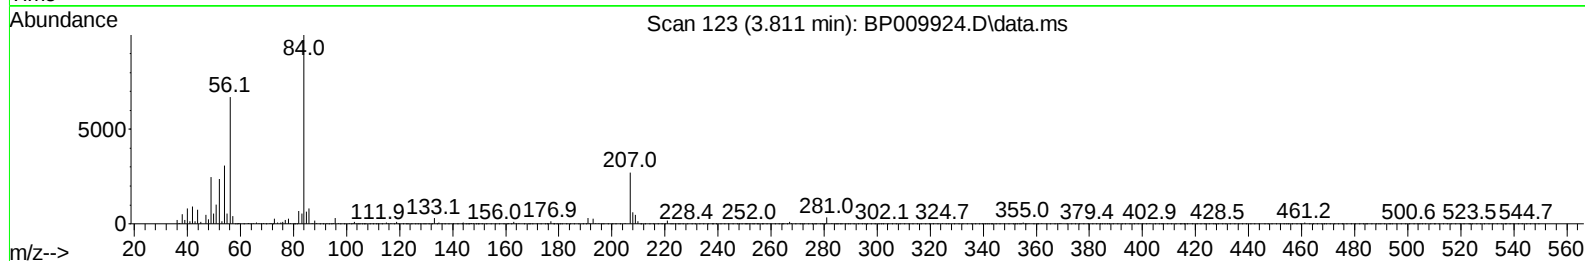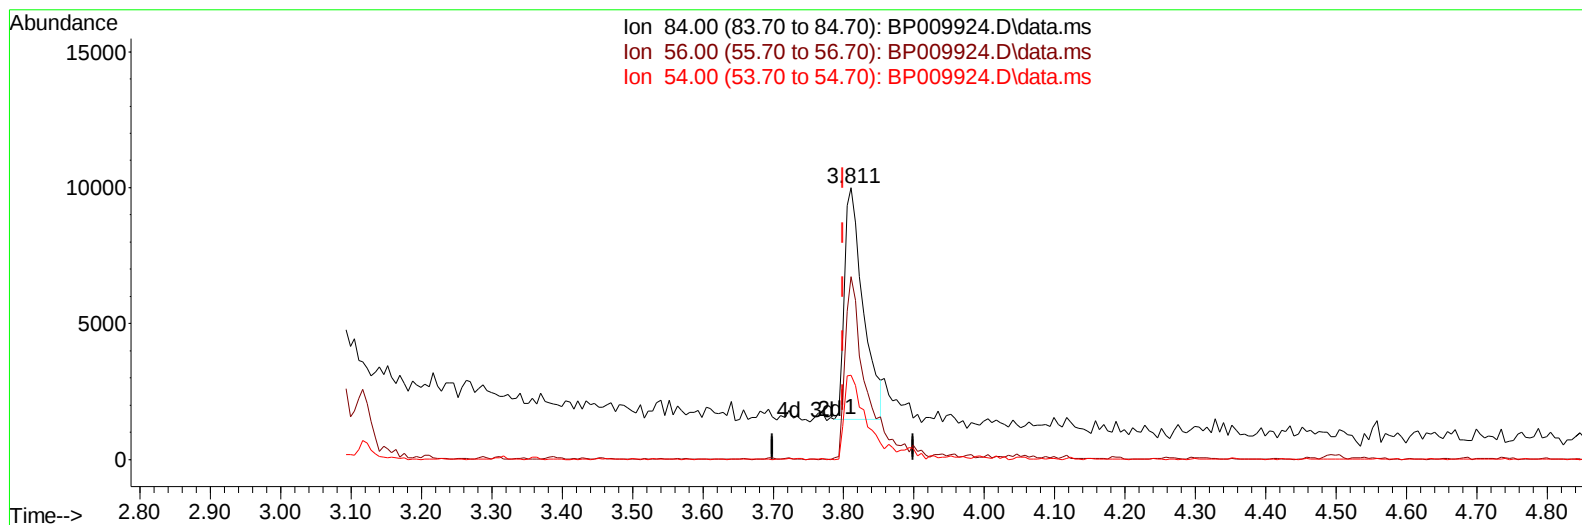

TIC: BP009924.D\data.ms

(4) Pyridine-d5 (S)

3.811min (+ 0.012) 2.41 ng/u1

response 15543

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	67.21#
54.00	24.80	30.93#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009924.D
 Acq On : 18 Apr 2022 20:03
 Operator : CG/JU
 Sample : N2421-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J74

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:58:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/22/2022

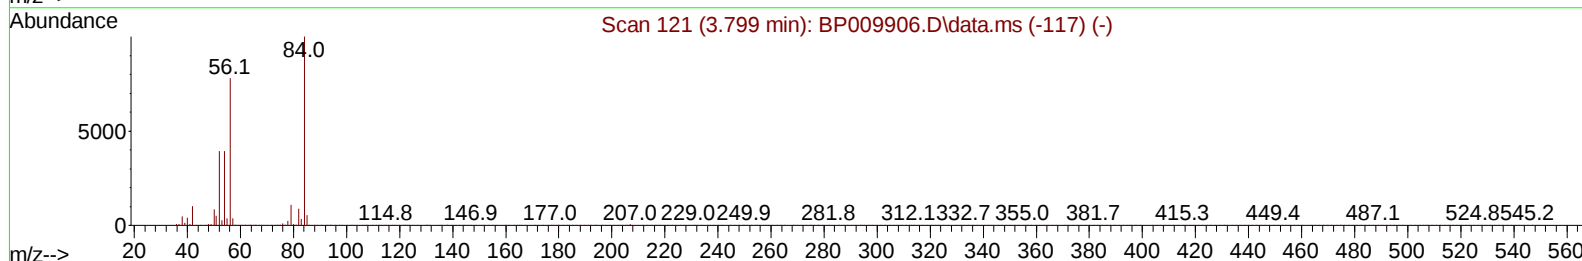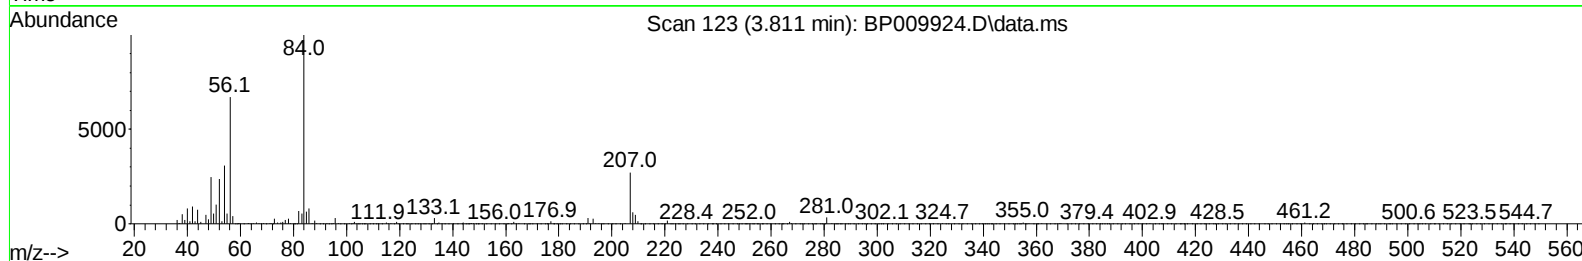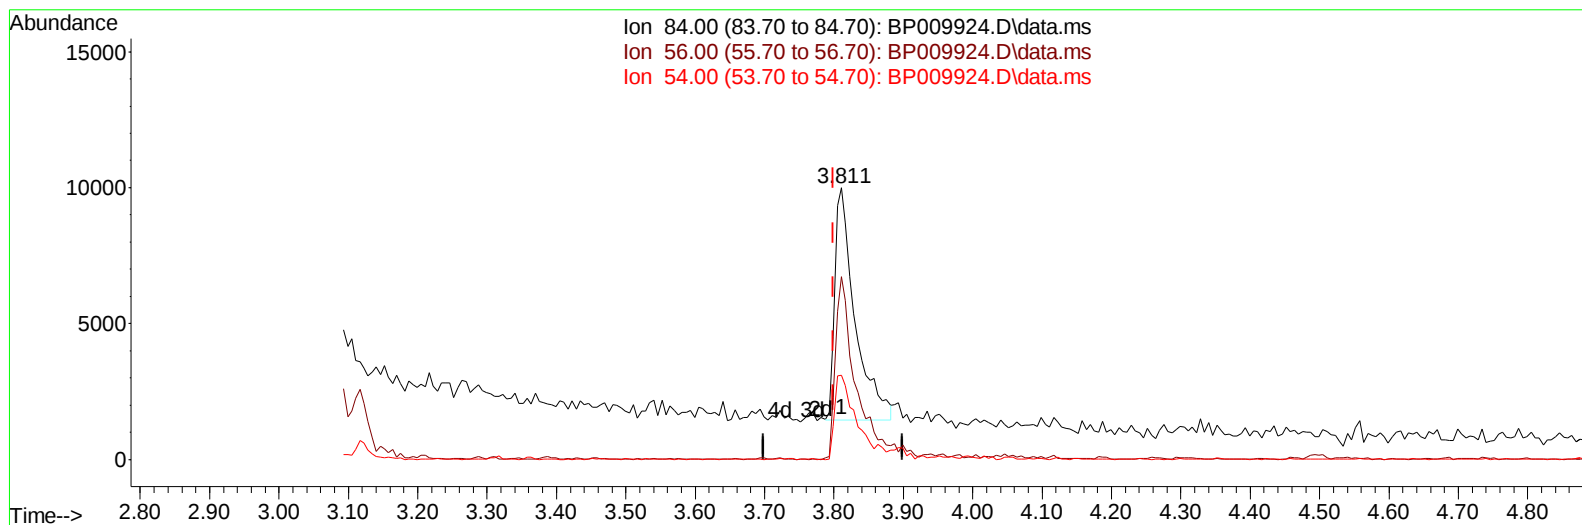

TIC: BP009924.D\data.ms

(4) Pyridine-d5 (S)

3.811min (+ 0.012) 2.67 ng/ul m

response 17266

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	67.21#
54.00	24.80	30.93#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009924.D
 Acq On : 18 Apr 2022 20:03
 Operator : CG/JU
 Sample : N2421-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J74

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/22/2022

Quant Time: Apr 19 00:58:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

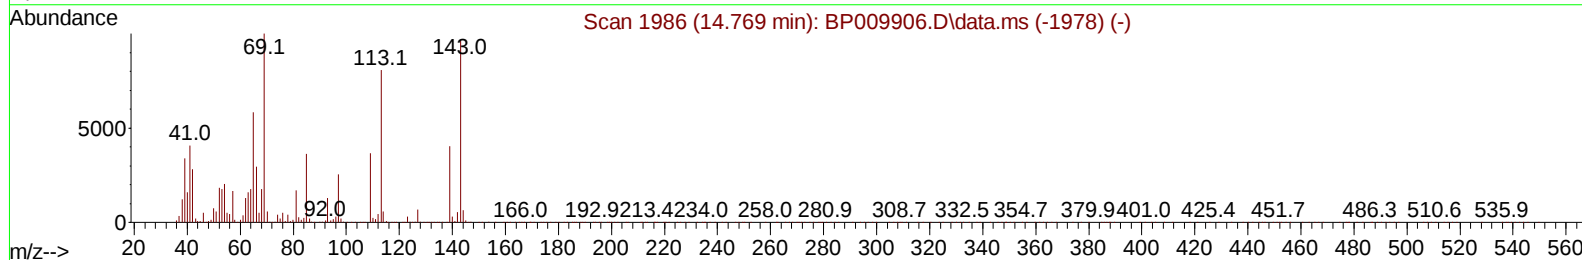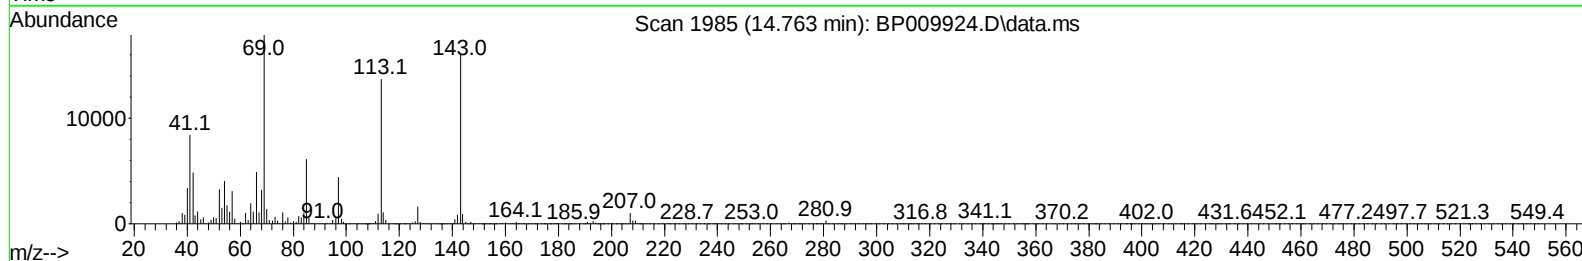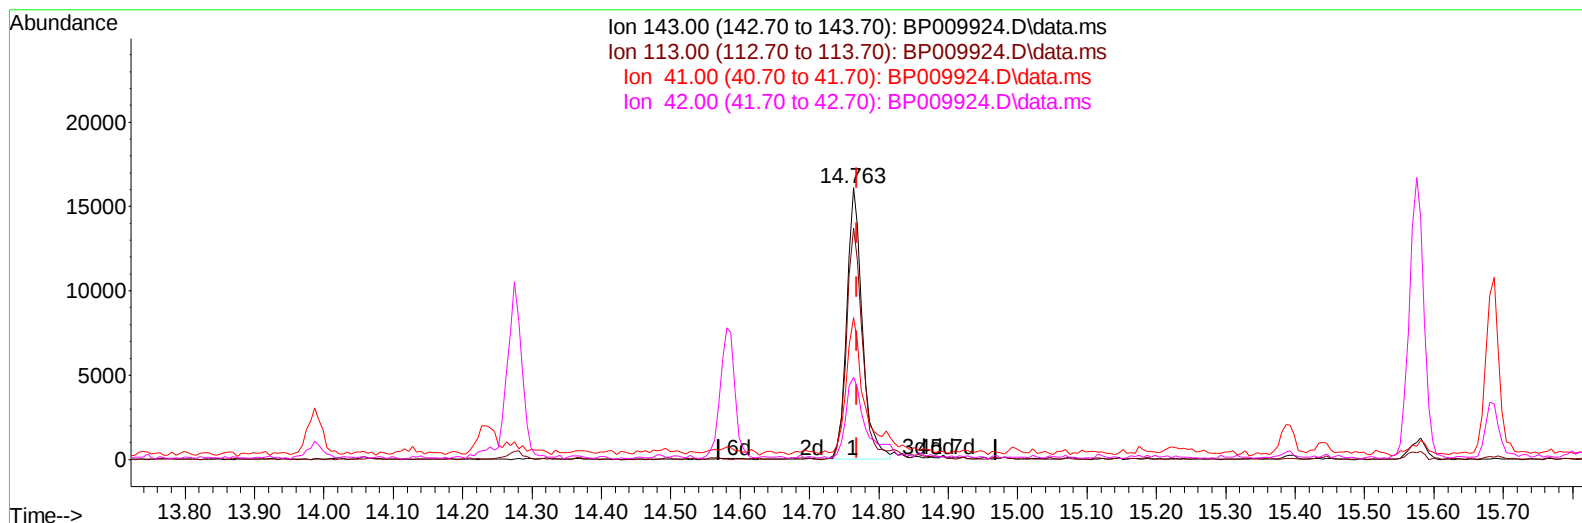

TIC: BP009924.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (-0.006) 5.32 ng/u1

response 25235

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	85.22#
41.00	23.20	52.28#
42.00	18.00	30.26#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009924.D
 Acq On : 18 Apr 2022 20:03
 Operator : CG/JU
 Sample : N2421-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J74

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:58:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/22/2022

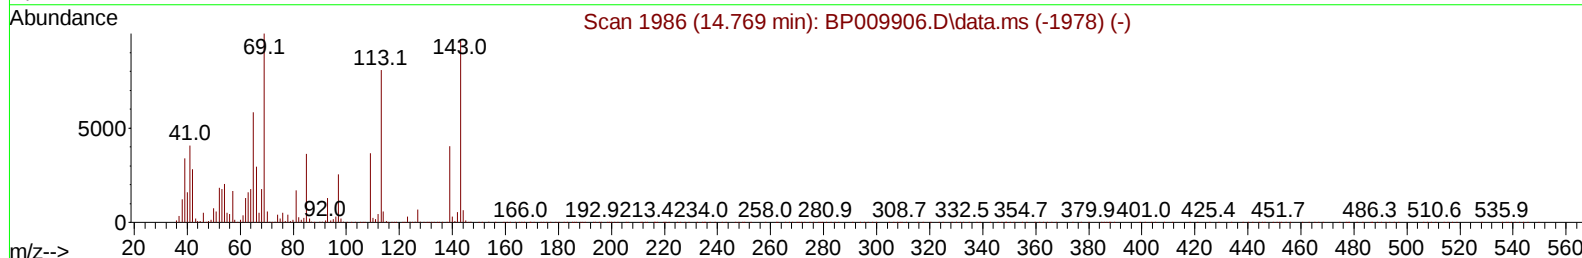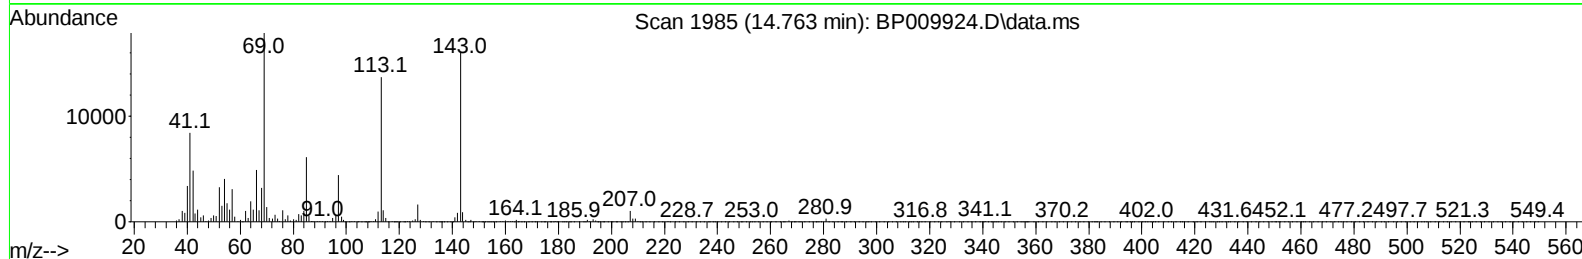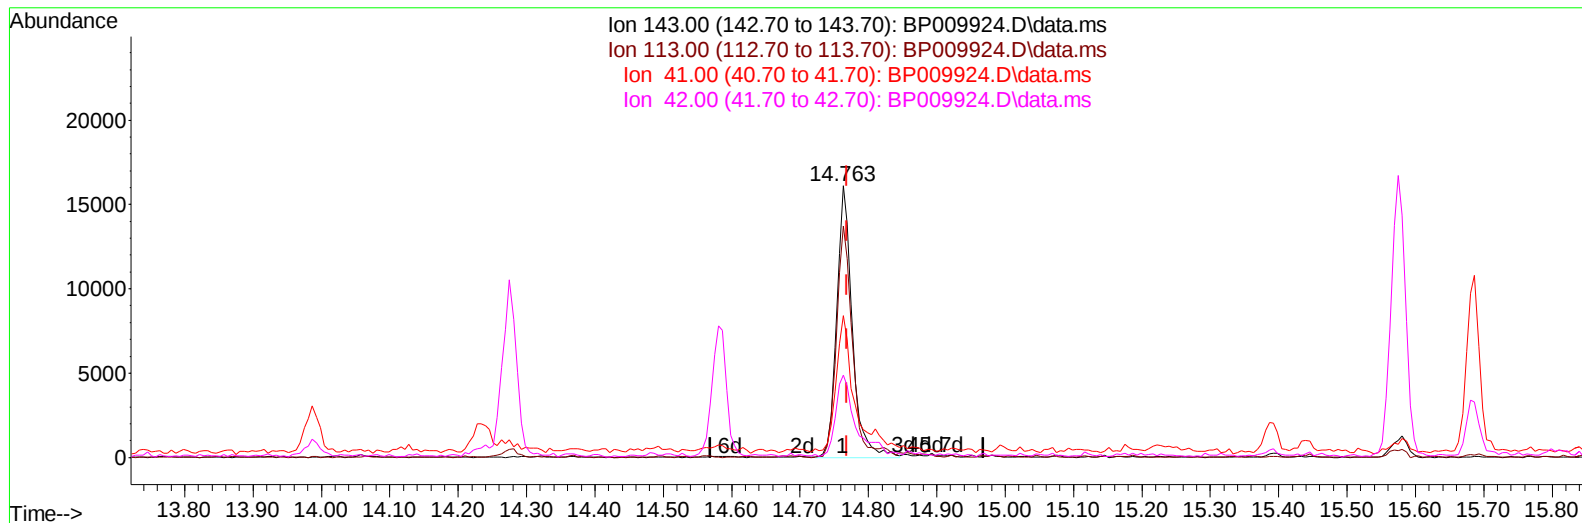

TIC: BP009924.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (-0.006) 5.43 ng/ul m

response 25760

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	85.22#
41.00	23.20	52.28#
42.00	18.00	30.26#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009924.D
 Acq On : 18 Apr 2022 20:03
 Operator : CG/JU
 Sample : N2421-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J74

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/22/2022

Quant Time: Apr 19 00:58:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	104573	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	458928	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.581	164	333233	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.334	188	756585	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.416	240	813252	20.000	ng/ul	0.00
88) Perylene-d12	23.874	264	765852	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	13097	5.590	ng/uL	0.00
4) Pyridine-d5	3.811	84	17266m	2.673	ng/ul	0.01
7) Phenol-d5	7.105	99	55394	6.034	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	190478	34.850	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	171919	24.825	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	119789	15.630	ng/ul	-0.01
21) Nitrobenzene-d5	9.110	128	125132	37.810	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	129196	35.608	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.375	165	222860	29.353	ng/ul	0.00
31) 4-Chloroaniline-d4	10.887	131	201944	18.674	ng/ul	0.00
46) Dimethylphthalate-d6	13.993	166	1009731	38.575	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	1074545	34.650	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.763	143	25760m	5.426	ng/ul	0.00
60) Fluorene-d10	15.575	176	875322	39.751	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	150612	33.604	ng/ul	0.00
73) Anthracene-d10	17.434	188	1523843	42.066	ng/ul	0.00
81) Pyrene-d10	19.663	212	1875977	42.237	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.721	264	1755538	44.017	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009924.D
Acq On : 18 Apr 2022 20:03
Operator : CG/JU
Sample : N2421-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J74

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/22/2022

Quant Time: Apr 19 00:58:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

