




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009925.D
 Acq On : 18 Apr 2022 20:37
 Operator : CG/JU
 Sample : N2421-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HX1

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:58:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/22/2022

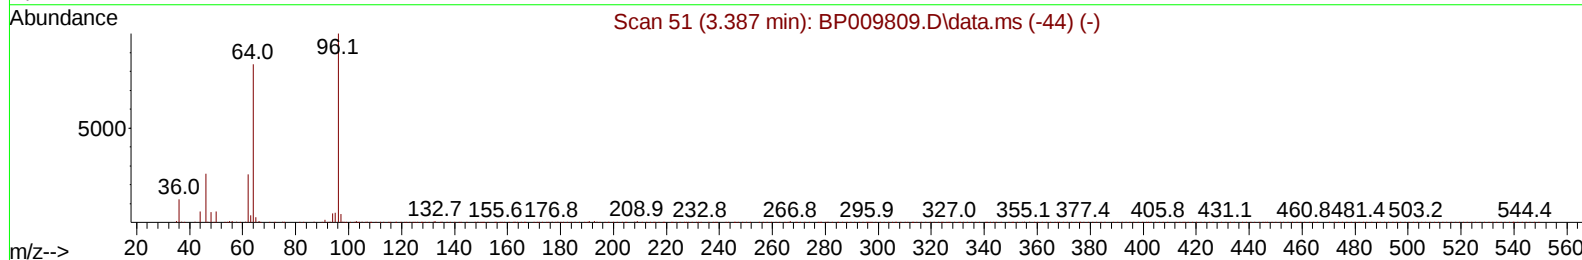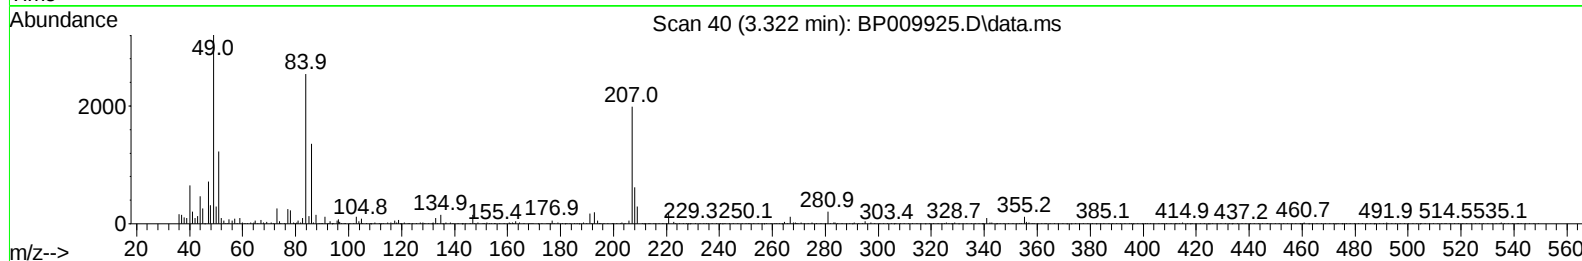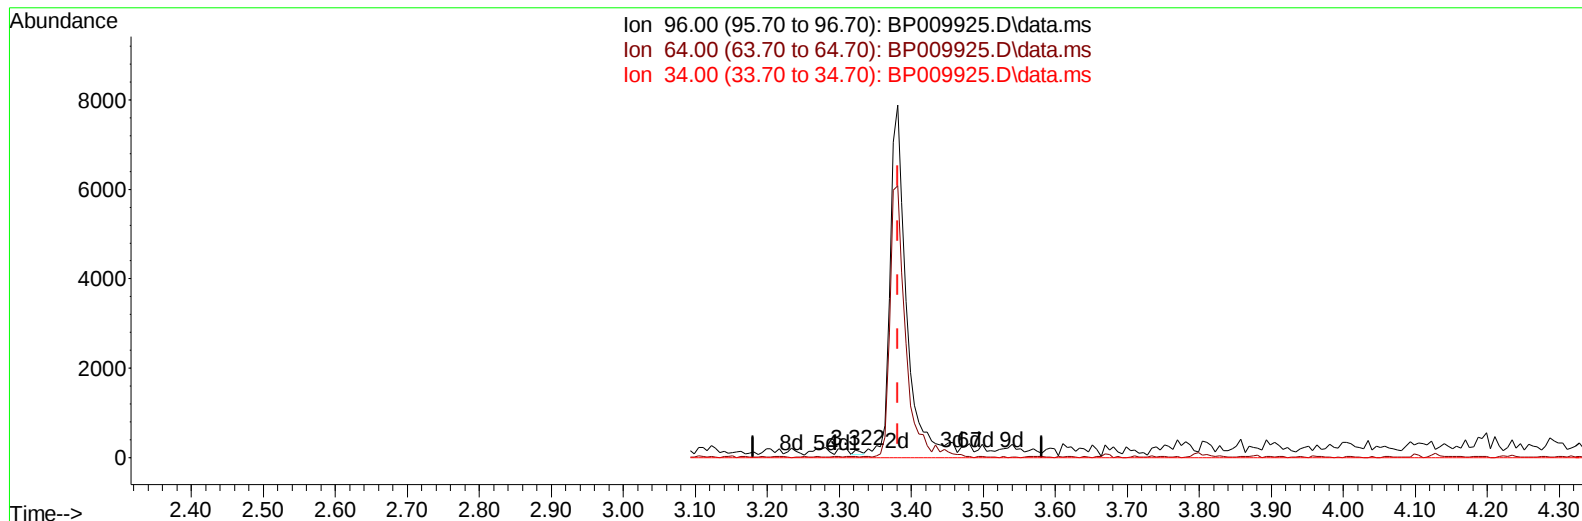

TIC: BP009925.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.322min (-0.059) 0.03 ng/uL

response 76

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	48.50
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009925.D
 Acq On : 18 Apr 2022 20:37
 Operator : CG/JU
 Sample : N2421-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HX1

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:58:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/22/2022

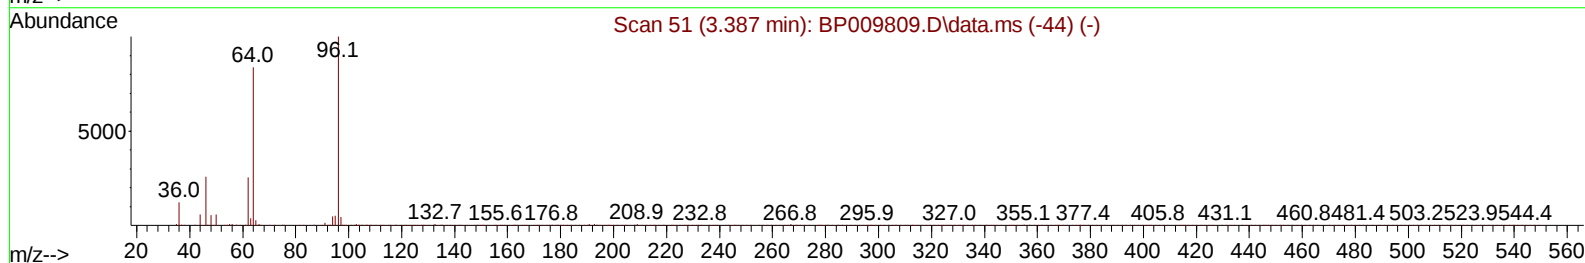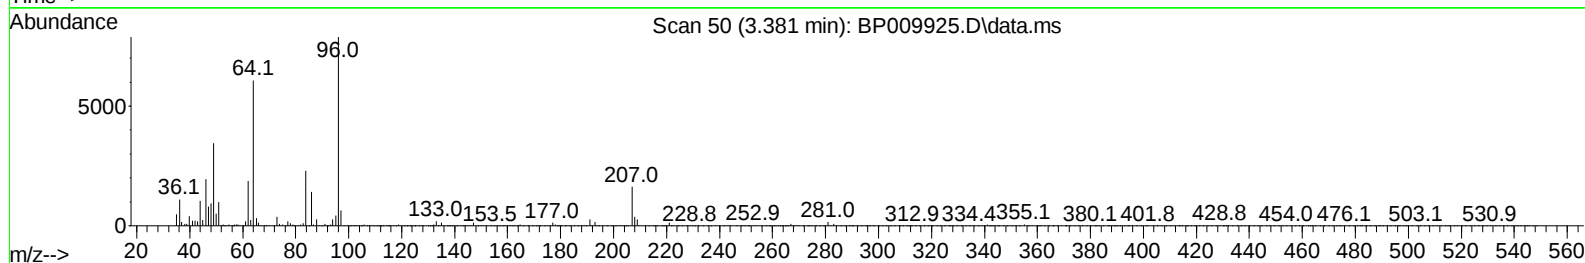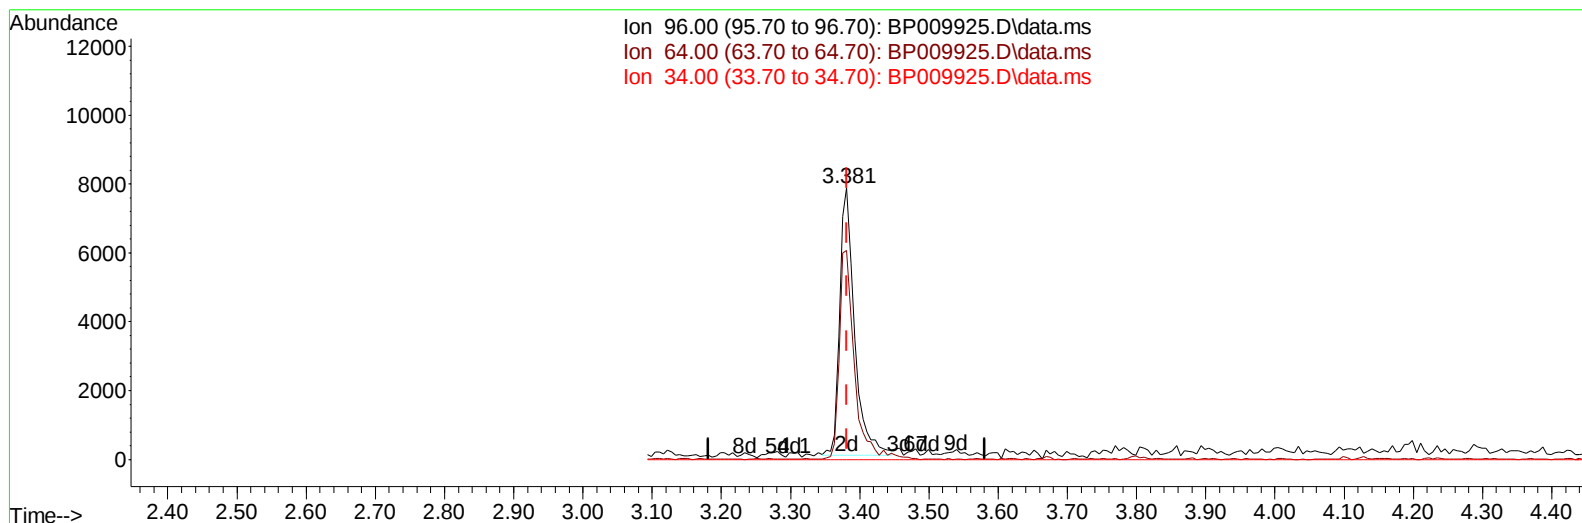

TIC: BP009925.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.381min (-0.000) 4.54 ng/uL m

response 11628

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	77.07#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009925.D
 Acq On : 18 Apr 2022 20:37
 Operator : CG/JU
 Sample : N2421-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HX1

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:58:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/22/2022

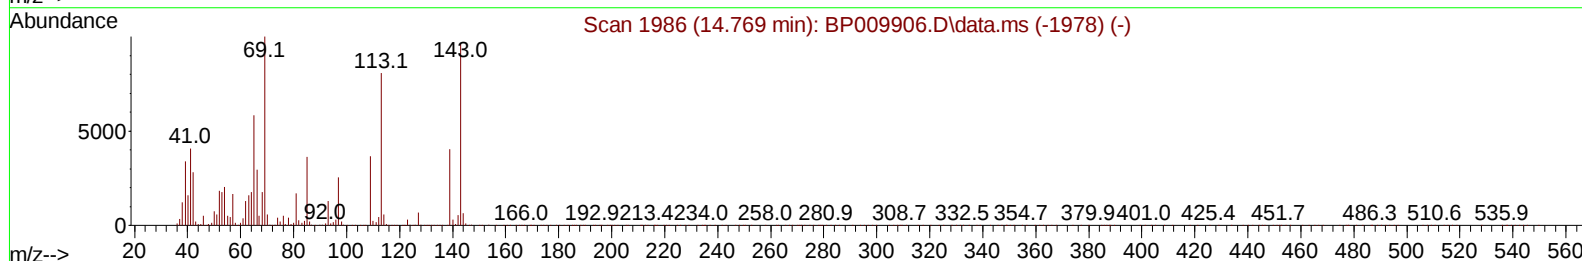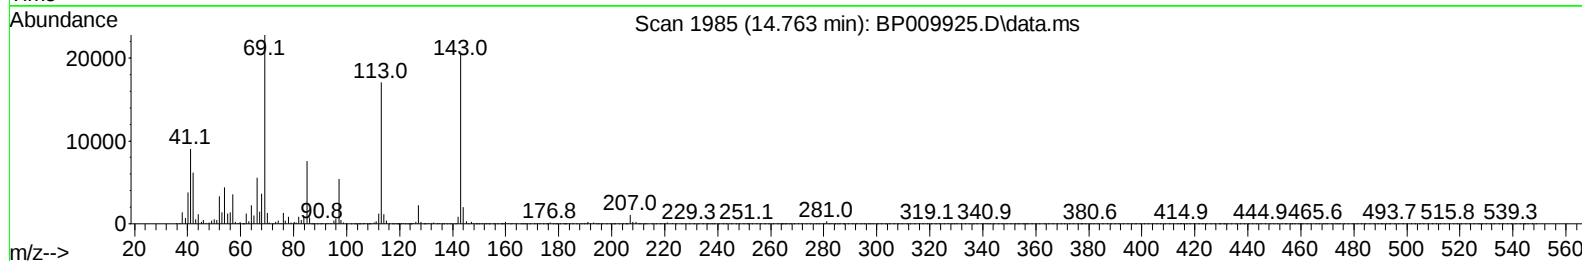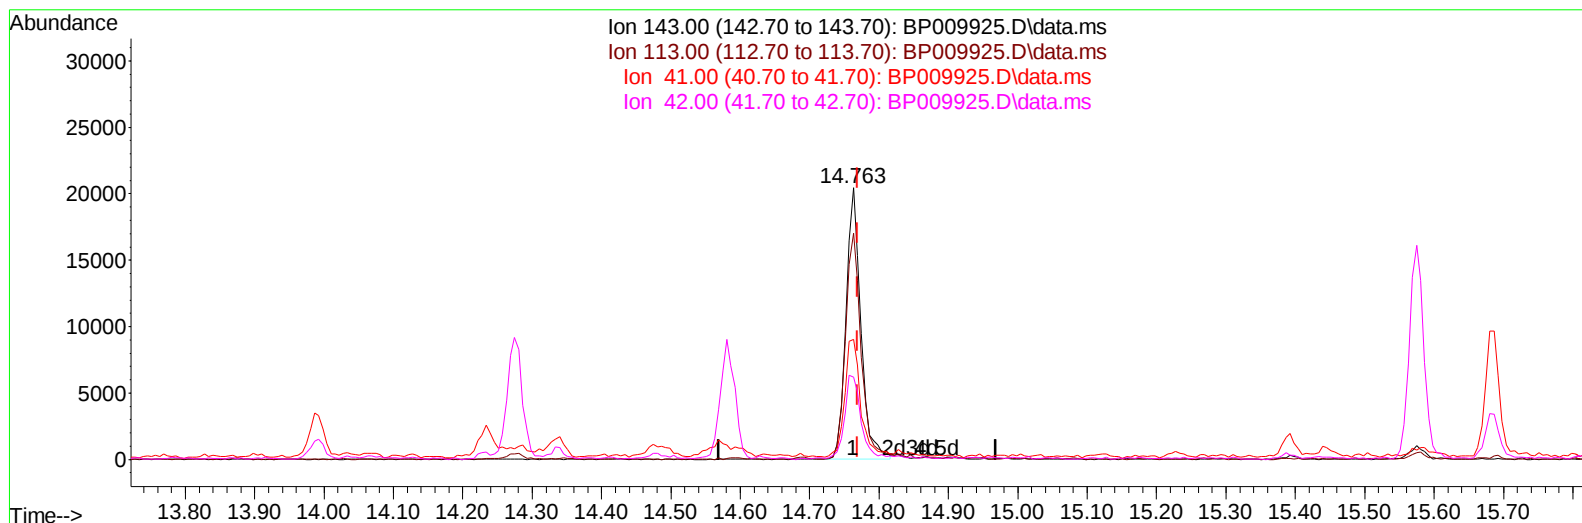

TIC: BP009925.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (-0.006) 6.06 ng/u1

response 30487

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	83.41#
41.00	23.20	44.27#
42.00	18.00	30.36#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009925.D
 Acq On : 18 Apr 2022 20:37
 Operator : CG/JU
 Sample : N2421-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HX1

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:58:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/22/2022

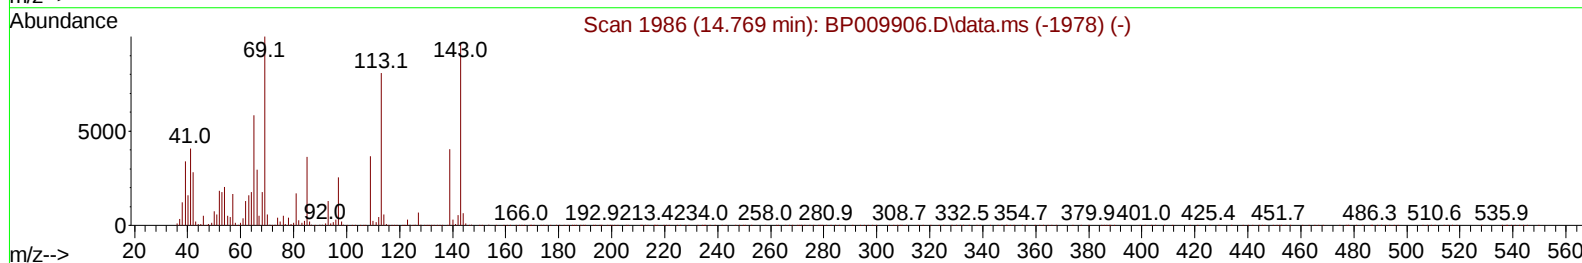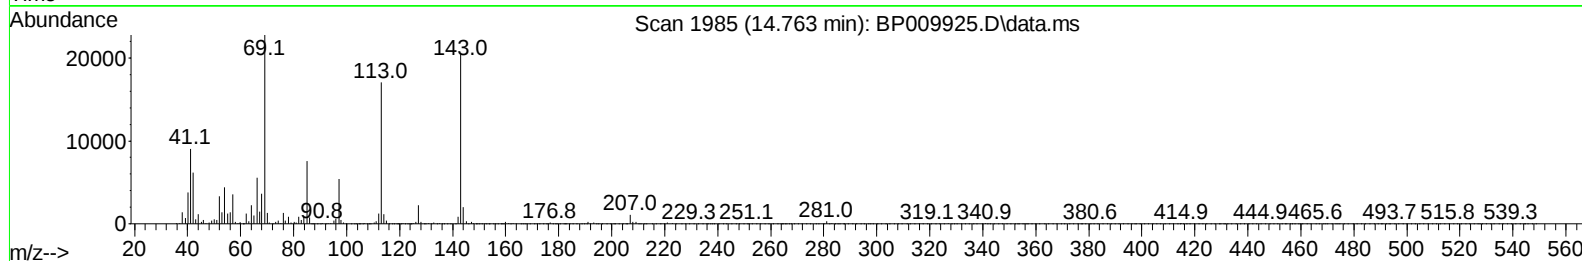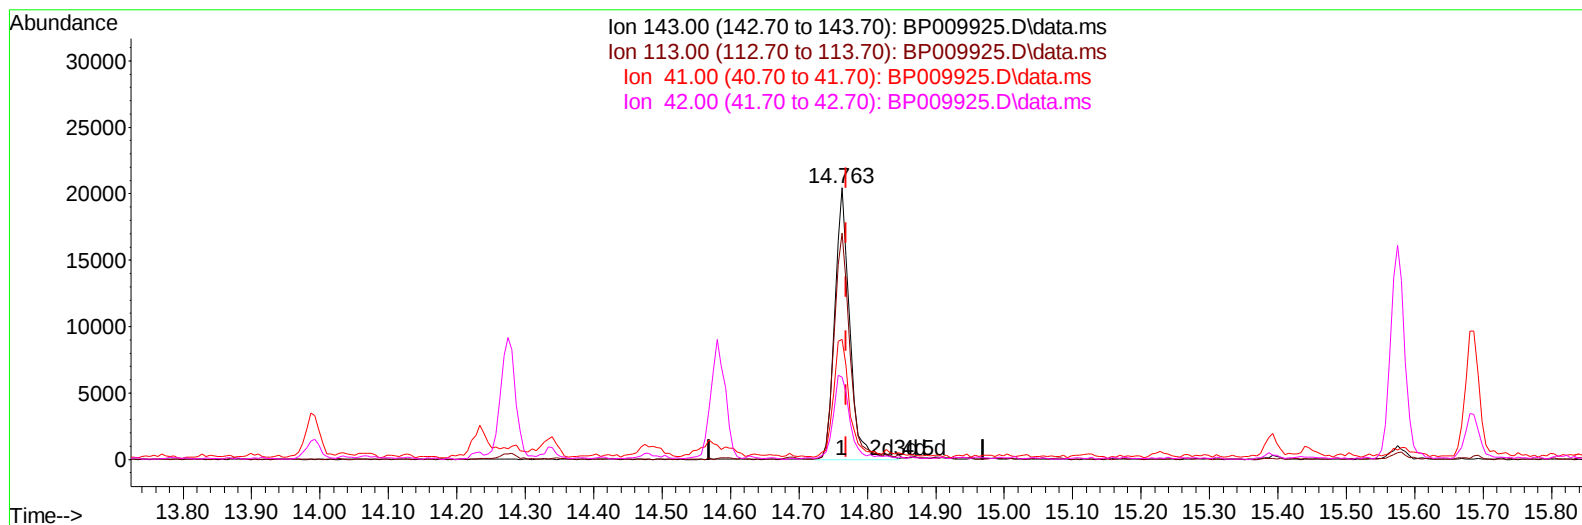

TIC: BP009925.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (-0.006) 6.16 ng/ul m

response 31031

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	83.41#
41.00	23.20	44.27#
42.00	18.00	30.36#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009925.D
 Acq On : 18 Apr 2022 20:37
 Operator : CG/JU
 Sample : N2421-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HX1

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:58:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/22/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	114347	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	499932	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.586	164	353438	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.333	188	802320	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.415	240	845712	20.000	ng/ul	# 0.00
88) Perylene-d12	23.874	264	771762	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	11628m	4.538	ng/uL	0.00
4) Pyridine-d5	3.799	84	63007	8.919	ng/ul	0.00
7) Phenol-d5	7.104	99	66170	6.591	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	185882	31.102	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	179862	23.752	ng/ul	0.00
15) 4-Methylphenol-d8	8.651	113	135708	16.194	ng/ul	-0.01
21) Nitrobenzene-d5	9.110	128	121559	33.718	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	126616	32.034	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.375	165	217643	26.314	ng/ul	0.00
31) 4-Chloroaniline-d4	10.887	131	143403	12.173	ng/ul	0.00
46) Dimethylphthalate-d6	13.986	166	947898	34.142	ng/ul	-0.01
49) Acenaphthylene-d8	14.275	160	1002848	30.490	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.763	143	31031m	6.163	ng/ul	0.00
60) Fluorene-d10	15.575	176	829695	35.525	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	152194	32.021	ng/ul	0.00
73) Anthracene-d10	17.433	188	1482887	38.602	ng/ul	0.00
81) Pyrene-d10	19.663	212	1835555	39.740	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.715	264	1630726	40.575	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009925.D
Acq On : 18 Apr 2022 20:37
Operator : CG/JU
Sample : N2421-09
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HX1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/22/2022

Quant Time: Apr 19 00:58:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

