




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009932.D
Acq On : 19 Apr 2022 00:33
Operator : CG/JU
Sample : N2421-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HY5

Manual IntegrationsAPPROVED

Quant Time: Apr 19 02:33:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
Supervised By :Yogesh Patel 04/22/2022

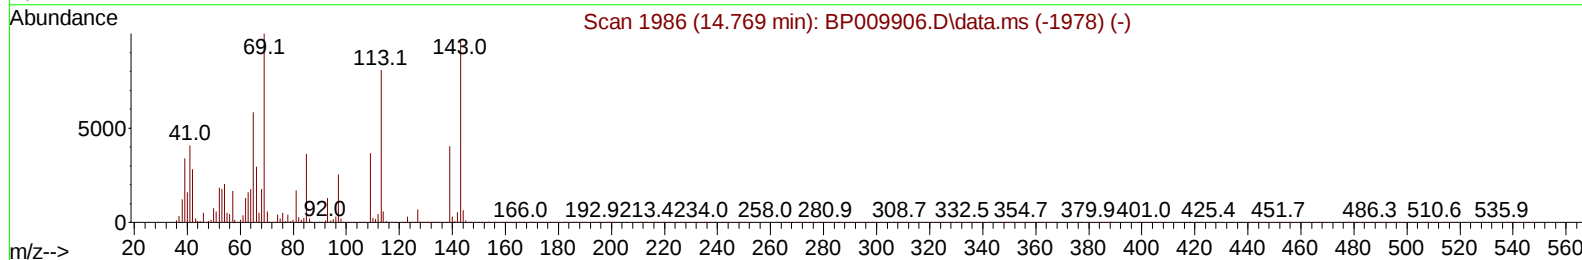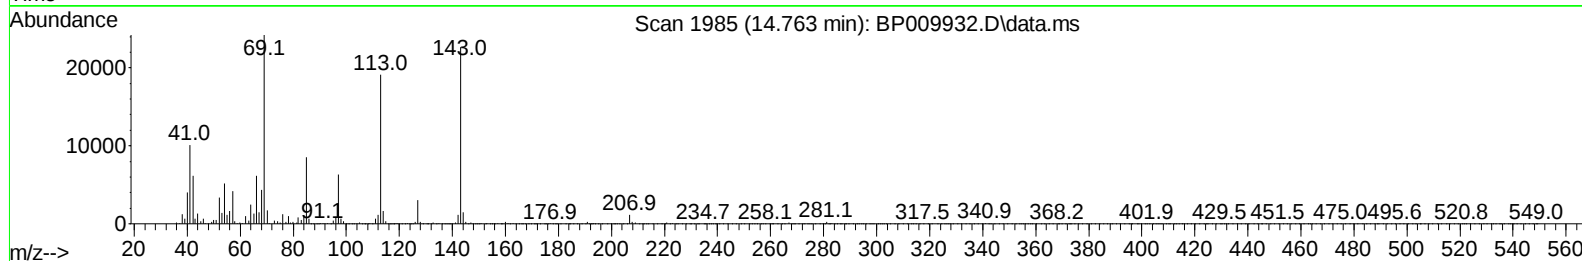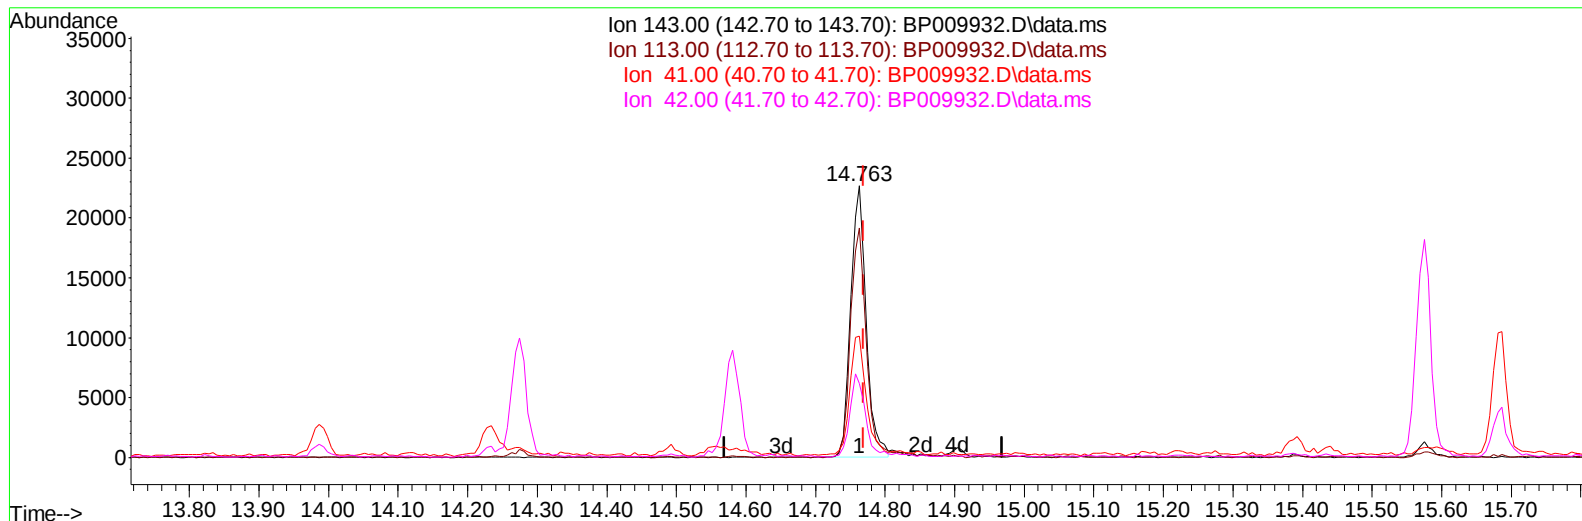

TIC: BP009932.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (-0.006) 6.68 ng/u1

response 34932

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	84.51#
41.00	23.20	44.59#
42.00	18.00	27.22#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009932.D
 Acq On : 19 Apr 2022 00:33
 Operator : CG/JU
 Sample : N2421-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HY5

Manual IntegrationsAPPROVED

Quant Time: Apr 19 02:33:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
 Supervised By :Yogesh Patel 04/22/2022

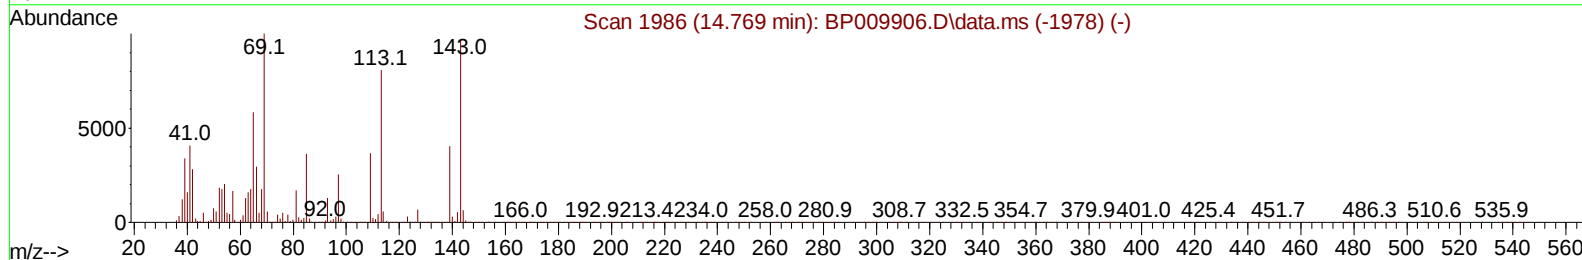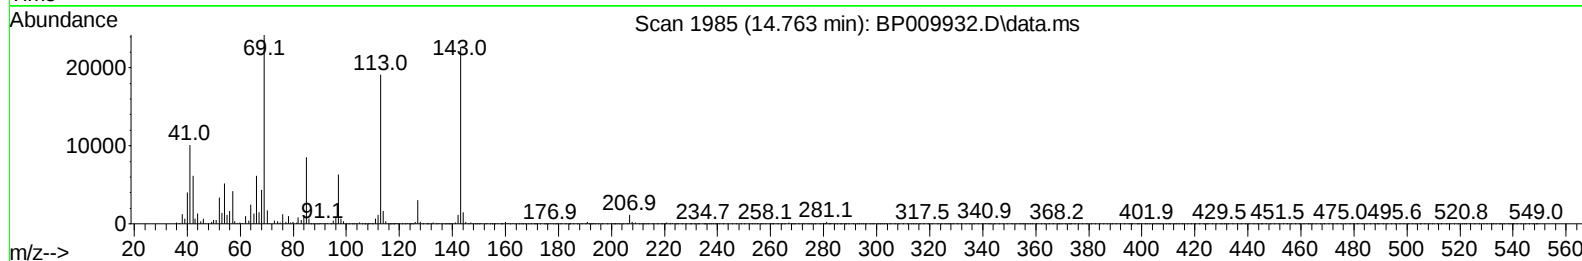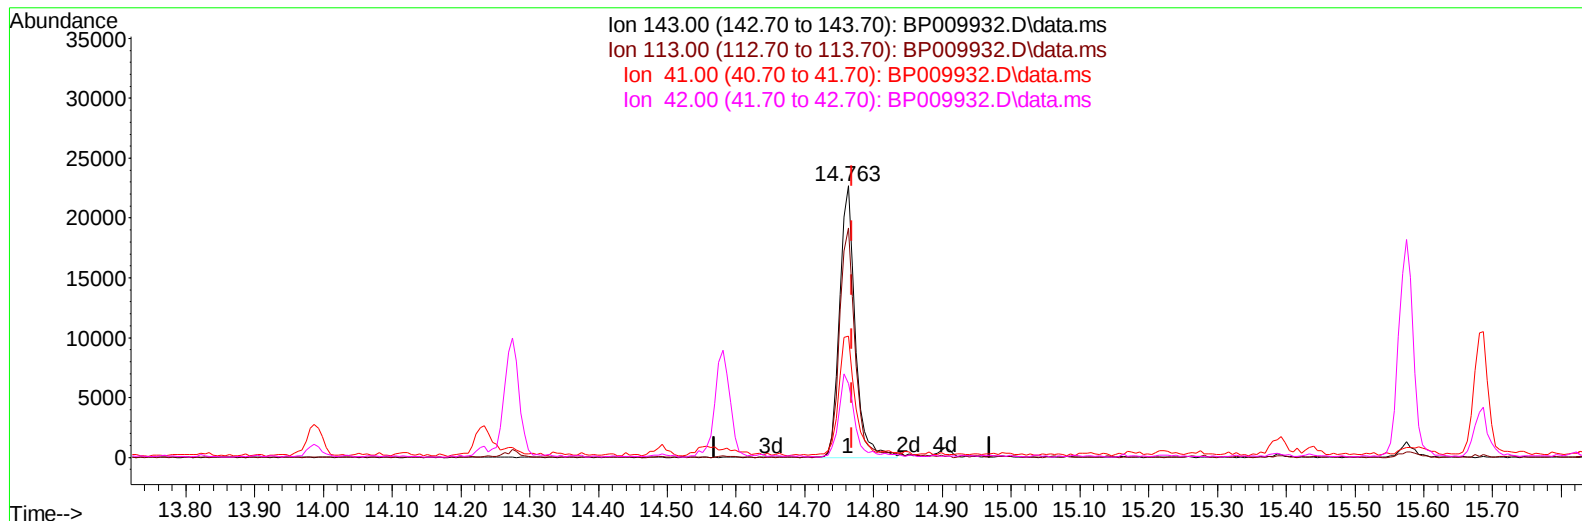

TIC: BP009932.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (-0.006) 6.83 ng/ul m

response 35707

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	84.51#
41.00	23.20	44.59#
42.00	18.00	27.22#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009932.D
 Acq On : 19 Apr 2022 00:33
 Operator : CG/JU
 Sample : N2421-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HY5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/20/2022
 Supervised By :Yogesh Patel 04/22/2022

Quant Time: Apr 19 02:33:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	119412	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	521671	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.581	164	366910	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.334	188	835337	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.416	240	868066	20.000	ng/ul	# 0.00
88) Perylene-d12	23.874	264	796351	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	13189	4.929	ng/uL	0.00
4) Pyridine-d5	3.799	84	85031	11.526	ng/ul	0.00
7) Phenol-d5	7.105	99	75127	7.166	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	209849	33.623	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	201608	25.494	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	143943	16.448	ng/ul	-0.01
21) Nitrobenzene-d5	9.110	128	136687	36.334	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	143379	34.764	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.369	165	248374	28.779	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.887	131	265401	21.591	ng/ul	0.00
46) Dimethylphthalate-d6	13.987	166	1051754	36.492	ng/ul	-0.01
49) Acenaphthylene-d8	14.275	160	1130404	33.106	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.763	143	35707m	6.831	ng/ul	0.00
60) Fluorene-d10	15.575	176	915694	37.768	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	166128	33.571	ng/ul	0.00
73) Anthracene-d10	17.434	188	1569418	39.240	ng/ul	0.00
81) Pyrene-d10	19.663	212	1926487	40.635	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.721	264	1696636	40.911	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.134	94	13660	1.302	ng/ul#	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009932.D
Acq On : 19 Apr 2022 00:33
Operator : CG/JU
Sample : N2421-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HY5

Manual IntegrationsAPPROVED

Quant Time: Apr 19 02:33:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
Supervised By :Yogesh Patel 04/22/2022

