




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009942.D
 Acq On : 19 Apr 2022 06:44
 Operator : CG/JU
 Sample : N2421-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COHX0

Manual IntegrationsAPPROVED

Quant Time: Apr 19 07:42:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
 Supervised By :Yogesh Patel 04/22/2022

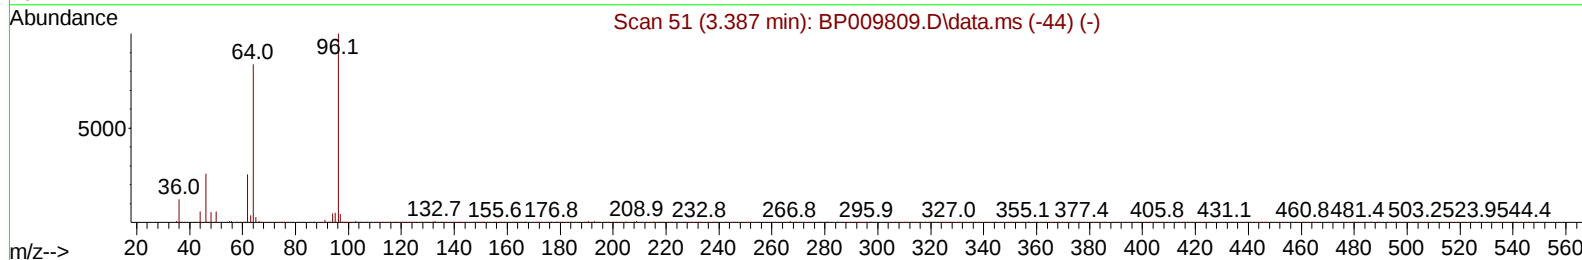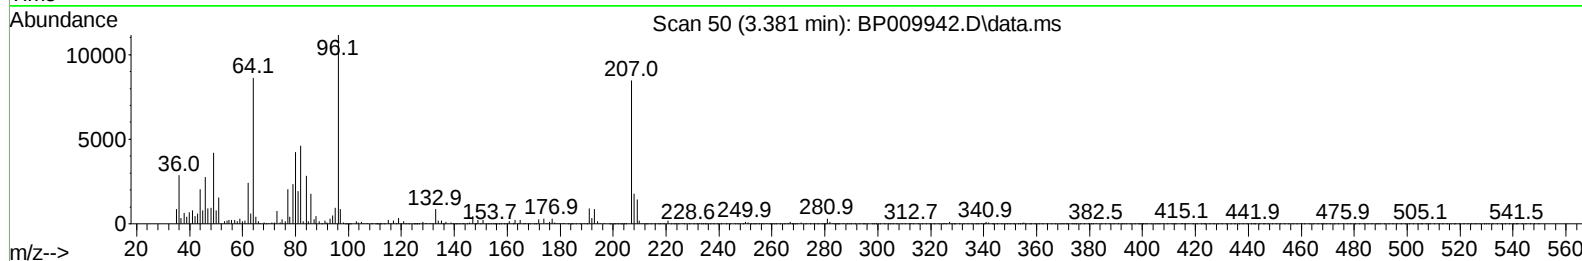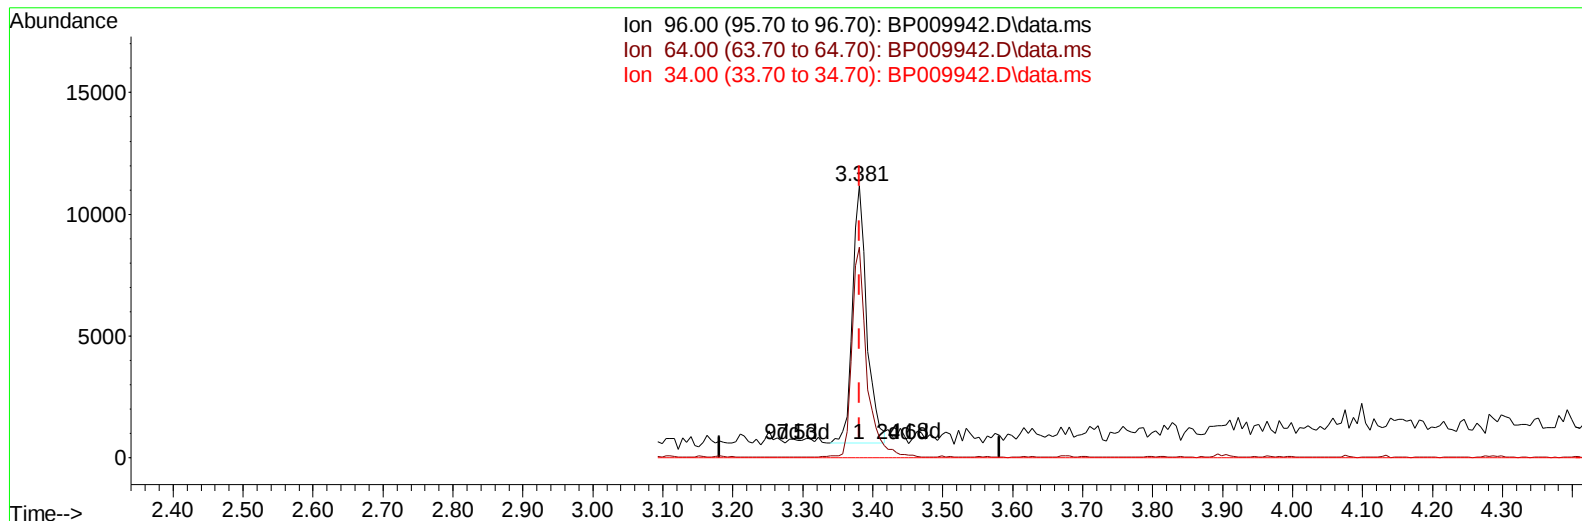

TIC: BP009942.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.381min (-0.000) 5.13 ng/uL

response 14858

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	77.45#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009942.D
Acq On : 19 Apr 2022 06:44
Operator : CG/JU
Sample : N2421-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COHX0

Manual IntegrationsAPPROVED

Quant Time: Apr 19 07:42:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
Supervised By :Yogesh Patel 04/22/2022

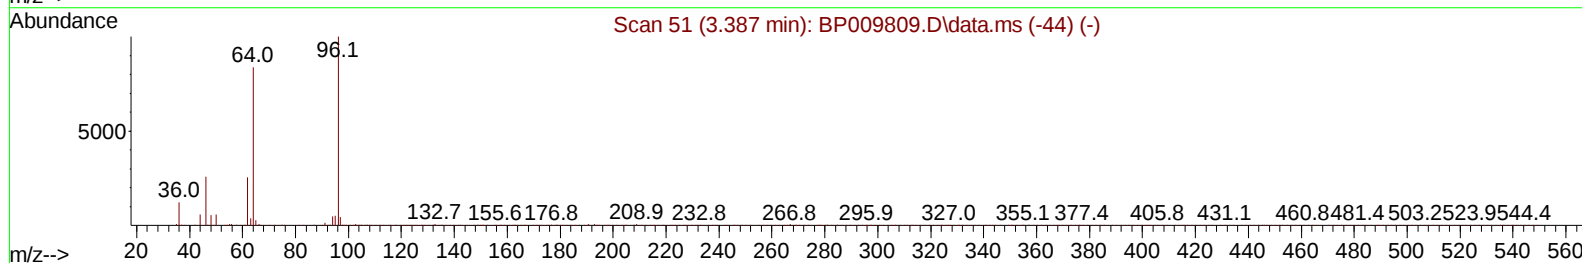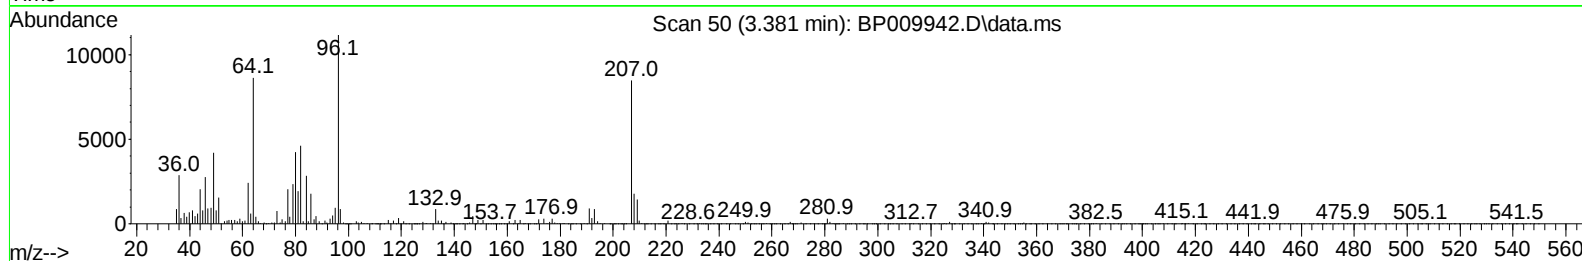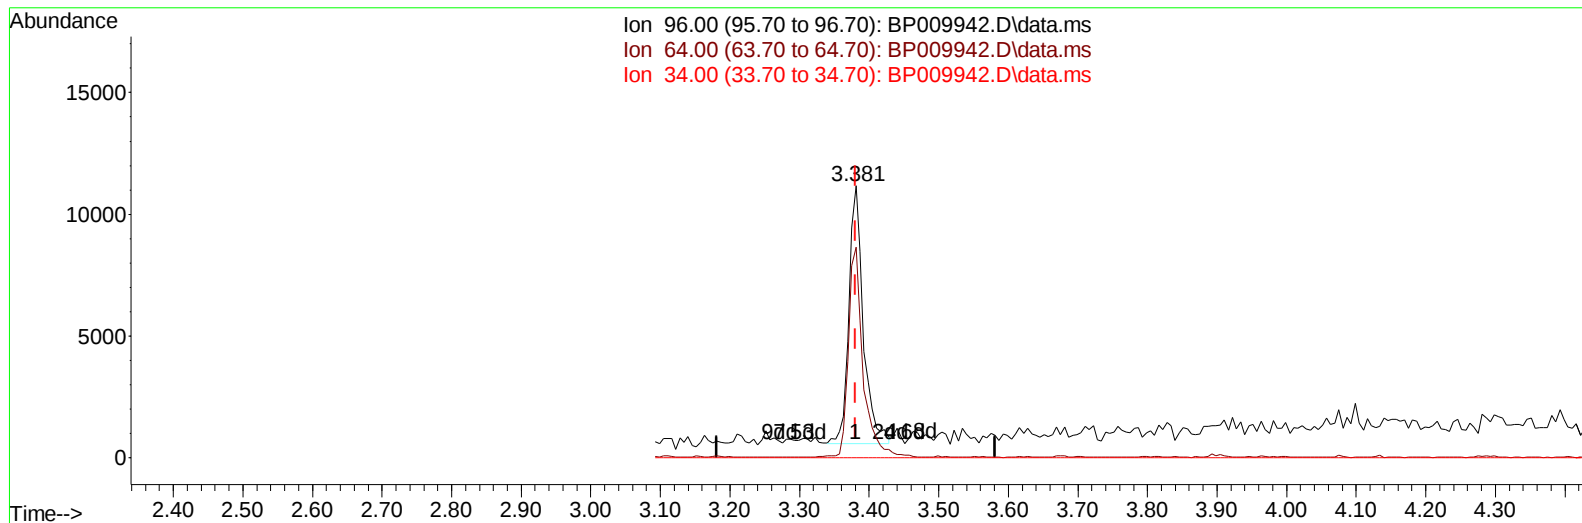

TIC: BP009942.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.381min (-0.000) 5.26 ng/uL m

response 15216

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	77.45#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009942.D
 Acq On : 19 Apr 2022 06:44
 Operator : CG/JU
 Sample : N2421-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COHX0

Manual IntegrationsAPPROVED

Quant Time: Apr 19 07:42:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
 Supervised By :Yogesh Patel 04/22/2022

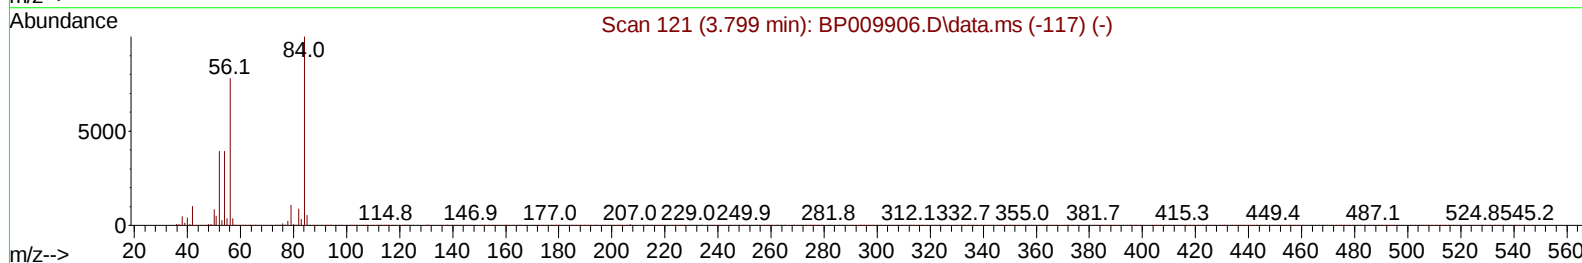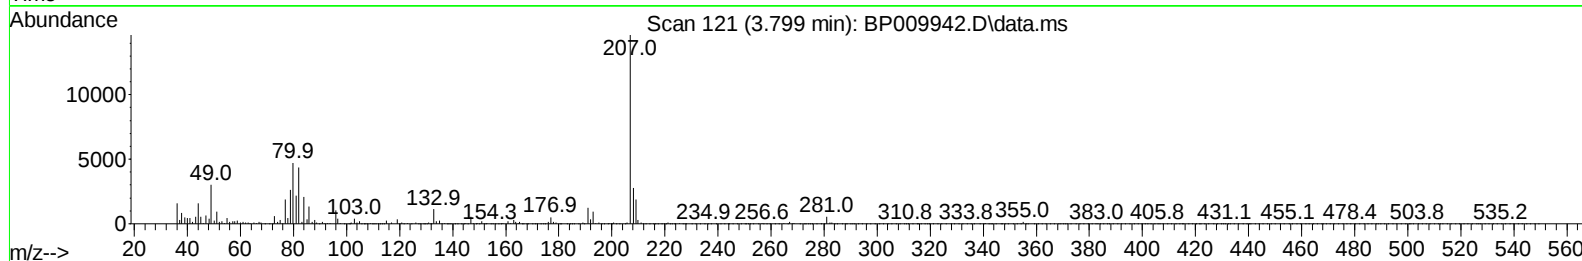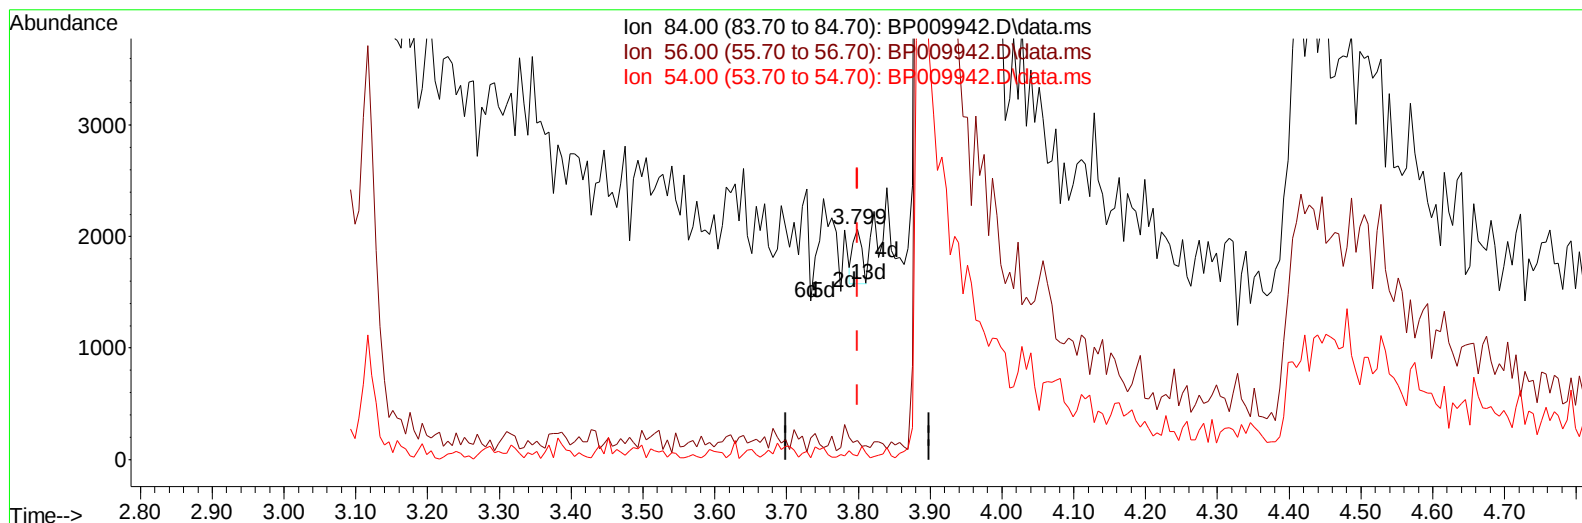

TIC: BP009942.D\data.ms

(4) Pyridine-d5 (S)

3.799min (-0.000) 0.05 ng/u1

response 413

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	8.28#
54.00	24.80	1.65#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009942.D
 Acq On : 19 Apr 2022 06:44
 Operator : CG/JU
 Sample : N2421-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COHX0

Manual IntegrationsAPPROVED

Quant Time: Apr 19 07:42:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
 Supervised By :Yogesh Patel 04/22/2022

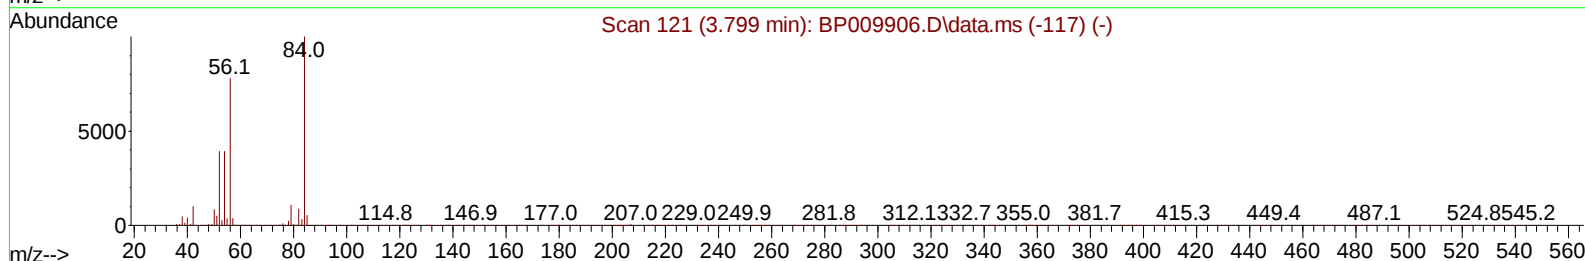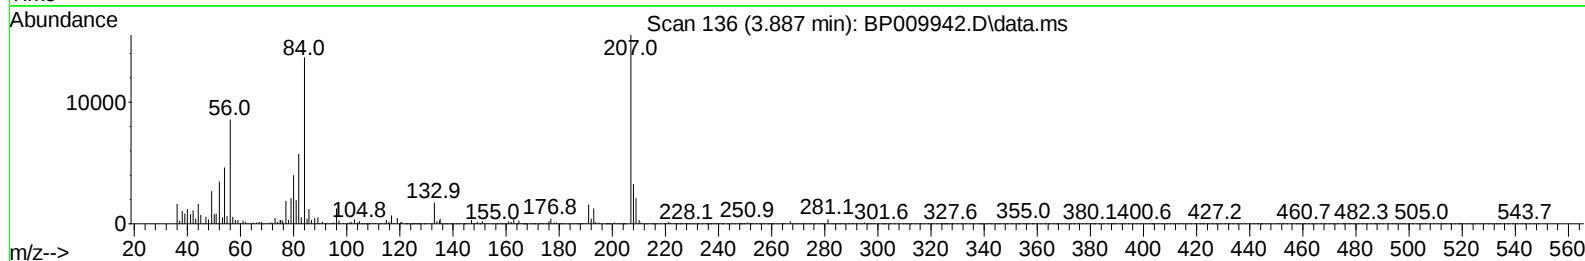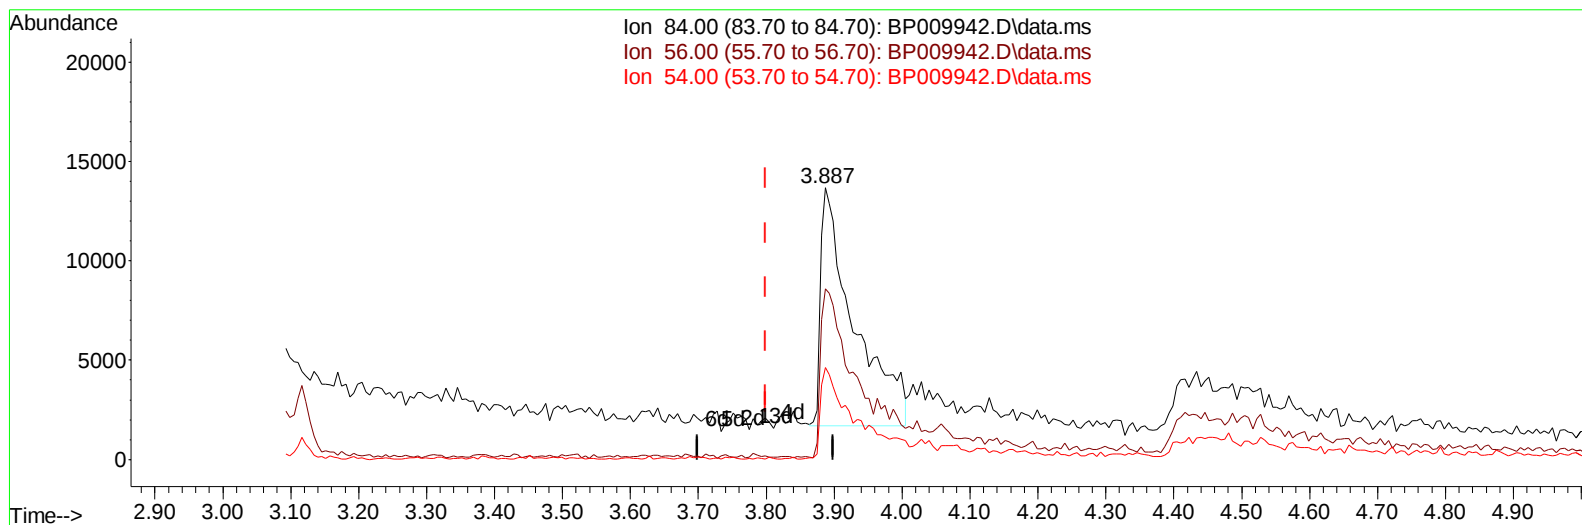

TIC: BP009942.D\data.ms

(4) Pyridine-d5 (S)

3.887min (+ 0.088) 5.13 ng/u1 m

response 40968

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	62.75#
54.00	24.80	33.90#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009942.D
 Acq On : 19 Apr 2022 06:44
 Operator : CG/JU
 Sample : N2421-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COHX0

Manual IntegrationsAPPROVED

Quant Time: Apr 19 07:42:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
 Supervised By :Yogesh Patel 04/22/2022

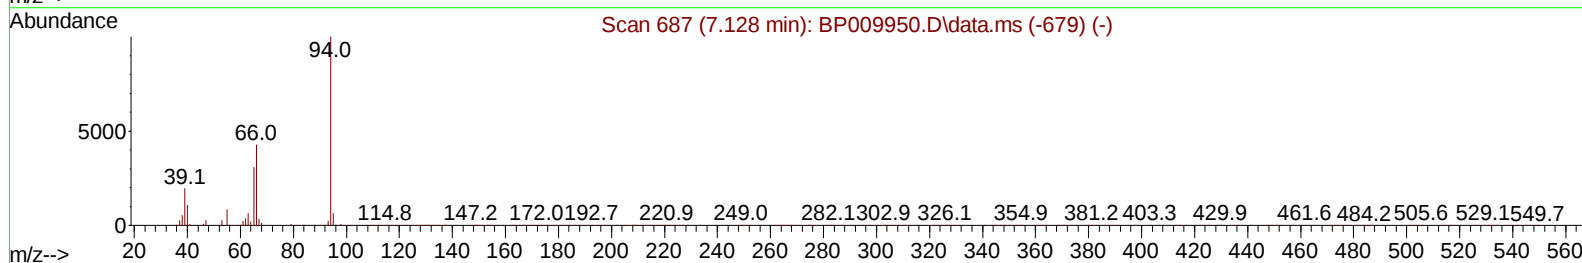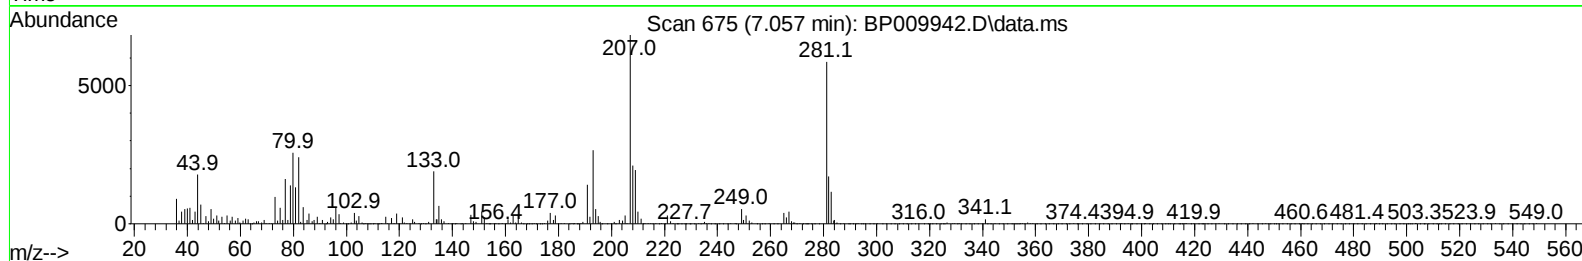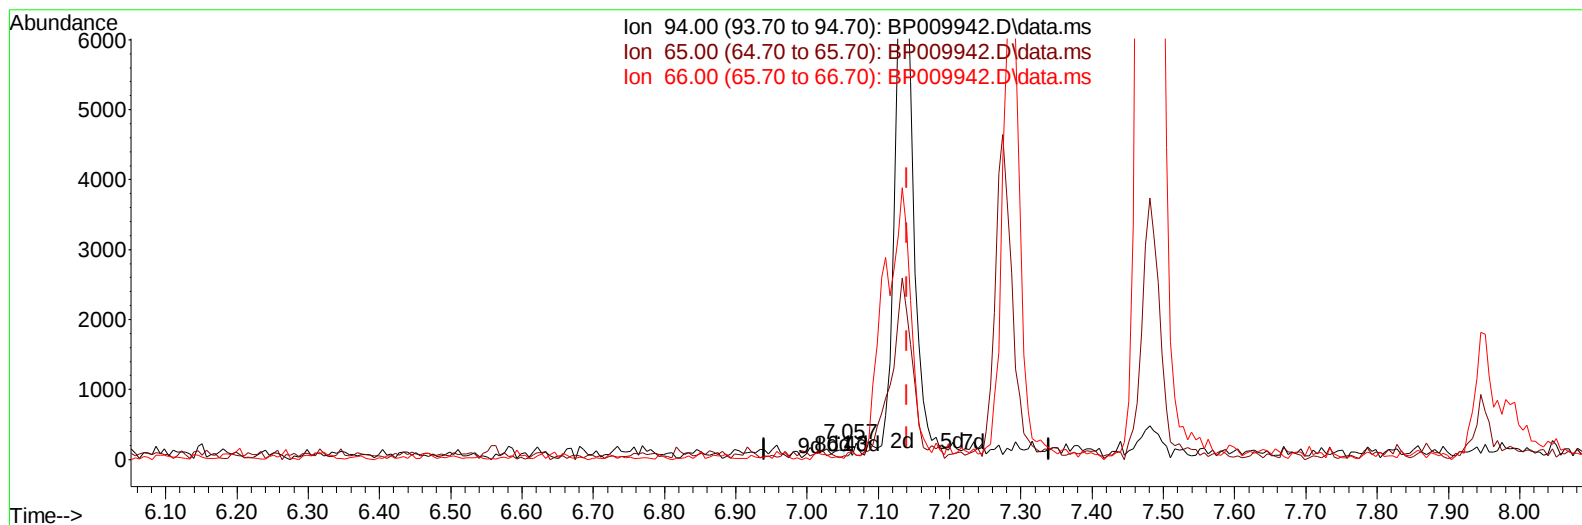

TIC: BP009942.D\data.ms

(8) Phenol

7.057min (-0.083) 0.01 ng/u1

response	64	
Ion	Exp%	Act%
94.00	100.00	100.00
65.00	23.80	23.48
66.00	43.20	43.91
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009942.D
 Acq On : 19 Apr 2022 06:44
 Operator : CG/JU
 Sample : N2421-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COHX0

Manual IntegrationsAPPROVED

Quant Time: Apr 19 07:42:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
 Supervised By :Yogesh Patel 04/22/2022

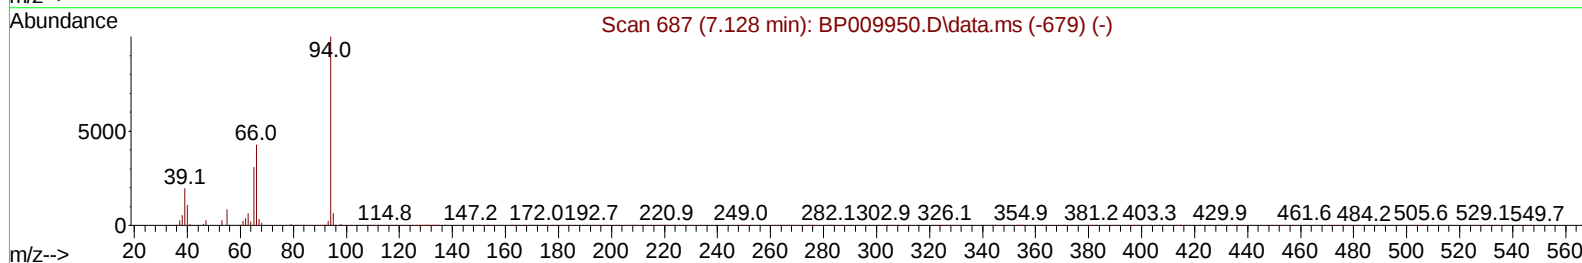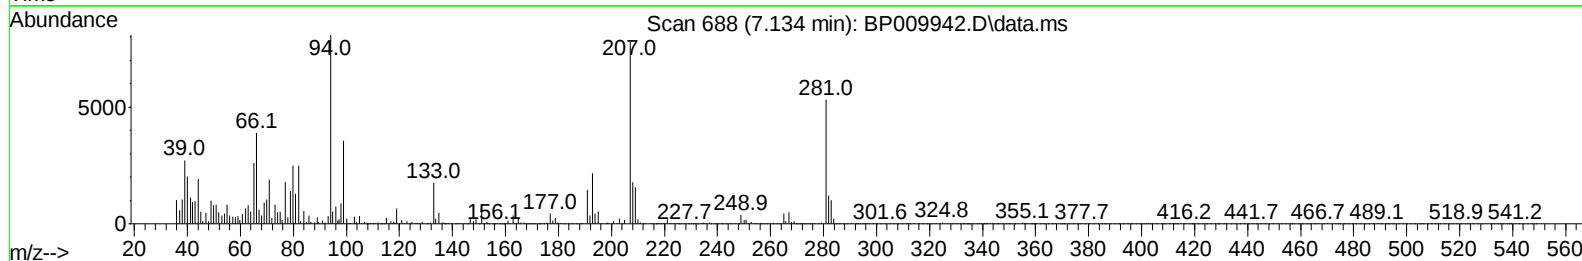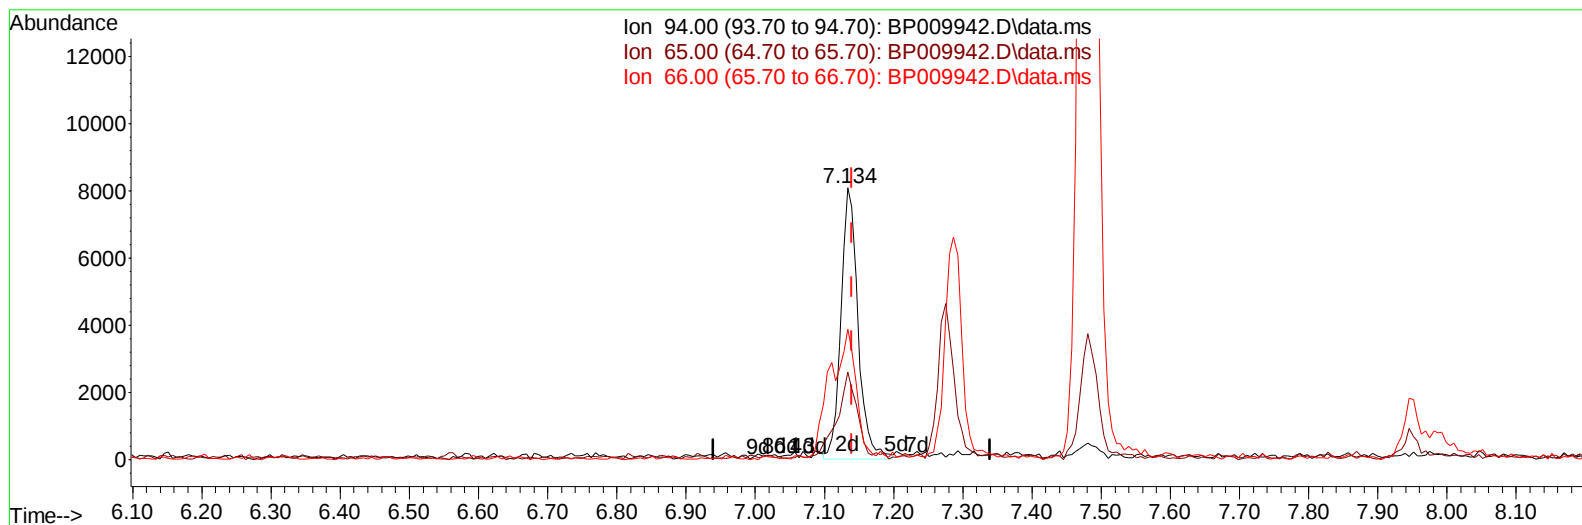

TIC: BP009942.D\data.ms

(8) Phenol

7.134min (-0.006) 1.22 ng/ul m

response 13859

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	23.80	32.11#
66.00	43.20	48.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009942.D
Acq On : 19 Apr 2022 06:44
Operator : CG/JU
Sample : N2421-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COHX0

Manual IntegrationsAPPROVED

Quant Time: Apr 19 07:42:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
Supervised By :Yogesh Patel 04/22/2022

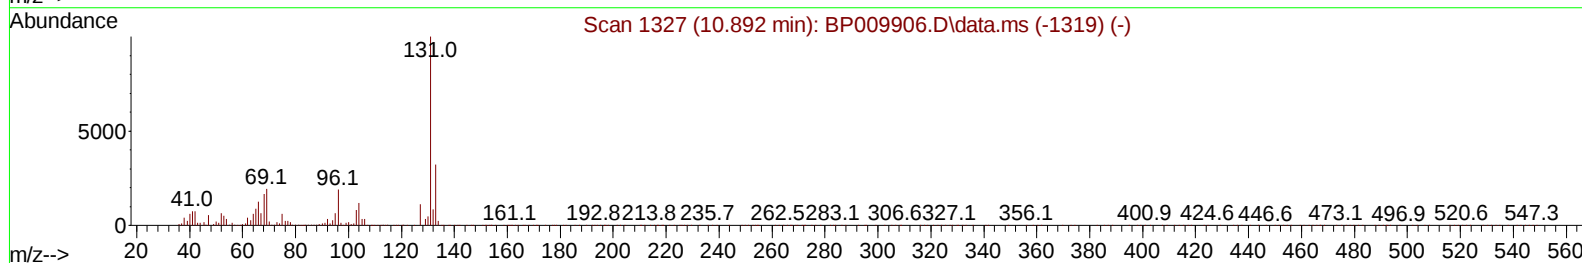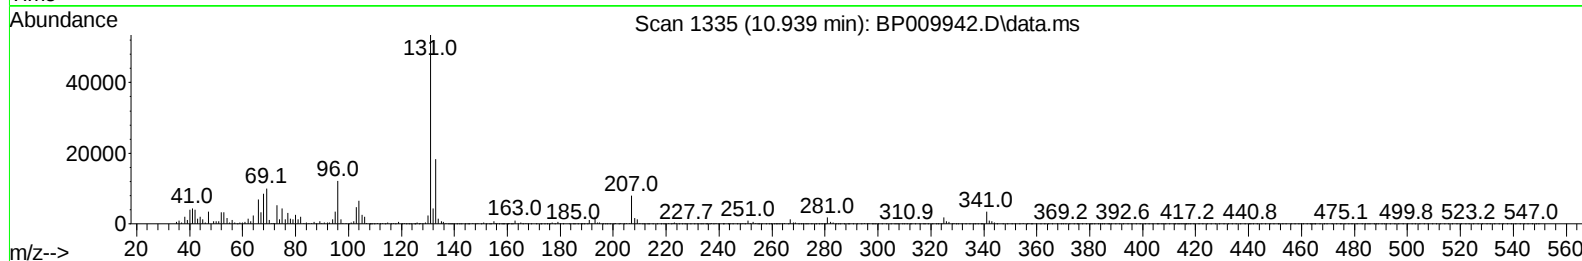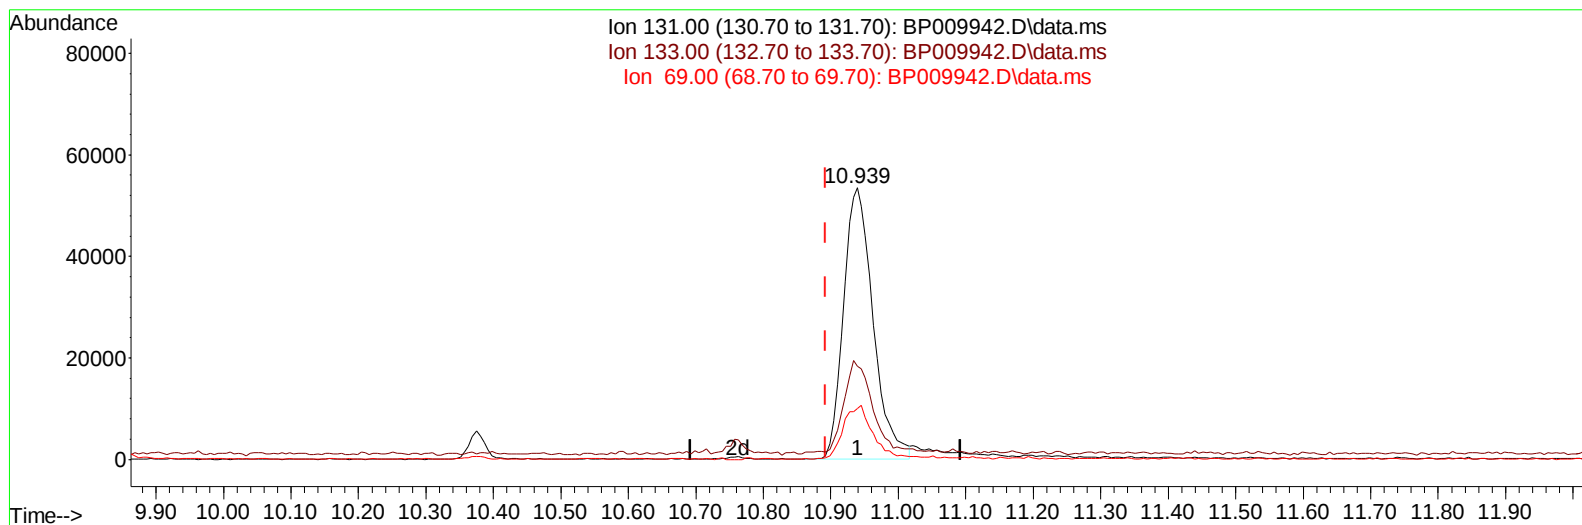

TIC: BP009942.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.939min (+ 0.047) 12.44 ng/u1

response 162471

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	34.22
69.00	26.10	18.75#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009942.D
Acq On : 19 Apr 2022 06:44
Operator : CG/JU
Sample : N2421-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COHX0

Manual IntegrationsAPPROVED

Quant Time: Apr 19 07:42:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
Supervised By :Yogesh Patel 04/22/2022

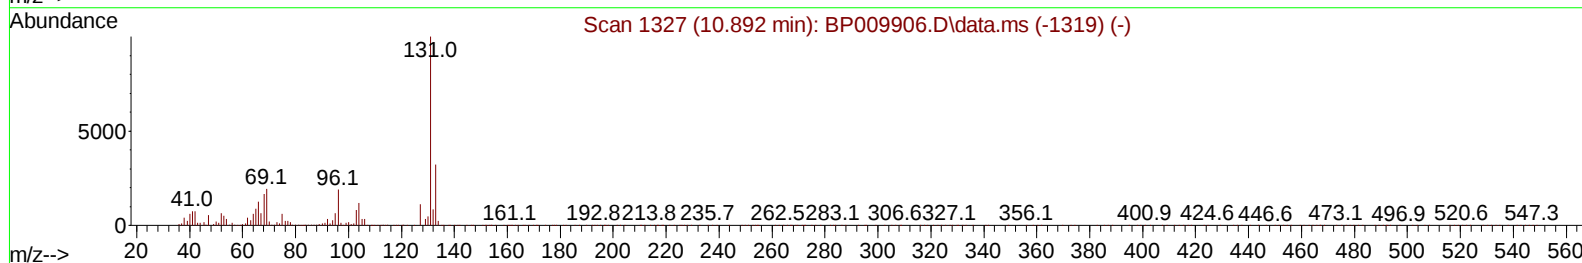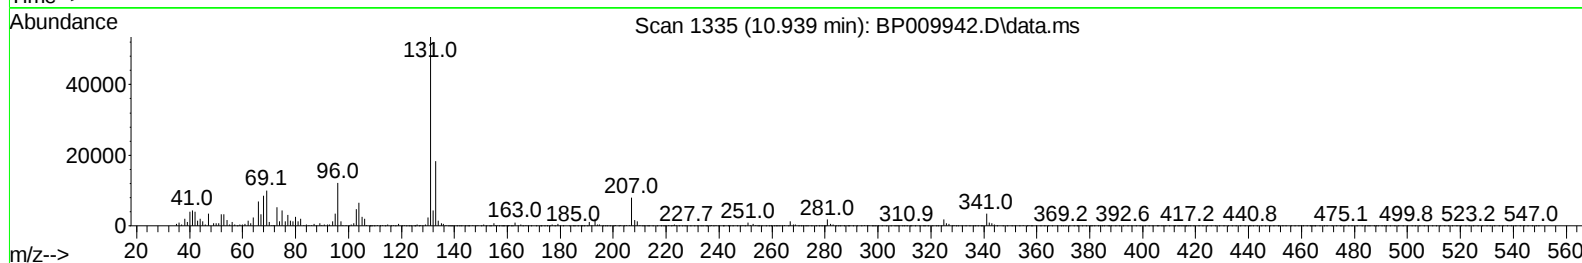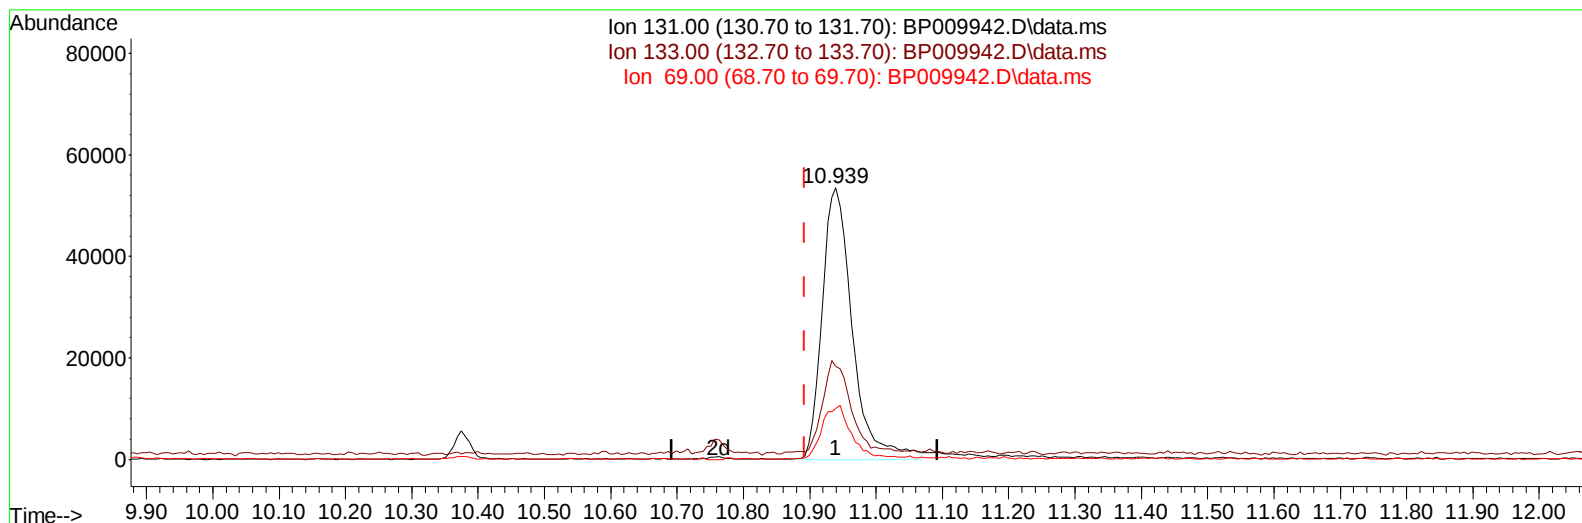

TIC: BP009942.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.939min (+ 0.047) 12.95 ng/ul m

response 169041

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	34.22
69.00	26.10	18.75#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009942.D
Acq On : 19 Apr 2022 06:44
Operator : CG/JU
Sample : N2421-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COHX0

Manual IntegrationsAPPROVED

Quant Time: Apr 19 07:42:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
Supervised By :Yogesh Patel 04/22/2022

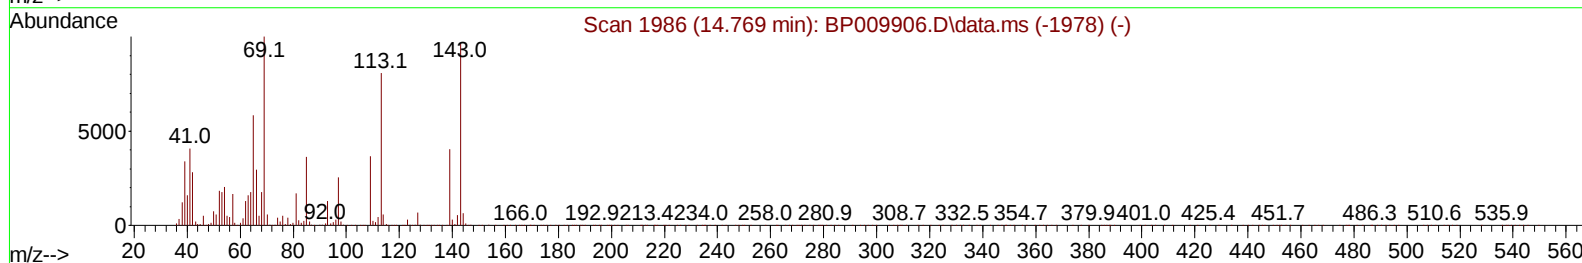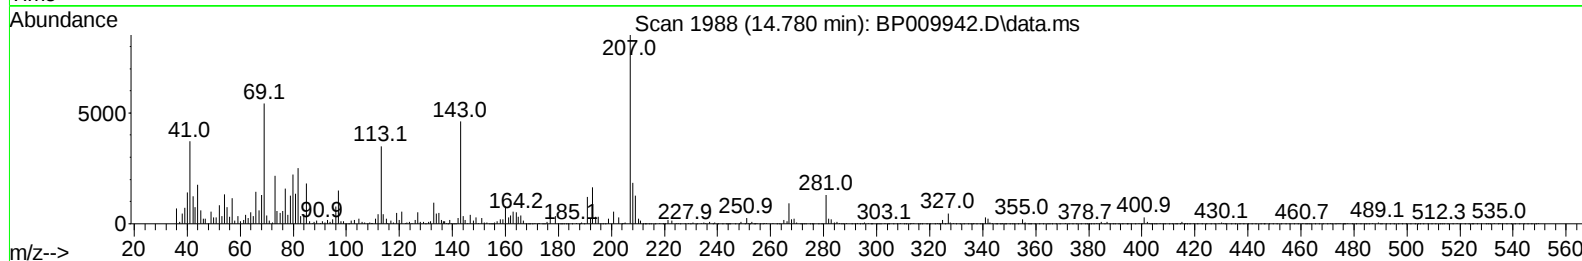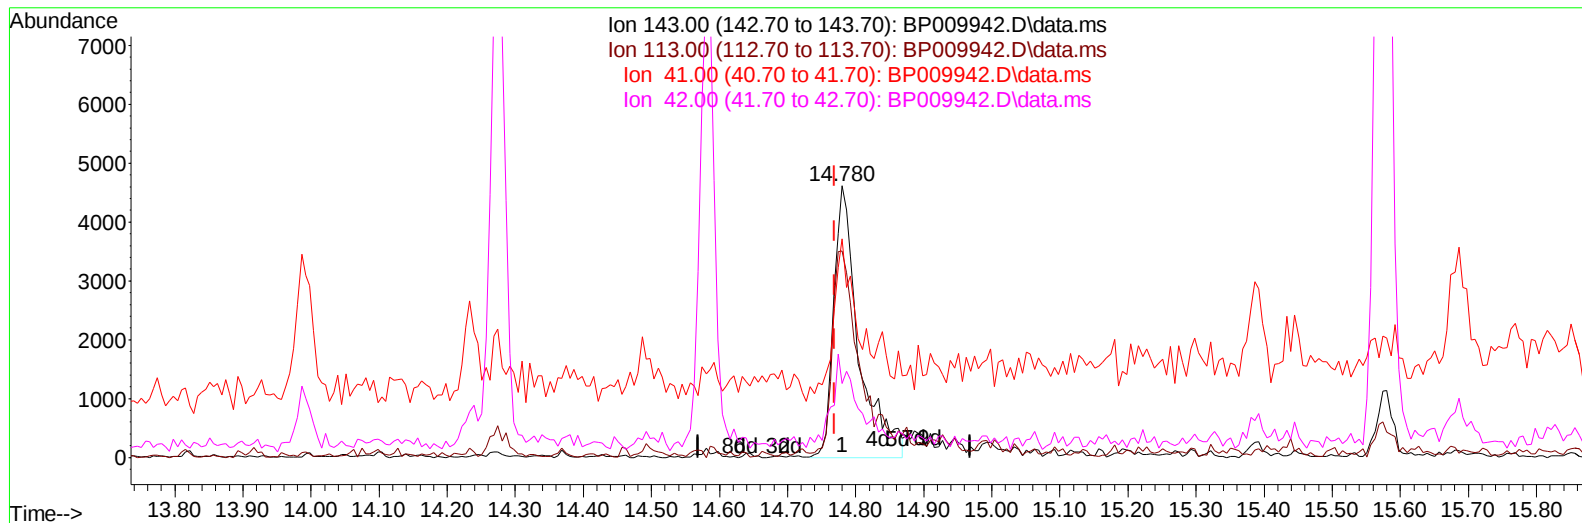

TIC: BP009942.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.780min (+ 0.011) 2.34 ng/ul m

response 11852

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	75.94#
41.00	23.20	80.49#
42.00	18.00	27.14#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009942.D
 Acq On : 19 Apr 2022 06:44
 Operator : CG/JU
 Sample : N2421-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COHX0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/20/2022
 Supervised By :Yogesh Patel 04/22/2022

Quant Time: Apr 19 07:42:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	129150	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	554066	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.580	164	355576	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.333	188	762541	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.415	240	541734	20.000	ng/ul	# 0.00
88) Perylene-d12	23.880	264	383109	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	15216m	5.258	ng/uL	0.00
4) Pyridine-d5	3.887	84	40968m	5.135	ng/ul	0.09
7) Phenol-d5	7.110	99	72686	6.411	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	241338	35.753	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	228909	26.764	ng/ul	0.00
15) 4-Methylphenol-d8	8.651	113	135442	14.309	ng/ul	-0.01
21) Nitrobenzene-d5	9.110	128	146737	36.725	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	69370	15.836	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.375	165	256490	27.981	ng/ul	0.00
31) 4-Chloroaniline-d4	10.939	131	169041m	12.948	ng/ul	0.05
46) Dimethylphthalate-d6	13.992	166	1061974	38.021	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	1073175	32.432	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.780	143	11852m	2.340	ng/ul	0.01
60) Fluorene-d10	15.574	176	926485	39.431	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	27687	6.129	ng/ul	0.00
73) Anthracene-d10	17.433	188	1497308	41.011	ng/ul	0.00
81) Pyrene-d10	19.662	212	1827042	61.752	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.721	264	835822	41.894	ng/ul	0.00
Target Compounds						
8) Phenol	7.134	94	13859m	1.221	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009942.D
Acq On : 19 Apr 2022 06:44
Operator : CG/JU
Sample : N2421-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HX0

Manual IntegrationsAPPROVED

Quant Time: Apr 19 07:42:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/20/2022
Supervised By :Yogesh Patel 04/22/2022

