




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009943.D
Acq On : 19 Apr 2022 07:17
Operator : CG/JU
Sample : N2421-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HY7

Manual IntegrationsAPPROVED

Quant Time: Apr 19 08:20:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/22/2022

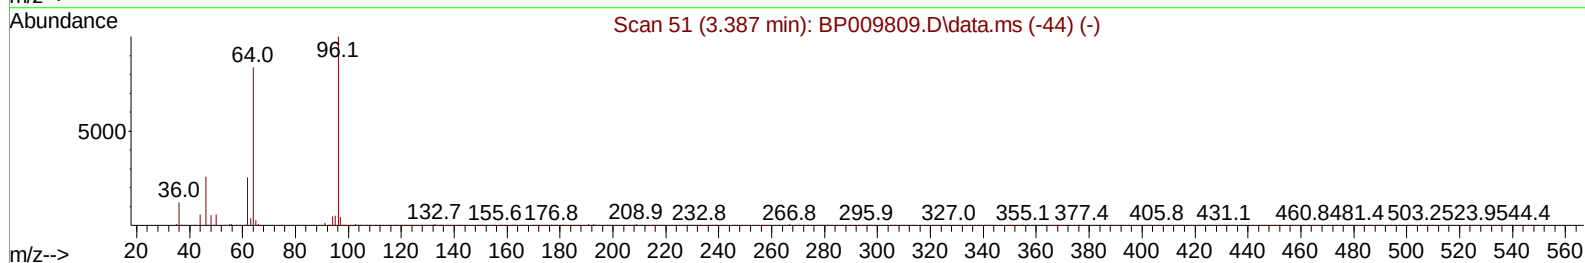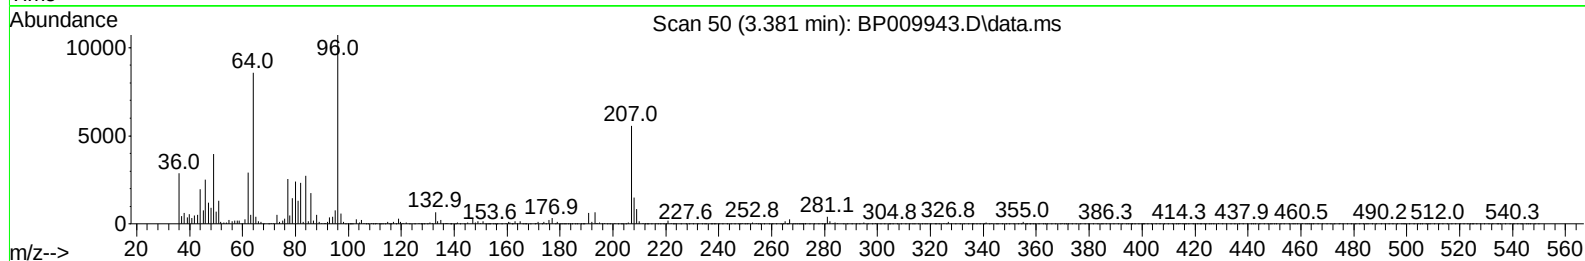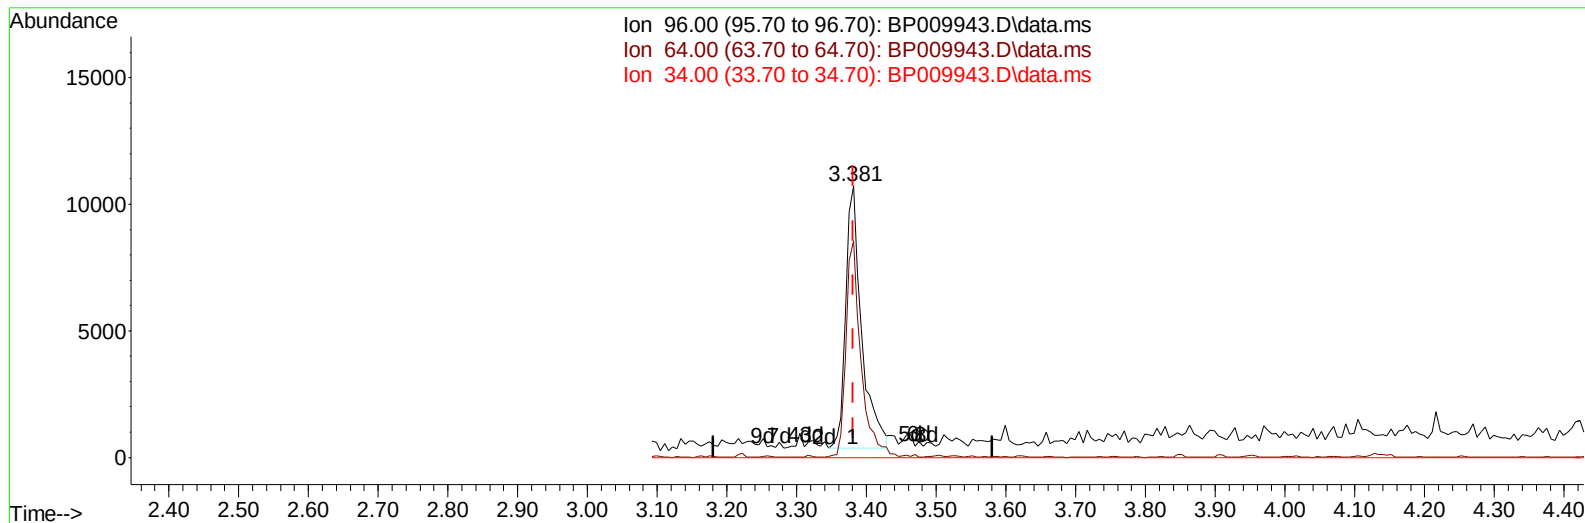

TIC: BP009943.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.381min (-0.000) 4.53 ng/uL

response 16418

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	79.89#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009943.D
Acq On : 19 Apr 2022 07:17
Operator : CG/JU
Sample : N2421-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HY7

Manual IntegrationsAPPROVED

Quant Time: Apr 19 08:20:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/22/2022

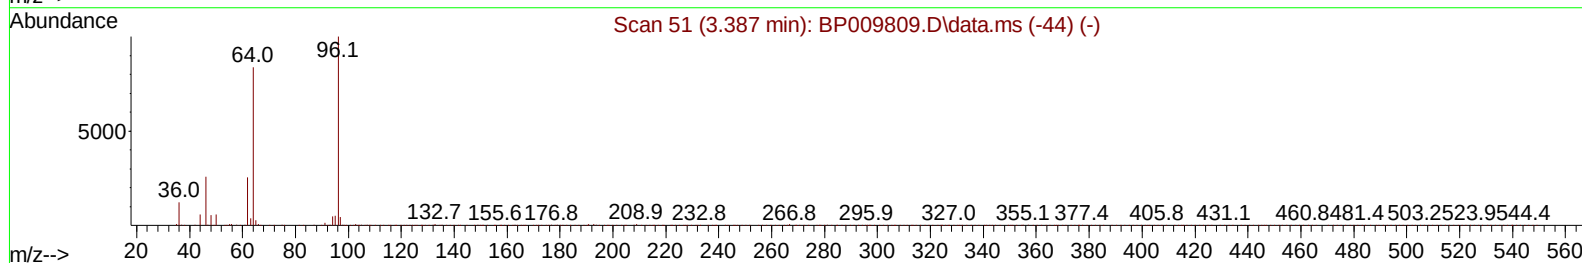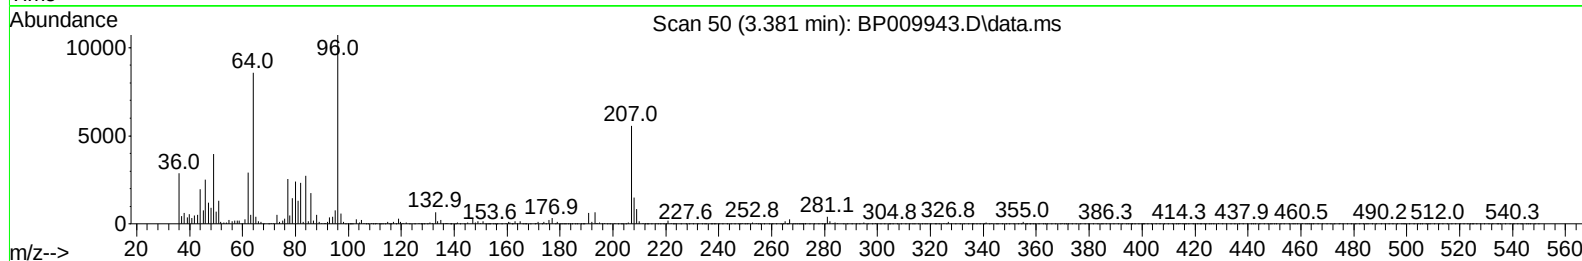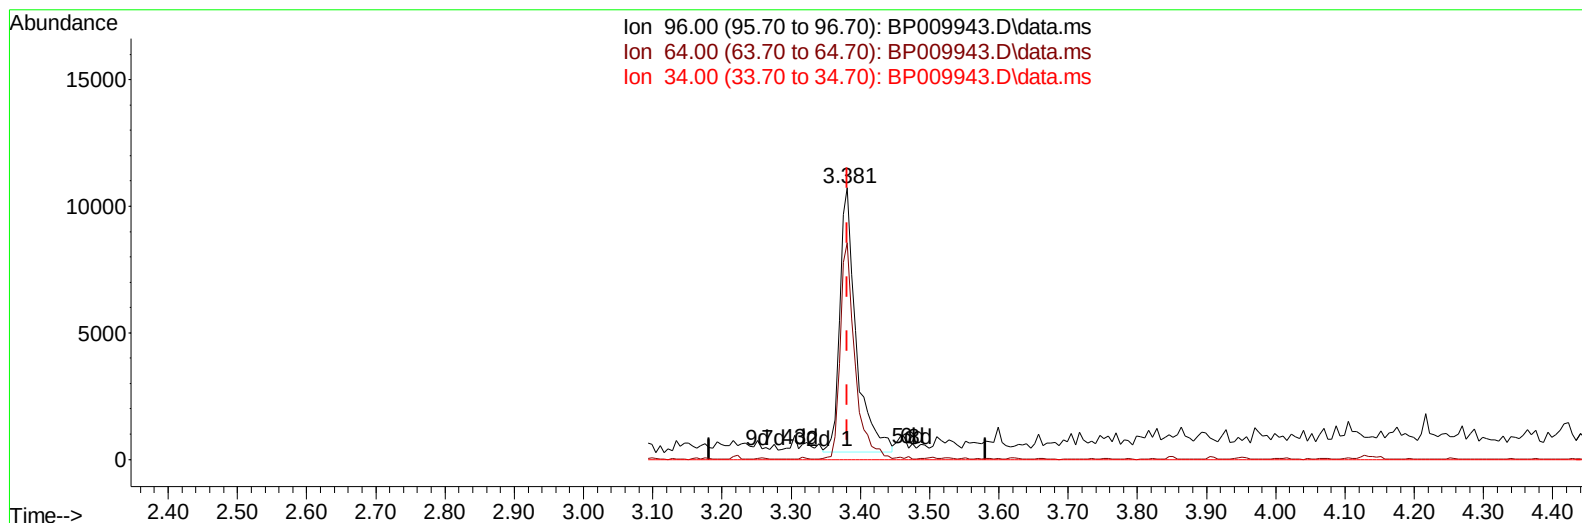

TIC: BP009943.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.381min (-0.000) 4.77 ng/uL m

response 17299

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	79.89#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009943.D
 Acq On : 19 Apr 2022 07:17
 Operator : CG/JU
 Sample : N2421-10
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HY7

Manual IntegrationsAPPROVED

Quant Time: Apr 19 08:20:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/22/2022

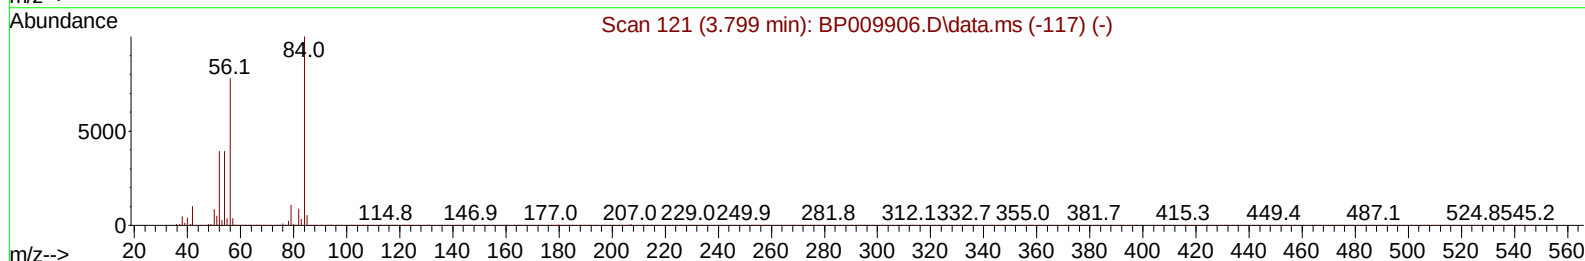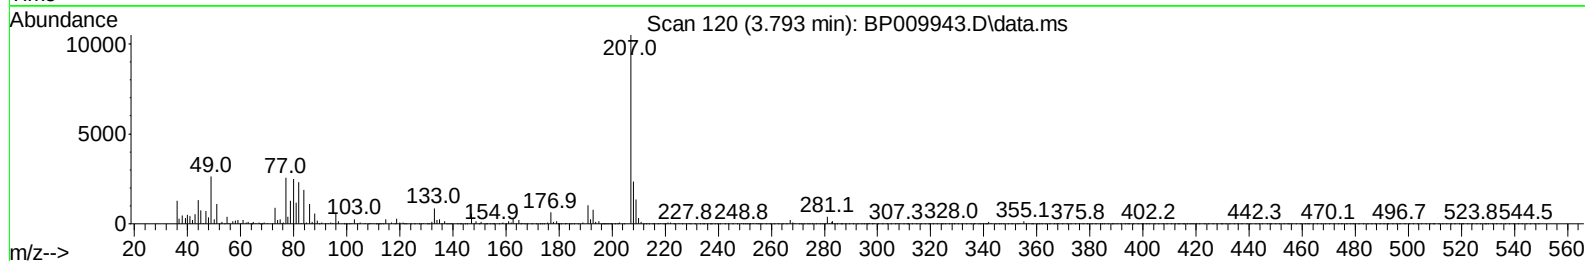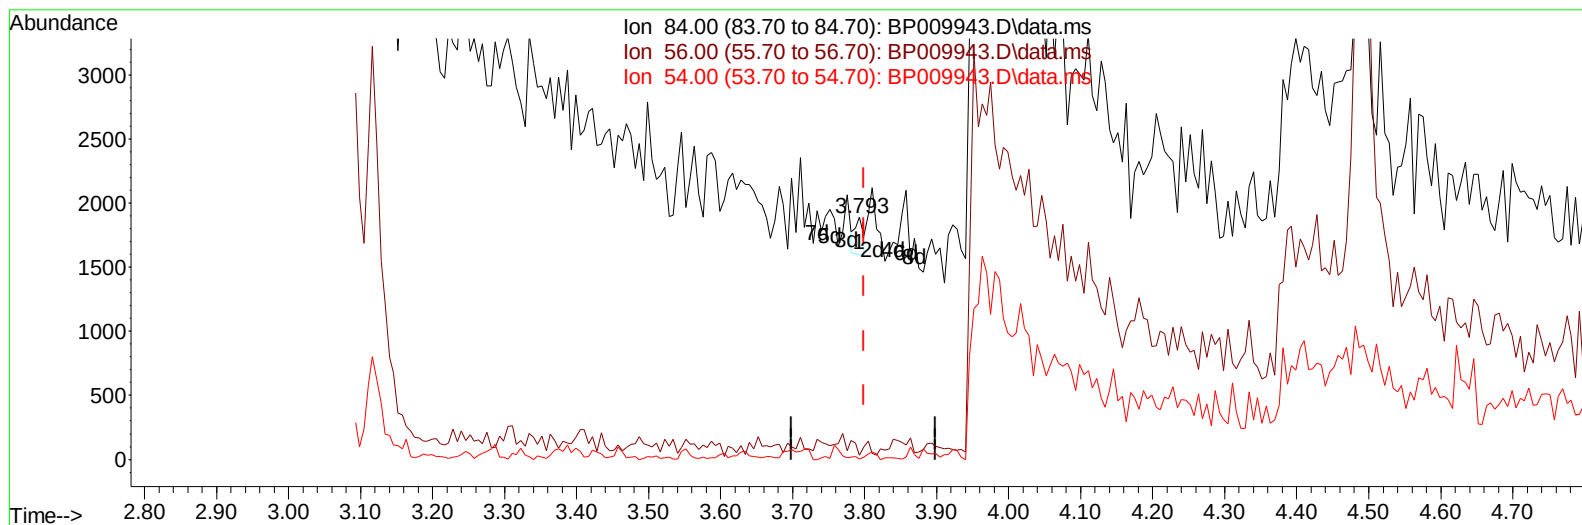

TIC: BP009943.D\data.ms

(4) Pyridine-d5 (S)

3.793min (-0.006) 0.02 ng/ul

response 225

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	1.64#
54.00	24.80	0.26#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009943.D
Acq On : 19 Apr 2022 07:17
Operator : CG/JU
Sample : N2421-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HY7

Manual IntegrationsAPPROVED

Quant Time: Apr 19 08:20:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/22/2022

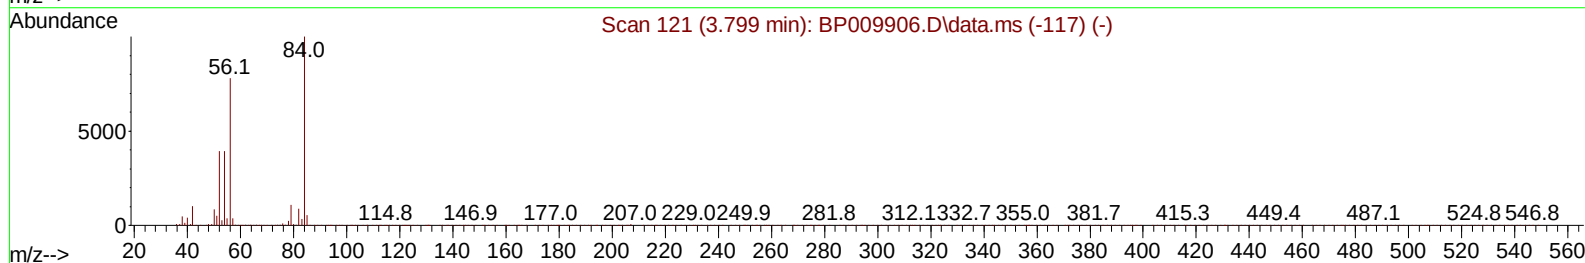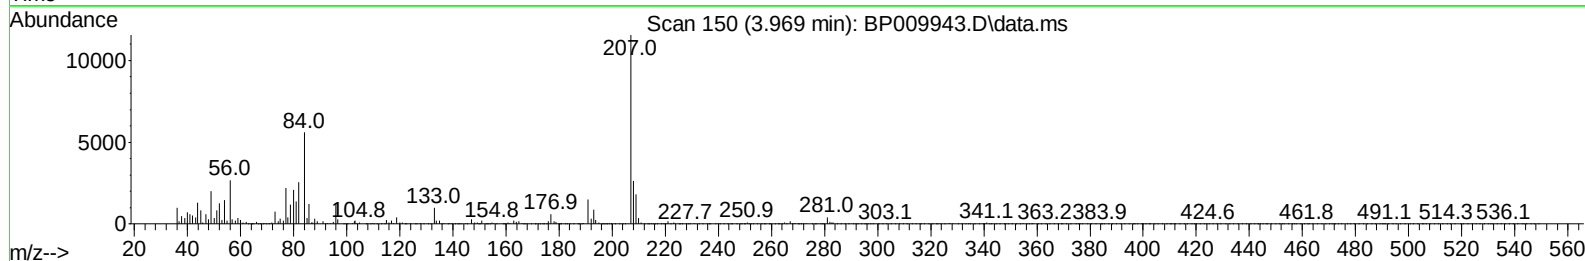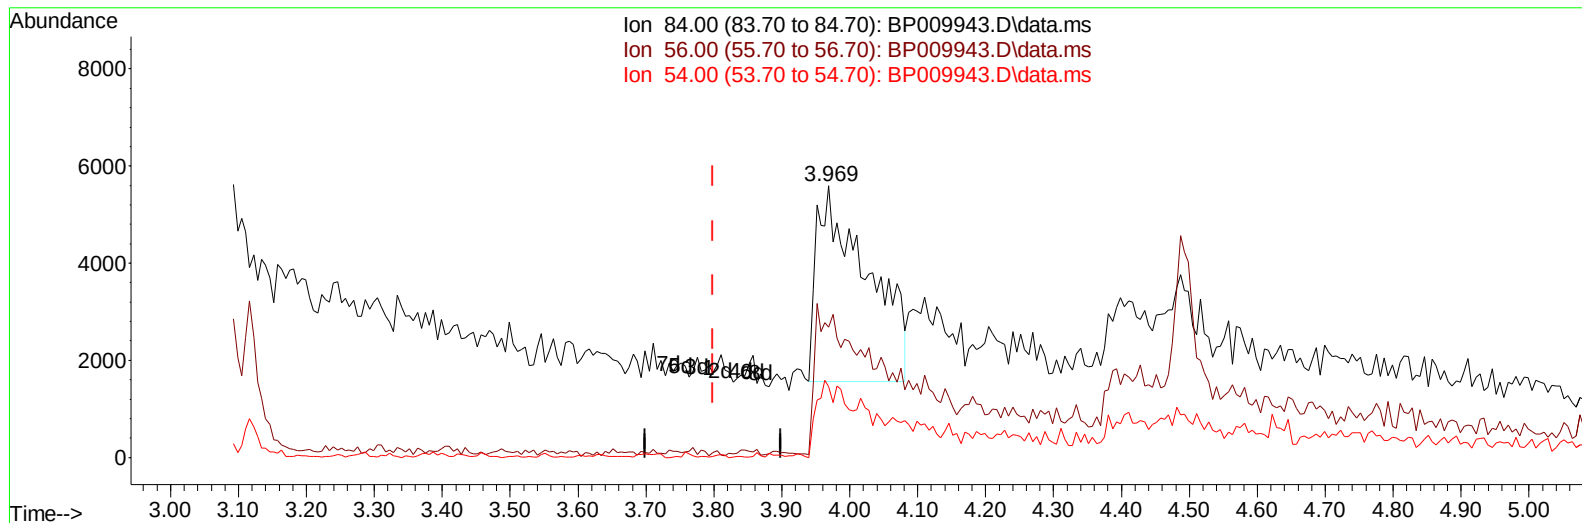

TIC: BP009943.D\data.ms

(4) Pyridine-d5 (S)

3.969min (+ 0.170) 2.10 ng/ul m

response 20936

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	48.01#
54.00	24.80	26.05
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009943.D
Acq On : 19 Apr 2022 07:17
Operator : CG/JU
Sample : N2421-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HY7

Manual IntegrationsAPPROVED

Quant Time: Apr 19 08:20:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/22/2022

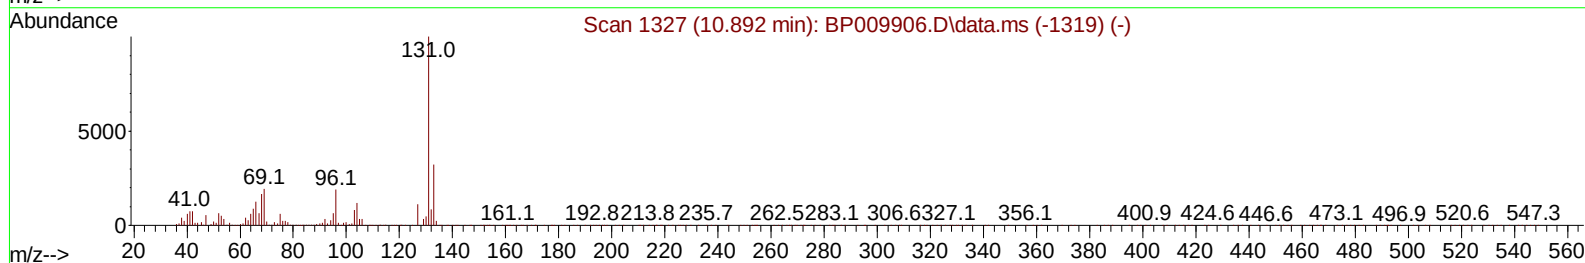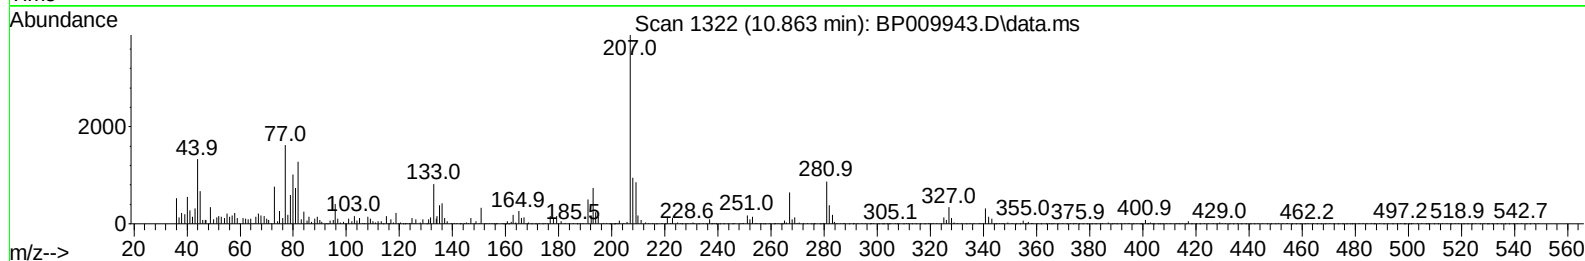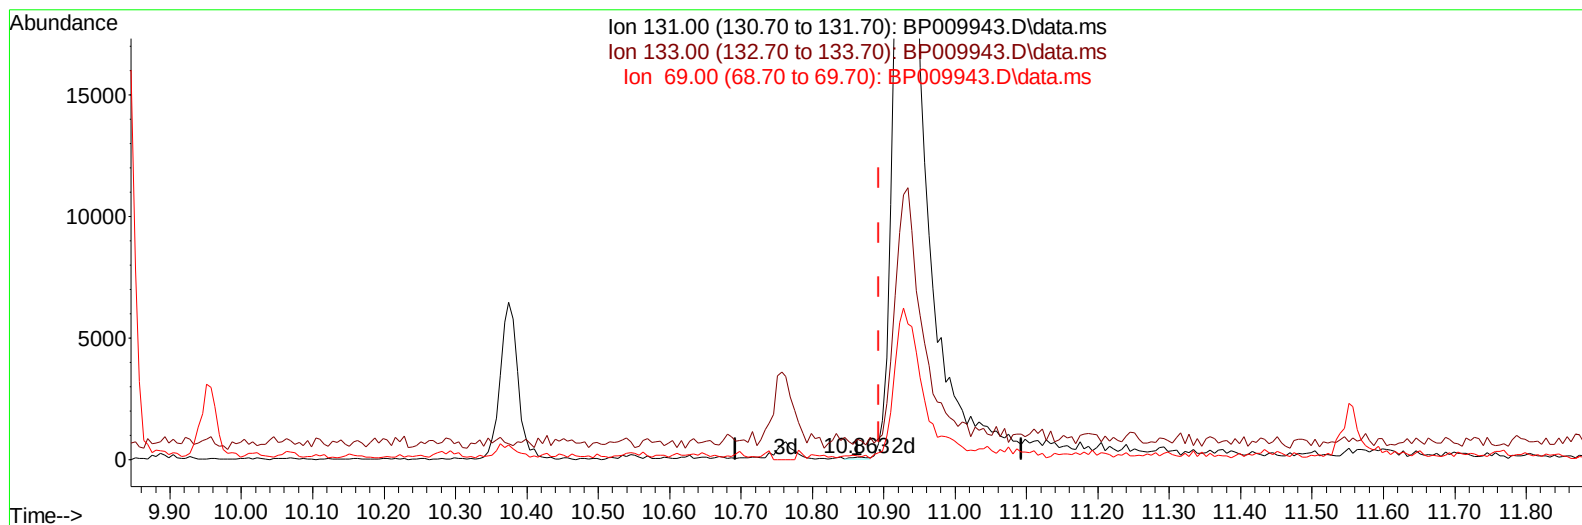

TIC: BP009943.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.863min (-0.030) 0.01 ng/u1

response 147

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	902.20#
69.00	26.10	174.73#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009943.D
Acq On : 19 Apr 2022 07:17
Operator : CG/JU
Sample : N2421-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HY7

Manual IntegrationsAPPROVED

Quant Time: Apr 19 08:20:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/22/2022

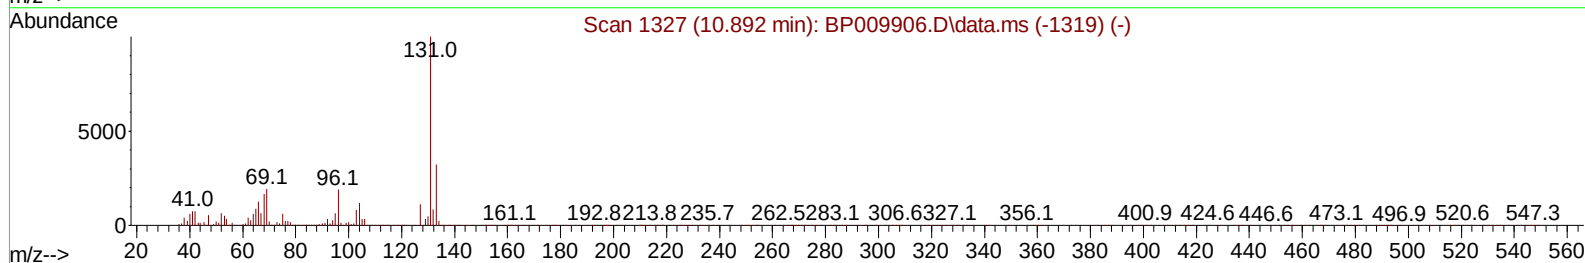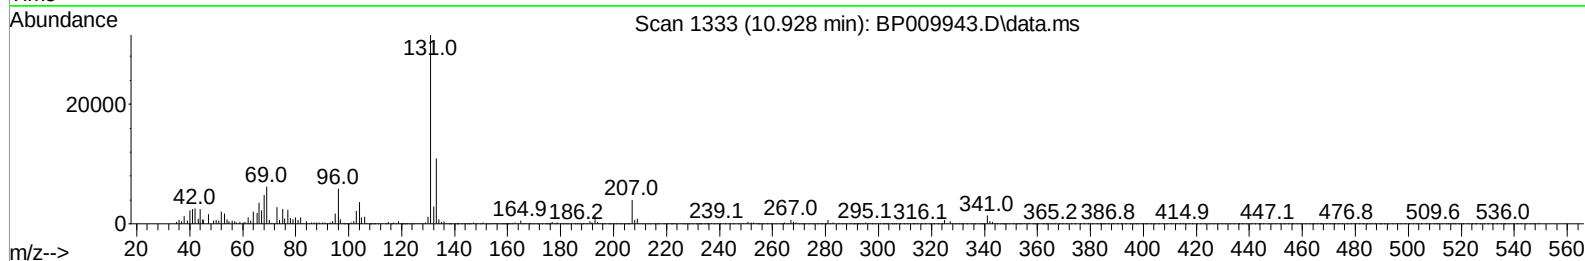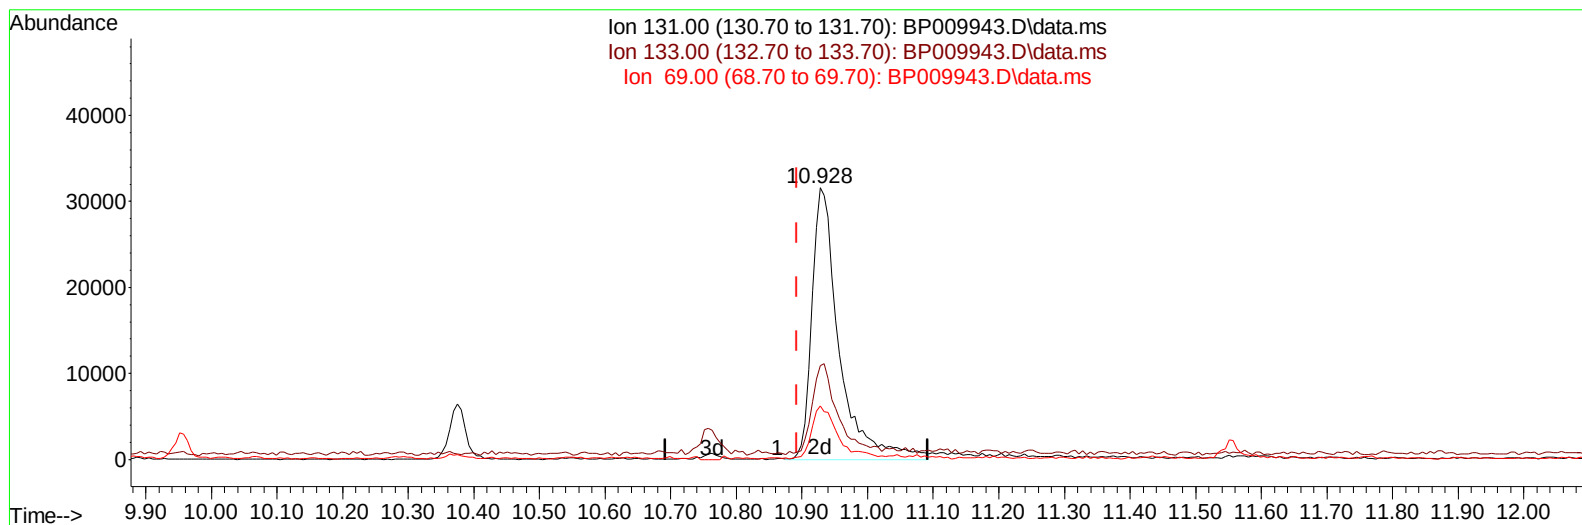

TIC: BP009943.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.928min (+ 0.035) 5.57 ng/ul m

response 91635

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	34.52
69.00	26.10	19.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009943.D
Acq On : 19 Apr 2022 07:17
Operator : CG/JU
Sample : N2421-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HY7

Manual IntegrationsAPPROVED

Quant Time: Apr 19 08:20:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/22/2022

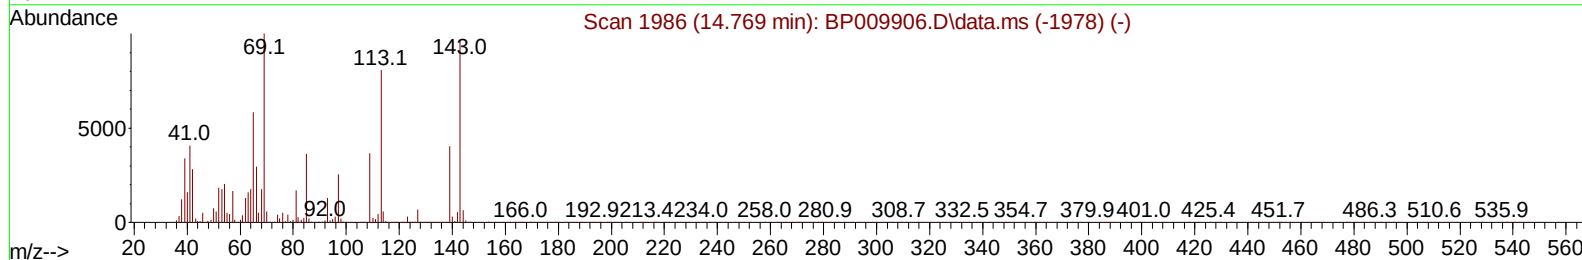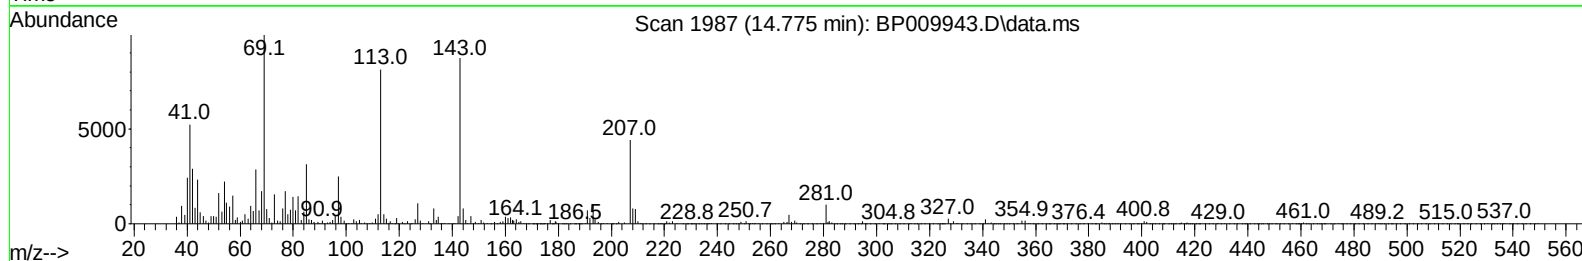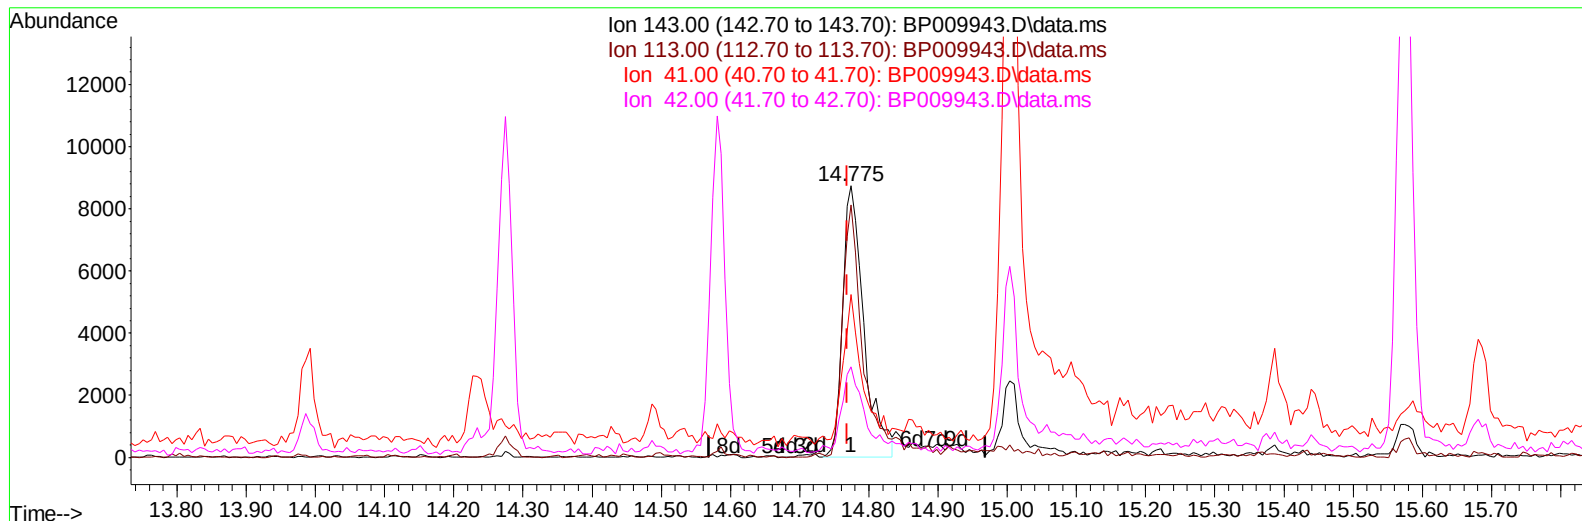

TIC: BP009943.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.775min (+ 0.006) 2.86 ng/ul

response 18539

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	93.12#
41.00	23.20	59.91#
42.00	18.00	33.28#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009943.D
Acq On : 19 Apr 2022 07:17
Operator : CG/JU
Sample : N2421-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HY7

Manual IntegrationsAPPROVED

Quant Time: Apr 19 08:20:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/22/2022

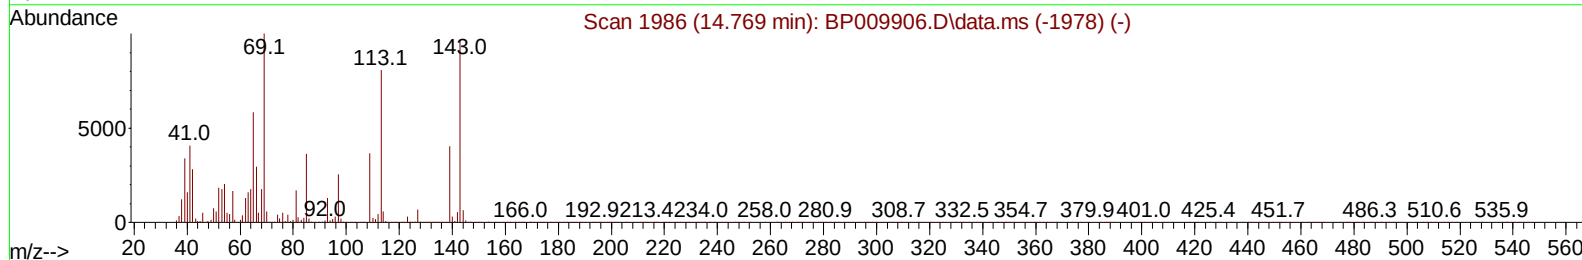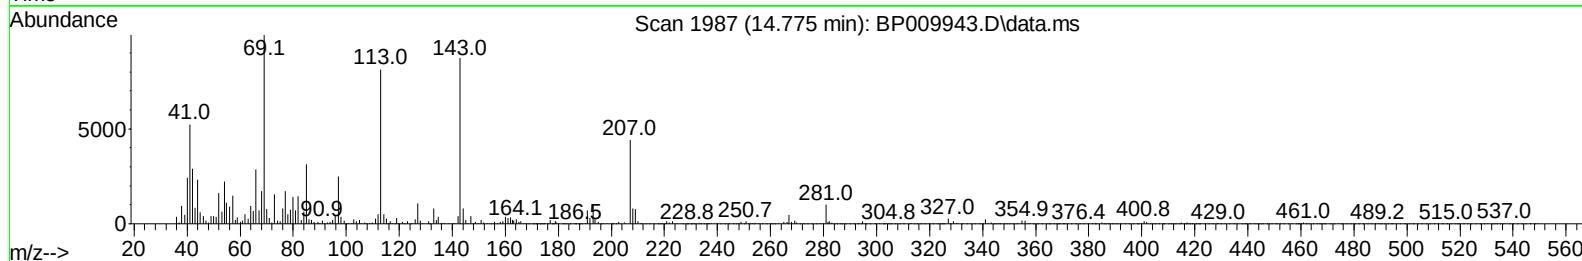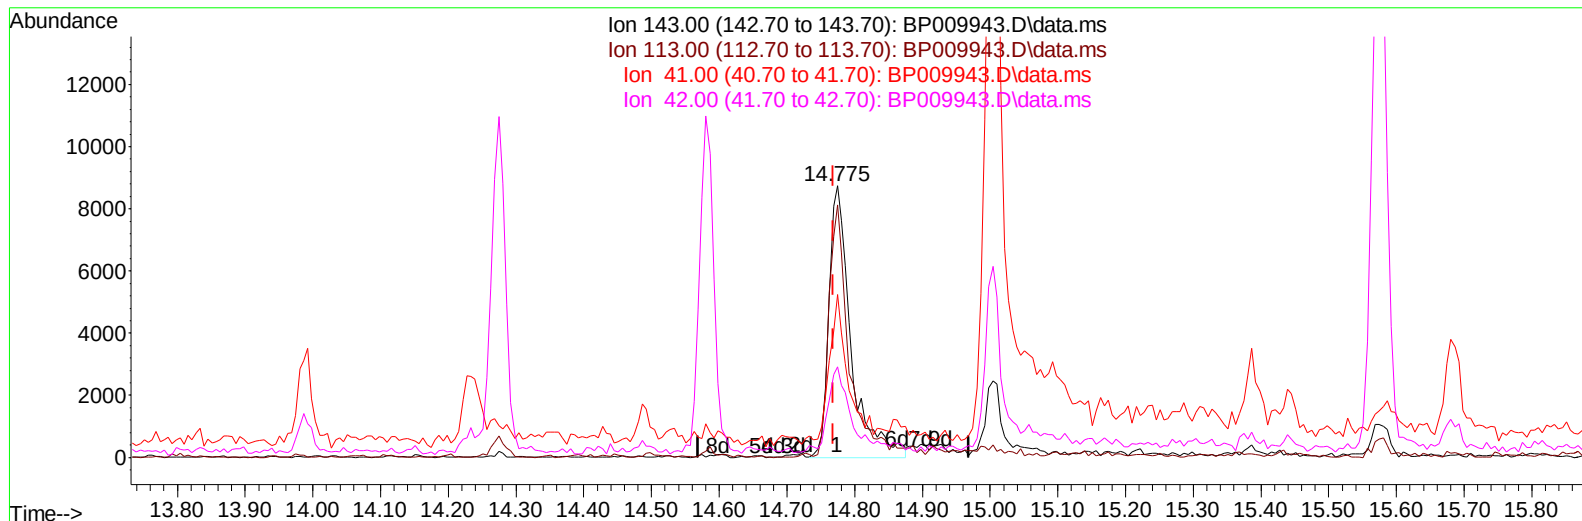

TIC: BP009943.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.775min (+ 0.006) 3.06 ng/ul m

response 19830

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	93.12#
41.00	23.20	59.91#
42.00	18.00	33.28#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009943.D
 Acq On : 19 Apr 2022 07:17
 Operator : CG/JU
 Sample : N2421-10
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HY7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/22/2022

Quant Time: Apr 19 08:20:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	161735	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	698689	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.580	164	454608	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.333	188	929594	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.415	240	751670	20.000	ng/ul	# 0.00
88) Perylene-d12	23.880	264	553657	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	17299m	4.774	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.110	99	94570	6.660	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	240327	28.430	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	246544	23.018	ng/ul	0.00
15) 4-Methylphenol-d8	8.651	113	153587	12.957	ng/ul	-0.01
21) Nitrobenzene-d5	9.110	128	148546	29.482	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	94347	17.080	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.375	165	305265	26.409	ng/ul	0.00
31) 4-Chloroaniline-d4	10.928	131	91635m	5.566	ng/ul	0.04
46) Dimethylphthalate-d6	13.986	166	1142559	31.995	ng/ul	-0.01
49) Acenaphthylene-d8	14.275	160	1178452	27.855	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.775	143	19830m	3.062	ng/ul	0.00
60) Fluorene-d10	15.575	176	948589	31.577	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	43381	7.878	ng/ul	0.00
73) Anthracene-d10	17.433	188	1442743	32.415	ng/ul	0.00
81) Pyrene-d10	19.663	212	1889961	46.037	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.721	264	1014807	35.197	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.134	94	17285	1.216	ng/ul#	81
86) Bis(2-ethylhexyl)phtha...	21.327	149	38186	1.292	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009943.D
Acq On : 19 Apr 2022 07:17
Operator : CG/JU
Sample : N2421-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HY7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/22/2022

Quant Time: Apr 19 08:20:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

