

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009930.D
 Acq On : 18 Apr 2022 23:26
 Operator : CG/JU
 Sample : N2422-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HZ8

Quant Time: Apr 19 00:59:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	111395	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	494427	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.581	164	359308	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.334	188	806533	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.416	240	843408	20.000	ng/ul	# 0.00
88) Perylene-d12	23.880	264	777563	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	12708	5.091	ng/uL	0.00
4) Pyridine-d5	3.799	84	59508	8.647	ng/ul	0.00
7) Phenol-d5	7.105	99	64881	6.634	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	192269	33.023	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	179162	24.286	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	129999	15.923	ng/ul	-0.01
21) Nitrobenzene-d5	9.111	128	122443	34.341	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	124614	31.879	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.375	165	221418	27.069	ng/ul	0.00
31) 4-Chloroaniline-d4	10.887	131	333741	28.646	ng/ul	0.00
46) Dimethylphthalate-d6	13.987	166	961644	34.072	ng/ul	-0.01
49) Acenaphthylene-d8	14.275	160	1026737	30.706	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.763	143	30437	5.946	ng/ul	0.00
60) Fluorene-d10	15.575	176	839237	35.346	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	146261	30.612	ng/ul	0.00
73) Anthracene-d10	17.434	188	1535258	39.757	ng/ul	0.00
81) Pyrene-d10	19.663	212	1889741	41.025	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.721	264	1660752	41.014	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	12.034	107	18905	1.967	ng/ul#	Qvalue 64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009930.D
Acq On : 18 Apr 2022 23:26
Operator : CG/JU
Sample : N2422-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ8


Quant Time: Apr 19 00:59:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

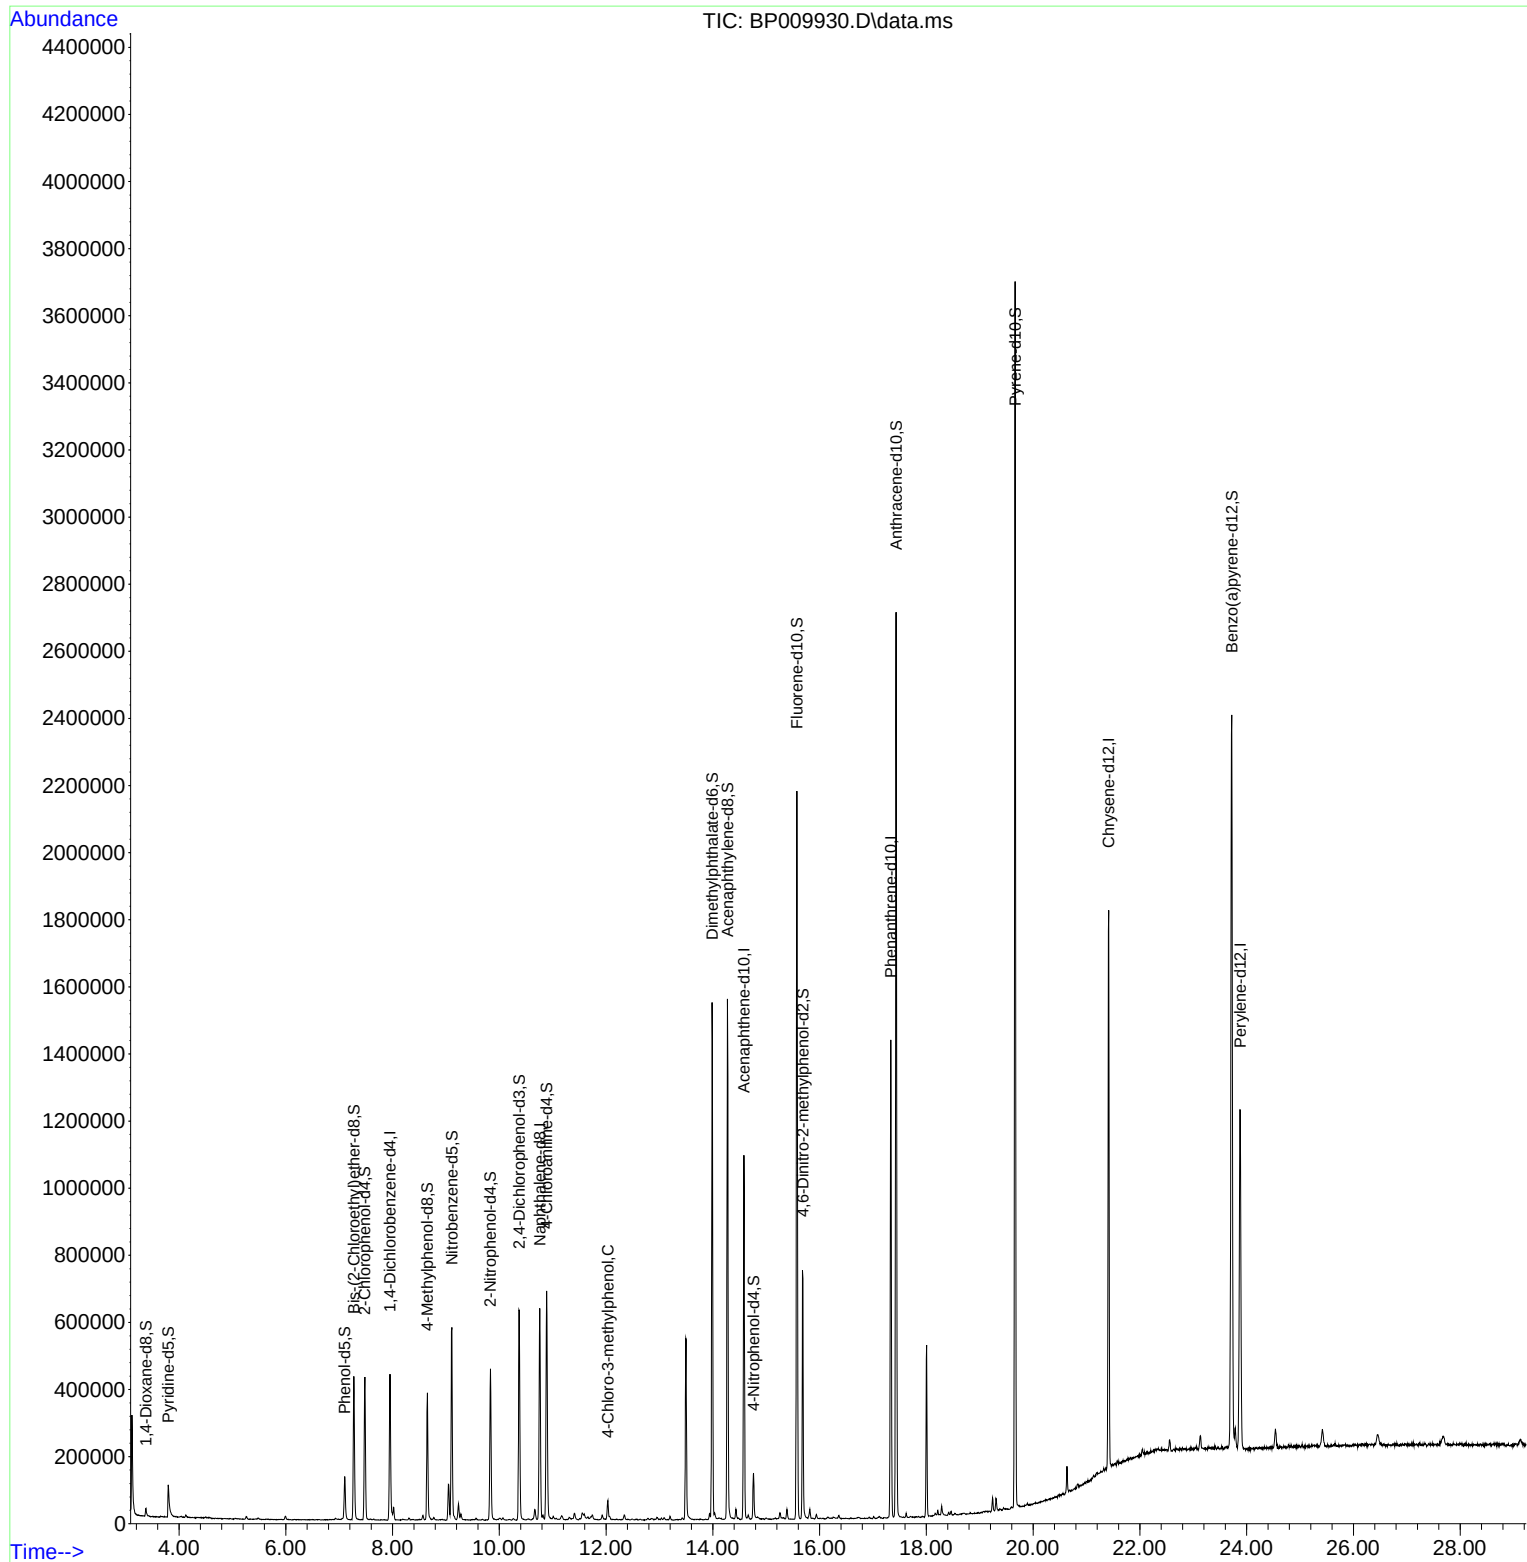

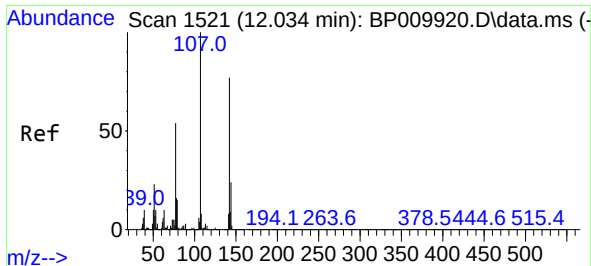

#35
 4-Chloro-3-methylphenol
 Concen: 1.967 ng/ul
 RT: 12.034 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BP009930.D
 Acq: 18 Apr 2022 23:26

Instrument :
 BNA_P
 ClientSampleId :
 C0HZ8

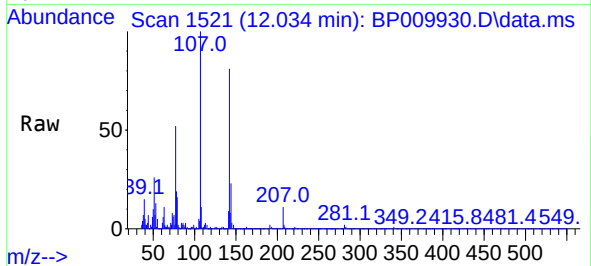

Tgt Ion:107 Resp: 18905
 Ion Ratio Lower Upper
 107 100
 144 23.3 15.8 23.8
 142 80.8 38.9 58.3#

