

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009942.D
 Acq On : 19 Apr 2022 06:44
 Operator : CG/JU
 Sample : N2421-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COHX0

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/20/2022
 Supervised By :Yogesh Patel 04/22/2022

Quant Time: Apr 19 07:42:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	129150	20.000	ng/u1	0.00
20) Naphthalene-d8	10.757	136	554066	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.580	164	355576	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.333	188	762541	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.415	240	541734	20.000	ng/u1	# 0.00
88) Perylene-d12	23.880	264	383109	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	15216m	5.258	ng/uL	0.00
4) Pyridine-d5	3.887	84	40968m	5.135	ng/u1	0.09
7) Phenol-d5	7.110	99	72686	6.411	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	241338	35.753	ng/u1	0.00
11) 2-Chlorophenol-d4	7.481	132	228909	26.764	ng/u1	0.00
15) 4-Methylphenol-d8	8.651	113	135442	14.309	ng/u1	-0.01
21) Nitrobenzene-d5	9.110	128	146737	36.725	ng/u1	0.00
24) 2-Nitrophenol-d4	9.834	143	69370	15.836	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.375	165	256490	27.981	ng/u1	0.00
31) 4-Chloroaniline-d4	10.939	131	169041m	12.948	ng/u1	0.05
46) Dimethylphthalate-d6	13.992	166	1061974	38.021	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	1073175	32.432	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.780	143	11852m	2.340	ng/u1	0.01
60) Fluorene-d10	15.574	176	926485	39.431	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	27687	6.129	ng/u1	0.00
73) Anthracene-d10	17.433	188	1497308	41.011	ng/u1	0.00
81) Pyrene-d10	19.662	212	1827042	61.752	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.721	264	835822	41.894	ng/u1	0.00
Target Compounds						
8) Phenol	7.134	94	13859m	1.221	ng/u1	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009942.D
Acq On : 19 Apr 2022 06:44
Operator : CG/JU
Sample : N2421-08
Misc :
ALS Vial : 38 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
C0HX0

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/20/2022
Supervised By :Yogesh Patel 04/22/2022


Quant Time: Apr 19 07:42:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

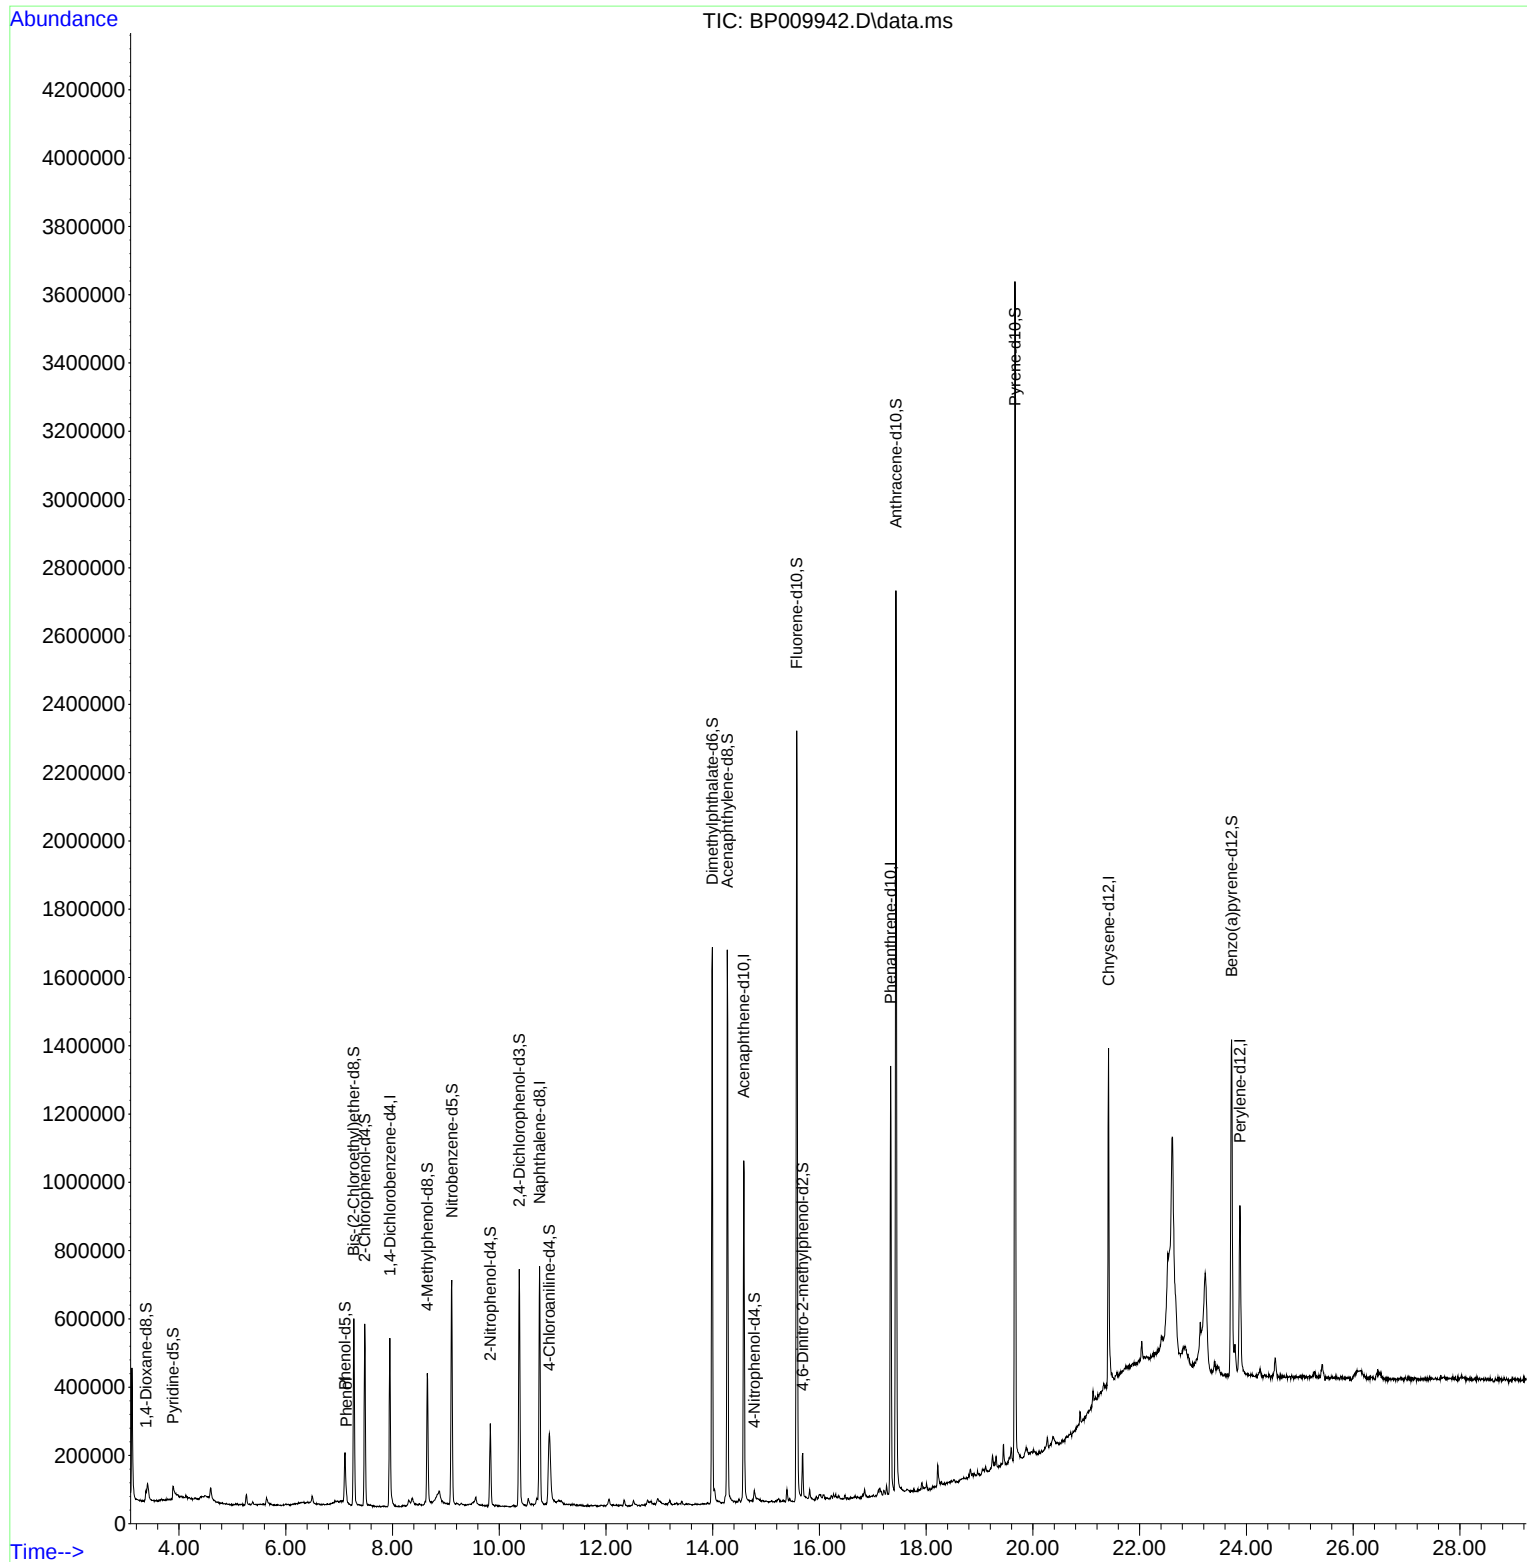

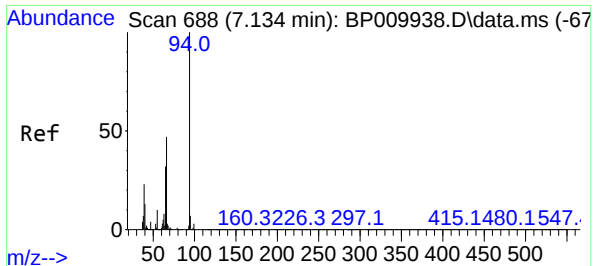

#8
Phenol
Concen: 1.221 ng/ul m
RT: 7.134 min Scan# 688
Delta R.T. -0.006 min
Lab File: BP009942.D
Acq: 19 Apr 2022 06:44

Instrument :
BNA_P
ClientSampleId :
COHX0

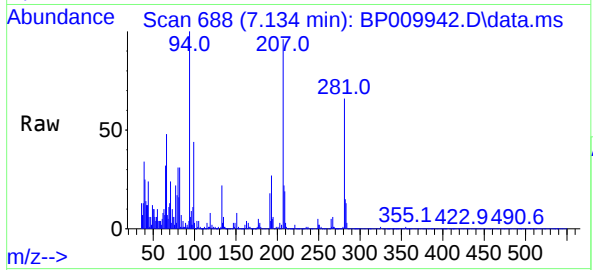

Tgt Ion: 94 Resp: 13859
Ion Ratio Lower Upper
94 100
65 32.1 19.0 28.6
66 48.0 34.6 51.8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/20/2022
Supervised By :Yogesh Patel 04/22/2022

