

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009944.D
 Acq On : 19 Apr 2022 07:51
 Operator : CG/JU
 Sample : N2422-12
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J42

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/22/2022

Quant Time: Apr 19 08:20:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 00:59:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	103344	20.000	ng/u1	0.00
20) Naphthalene-d8	10.757	136	472741	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.581	164	331254	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.334	188	701232	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.416	240	581405	20.000	ng/u1	# 0.00
88) Perylene-d12	23.880	264	469877	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	10505	4.537	ng/uL	0.00
4) Pyridine-d5	3.887	84	21138m	3.311	ng/u1	0.09
7) Phenol-d5	7.111	99	44351	4.888	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	121382	22.472	ng/u1	0.00
11) 2-Chlorophenol-d4	7.481	132	117365	17.149	ng/u1	0.00
15) 4-Methylphenol-d8	8.652	113	81959	10.821	ng/u1	-0.01
21) Nitrobenzene-d5	9.110	128	72781	21.349	ng/u1	0.00
24) 2-Nitrophenol-d4	9.834	143	45032	12.049	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.375	165	139900	17.888	ng/u1	0.00
31) 4-Chloroaniline-d4	10.904	131	155751	13.982	ng/u1	0.01
46) Dimethylphthalate-d6	13.987	166	604676	23.239	ng/u1	-0.01
49) Acenaphthylene-d8	14.275	160	615565	19.968	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.775	143	10638m	2.254	ng/u1	0.00
60) Fluorene-d10	15.575	176	504390	23.043	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	18465	4.445	ng/u1	0.00
73) Anthracene-d10	17.433	188	798223	23.775	ng/u1	0.00
81) Pyrene-d10	19.663	212	1102228	34.712	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.716	264	633520	25.890	ng/u1	-0.01
Target Compounds					Qvalue	
8) Phenol	7.134	94	16550	1.822	ng/u1#	93
78) Di-n-butylphthalate	18.286	149	156214	3.704	ng/u1#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009944.D
Acq On : 19 Apr 2022 07:51
Operator : CG/JU
Sample : N2422-12
Misc :
ALS Vial : 40 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
C0J42

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/22/2022


Quant Time: Apr 19 08:20:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 00:59:30 2022
Response via : Initial Calibration

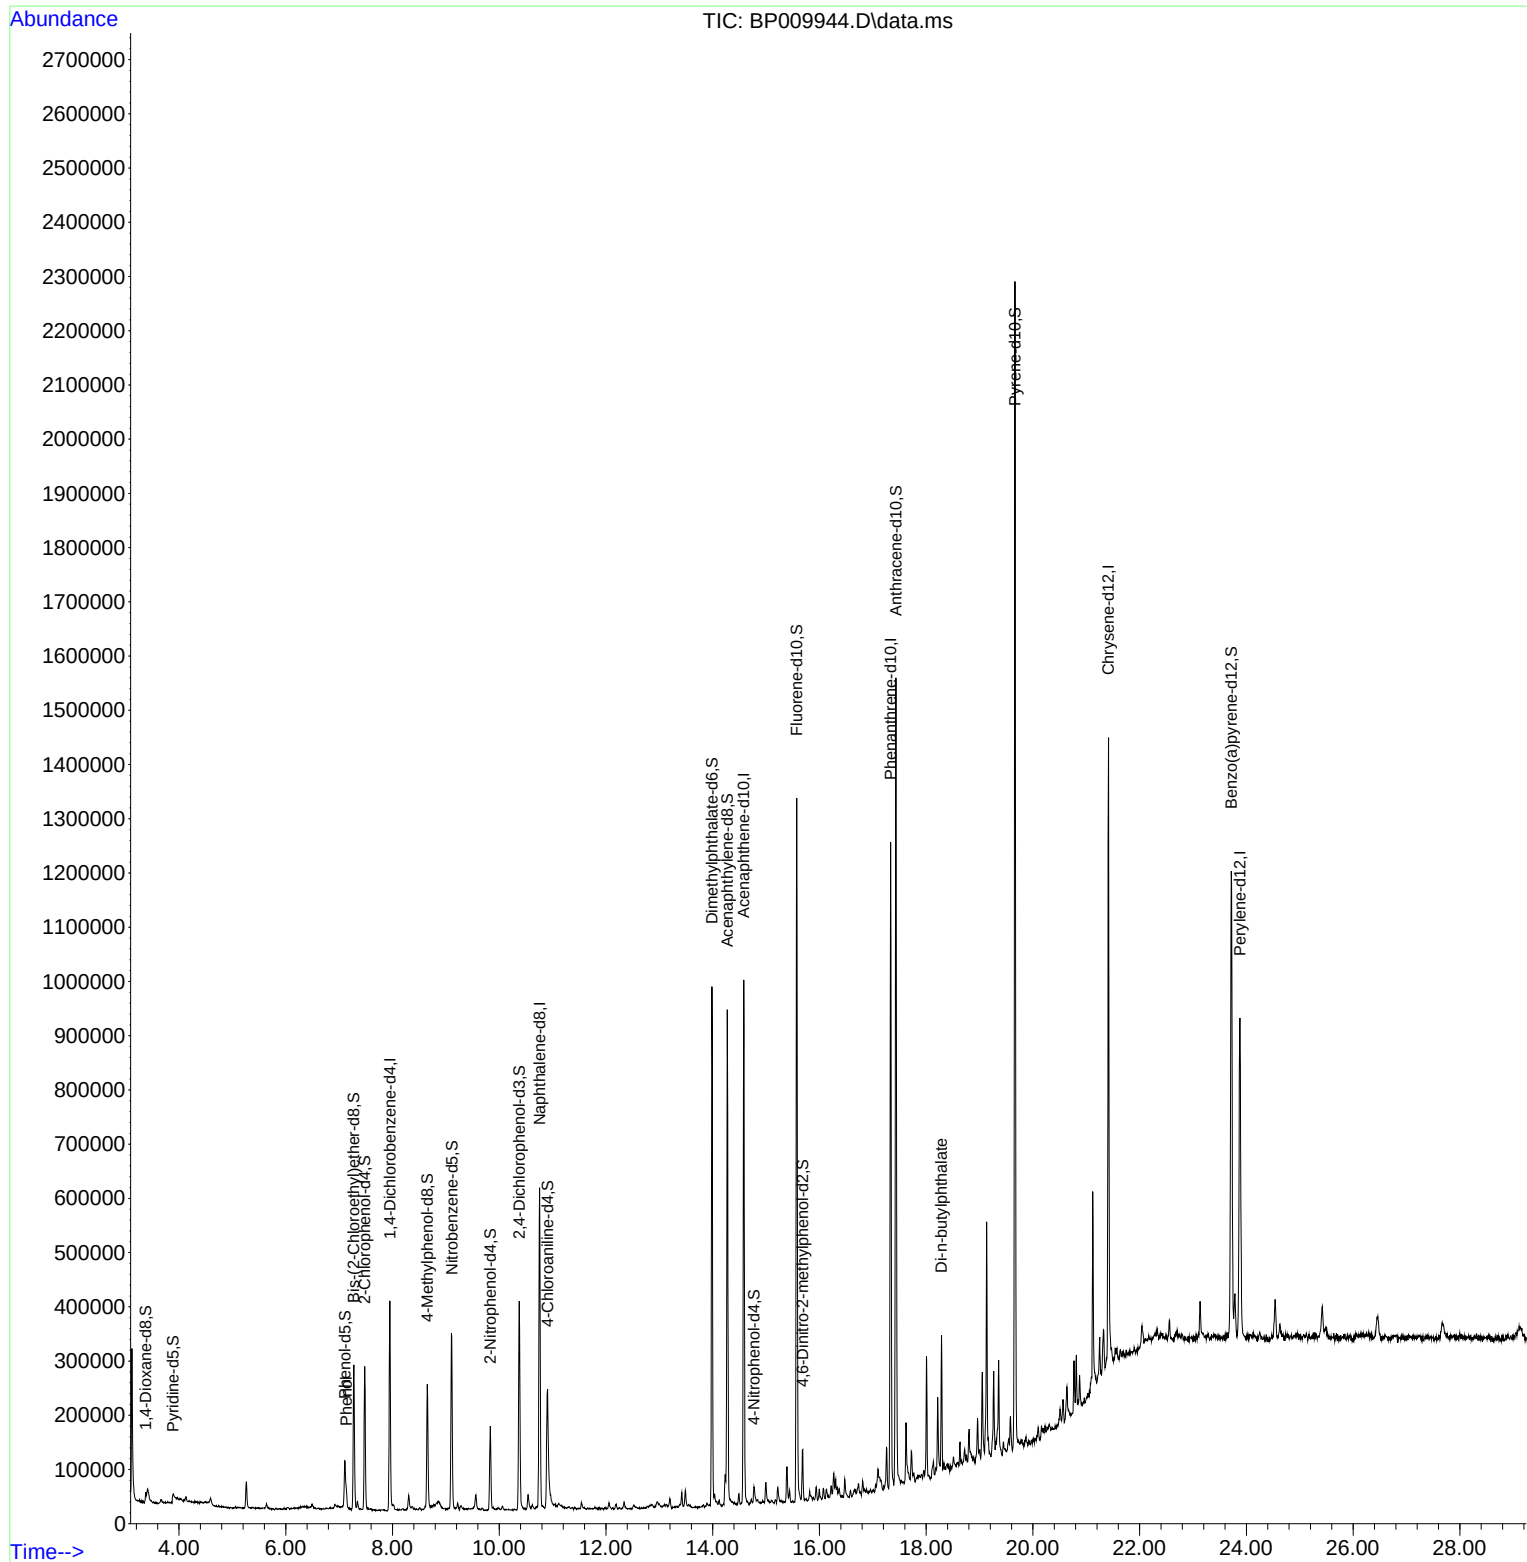

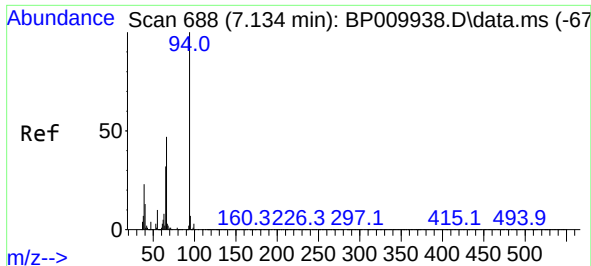

#8
Phenol
Concen: 1.822 ng/ul
RT: 7.134 min Scan# 688
Delta R.T. -0.006 min
Lab File: BP009944.D
Acq: 19 Apr 2022 07:51




Instrument :
BNA_P
ClientSampleId :
C0J42

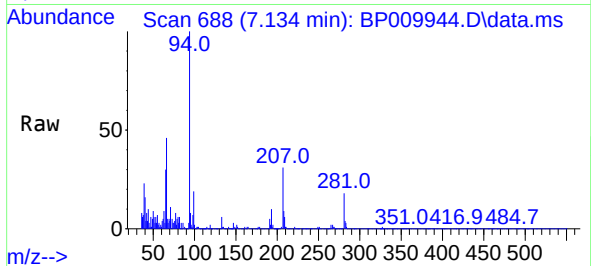


Tgt Ion: 94 Resp: 16550
Ion Ratio Lower Upper
94 100
65 29.6 19.0 28.6
66 45.6 34.6 51.8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/22/2022

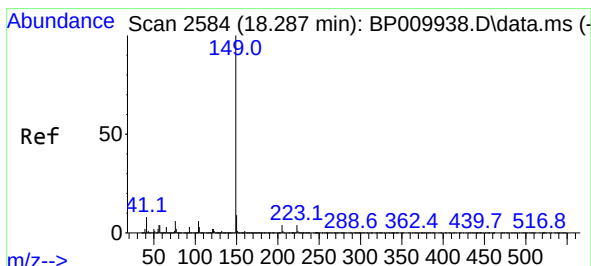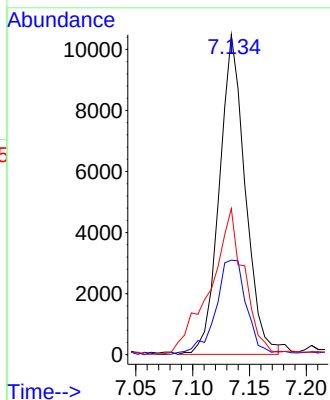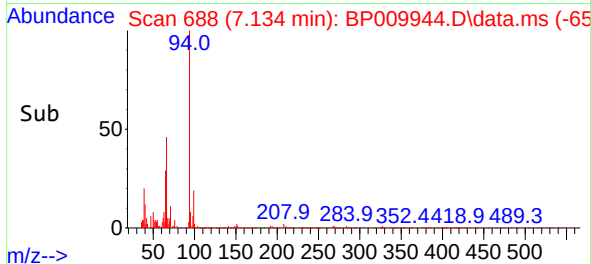

#78
Di-n-butylphthalate
Concen: 3.704 ng/ul
RT: 18.286 min Scan# 2584
Delta R.T. -0.012 min
Lab File: BP009944.D
Acq: 19 Apr 2022 07:51

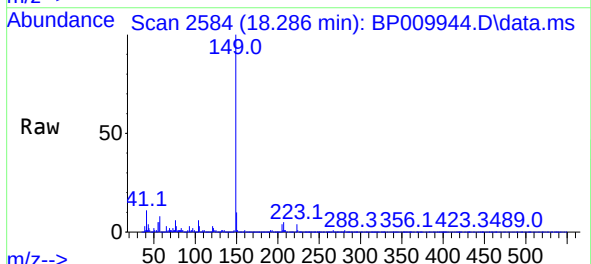

Tgt Ion:149 Resp: 156214
Ion Ratio Lower Upper
149 100
150 9.8 9.6 14.4
104 6.1 6.2 9.4

