

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009908.D
 Acq On : 18 Apr 2022 11:06
 Operator : CG/JU
 Sample : PB144126BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK126

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.123	3	6	11	rVB2	14237	18730	0.47%	0.049%
2	3.381	46	50	58	rVB	31011	47209	1.19%	0.124%
3	3.793	117	120	142	rBV	376553	696226	17.50%	1.829%
4	4.134	174	178	183	rVB2	9371	14641	0.37%	0.038%
5	7.111	677	684	695	rBV	526151	858916	21.59%	2.256%
6	7.281	705	713	725	rBV	418342	678785	17.06%	1.783%
7	7.481	737	747	757	rBV	548421	882678	22.18%	2.319%
8	7.952	819	827	838	rBV	434015	732770	18.42%	1.925%
9	8.658	939	947	958	rBV	685174	1134803	28.52%	2.981%
10	9.110	1015	1024	1035	rBV	583878	954252	23.98%	2.507%
11	9.834	1139	1147	1157	rBV	455747	766788	19.27%	2.014%
12	10.375	1231	1239	1257	rBV	704063	1181532	29.70%	3.104%
13	10.757	1297	1304	1318	rBV	634233	1108812	27.87%	2.913%
14	10.887	1318	1326	1341	rBV	712303	1277511	32.11%	3.356%
15	12.346	1568	1574	1582	rVB2	15369	26705	0.67%	0.070%
16	13.993	1847	1854	1869	rBV	1415576	2011194	50.55%	5.283%
17	14.275	1892	1902	1914	rBV	1452502	2176407	54.70%	5.717%
18	14.587	1947	1955	1963	rBV	1104582	1644394	41.33%	4.320%
19	14.763	1977	1985	1998	rBV	639689	934439	23.49%	2.455%
20	15.575	2116	2123	2136	rBV	1943105	2864640	72.00%	7.525%
21	15.687	2136	2142	2153	rBV	645818	881833	22.16%	2.317%
22	15.816	2158	2164	2170	rVB2	23836	37856	0.95%	0.099%
23	16.363	2253	2257	2261	rVB4	7839	9828	0.25%	0.026%
24	17.010	2364	2367	2372	rBV7	4043	6006	0.15%	0.016%
25	17.334	2414	2422	2432	rBV	1445737	2128909	53.51%	5.593%
26	17.434	2432	2439	2452	rVV	2268165	3275519	82.32%	8.605%
27	19.239	2742	2746	2751	rBV3	29220	38337	0.96%	0.101%
28	19.310	2754	2758	2762	rBV2	31836	40167	1.01%	0.106%
29	19.663	2812	2818	2827	rBV	3097355	3978838	100.00%	10.452%
30	21.416	3111	3116	3122	rBV	1791690	2324602	58.42%	6.107%
31	23.716	3500	3507	3515	rBV2	1680964	3309977	83.19%	8.695%
32	23.874	3527	3534	3543	rVB2	983639	2022886	50.84%	5.314%




Sum of corrected areas: 38066190

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009908.D
Acq On : 18 Apr 2022 11:06
Operator : CG/JU
Sample : PB144126BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK126

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

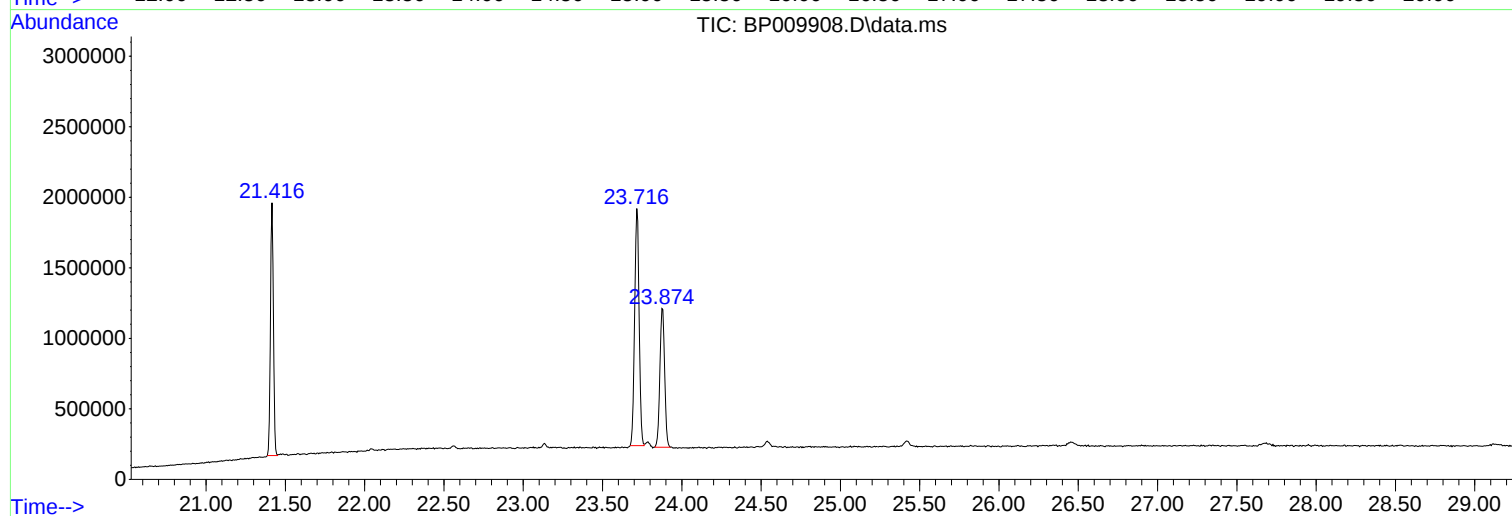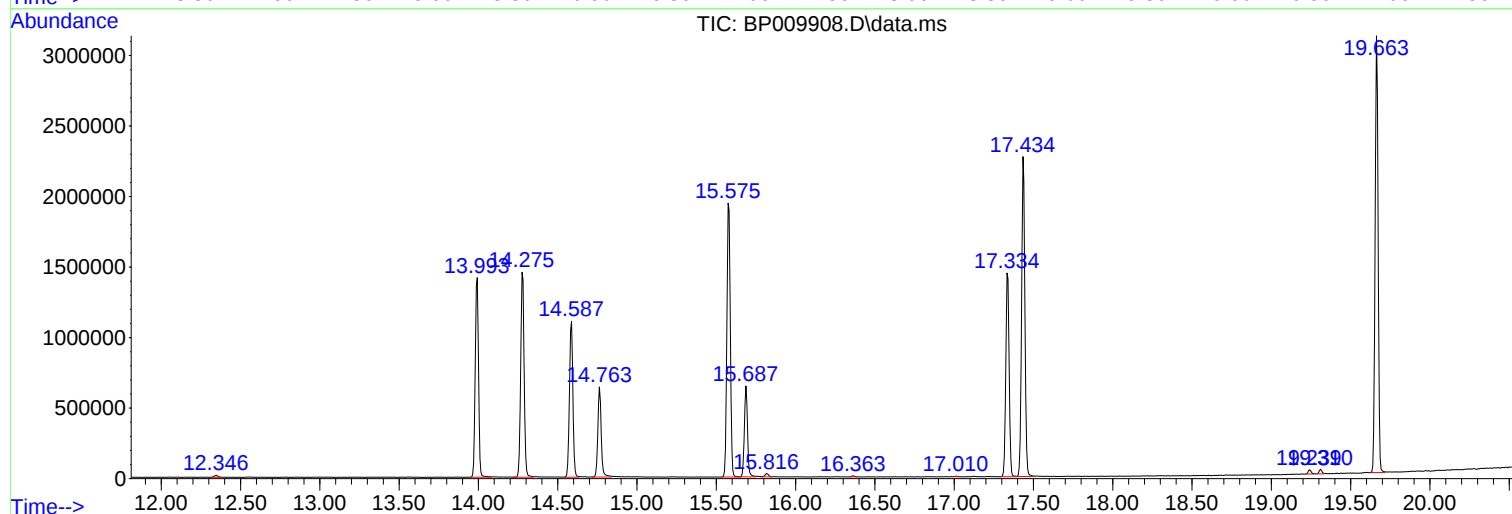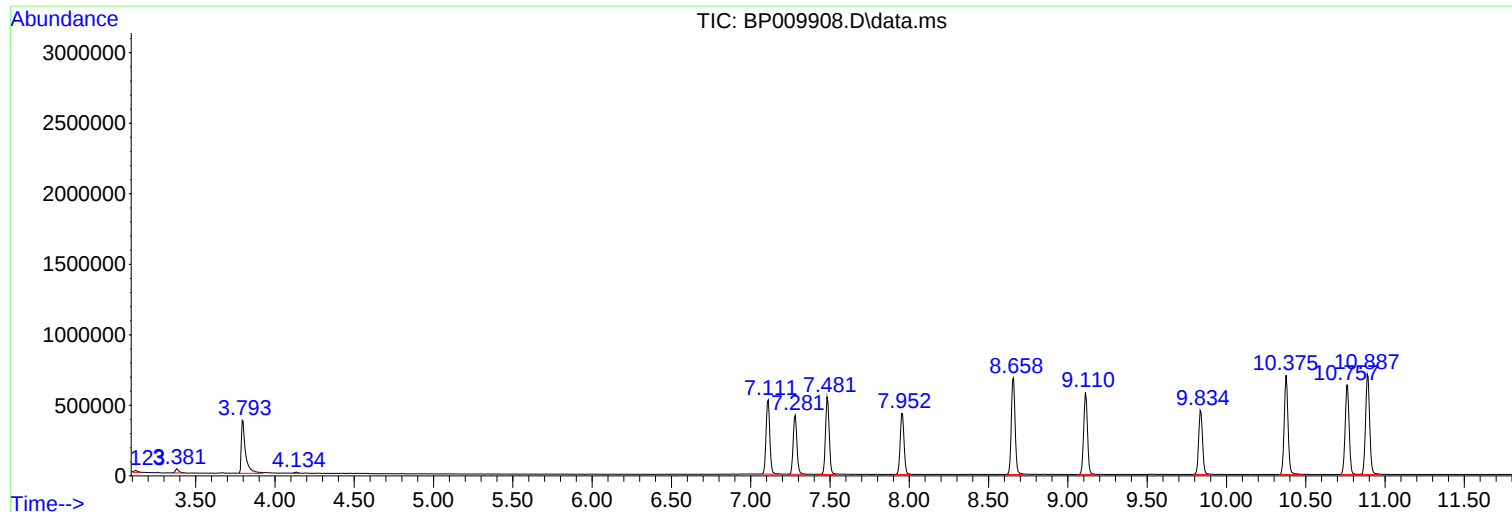

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009908.D
Acq On : 18 Apr 2022 11:06
Operator : CG/JU
Sample : PB144126BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK126

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009908.D
Acq On : 18 Apr 2022 11:06
Operator : CG/JU
Sample : PB144126BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK126

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------