

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009921.D
 Acq On : 18 Apr 2022 18:22
 Operator : CG/JU
 Sample : PB144145BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK145

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009921.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	3	5	11	rVB3	12102	17233	0.38%	0.038%
2	3.381	46	50	57	rBV	29571	43661	0.96%	0.097%
3	3.793	116	120	138	rBV	407730	727988	15.99%	1.618%
4	4.134	173	178	183	rBV3	8355	13732	0.30%	0.031%
5	7.105	676	683	696	rBV	598600	958664	21.06%	2.131%
6	7.275	704	712	725	rVB	485666	778915	17.11%	1.731%
7	7.481	740	747	756	rBV	610060	974993	21.42%	2.167%
8	7.952	820	827	841	rVB	537861	864140	18.99%	1.921%
9	8.652	938	946	963	rBV	800994	1312250	28.83%	2.917%
10	9.110	1016	1024	1034	rBV	655409	1089286	23.93%	2.421%
11	9.834	1139	1147	1158	rBV	524813	886966	19.49%	1.972%
12	10.375	1231	1239	1256	rBV	790032	1349211	29.64%	2.999%
13	10.757	1292	1304	1316	rBV	809764	1386940	30.47%	3.083%
14	10.887	1319	1326	1343	rVB	848556	1468433	32.26%	3.264%
15	12.345	1568	1574	1583	rVB	17322	29053	0.64%	0.065%
16	13.987	1846	1853	1870	rBV	1628895	2377023	52.22%	5.284%
17	14.275	1892	1902	1914	rBV	1770469	2612280	57.39%	5.807%
18	14.587	1947	1955	1968	rBV	1374433	2114755	46.46%	4.701%
19	14.763	1978	1985	1998	rBV	751122	1103196	24.24%	2.452%
20	15.398	2089	2093	2098	rBV8	3312	5750	0.13%	0.013%
21	15.575	2115	2123	2134	rBV	2366197	3405975	74.83%	7.571%
22	15.686	2134	2142	2155	rVV	748608	1072459	23.56%	2.384%
23	15.816	2159	2164	2171	rVB2	26615	44166	0.97%	0.098%
24	16.363	2251	2257	2264	rVB9	8554	16797	0.37%	0.037%
25	17.016	2364	2368	2374	rVB9	5130	7762	0.17%	0.017%
26	17.122	2377	2386	2390	rBV4	8455	16850	0.37%	0.037%
27	17.333	2415	2422	2432	rBV	1828473	2636614	57.93%	5.861%
28	17.433	2432	2439	2449	rBV	2660119	3799009	83.46%	8.445%
29	17.704	2482	2485	2487	rBV4	3817	5090	0.11%	0.011%
30	19.239	2742	2746	2751	rBV3	31462	46668	1.03%	0.104%
31	19.310	2753	2758	2762	rBV	34588	46413	1.02%	0.103%
32	19.663	2812	2818	2825	rBV	3460373	4551661	100.00%	10.118%
33	21.416	3111	3116	3125	rBV	2220049	2854469	62.71%	6.345%
34	23.721	3500	3508	3515	rBV2	1913632	3837576	84.31%	8.531%
35	23.880	3527	3535	3543	rVB	1243218	2529857	55.58%	5.624%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009921.D
Acq On : 18 Apr 2022 18:22
Operator : CG/JU
Sample : PB144145BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK145

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Title : SVOA CALIBRATION




Sum of corrected areas: 44985835

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009921.D
Acq On : 18 Apr 2022 18:22
Operator : CG/JU
Sample : PB144145BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK145

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

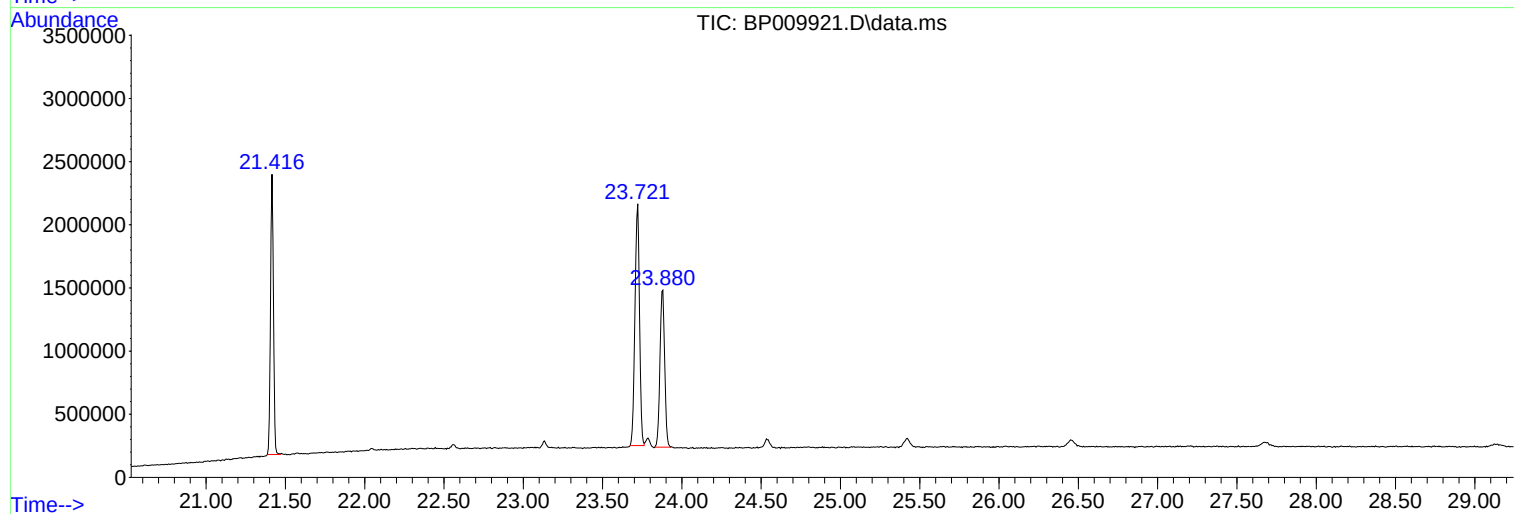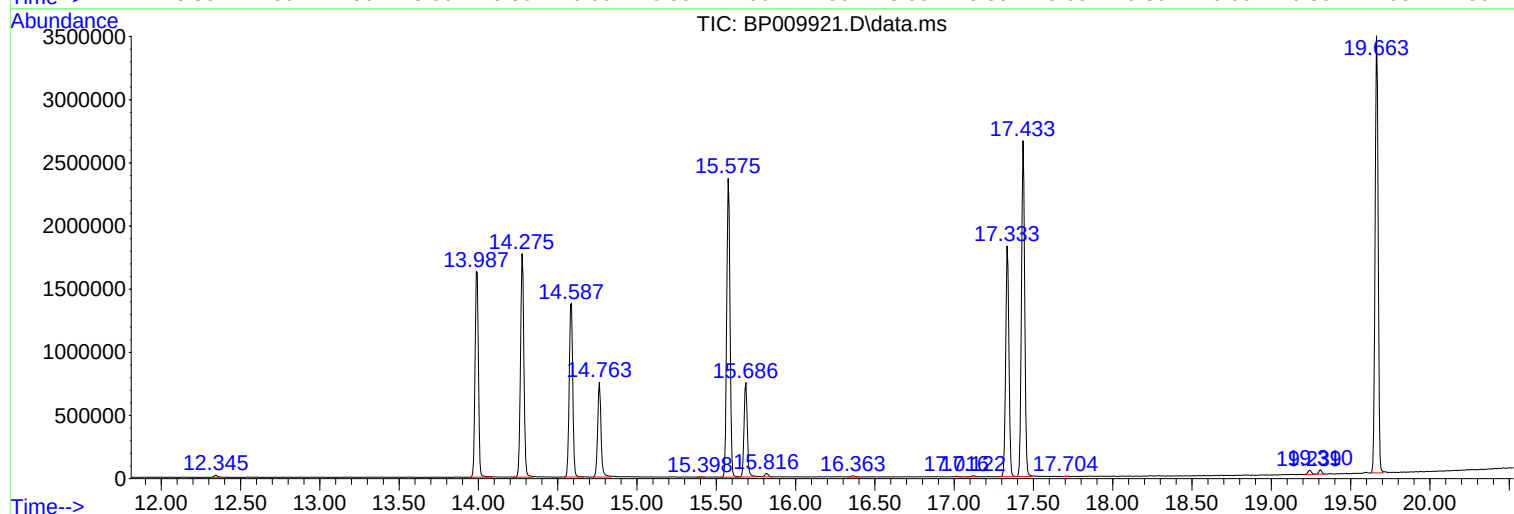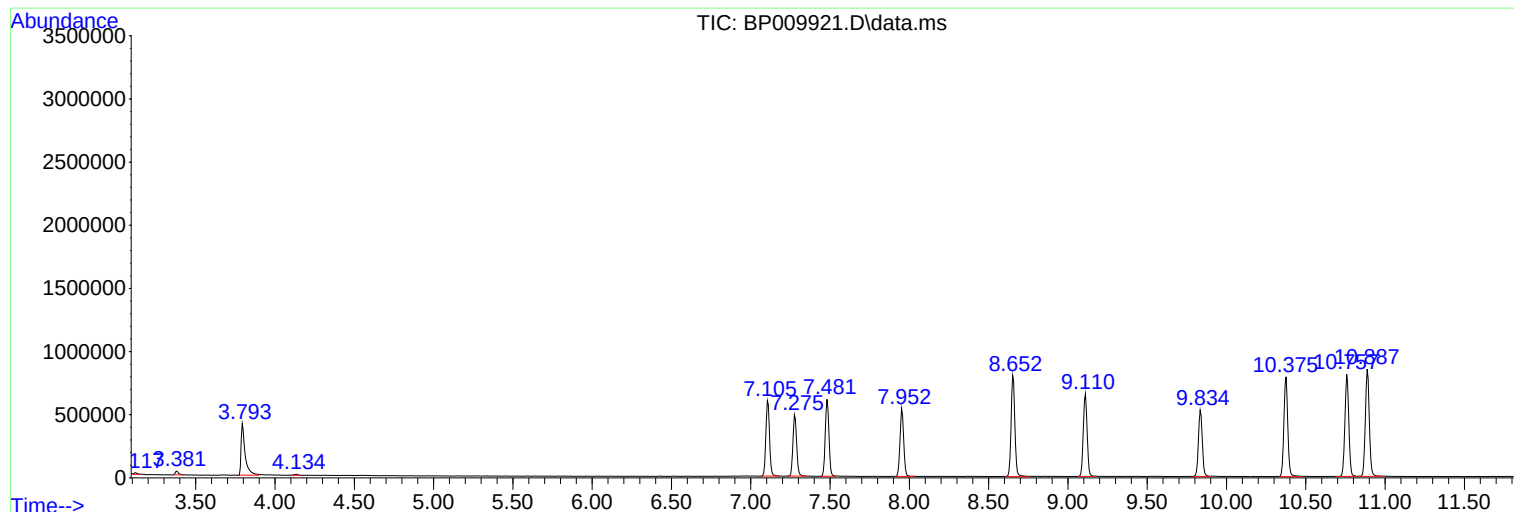

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009921.D
Acq On : 18 Apr 2022 18:22
Operator : CG/JU
Sample : PB144145BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK145

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009921.D
Acq On : 18 Apr 2022 18:22
Operator : CG/JU
Sample : PB144145BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK145

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------