

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009927.D
 Acq On : 18 Apr 2022 21:44
 Operator : CG/JU
 Sample : N2421-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	3	5	18	rVB	268505	371802	7.41%	0.944%
2	3.381	46	50	55	rBV	22485	33377	0.67%	0.085%
3	3.658	95	97	105	rBV9	2873	5661	0.11%	0.014%
4	3.811	120	123	131	rBV2	25723	52194	1.04%	0.133%
5	4.134	174	178	184	rVB5	7662	12167	0.24%	0.031%
6	5.263	364	370	376	rVB3	13066	22282	0.44%	0.057%
7	5.387	387	391	396	rVB8	4230	6532	0.13%	0.017%
8	6.981	656	662	666	rVB2	8559	15504	0.31%	0.039%
9	7.105	674	683	695	rBV	142449	253556	5.05%	0.644%
10	7.275	705	712	727	rBV	432273	714121	14.23%	1.814%
11	7.481	740	747	761	rBV	462487	743154	14.81%	1.888%
12	7.952	820	827	838	rBV	396652	662503	13.20%	1.683%
13	8.310	883	888	893	rVB3	9241	15466	0.31%	0.039%
14	8.652	938	946	958	rBV	423528	677007	13.49%	1.720%
15	9.110	1016	1024	1032	rBV	593526	1008640	20.10%	2.562%
16	9.569	1095	1102	1107	rBV6	5635	10229	0.20%	0.026%
17	9.834	1138	1147	1159	rBV	487361	808181	16.10%	2.053%
18	10.375	1230	1239	1256	rBV	694748	1187804	23.67%	3.017%
19	10.540	1262	1267	1276	rBV	29639	58091	1.16%	0.148%
20	10.757	1297	1304	1316	rBV	580538	1032724	20.58%	2.623%
21	10.887	1319	1326	1337	rVV	224212	397163	7.91%	1.009%
22	11.716	1459	1467	1472	rBV	3320	7579	0.15%	0.019%
23	12.340	1569	1573	1580	rVB	15133	25521	0.51%	0.065%
24	12.775	1643	1647	1651	rBV6	3655	6467	0.13%	0.016%
25	12.963	1674	1679	1680	rBV5	3470	5520	0.11%	0.014%
26	12.992	1680	1684	1694	rVB5	17339	31313	0.62%	0.080%
27	13.204	1715	1720	1725	rBV3	9507	14313	0.29%	0.036%
28	13.251	1725	1728	1734	rBV8	3446	6507	0.13%	0.017%
29	13.428	1752	1758	1761	rBV7	5263	8043	0.16%	0.020%
30	13.492	1764	1769	1776	rVB7	3791	7137	0.14%	0.018%
31	13.557	1776	1780	1787	rBV10	2486	5760	0.11%	0.015%
32	13.992	1847	1854	1864	rBV	1552485	2253980	44.91%	5.726%
33	14.122	1871	1876	1881	rVB8	7332	11376	0.23%	0.029%
34	14.234	1890	1895	1896	rBV2	28073	34260	0.68%	0.087%
35	14.275	1896	1902	1915	rVB	1630443	2428005	48.38%	6.168%
36	14.492	1936	1939	1944	rVB4	5037	6111	0.12%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009927.D
 Acq On : 18 Apr 2022 21:44
 Operator : CG/JU
 Sample : N2421-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

37	14.581	1947	1954	1965	rBV	980849	1467085	29.23%	3.727%
38	14.763	1978	1985	1995	rBV	158223	260199	5.18%	0.661%
39	14.904	2005	2009	2013	rBV7	4298	6879	0.14%	0.017%
40	14.987	2019	2023	2028	rVB8	3821	7172	0.14%	0.018%
41	15.222	2058	2063	2069	rBV5	9700	21816	0.43%	0.055%
42	15.398	2087	2093	2098	rBV2	19596	33942	0.68%	0.086%
43	15.445	2098	2101	2107	rVB8	7038	9815	0.20%	0.025%
44	15.575	2116	2123	2132	rBV	2307677	3310060	65.95%	8.408%
45	15.686	2135	2142	2150	rBV	862366	1229492	24.50%	3.123%
46	15.816	2160	2164	2171	rVB2	25913	39656	0.79%	0.101%
47	15.939	2180	2185	2191	rBV9	6553	12291	0.24%	0.031%
48	16.004	2191	2196	2204	rBV9	4676	9255	0.18%	0.024%
49	16.145	2214	2220	2225	rBV9	4254	8918	0.18%	0.023%
50	16.222	2229	2233	2236	rVB6	4652	5516	0.11%	0.014%
51	16.263	2236	2240	2243	rBV5	12895	16823	0.34%	0.043%
52	16.363	2254	2257	2264	rVB5	13100	21140	0.42%	0.054%
53	16.475	2272	2276	2281	rBV4	10367	16252	0.32%	0.041%
54	16.663	2301	2308	2311	rBV9	3599	9039	0.18%	0.023%
55	16.816	2330	2334	2337	rBV6	8648	12277	0.24%	0.031%
56	17.016	2365	2368	2372	rBV5	4595	7874	0.16%	0.020%
57	17.104	2378	2383	2389	rBV7	12010	26788	0.53%	0.068%
58	17.151	2389	2391	2397	rVB6	6703	9145	0.18%	0.023%
59	17.263	2405	2410	2413	rBV	24299	29657	0.59%	0.075%
60	17.333	2416	2422	2432	rVV	1275220	1851190	36.88%	4.703%
61	17.433	2432	2439	2454	rVV	2937033	4168069	83.05%	10.588%
62	17.645	2472	2475	2481	rBV8	5950	10612	0.21%	0.027%
63	18.004	2533	2536	2541	rVB4	15922	21856	0.44%	0.056%
64	18.216	2568	2572	2580	rBV4	39630	60466	1.20%	0.154%
65	18.510	2619	2622	2624	rBV4	6964	9452	0.19%	0.024%
66	19.239	2742	2746	2750	rBV4	39989	53999	1.08%	0.137%
67	19.275	2750	2752	2754	rVV3	10541	12313	0.25%	0.031%
68	19.310	2754	2758	2762	rVB	35485	47960	0.96%	0.122%
69	19.663	2812	2818	2829	rBV	3825501	5018845	100.00%	12.749%
70	21.121	3063	3066	3073	rBV3	103072	148850	2.97%	0.378%
71	21.416	3111	3116	3122	rBV	1670168	2060399	41.05%	5.234%
72	23.715	3500	3507	3515	rBV2	2255639	4468021	89.02%	11.350%
73	23.874	3527	3534	3545	rVB2	924374	1922753	38.31%	4.884%




Sum of corrected areas: 39365926

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009927.D
Acq On : 18 Apr 2022 21:44
Operator : CG/JU
Sample : N2421-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

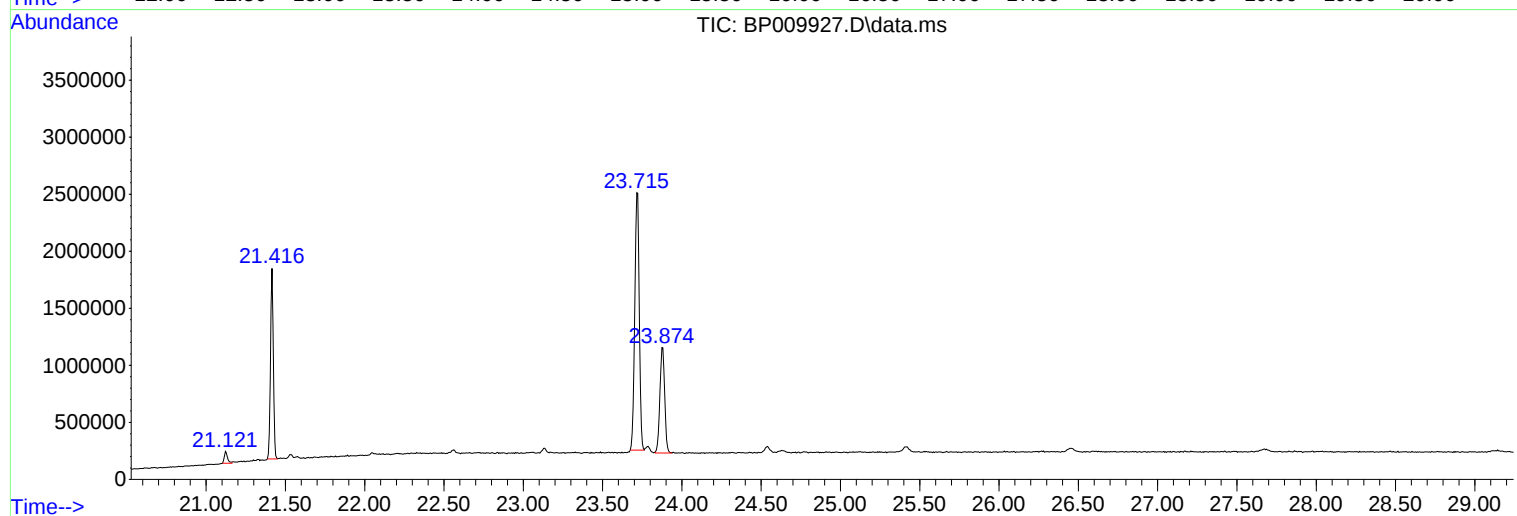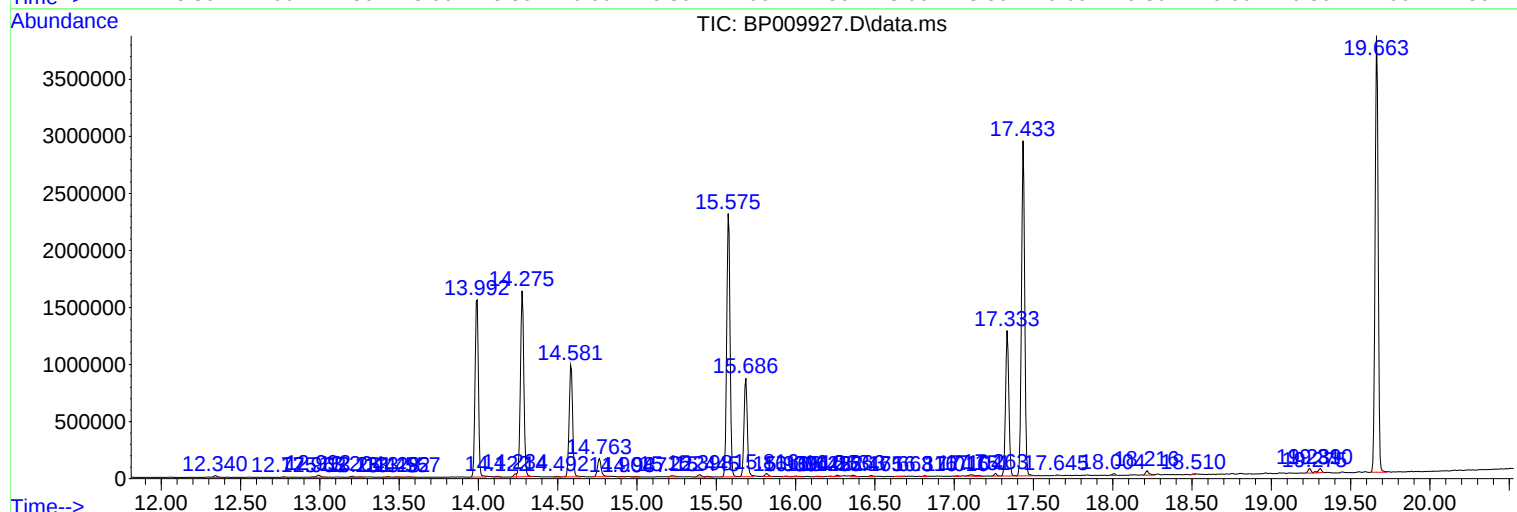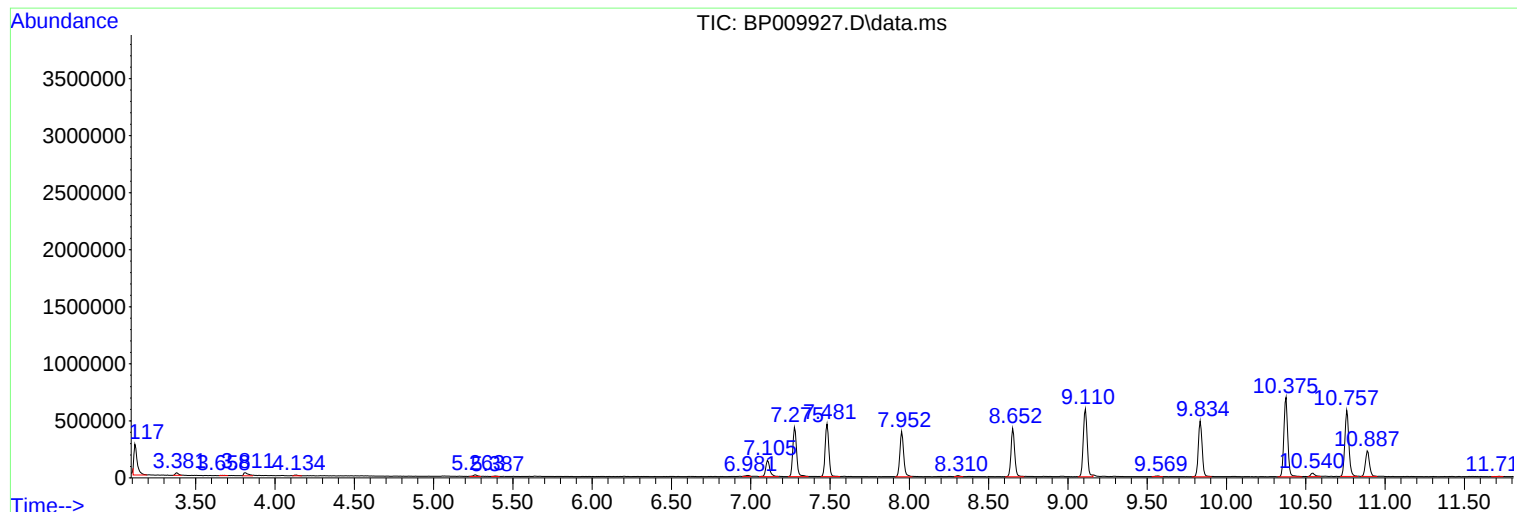

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009927.D
Acq On : 18 Apr 2022 21:44
Operator : CG/JU
Sample : N2421-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J72










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.117	11.22 ng/ul	371802	1,4-Dichlorobenzene-d4	7.952

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	35
5			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	33

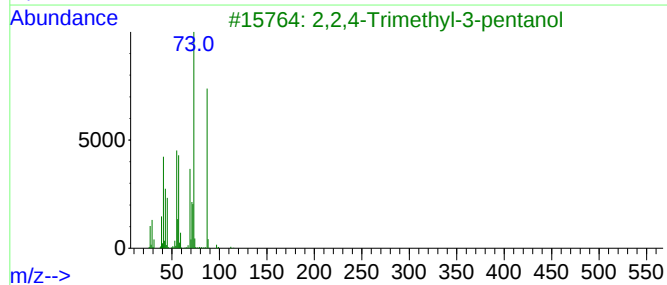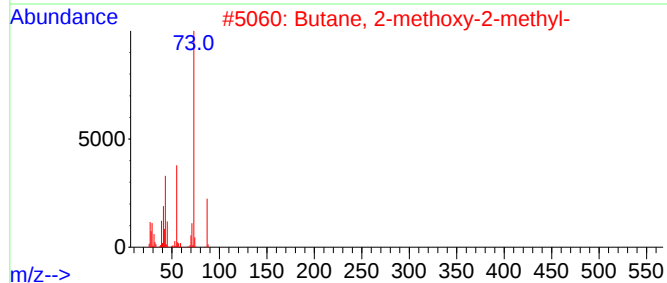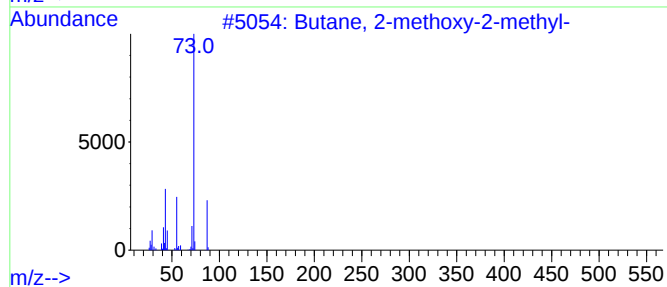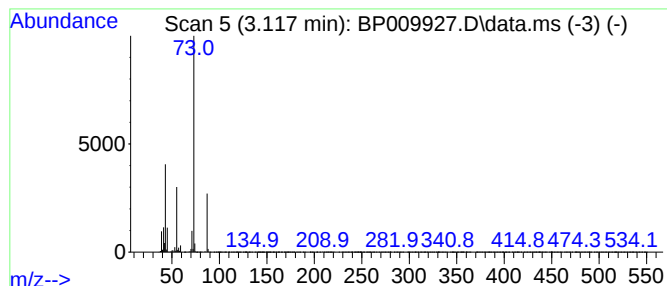

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009927.D
Acq On : 18 Apr 2022 21:44
Operator : CG/JU
Sample : N2421-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.117	11.2	ng/u1	371802	1	7.952	662503	20.0