

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009929.D
 Acq On : 18 Apr 2022 22:52
 Operator : CG/JU
 Sample : N2421-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009929.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	3	5	18	rVB	363527	476989	9.41%	1.148%
2	3.375	46	49	55	rBV	24653	32115	0.63%	0.077%
3	3.799	118	121	131	rBV	111758	183922	3.63%	0.443%
4	4.128	173	177	182	rBV2	9489	14631	0.29%	0.035%
5	5.258	366	369	374	rBV5	4543	6002	0.12%	0.014%
6	7.105	676	683	694	rVB2	137323	266109	5.25%	0.641%
7	7.275	703	712	721	rBV	460654	736427	14.53%	1.773%
8	7.481	740	747	755	rBV	481116	754525	14.88%	1.816%
9	7.952	820	827	836	rBV	463937	744038	14.68%	1.791%
10	8.310	881	888	893	rBV9	5160	11777	0.23%	0.028%
11	8.651	936	946	958	rBV	400569	644542	12.71%	1.551%
12	8.769	964	966	974	rVB7	3577	5771	0.11%	0.014%
13	9.110	1010	1024	1033	rBV	616801	1045694	20.63%	2.517%
14	9.228	1037	1044	1047	rVV8	2806	7247	0.14%	0.017%
15	9.287	1049	1054	1061	rVB10	5014	9595	0.19%	0.023%
16	9.563	1094	1101	1107	rVB5	12270	23907	0.47%	0.058%
17	9.834	1137	1147	1156	rBV	487489	820267	16.18%	1.974%
18	10.075	1182	1188	1191	rBV7	2613	5977	0.12%	0.014%
19	10.369	1231	1238	1252	rBV	674141	1182743	23.33%	2.847%
20	10.540	1261	1267	1276	rBV	47448	93974	1.85%	0.226%
21	10.757	1295	1304	1314	rBV	657598	1125677	22.20%	2.710%
22	10.887	1319	1326	1339	rVV	613460	1047531	20.66%	2.521%
23	12.063	1520	1526	1530	rBV8	3060	5137	0.10%	0.012%
24	12.281	1558	1563	1568	rVV	14251	22463	0.44%	0.054%
25	12.345	1568	1574	1580	rVB3	16187	28959	0.57%	0.070%
26	12.957	1672	1678	1682	rBV6	5210	8503	0.17%	0.020%
27	13.098	1695	1702	1706	rBV10	2692	5930	0.12%	0.014%
28	13.198	1715	1719	1725	rVB2	9394	13686	0.27%	0.033%
29	13.392	1746	1752	1755	rBV3	19333	31646	0.62%	0.076%
30	13.422	1755	1757	1763	rVB2	10274	12727	0.25%	0.031%
31	13.551	1775	1779	1782	rBV6	4186	6836	0.13%	0.016%
32	13.587	1782	1785	1793	rVB2	8615	15097	0.30%	0.036%
33	13.987	1846	1853	1867	rBV	1627318	2249951	44.38%	5.416%
34	14.116	1871	1875	1880	rVB8	4595	8755	0.17%	0.021%
35	14.234	1890	1895	1896	rBV2	27506	35942	0.71%	0.087%
36	14.275	1896	1902	1912	rVB	1623000	2415102	47.64%	5.813%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009929.D
 Acq On : 18 Apr 2022 22:52
 Operator : CG/JU
 Sample : N2421-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

37	14.492	1935	1939	1943	rVB4	6434	10166	0.20%	0.024%
38	14.581	1947	1954	1965	rBV	1112808	1627209	32.10%	3.917%
39	14.763	1976	1985	1994	rBV2	130801	223888	4.42%	0.539%
40	14.828	1994	1996	2002	rVB7	4880	7153	0.14%	0.017%
41	15.222	2058	2063	2068	rVB2	12634	20403	0.40%	0.049%
42	15.392	2083	2092	2096	rBV2	38166	62308	1.23%	0.150%
43	15.439	2098	2100	2105	rVB4	9536	10282	0.20%	0.025%
44	15.575	2116	2123	2134	rBV	2380723	3404510	67.16%	8.195%
45	15.686	2135	2142	2150	rBV	854289	1204673	23.76%	2.900%
46	15.816	2158	2164	2169	rBV	26784	40407	0.80%	0.097%
47	15.939	2179	2185	2190	rBV8	8551	14528	0.29%	0.035%
48	15.998	2192	2195	2196	rBV3	6995	7237	0.14%	0.017%
49	16.128	2213	2217	2225	rBV10	4669	10827	0.21%	0.026%
50	16.216	2229	2232	2236	rVV6	6619	10186	0.20%	0.025%
51	16.263	2236	2240	2244	rVV6	13625	23545	0.46%	0.057%
52	16.304	2244	2247	2250	rVV5	12530	16900	0.33%	0.041%
53	16.357	2253	2256	2262	rVB6	11726	20136	0.40%	0.048%
54	16.475	2271	2276	2280	rBV3	10438	16995	0.34%	0.041%
55	16.645	2302	2305	2309	rBV6	2813	5652	0.11%	0.014%
56	16.810	2329	2333	2337	rVB7	7024	10700	0.21%	0.026%
57	16.875	2341	2344	2348	rVB5	6673	9730	0.19%	0.023%
58	17.016	2364	2368	2371	rBV6	5421	6155	0.12%	0.015%
59	17.104	2379	2383	2388	rBV3	11179	21293	0.42%	0.051%
60	17.157	2389	2392	2399	rVB8	8684	11055	0.22%	0.027%
61	17.263	2406	2410	2415	rVB	28032	37835	0.75%	0.091%
62	17.333	2415	2422	2432	rBV	1464133	2069342	40.82%	4.981%
63	17.433	2432	2439	2451	rVV	3072911	4198069	82.81%	10.105%
64	17.522	2451	2454	2460	rVB8	8134	14820	0.29%	0.036%
65	18.004	2533	2536	2541	rVB3	18372	23545	0.46%	0.057%
66	18.127	2551	2557	2563	rBV10	6708	18158	0.36%	0.044%
67	18.216	2568	2572	2578	rVV2	70123	98609	1.95%	0.237%
68	18.280	2580	2583	2588	rVB4	13608	22850	0.45%	0.055%
69	18.510	2619	2622	2624	rBV3	9070	10175	0.20%	0.024%
70	18.751	2661	2663	2667	rVB5	7540	8341	0.16%	0.020%
71	18.963	2696	2699	2701	rBV3	8402	9761	0.19%	0.023%
72	19.045	2711	2713	2717	rBV5	12960	16868	0.33%	0.041%
73	19.116	2723	2725	2731	rVB6	9723	13838	0.27%	0.033%
74	19.239	2742	2746	2750	rBV	43470	54807	1.08%	0.132%
75	19.310	2754	2758	2764	rVB	39995	59012	1.16%	0.142%
76	19.445	2778	2781	2787	rBV7	12368	17264	0.34%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009929.D
Acq On : 18 Apr 2022 22:52
Operator : CG/JU
Sample : N2421-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J56

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Title : SVOA CALIBRATION

77	19.663	2812	2818	2829	rBV	3903627	5069550	100.00%	12.203%
78	21.121	3062	3066	3073	rBV	142380	200738	3.96%	0.483%
79	21.416	3110	3116	3122	rBV	1690577	2282082	45.02%	5.493%
80	23.715	3499	3507	3515	rBV2	2190579	4385481	86.51%	10.556%

81	23.874	3527	3534	3544	rVB2	981553	2036773	40.18%	4.903%
----	--------	------	------	------	------	--------	---------	--------	--------




Sum of corrected areas: 41544050

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009929.D
Acq On : 18 Apr 2022 22:52
Operator : CG/JU
Sample : N2421-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

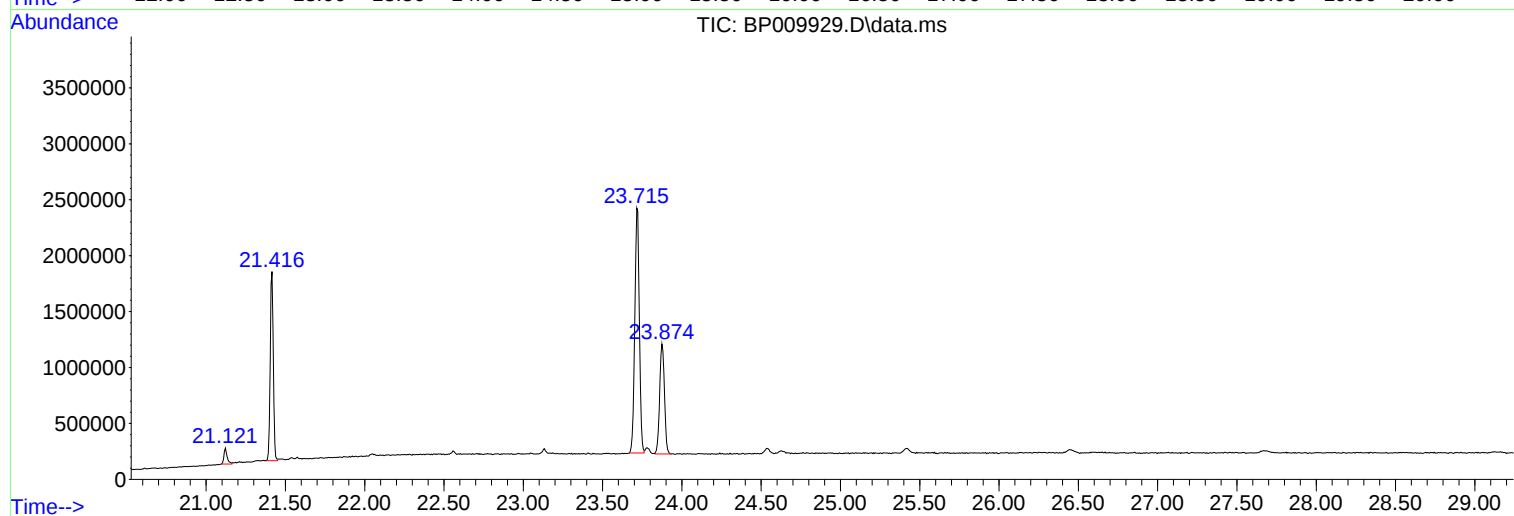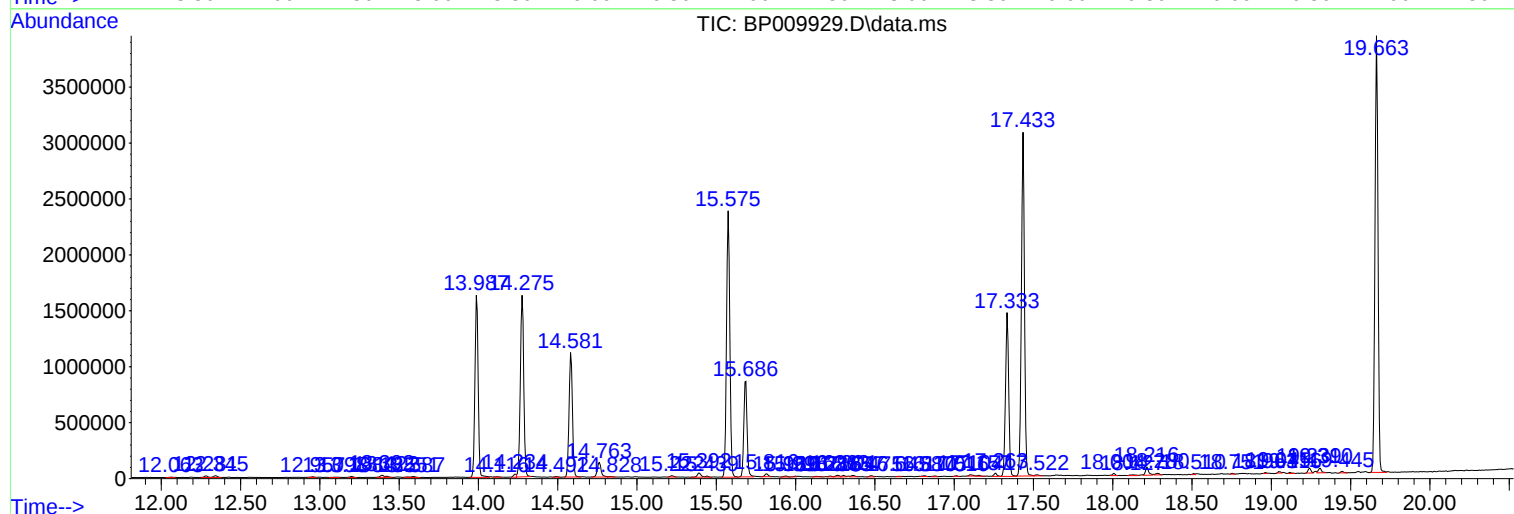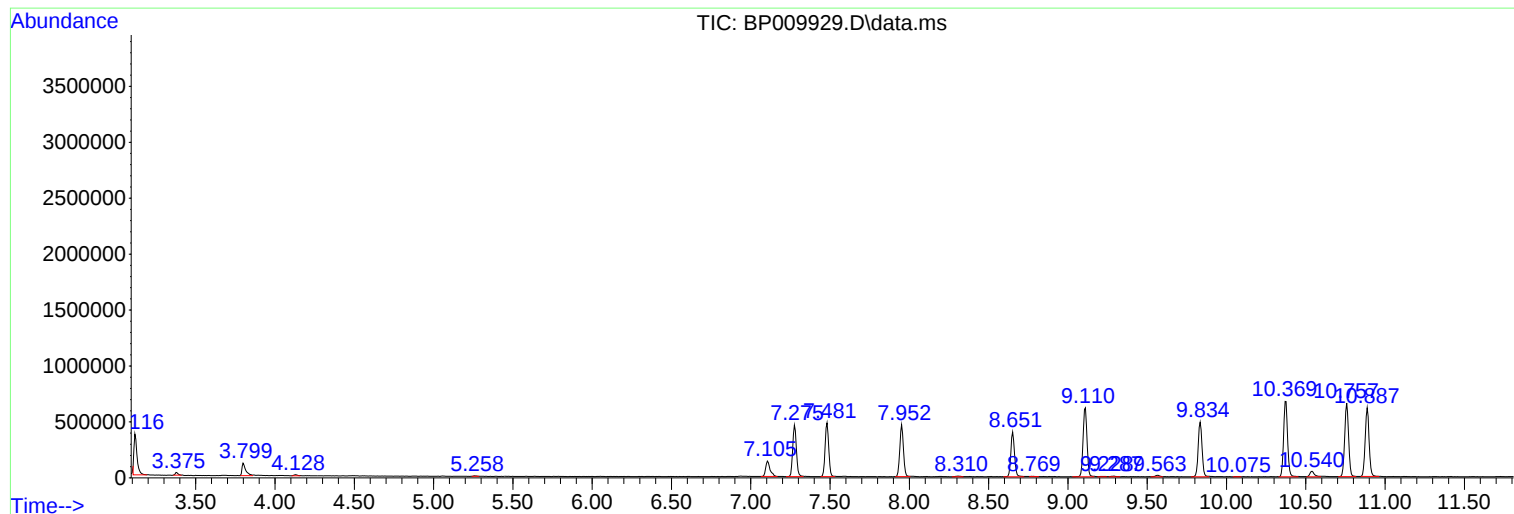

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009929.D
Acq On : 18 Apr 2022 22:52
Operator : CG/JU
Sample : N2421-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J56










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.116	12.82 ng/ul	476989	1,4-Dichlorobenzene-d4	7.952

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
4			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	32
5			1,3-Dioxolane, 2-propyl-	116	C6H12O2	003390-13-4	23

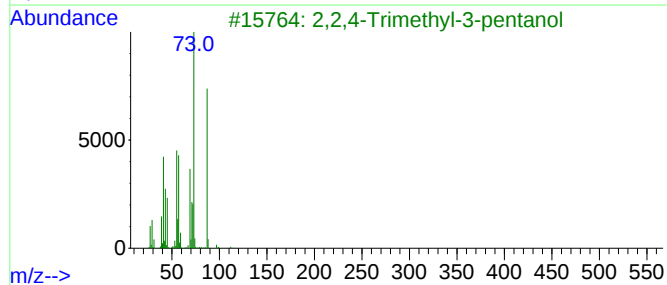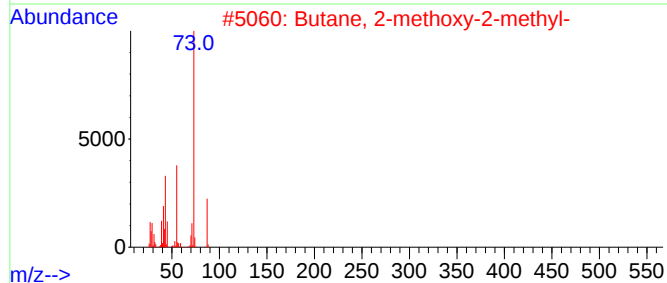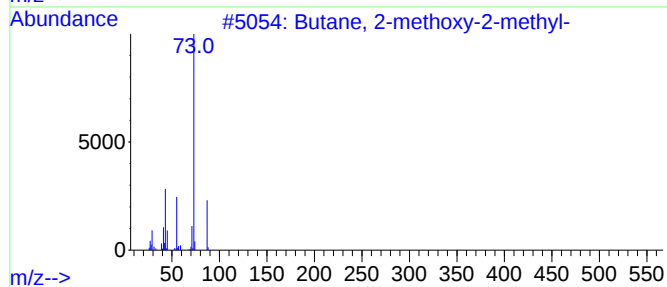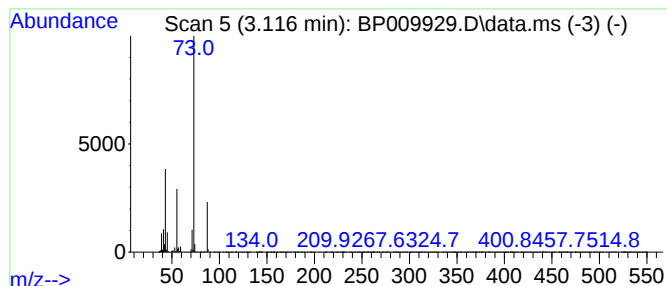

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009929.D
Acq On : 18 Apr 2022 22:52
Operator : CG/JU
Sample : N2421-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.116	12.8	ng/ul	476989	1	7.952	744038	20.0