

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009942.D
 Acq On : 19 Apr 2022 06:44
 Operator : CG/JU
 Sample : N2421-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COHX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	3	5	17	rVB	384964	511336	10.80%	1.442%
2	3.381	45	50	51	rBV2	32297	38138	0.81%	0.108%
3	3.410	51	55	69	rVB2	50010	125661	2.65%	0.354%
4	3.887	132	136	144	rBV	39971	101482	2.14%	0.286%
5	4.128	175	177	180	rBV4	7915	7017	0.15%	0.020%
6	4.416	220	226	227	rBV5	8400	14377	0.30%	0.041%
7	4.593	251	256	268	rVB2	37262	84840	1.79%	0.239%
8	5.263	365	370	376	rBV	30291	50503	1.07%	0.142%
9	5.381	384	390	394	rBV9	10040	18173	0.38%	0.051%
10	5.640	429	434	444	rBV3	21473	50517	1.07%	0.142%
11	6.004	489	496	498	rBV8	5108	8615	0.18%	0.024%
12	6.046	499	503	508	rVB8	3876	7199	0.15%	0.020%
13	6.493	574	579	586	rVB3	22587	42899	0.91%	0.121%
14	6.598	594	597	602	rBV7	3750	6518	0.14%	0.018%
15	6.922	649	652	654	rBV4	6063	6154	0.13%	0.017%
16	7.069	674	677	678	rVV3	4866	5374	0.11%	0.015%
17	7.110	678	684	693	rVB2	147045	279605	5.91%	0.788%
18	7.275	706	712	724	rVB	546225	862087	18.21%	2.431%
19	7.481	740	747	756	rBV	532320	858997	18.15%	2.422%
20	7.581	762	764	772	rVB9	6860	14692	0.31%	0.041%
21	7.951	819	827	844	rBV	494548	853478	18.03%	2.406%
22	8.216	869	872	875	rVB4	4272	5389	0.11%	0.015%
23	8.304	880	887	893	rVV7	17249	44336	0.94%	0.125%
24	8.369	893	898	910	rVB2	20078	56470	1.19%	0.159%
25	8.610	936	939	941	rVV4	9260	11723	0.25%	0.033%
26	8.651	941	946	956	rVB	379990	634771	13.41%	1.790%
27	8.934	993	994	998	rVB4	6171	6438	0.14%	0.018%
28	9.110	1016	1024	1037	rVB	657317	1105830	23.36%	3.118%
29	9.287	1050	1054	1059	rBV8	4214	6370	0.13%	0.018%
30	9.510	1087	1092	1093	rBV5	5689	9305	0.20%	0.026%
31	9.528	1093	1095	1096	rVV2	8634	8439	0.18%	0.024%
32	9.563	1096	1101	1110	rVB6	23022	47177	1.00%	0.133%
33	9.834	1139	1147	1155	rBV	242831	414147	8.75%	1.168%
34	9.939	1161	1165	1168	rBV6	4267	6702	0.14%	0.019%
35	10.269	1216	1221	1222	rVB4	4270	5581	0.12%	0.016%
36	10.375	1229	1239	1254	rBV	694997	1243789	26.28%	3.507%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009942.D
 Acq On : 19 Apr 2022 06:44
 Operator : CG/JU
 Sample : N2421-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COHX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

37	10.545	1262	1268	1275	rBV3	21446	47118	1.00%	0.133%
38	10.704	1289	1295	1298	rBV4	17572	34882	0.74%	0.098%
39	10.757	1298	1304	1318	rVB	697981	1186240	25.06%	3.345%
40	10.939	1326	1335	1348	rBV2	205927	634595	13.41%	1.789%
41	11.116	1357	1365	1369	rBV2	7618	17421	0.37%	0.049%
42	11.310	1396	1398	1402	rVB5	3804	5112	0.11%	0.014%
43	12.057	1515	1525	1532	rBV2	20927	55947	1.18%	0.158%
44	12.339	1569	1573	1580	rBV2	17921	32355	0.68%	0.091%
45	12.516	1598	1603	1610	rBV5	14675	29109	0.61%	0.082%
46	12.675	1626	1630	1632	rBV5	3996	6867	0.15%	0.019%
47	12.780	1643	1648	1651	rBV5	13411	23934	0.51%	0.067%
48	12.969	1673	1680	1685	rBV7	18531	48445	1.02%	0.137%
49	13.180	1712	1716	1717	rBV4	6666	9637	0.20%	0.027%
50	13.198	1717	1719	1724	rVB6	12772	14204	0.30%	0.040%
51	13.422	1754	1757	1760	rBV5	8764	11535	0.24%	0.033%
52	13.898	1834	1838	1839	rBV4	4165	4736	0.10%	0.013%
53	13.992	1846	1854	1859	rBV	1630744	2331671	49.26%	6.574%
54	14.275	1896	1902	1912	rVB	1607583	2293136	48.44%	6.465%
55	14.451	1929	1932	1933	rBV3	5232	5170	0.11%	0.015%
56	14.492	1936	1939	1944	rVB7	10209	14980	0.32%	0.042%
57	14.580	1944	1954	1969	rBV	1000869	1605798	33.92%	4.528%
58	14.780	1983	1988	1995	rBV2	33175	71947	1.52%	0.203%
59	15.110	2040	2044	2047	rVB6	4543	6559	0.14%	0.018%
60	15.180	2053	2056	2059	rBV4	4928	4978	0.11%	0.014%
61	15.239	2061	2066	2069	rVB7	8460	16152	0.34%	0.046%
62	15.392	2086	2092	2097	rBV2	37259	63568	1.34%	0.179%
63	15.574	2117	2123	2136	rBV	2254997	3476558	73.44%	9.802%
64	15.686	2137	2142	2151	rVB	131130	209736	4.43%	0.591%
65	15.816	2160	2164	2170	rVB2	26141	35104	0.74%	0.099%
66	15.939	2182	2185	2188	rBV5	10010	12104	0.26%	0.034%
67	16.004	2188	2196	2198	rBV9	14150	32375	0.68%	0.091%
68	16.069	2204	2207	2209	rBV4	9239	11852	0.25%	0.033%
69	16.221	2229	2233	2237	rBV7	10939	17659	0.37%	0.050%
70	16.263	2237	2240	2244	rVV6	15319	23155	0.49%	0.065%
71	16.304	2245	2247	2251	rVV4	15013	18080	0.38%	0.051%
72	16.363	2255	2257	2263	rVB7	10345	13280	0.28%	0.037%
73	16.480	2274	2277	2282	rVB7	12552	16345	0.35%	0.046%
74	16.798	2329	2331	2332	rVV2	5425	4807	0.10%	0.014%
75	16.816	2332	2334	2336	rVV3	11117	12510	0.26%	0.035%
76	16.845	2336	2339	2344	rVB	22117	31265	0.66%	0.088%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
 Data File : BP009942.D
 Acq On : 19 Apr 2022 06:44
 Operator : CG/JU
 Sample : N2421-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COHX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

77	17.104	2381	2383	2385	rBV2	8184	6848	0.14%	0.019%
78	17.133	2385	2388	2396	rVB5	21386	44118	0.93%	0.124%
79	17.210	2397	2401	2405	rBV7	14696	23975	0.51%	0.068%
80	17.257	2405	2409	2413	rVB5	26042	31567	0.67%	0.089%
81	17.333	2416	2422	2433	rBV	1253307	1868157	39.47%	5.267%
82	17.433	2433	2439	2455	rBV	2635736	3888313	82.14%	10.963%
83	17.921	2519	2522	2525	rBV3	18822	24864	0.53%	0.070%
84	18.004	2534	2536	2541	rVB4	20746	24820	0.52%	0.070%
85	18.215	2569	2572	2580	rBV4	60785	99729	2.11%	0.281%
86	19.451	2779	2782	2787	rVB6	57566	72684	1.54%	0.205%
87	19.662	2812	2818	2834	rBV	3455435	4733668	100.00%	13.346%
88	21.415	3111	3116	3125	rBV	989789	1489893	31.47%	4.201%
89	23.721	3501	3508	3515	rBV2	974684	2108575	44.54%	5.945%
90	23.880	3529	3535	3545	rVB2	484119	1005244	21.24%	2.834%




Sum of corrected areas: 35467510

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009942.D
Acq On : 19 Apr 2022 06:44
Operator : CG/JU
Sample : N2421-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COHX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

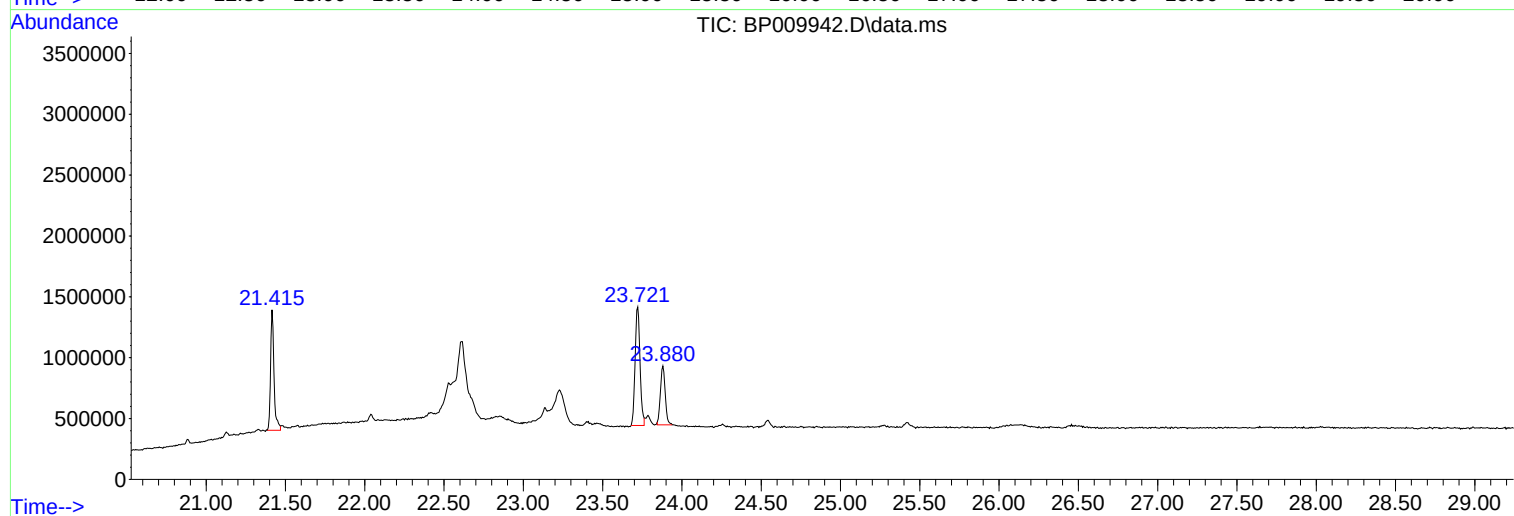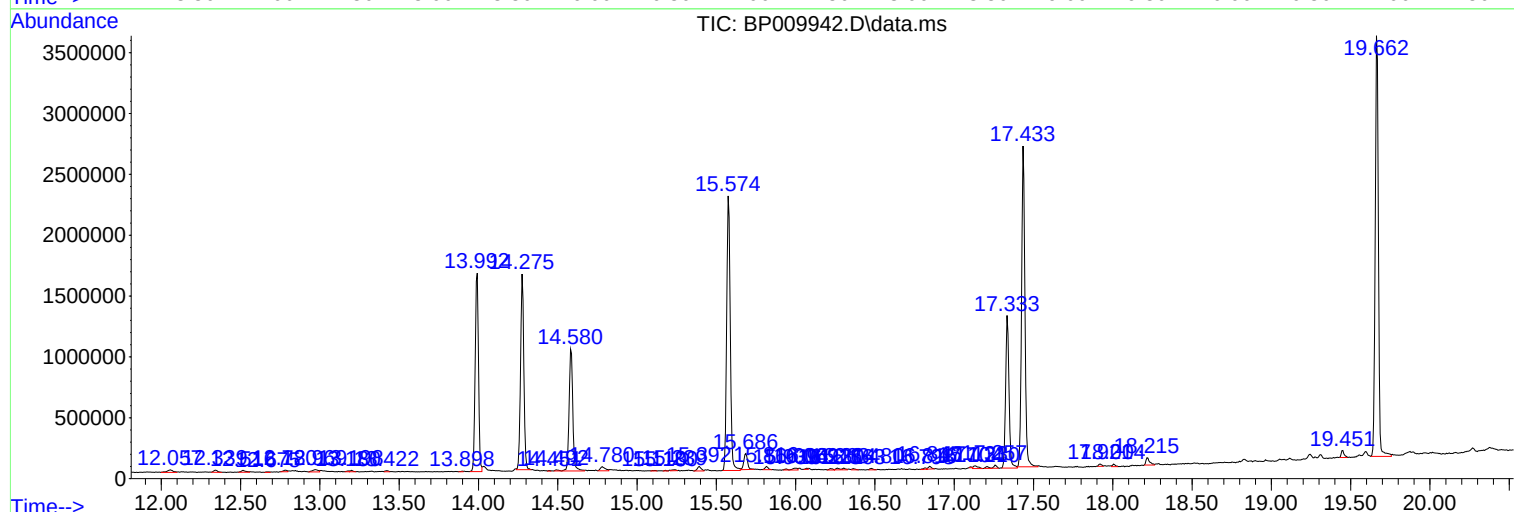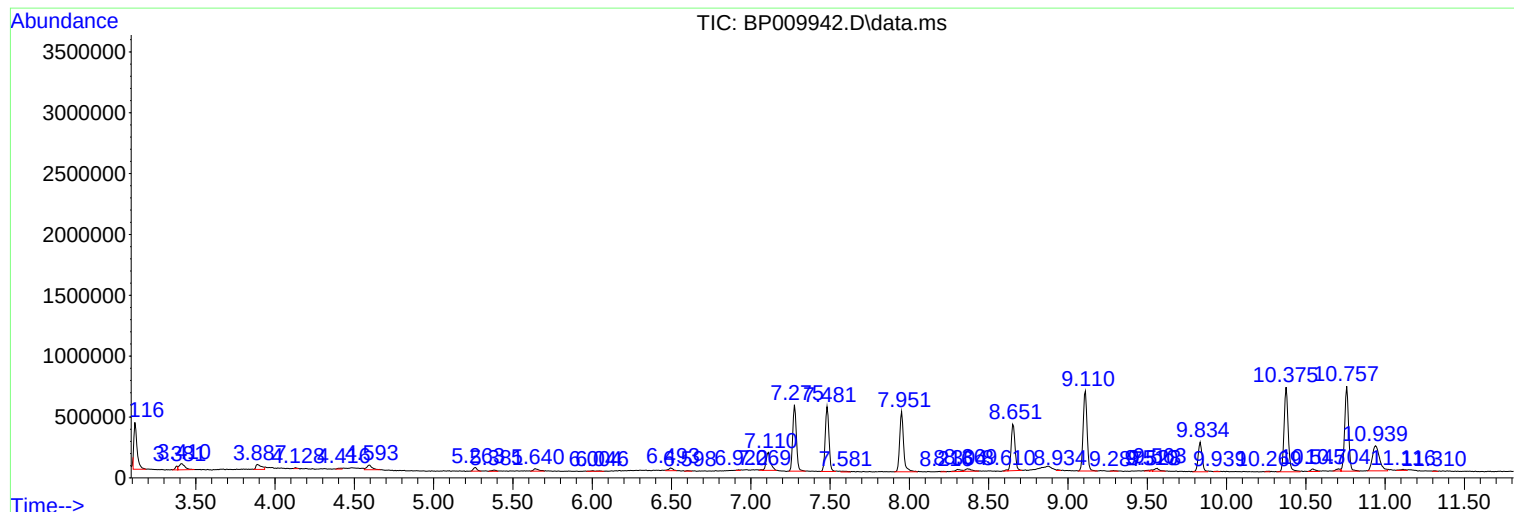

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009942.D
Acq On : 19 Apr 2022 06:44
Operator : CG/JU
Sample : N2421-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COHX0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.116	11.98 ng/ul	511336	1,4-Dichlorobenzene-d4	7.951

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
4			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	23
5			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12

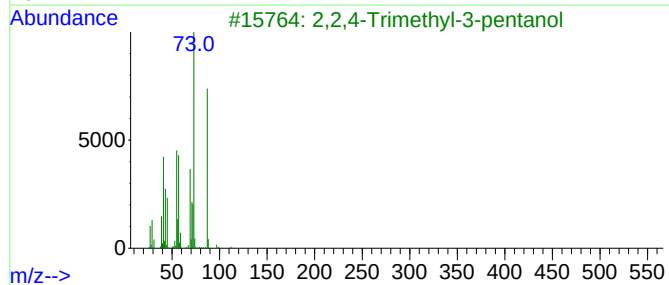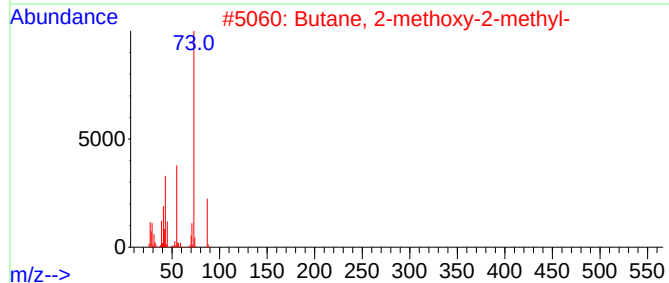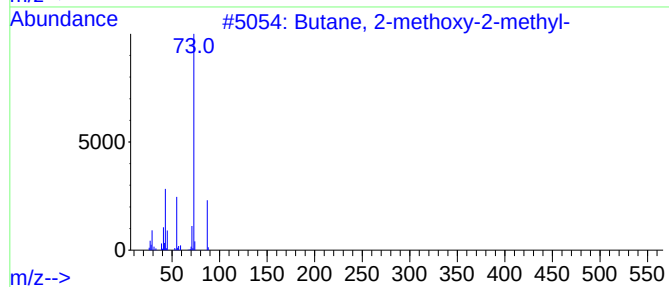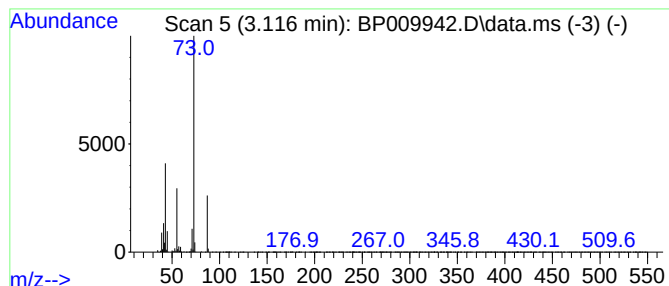

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041822\
Data File : BP009942.D
Acq On : 19 Apr 2022 06:44
Operator : CG/JU
Sample : N2421-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.116	12.0	ng/ul	511336	1	7.951	853478	20.0