
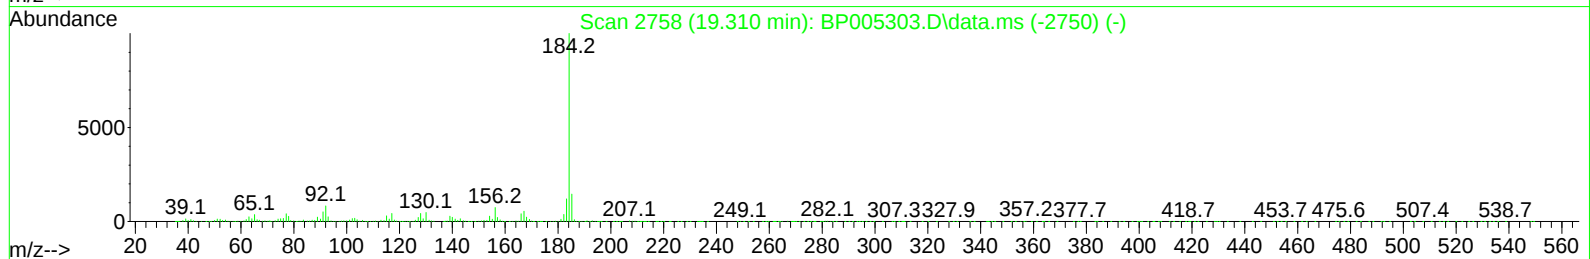
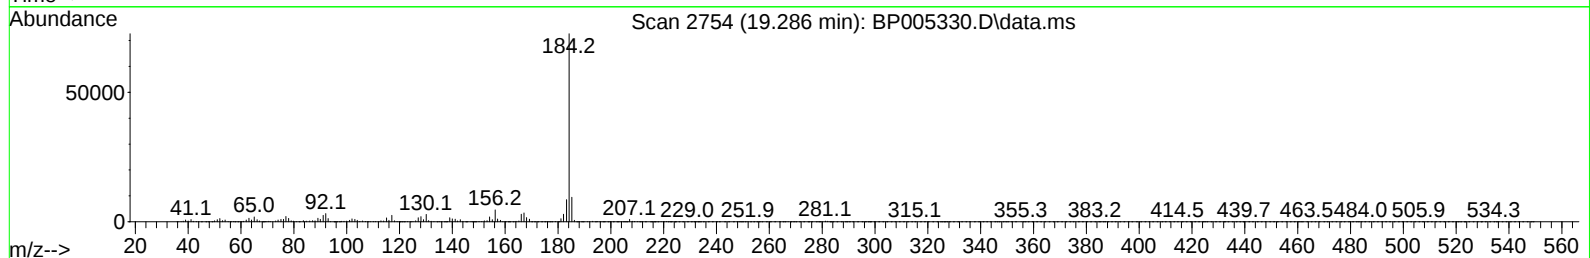


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041921\
Data File : BP005330.D
Acq On : 19 Apr 2021 15:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 15:54:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 11:02:58 2021
Response via : Initial Calibration

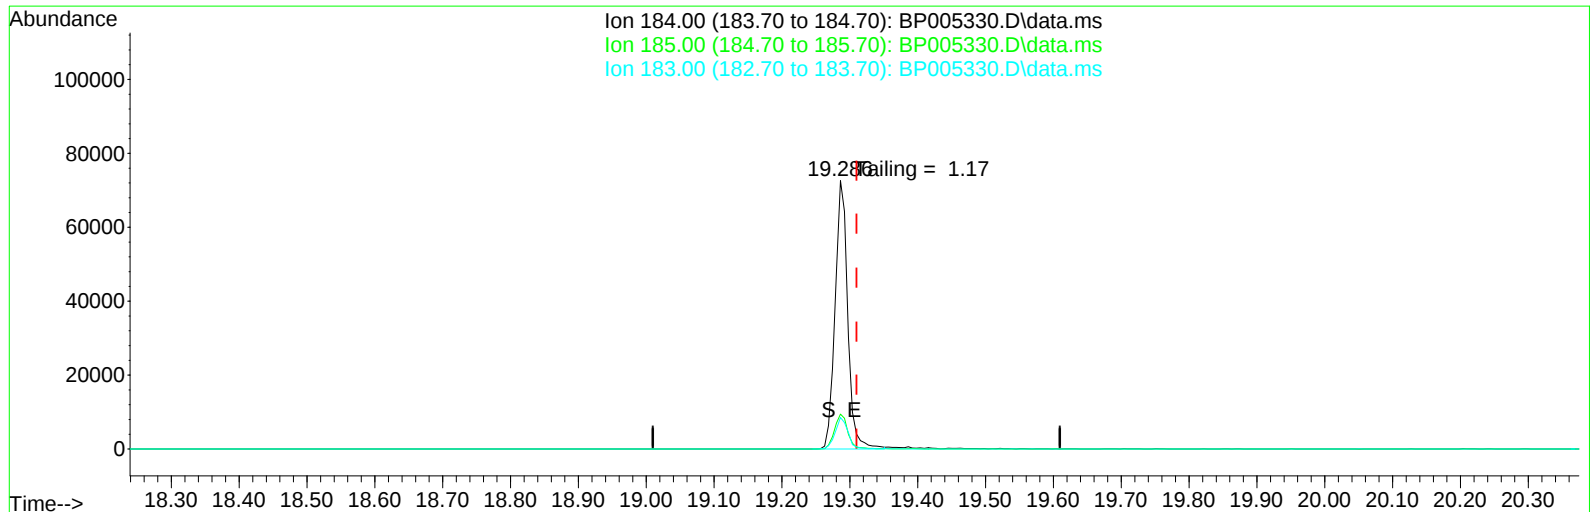




TIC: BP005330.D\data.ms

(77) Benzidine**19.286min (-0.024) 764027.26 ng****response 94491**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.04
183.00	12.10	11.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041921\
 Data File : BP005330.D
 Acq On : 19 Apr 2021 15:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 15:54:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 11:02:58 2021
 Response via : Initial Calibration

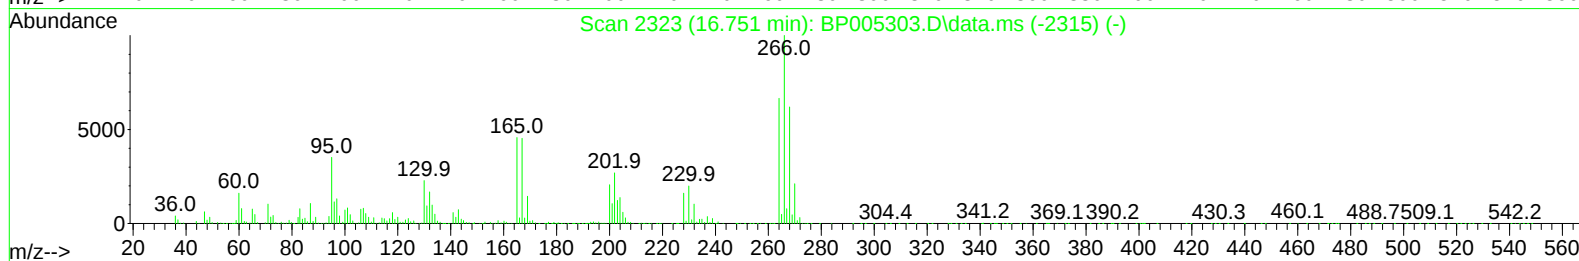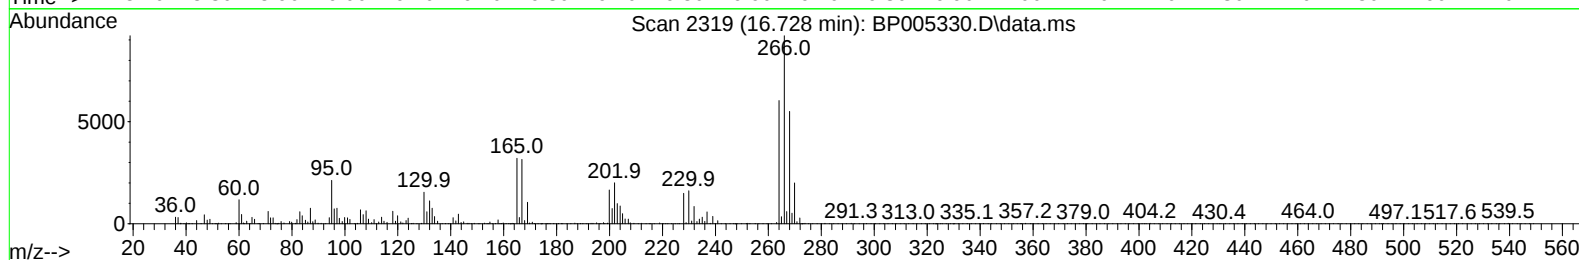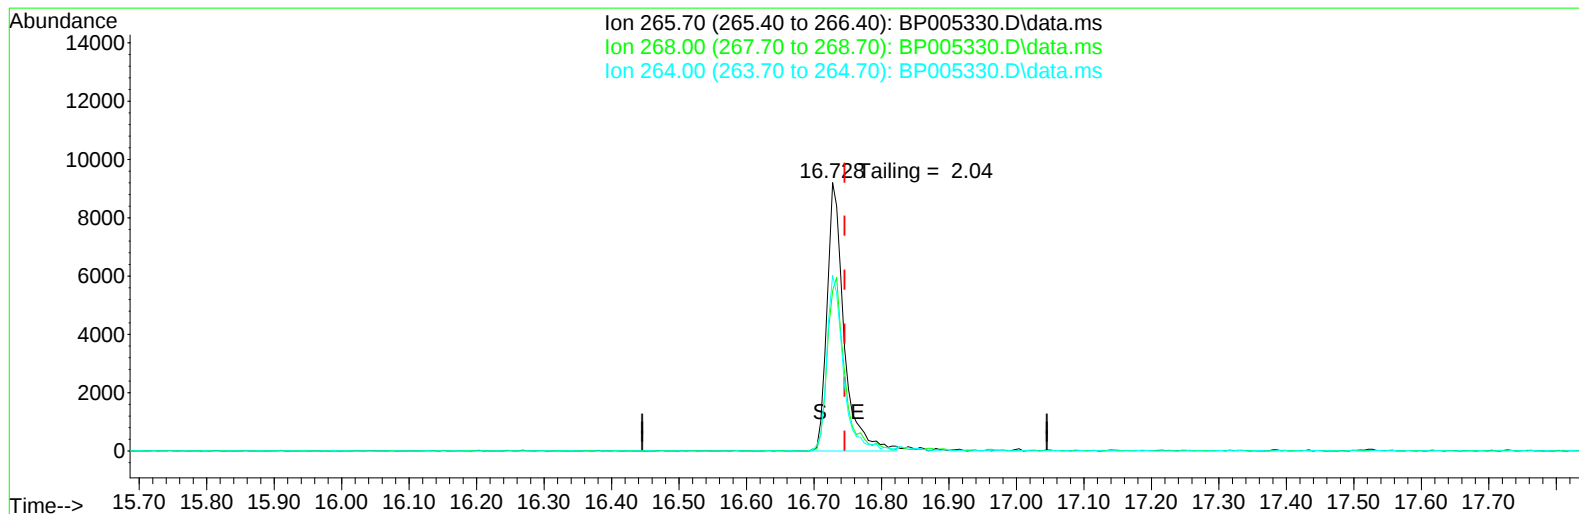

TIC: BP005330.D\data.ms

(70) Pentachlorophenol (C)

16.728min (-0.018) 205171.40 ng

response 16137

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	59.75
264.00	66.60	65.49
0.00	0.00	0.00