

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041921\
 Data File : BP005340.D
 Acq On : 19 Apr 2021 21:17
 Operator : CG/JU
 Sample : PB135822BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB135822BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005340.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.252	364	368	377	rVB	669684	879589	75.73%	15.851%
2	6.840	633	638	649	rVB	596528	883711	76.09%	15.925%
3	7.646	771	775	783	rVB2	114774	186298	16.04%	3.357%
4	8.810	967	973	991	rVB	306855	500066	43.05%	9.012%
5	10.440	1243	1250	1257	rBV	62493	104834	9.03%	1.889%
6	12.922	1663	1672	1690	rBV	586242	732879	63.10%	13.207%
7	14.310	1900	1908	1918	rBV	92000	133679	11.51%	2.409%
8	15.810	2155	2163	2180	rBV	321948	456110	39.27%	8.220%
9	17.075	2372	2378	2391	rBV	91703	136113	11.72%	2.453%
10	19.651	2810	2816	2825	rBV	1100006	1161461	100.00%	20.931%
11	21.175	3070	3075	3084	rBV	152570	196252	16.90%	3.537%
12	23.427	3452	3458	3466	rBV2	92986	178102	15.33%	3.210%




Sum of corrected areas: 5549094

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041921\
Data File : BP005340.D
Acq On : 19 Apr 2021 21:17
Operator : CG/JU
Sample : PB135822BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135822BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

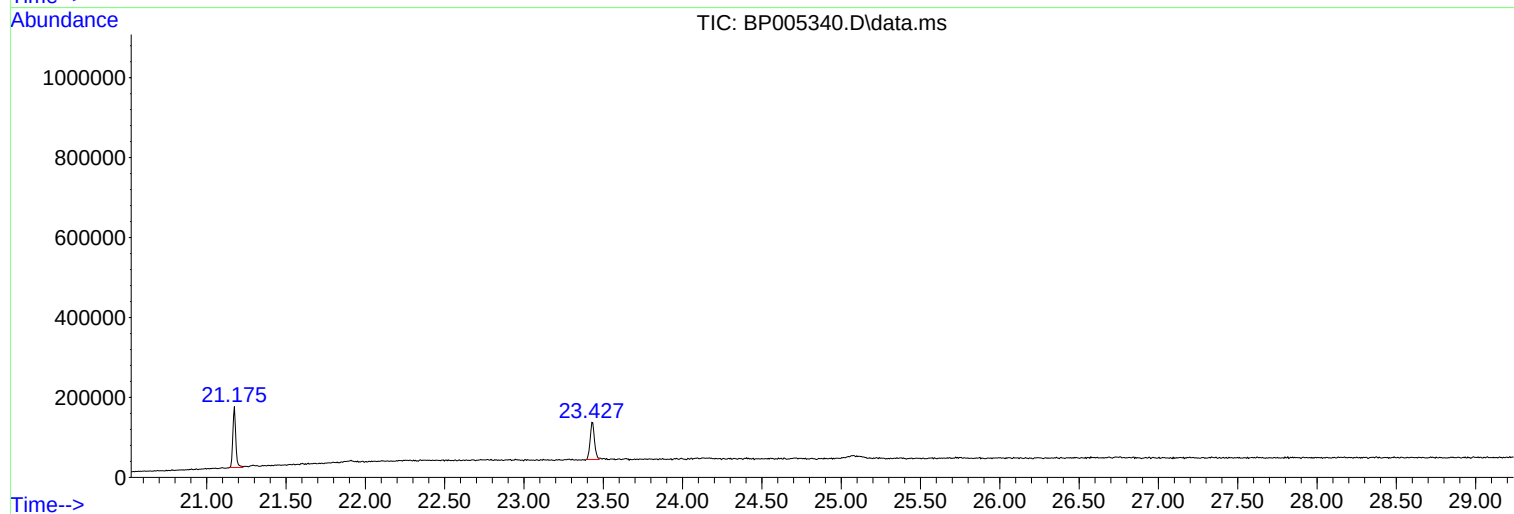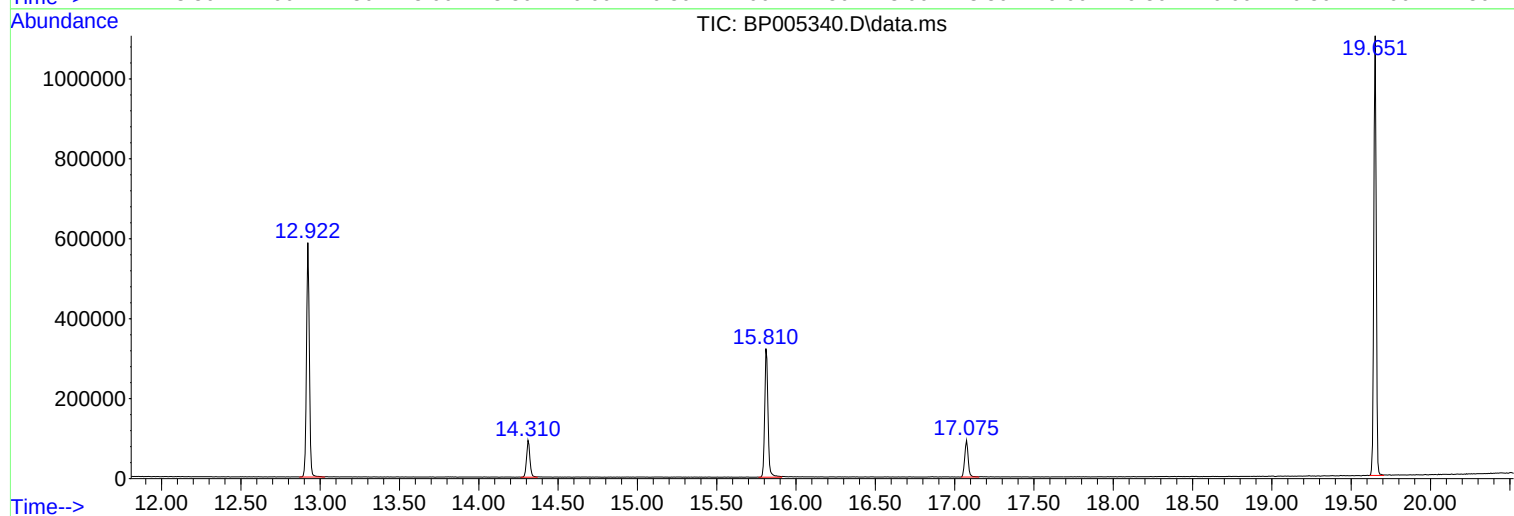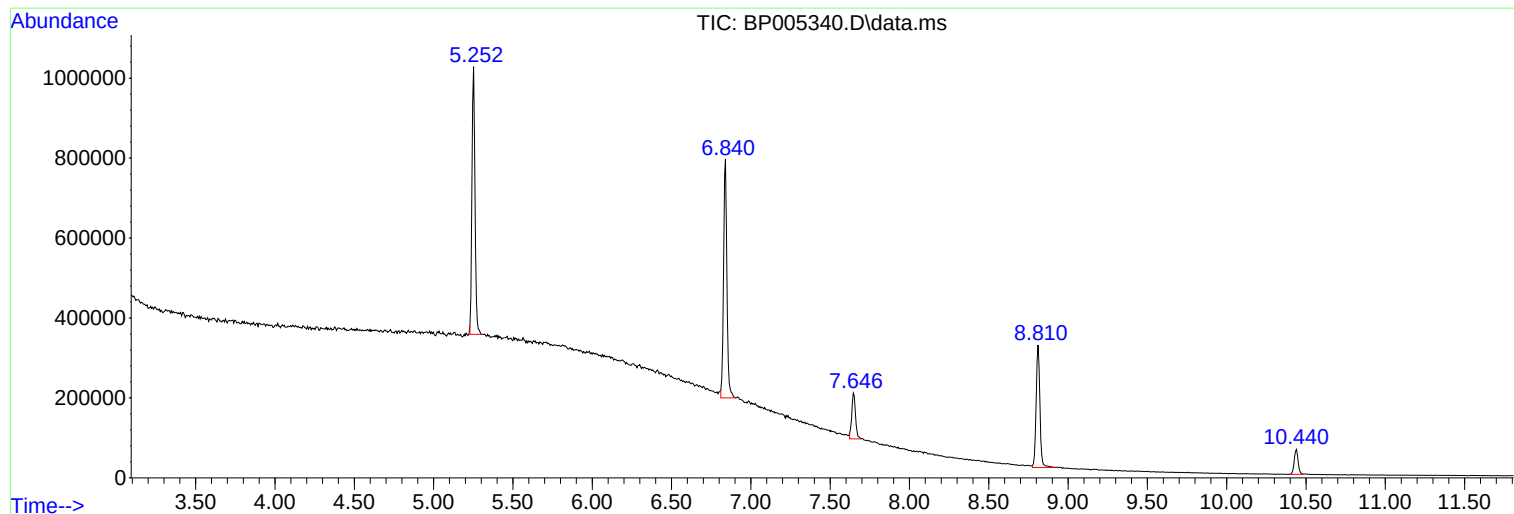

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041921\
Data File : BP005340.D
Acq On : 19 Apr 2021 21:17
Operator : CG/JU
Sample : PB135822BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135822BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041921\
Data File : BP005340.D
Acq On : 19 Apr 2021 21:17
Operator : CG/JU
Sample : PB135822BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135822BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------