
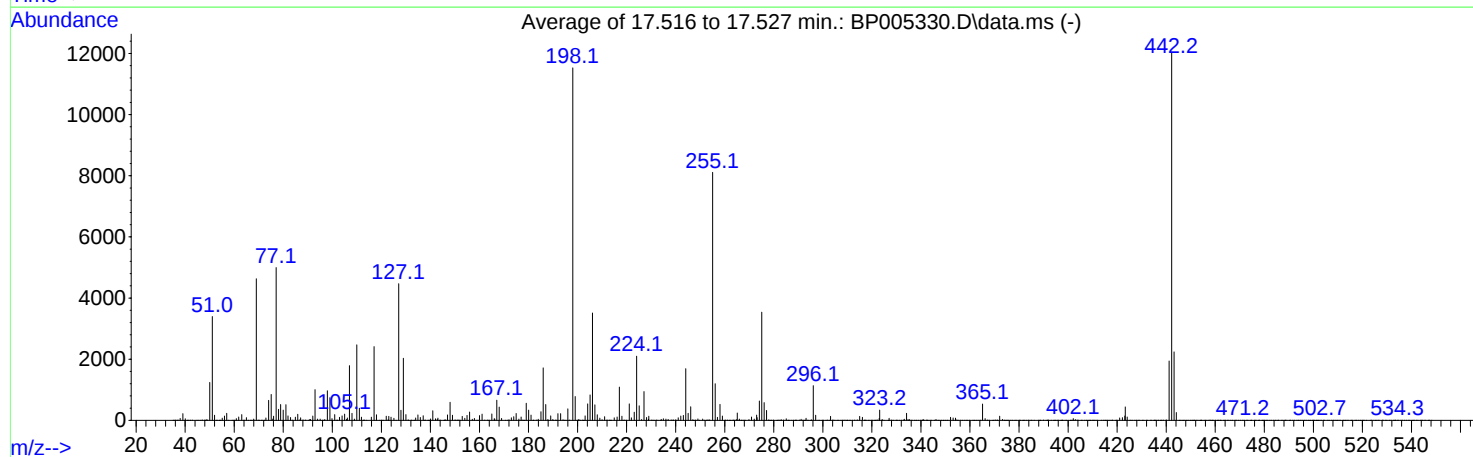


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041921\
 Data File : BP005330.D
 Acq On : 19 Apr 2021 15:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 20 02:04:17 2021

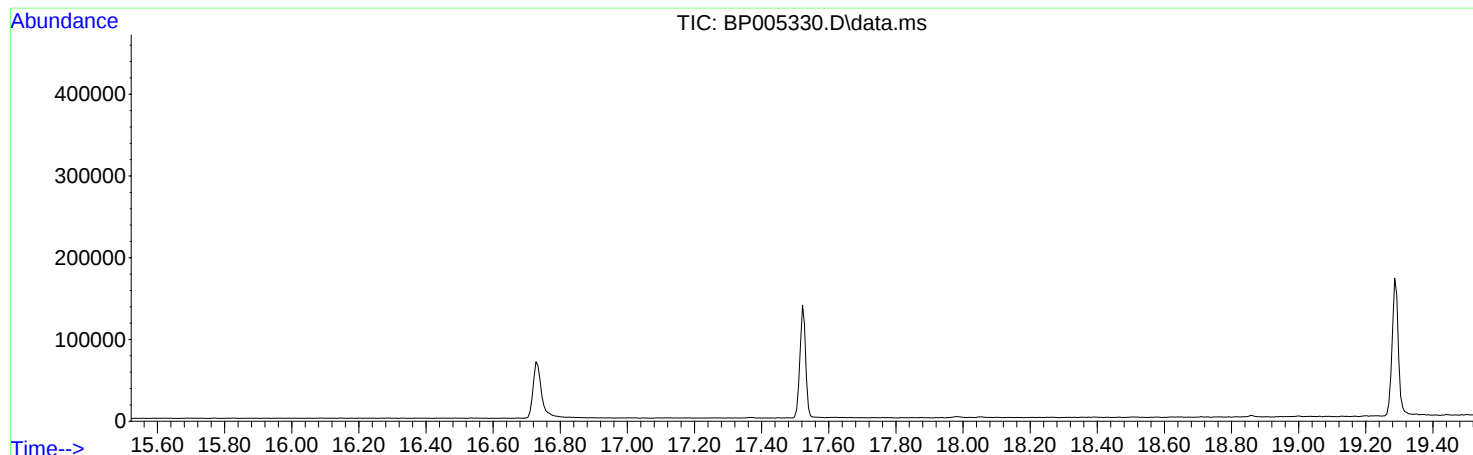




AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	3398	PASS
68	69	0.00	2	0.9	44	PASS
69	198	0.00	100	40.2	4633	PASS
70	69	0.00	2	0.2	11	PASS
127	198	10	80	38.7	4467	PASS
197	198	0.00	2	0.1	9	PASS
198	198	100	100	100.0	11529	PASS
199	198	5	9	6.8	779	PASS
275	198	10	60	30.7	3536	PASS
365	198	1	100	4.6	532	PASS
441	198	0.01	100	16.8	1940	PASS
442	442	100	100	100.0	12030	PASS
443	442	15	24	18.6	2241	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041921\
Data File : BP005330.D
Acq On : 19 Apr 2021 15:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 19 15:54:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 11:02:58 2021
Response via : Initial Calibration

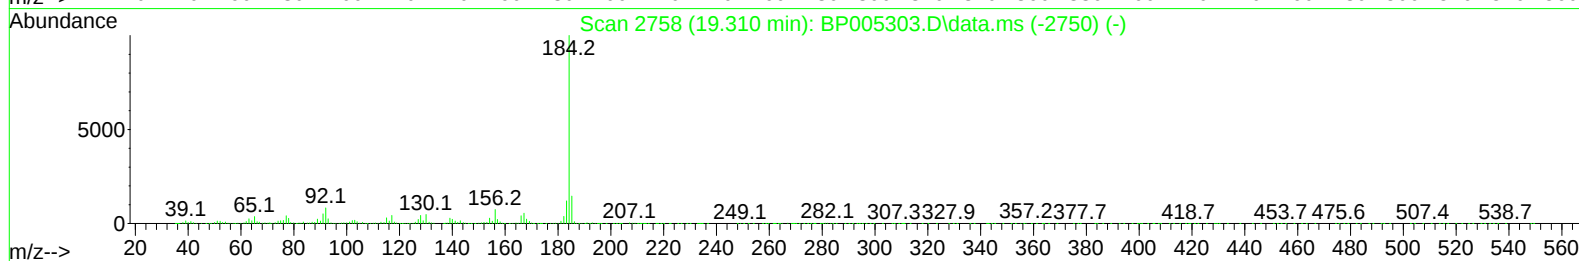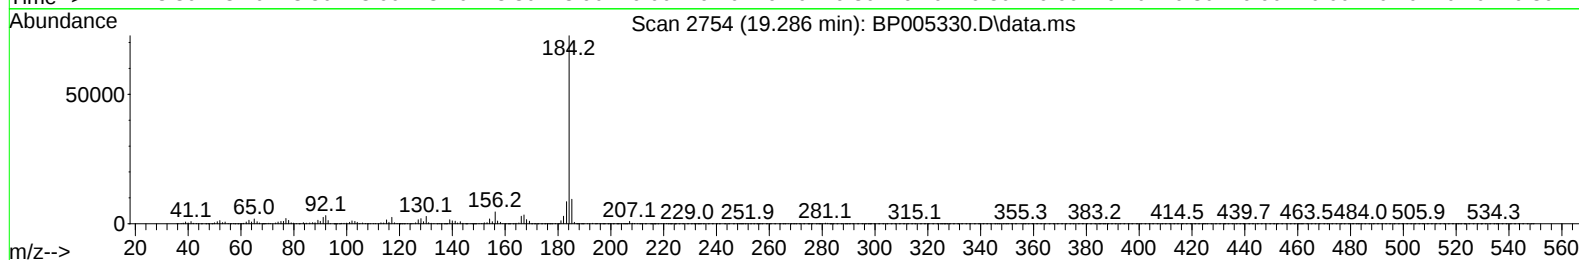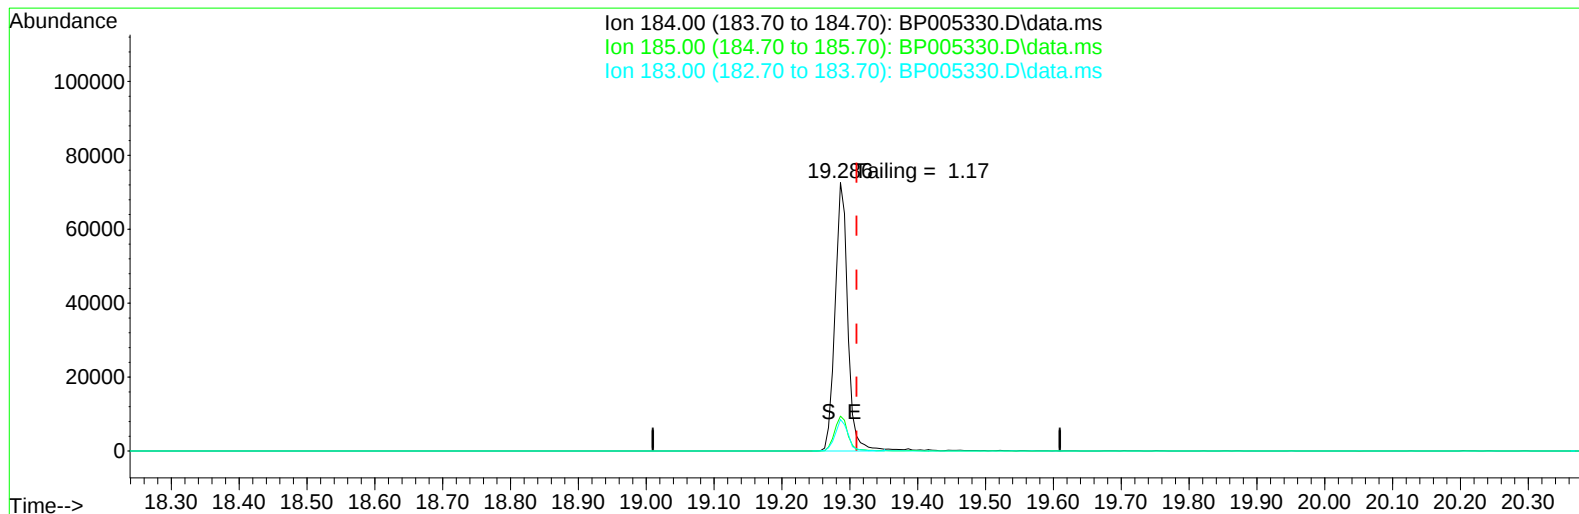

TIC: BP005330.D\data.ms

(77) Benzidine

19.286min (-0.024) 764027.26 ng




response 94491

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.04
183.00	12.10	11.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041921\
Data File : BP005330.D
Acq On : 19 Apr 2021 15:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 19 15:54:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 11:02:58 2021
Response via : Initial Calibration

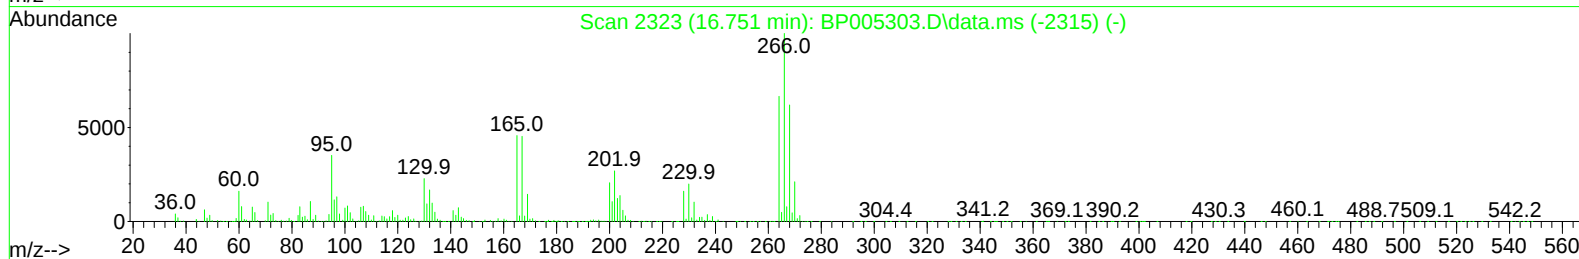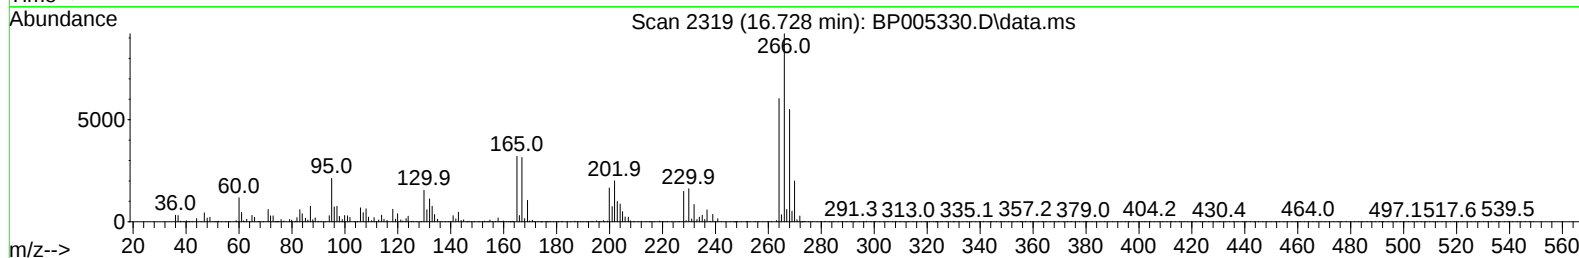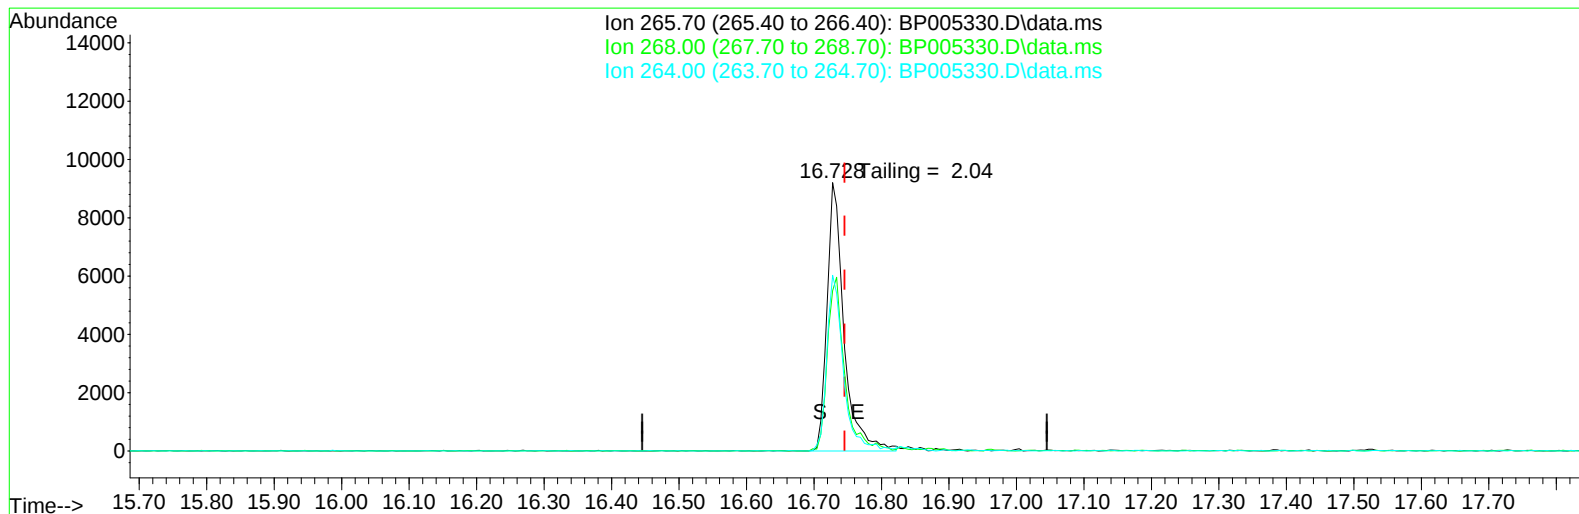

TIC: BP005330.D\data.ms

(70) Pentachlorophenol (C)

16.728min (-0.018) 205171.40 ng

response 16137

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	59.75
264.00	66.60	65.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/19/2021	BNA_P	BP005330.D
Compound Name	Response	Retention Time
DDT	65130	20.48
DDD	290	20.1
DDE	95	19.56
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
385	65515	0.59

Instrument :
BNA_P
ClientSampleId :
DFTPP