
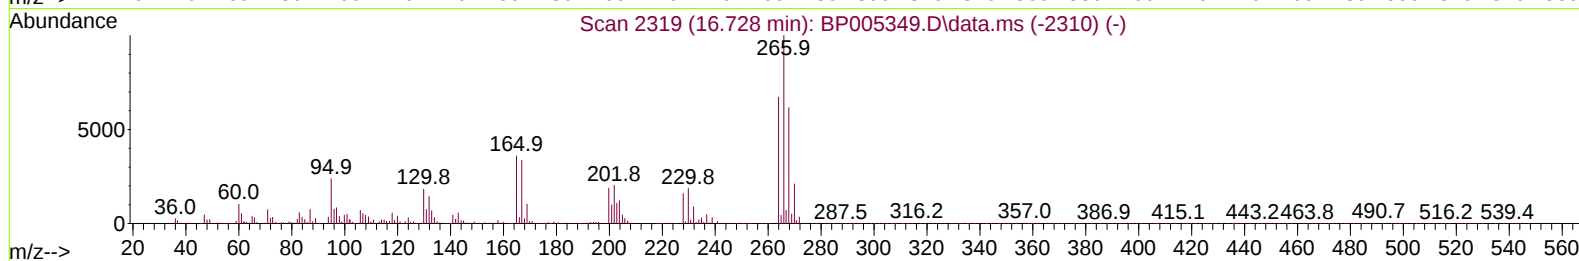
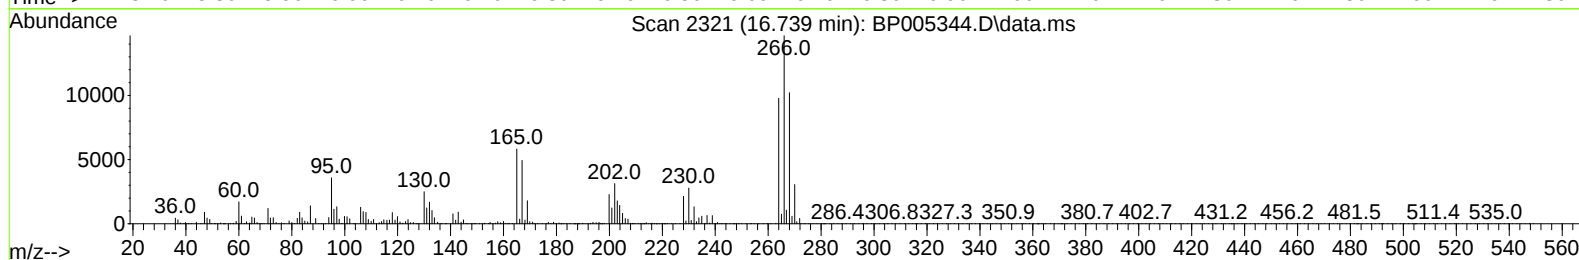


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042021\
Data File : BP005344.D
Acq On : 20 Apr 2021 08:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 06:11:27 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 13:58:01 2021
Response via : Initial Calibration

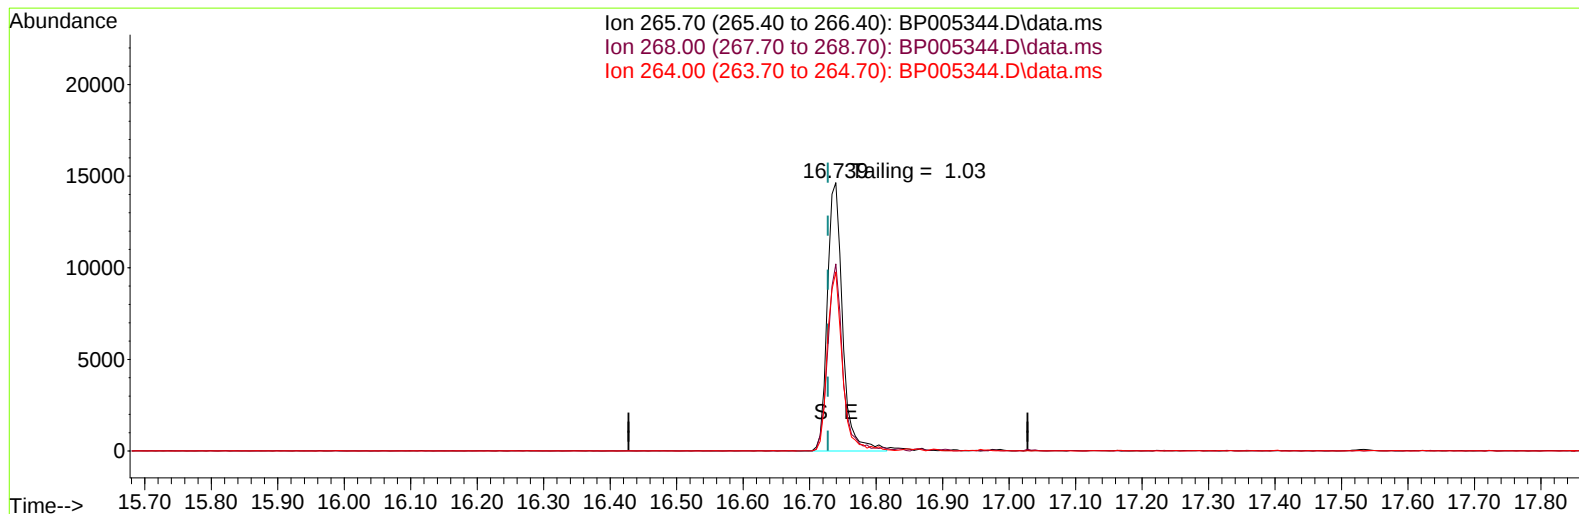

TIC: BP005344.D\data.ms

(70) Pentachlorophenol (C)




16.739min (+ 0.012) 157824.17 ng

response 23719

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	69.68
264.00	67.10	66.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042021\
 Data File : BP005344.D
 Acq On : 20 Apr 2021 08:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 06:11:27 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 20 13:58:01 2021
 Response via : Initial Calibration

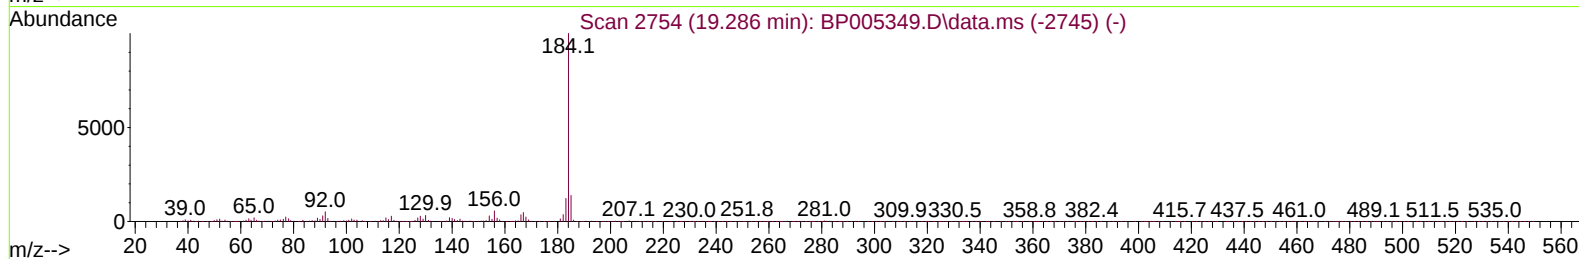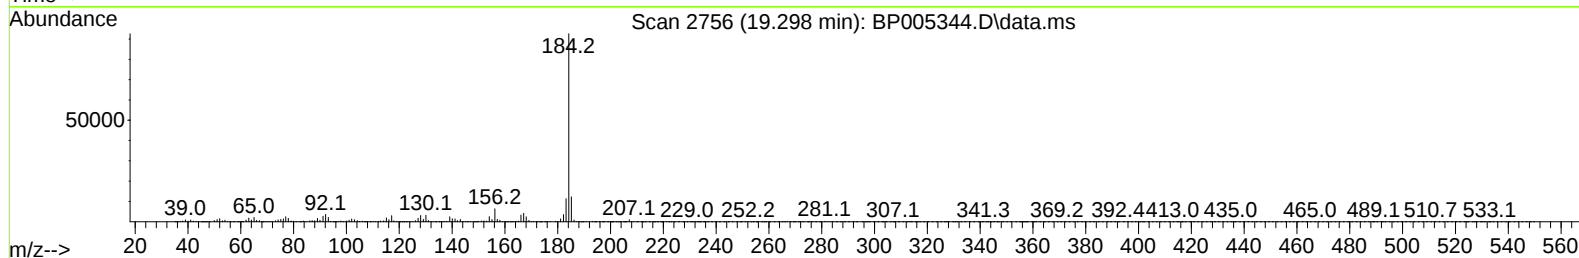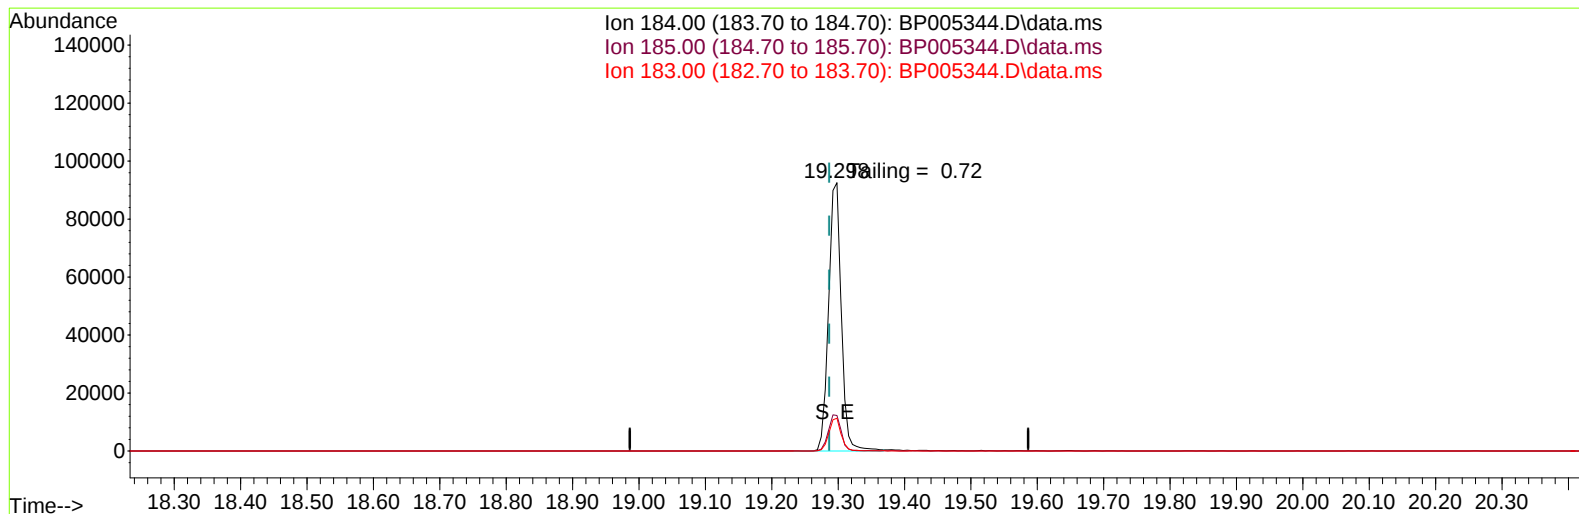

TIC: BP005344.D\data.ms

(77) Benzidine**19.298min (+ 0.012) 5244.03 ng****response 123912**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.26
183.00	12.30	12.27
0.00	0.00	0.00