
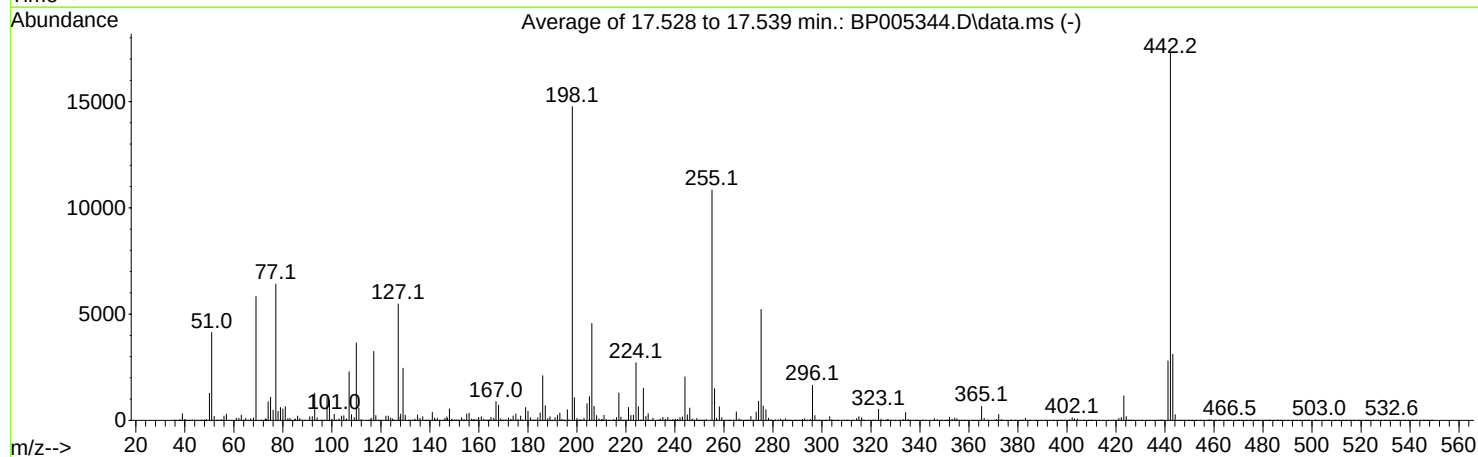


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042021\
 Data File : BP005344.D
 Acq On : 20 Apr 2021 08:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 20 13:58:01 2021

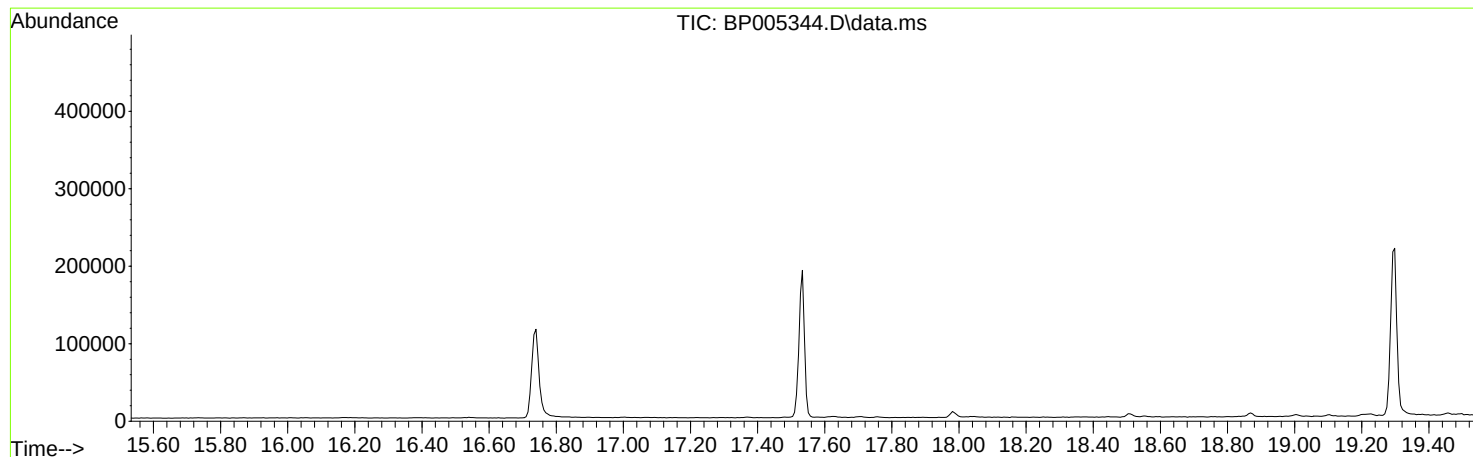

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	4134	PASS
68	69	0.00	2	1.9	113	PASS
69	198	0.00	100	39.5	5827	PASS
70	69	0.00	2	0.1	6	PASS
127	198	10	80	37.1	5473	PASS
197	198	0.00	2	0.2	26	PASS
198	198	100	100	100.0	14764	PASS
199	198	5	9	7.2	1066	PASS
275	198	10	60	35.3	5219	PASS
365	198	1	100	4.4	655	PASS
441	198	0.01	100	19.0	2803	PASS
442	442	100	100	100.0	17308	PASS
443	442	15	24	18.0	3120	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
4/20/2021	BNA_P	<u>BP005344.D</u>
Compound Name	Response	Retention Time
DDT	84741	20.492
DDD	602	20.069
DDE	111	19.563
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
713	85454	0.83

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042021\
 Data File : BP005344.D
 Acq On : 20 Apr 2021 08:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 21 06:11:27 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 20 13:58:01 2021
 Response via : Initial Calibration

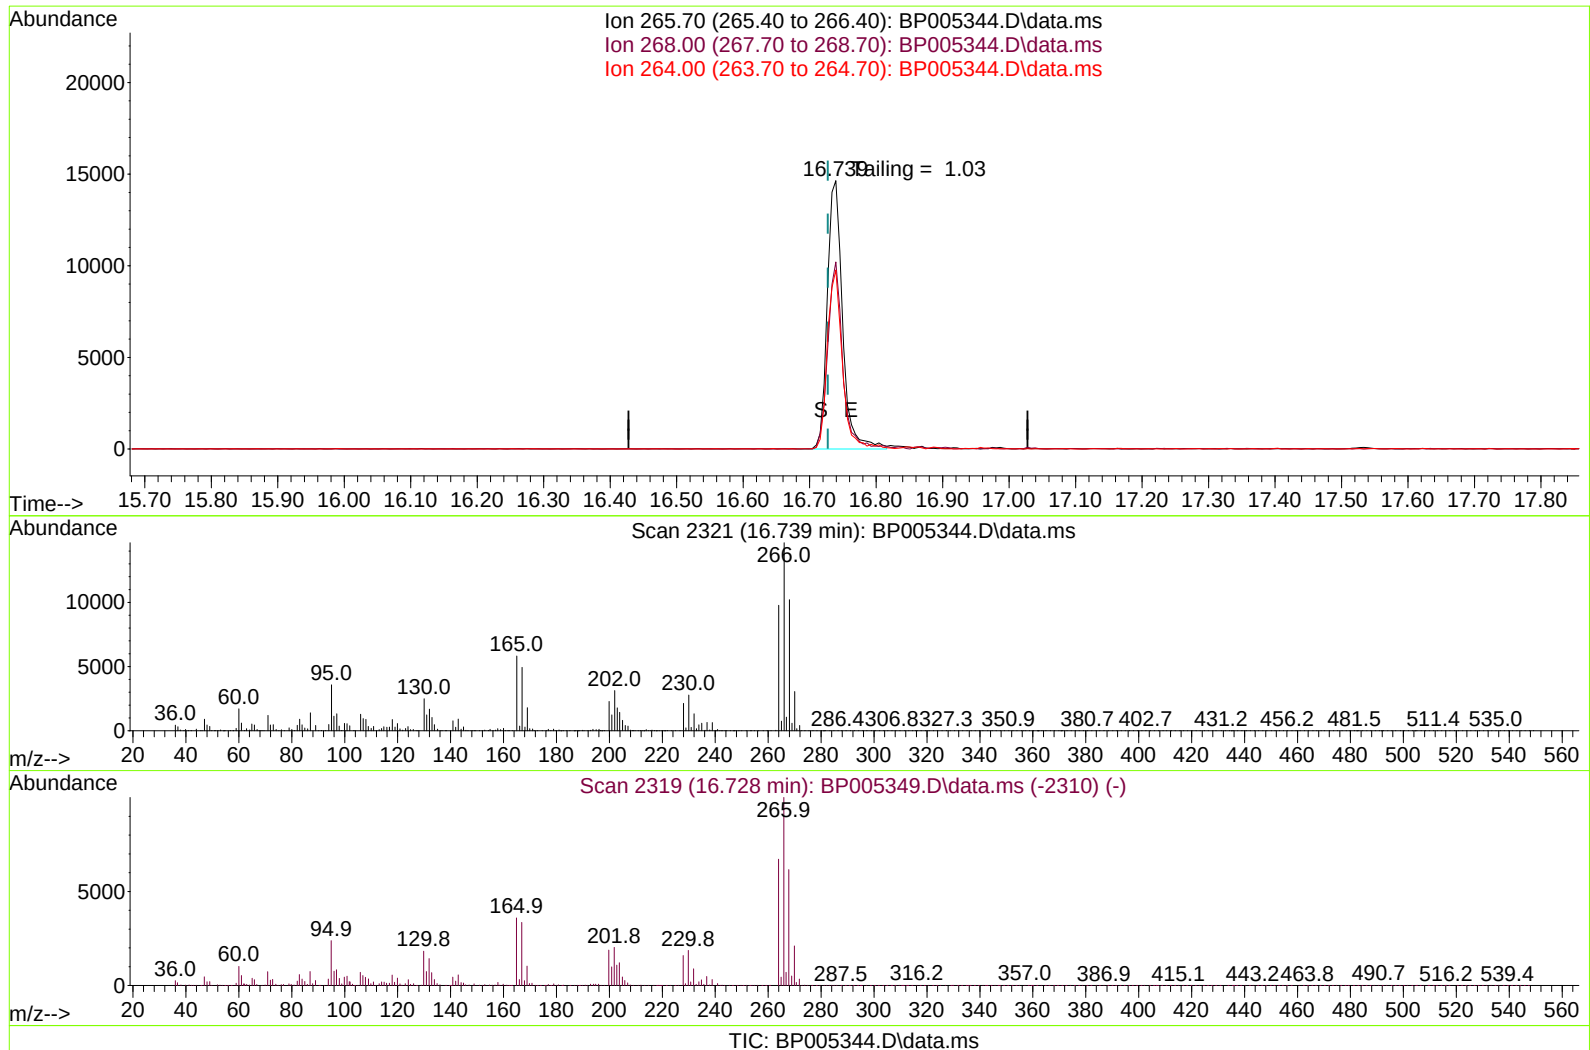

TIC: BP005344.D\data.ms

(70) Pentachlorophenol (C)

16.739min (+ 0.012) 157824.17 ng




response 23719

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	69.68
264.00	67.10	66.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042021\
 Data File : BP005344.D
 Acq On : 20 Apr 2021 08:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 21 06:11:27 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 20 13:58:01 2021
 Response via : Initial Calibration

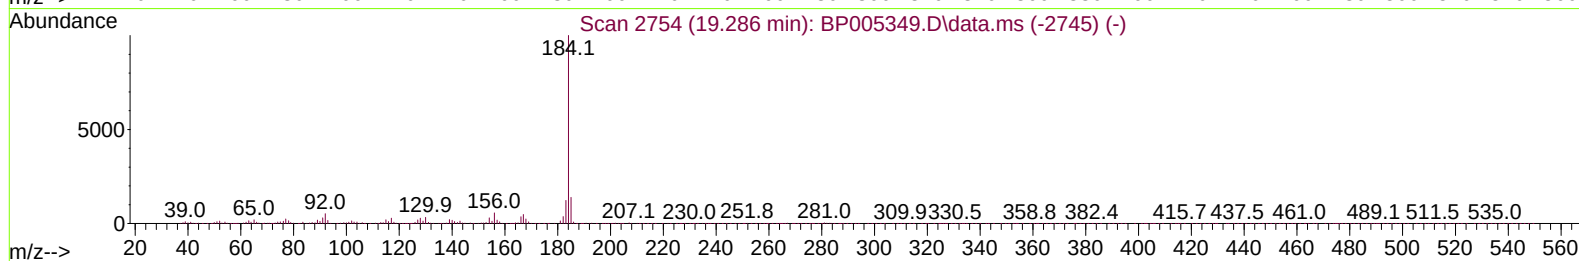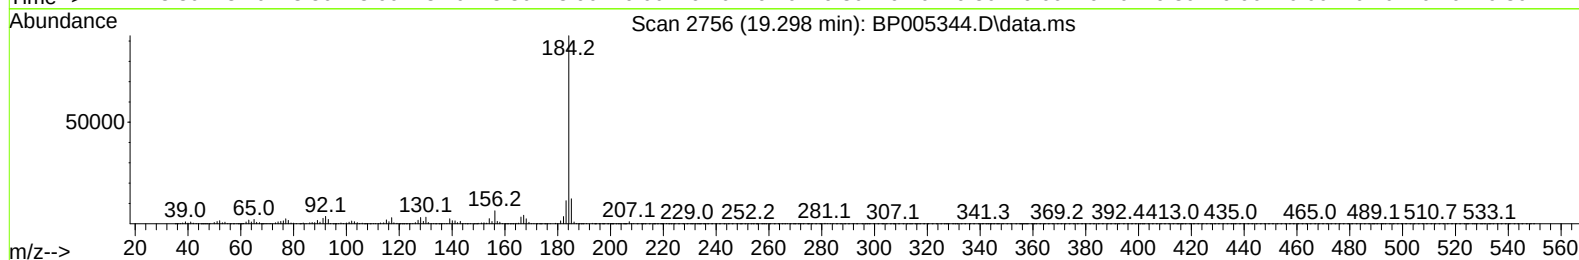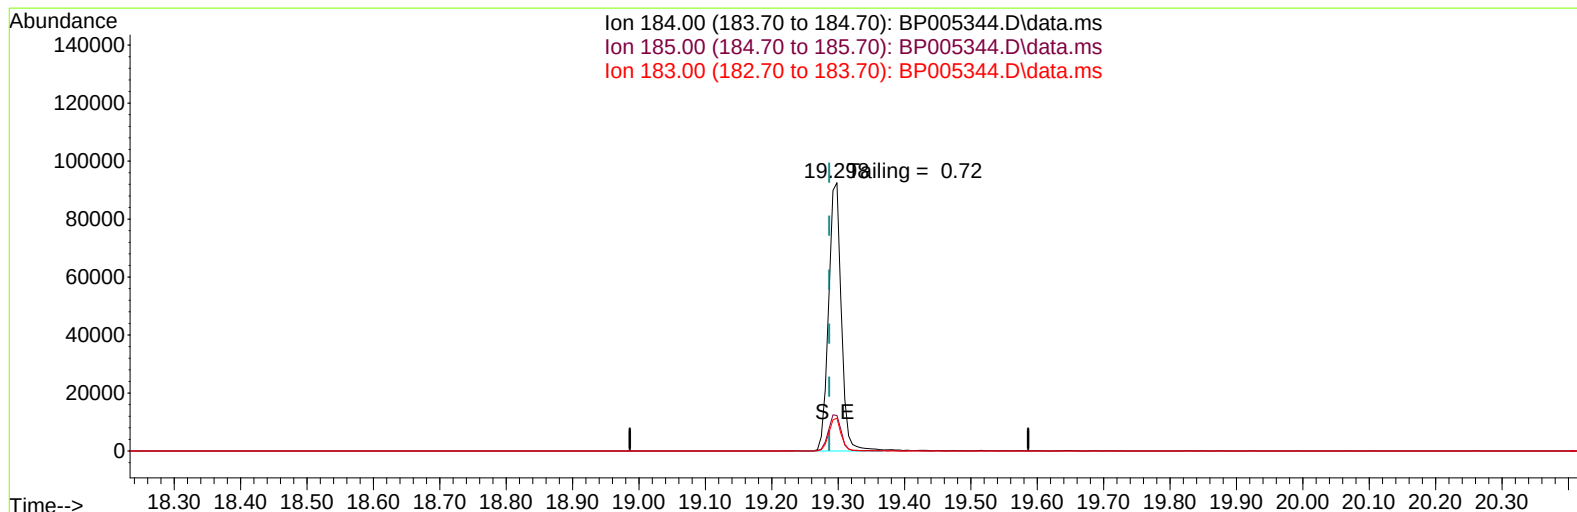

TIC: BP005344.D\data.ms

(77) Benzidine

19.298min (+ 0.012) 5244.03 ng

response 123912

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.26
183.00	12.30	12.27
0.00	0.00	0.00