




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020042.D
 Acq On : 20 Apr 2024 13:37
 Operator : MA/JU
 Sample : P2161-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R93

Manual IntegrationsAPPROVED

Quant Time: Apr 21 23:42:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 20 01:32:50 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/30/2024

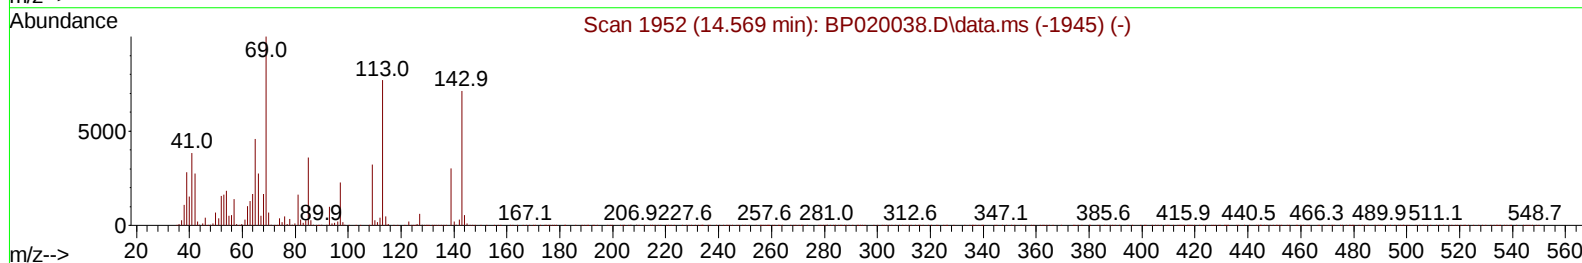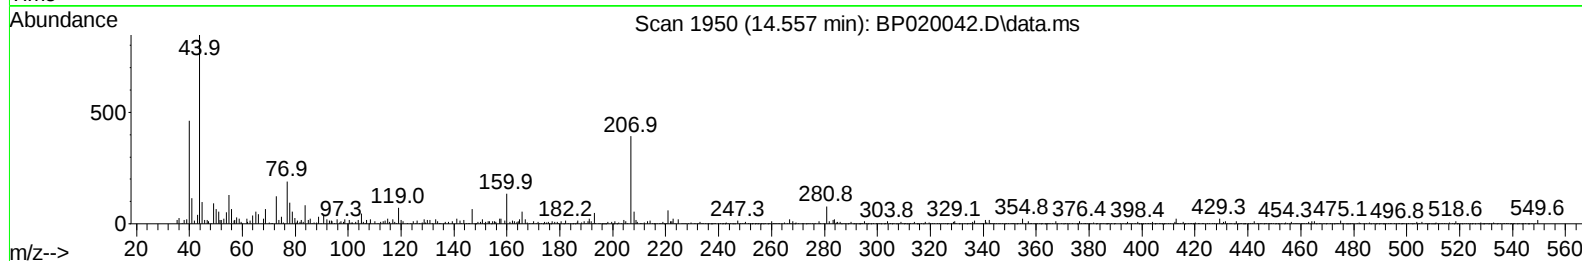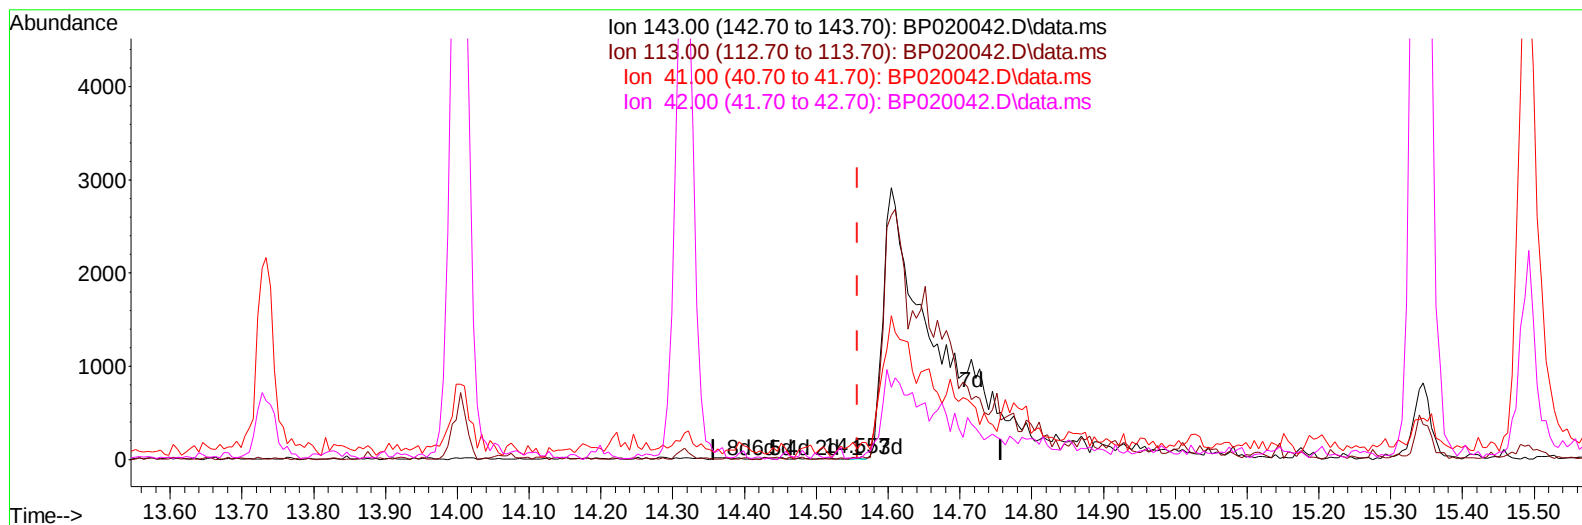

TIC: BP020042.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.557min (+ 0.000) 0.00 ng/ul

response 8

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.80	57.89#
41.00	50.70	605.26#
42.00	34.00	78.95#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020042.D
 Acq On : 20 Apr 2024 13:37
 Operator : MA/JU
 Sample : P2161-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R93

Manual IntegrationsAPPROVED

Quant Time: Apr 21 23:42:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 20 01:32:50 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/30/2024

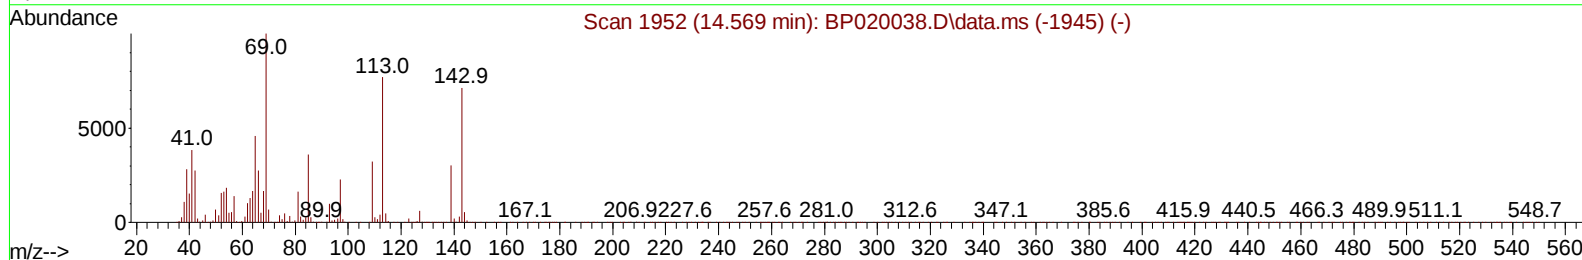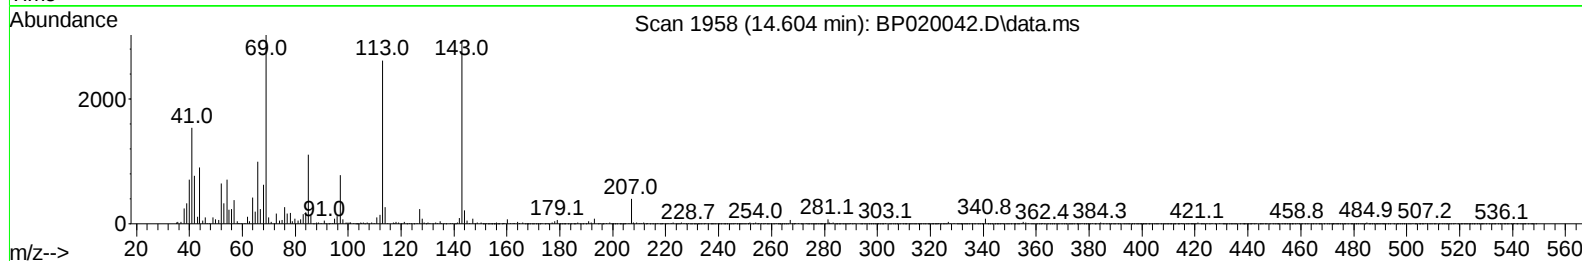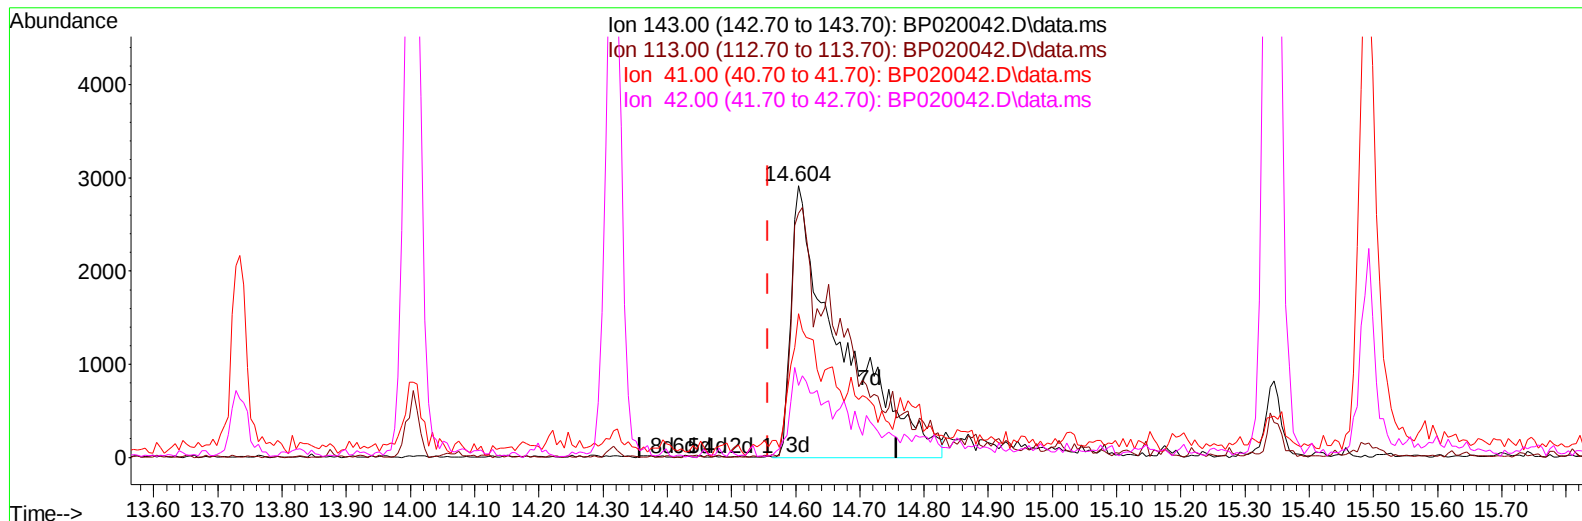

TIC: BP020042.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.604min (+ 0.047) 6.10 ng/ul m

response 15488

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.80	89.91
41.00	50.70	52.83
42.00	34.00	26.48#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020042.D
 Acq On : 20 Apr 2024 13:37
 Operator : MA/JU
 Sample : P2161-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R93

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/30/2024

Quant Time: Apr 21 23:56:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 20 01:32:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	81649	20.000	ng/ul	0.00
20) Naphthalene-d8	10.416	136	343065	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.316	164	244104	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.157	188	500886	20.000	ng/ul	0.00
79) Chrysene-d12	21.663	240	421854	20.000	ng/ul	0.00
88) Perylene-d12	25.057	264	479168	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	9628	4.832	ng/uL	0.00
4) Pyridine-d5	3.646	84	18283	3.117	ng/ul	0.01
7) Phenol-d5	6.828	99	45862	6.445	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67	190776	38.355	ng/ul	0.00
11) 2-Chlorophenol-d4	7.175	132	136464	28.087	ng/ul	0.00
15) 4-Methylphenol-d8	8.346	113	93052	16.740	ng/ul	0.00
21) Nitrobenzene-d5	8.799	128	102533	41.549	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	109143	40.916	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.046	165	168654	31.871	ng/ul	0.00
31) 4-Chloroaniline-d4	10.575	131	130141	18.422	ng/ul	0.00
46) Dimethylphthalate-d6	13.734	166	739467	44.326	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	816989	41.088	ng/ul	0.00
54) 4-Nitrophenol-d4	14.604	143	15488m	6.099	ng/ul	0.05
60) Fluorene-d10	15.345	176	651387	43.864	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.492	200	106744	36.478	ng/ul	0.00
73) Anthracene-d10	17.263	188	998294	44.487	ng/ul	0.00
81) Pyrene-d10	19.663	212	1092537	48.191	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.816	264	1099165	46.958	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020042.D
Acq On : 20 Apr 2024 13:37
Operator : MA/JU
Sample : P2161-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0R93

Manual IntegrationsAPPROVED

Quant Time: Apr 21 23:56:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 20 01:32:50 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/30/2024

