




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020056.D
 Acq On : 21 Apr 2024 00:35
 Operator : MA/JU
 Sample : P2161-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CORE4

Manual IntegrationsAPPROVED

Quant Time: Apr 22 00:29:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 20 01:32:50 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/30/2024

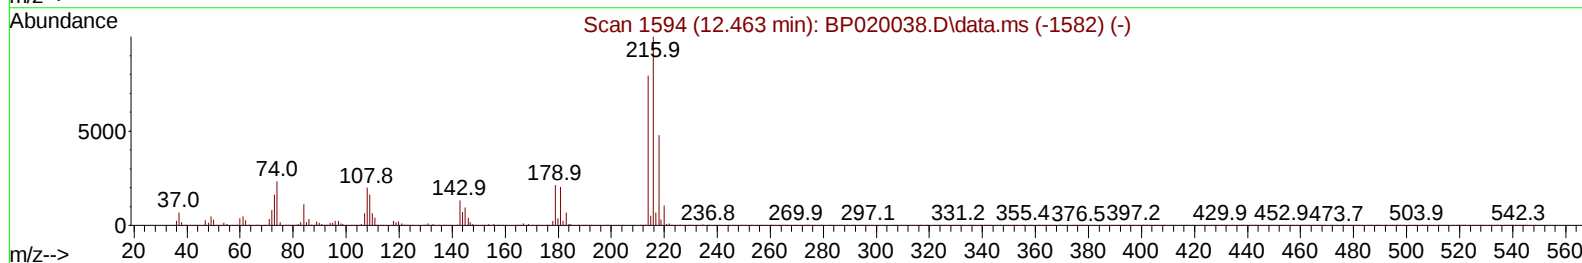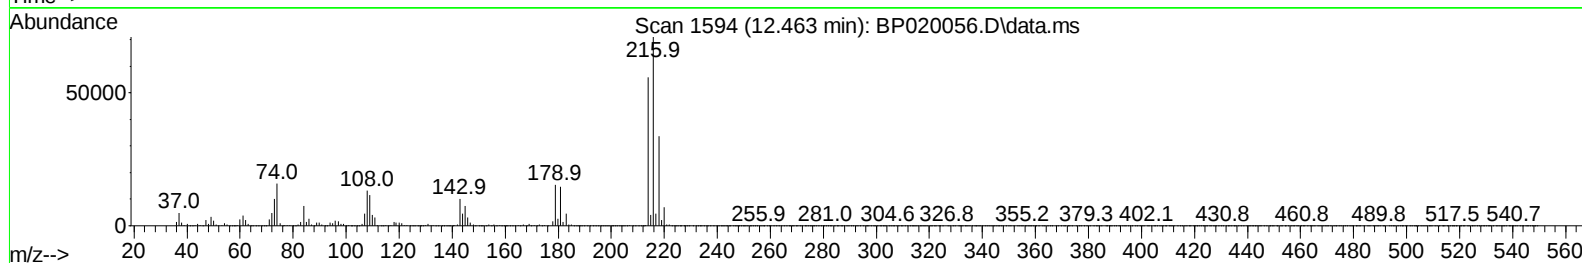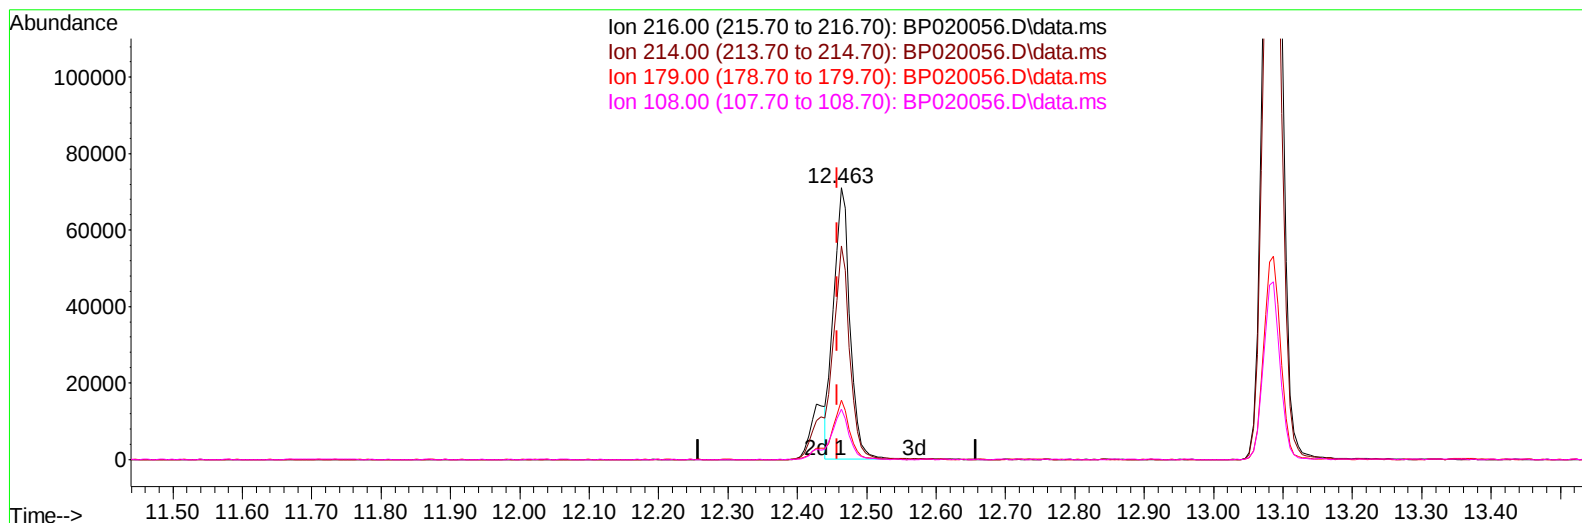

TIC: BP020056.D\data.ms

(39) 1,2,4,5-Tetrachlorobenzene

12.463min (+ 0.006) 14.59 ng/u1

response 116313

Ion	Exp%	Act%
216.00	100.00	100.00
214.00	80.20	78.62
179.00	21.60	21.77
108.00	21.00	18.60




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020056.D
 Acq On : 21 Apr 2024 00:35
 Operator : MA/JU
 Sample : P2161-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CORE4

Manual IntegrationsAPPROVED

Quant Time: Apr 22 00:29:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 20 01:32:50 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/30/2024

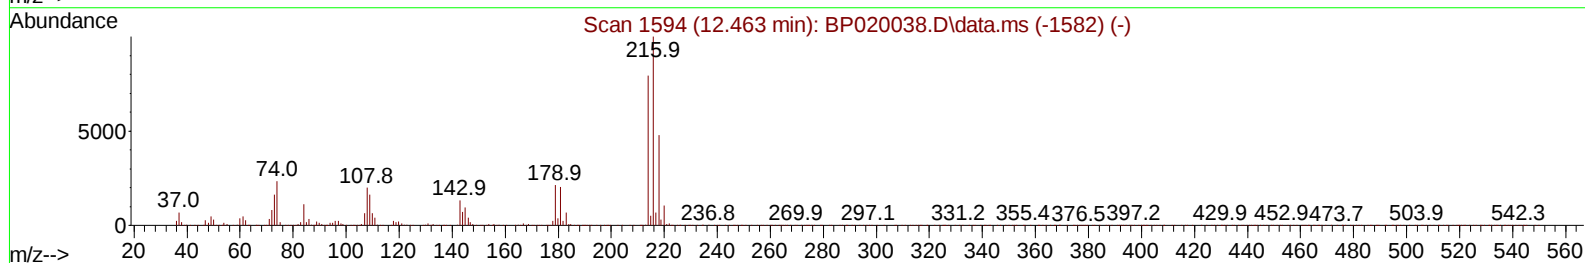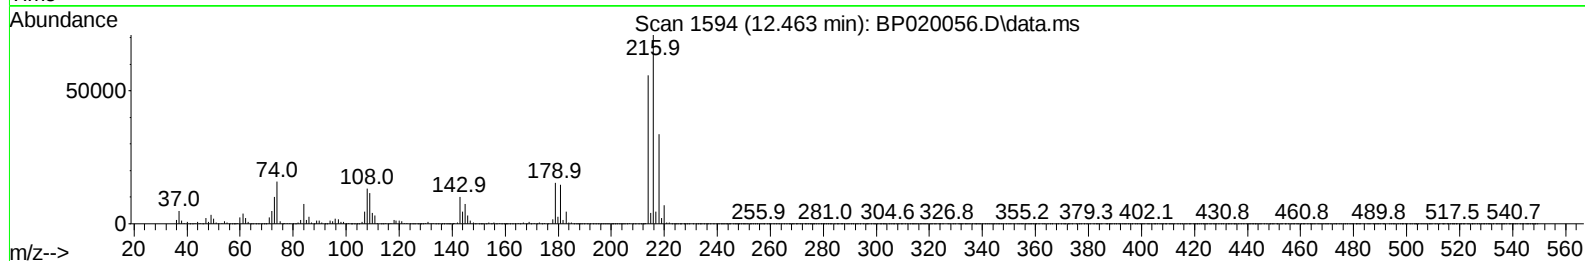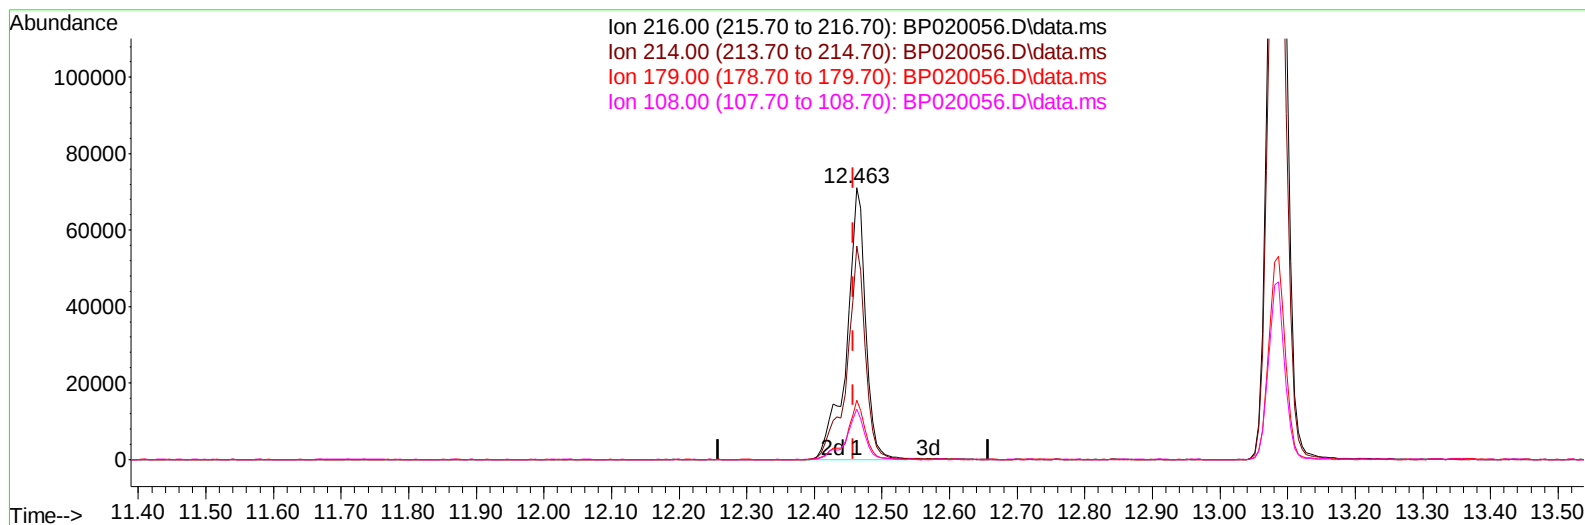

TIC: BP020056.D\data.ms

(39) 1,2,4,5-Tetrachlorobenzene

12.463min (+ 0.006) 17.41 ng/ul m

response 138798

Ion	Exp%	Act%
216.00	100.00	100.00
214.00	80.20	78.62
179.00	21.60	21.77
108.00	21.00	18.60




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020056.D
Acq On : 21 Apr 2024 00:35
Operator : MA/JU
Sample : P2161-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CORE4

Manual IntegrationsAPPROVED

Quant Time: Apr 22 00:29:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 20 01:32:50 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/30/2024

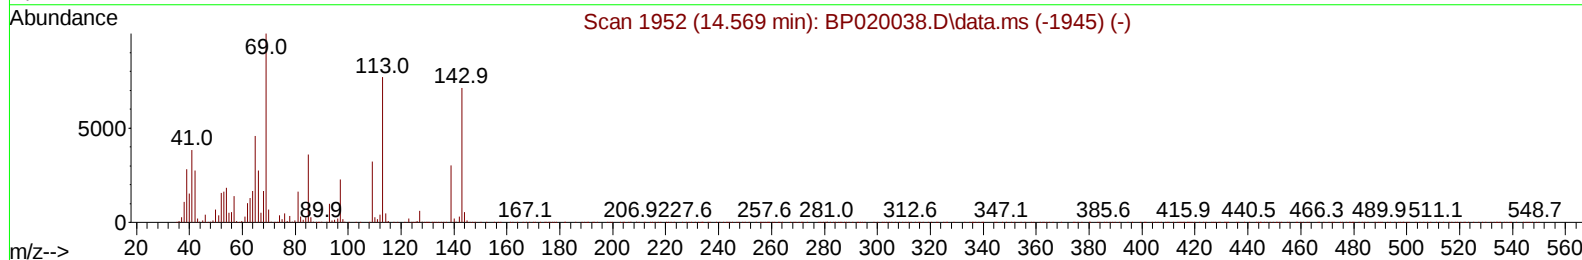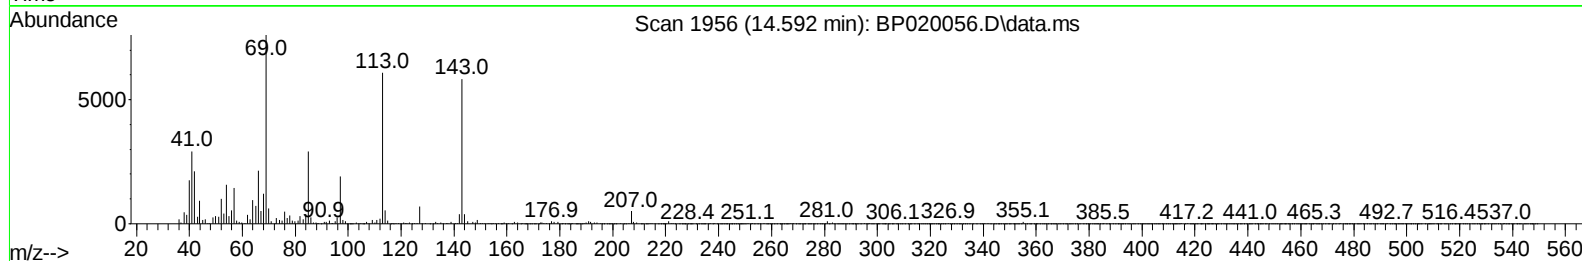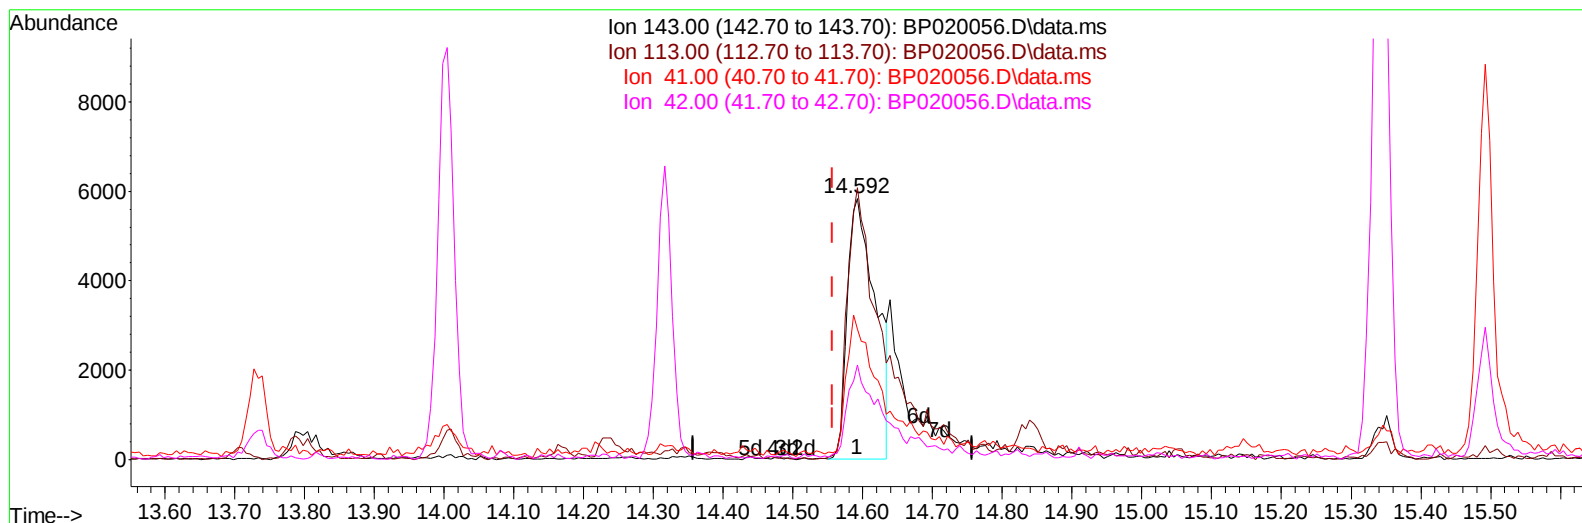

TIC: BP020056.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.592min (+ 0.035) 6.43 ng/u1

response 16354

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.80	104.04
41.00	50.70	50.01
42.00	34.00	36.30




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020056.D
Acq On : 21 Apr 2024 00:35
Operator : MA/JU
Sample : P2161-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0RE4

Manual IntegrationsAPPROVED

Quant Time: Apr 22 00:29:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 20 01:32:50 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/30/2024

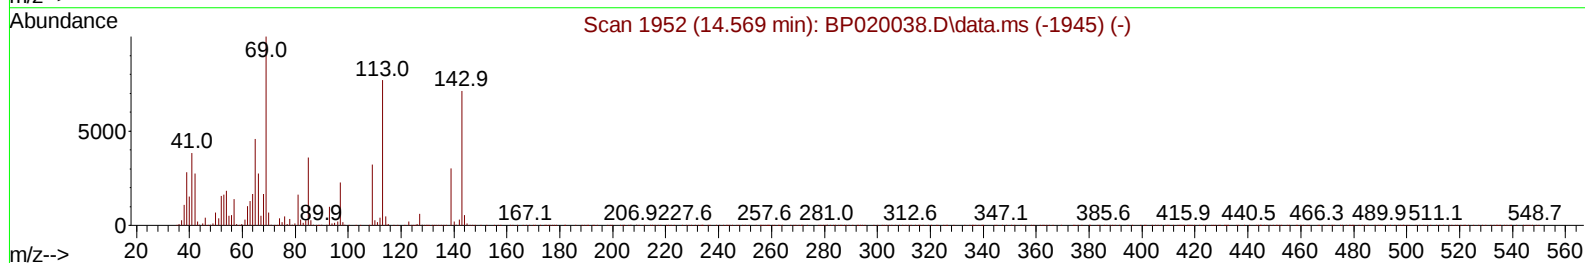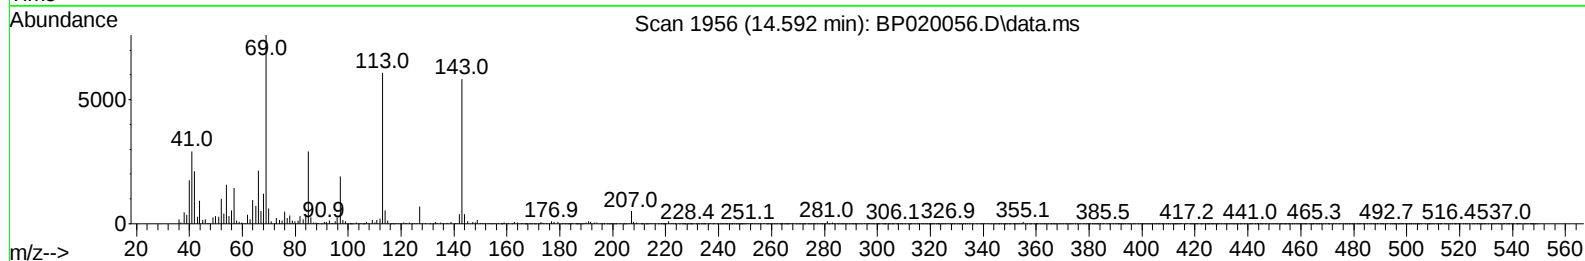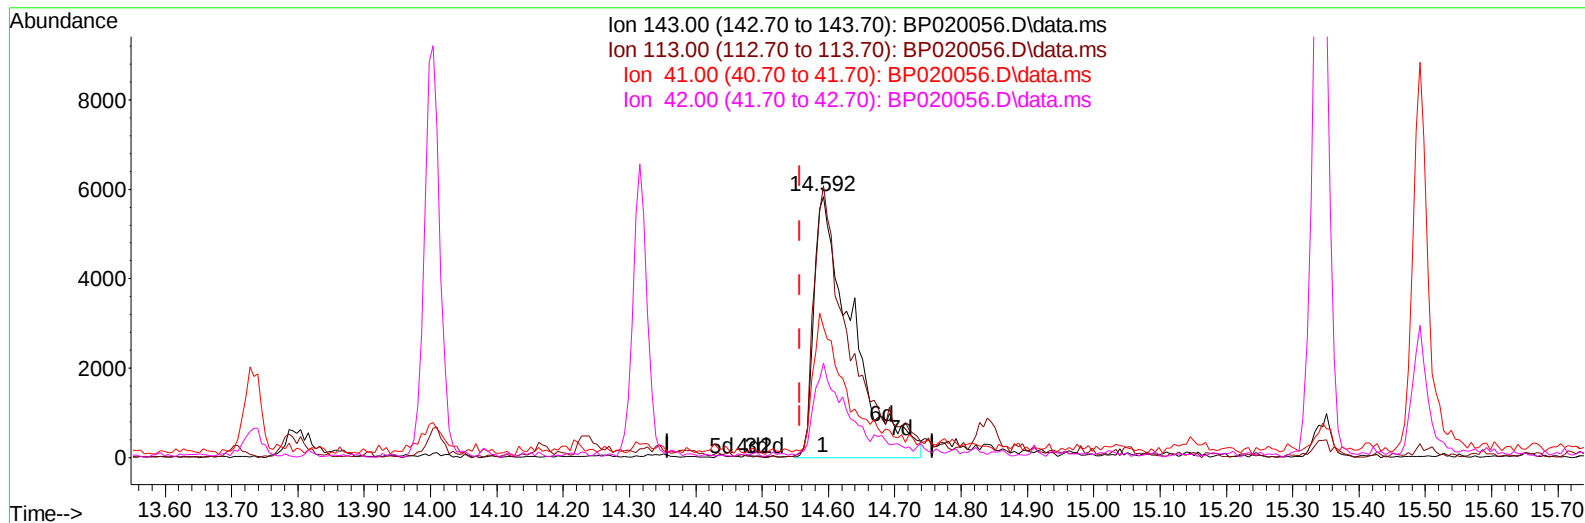

TIC: BP020056.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.592min (+ 0.035) 9.20 ng/ul m

response 23405

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.80	104.04
41.00	50.70	50.01
42.00	34.00	36.30

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020056.D
 Acq On : 21 Apr 2024 00:35
 Operator : MA/JU
 Sample : P2161-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CORE4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/30/2024

Quant Time: Apr 22 00:39:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 20 01:32:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.646	152	88773	20.000	ng/ul	0.00
20) Naphthalene-d8	10.422	136	363538	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.316	164	244631	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.163	188	512255	20.000	ng/ul	0.00
79) Chrysene-d12	21.651	240	446793	20.000	ng/ul	0.00
88) Perylene-d12	25.045	264	509951	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	9678	4.467	ng/uL	0.00
4) Pyridine-d5	3.634	84	82846	12.991	ng/ul	0.00
7) Phenol-d5	6.822	99	62746	8.110	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67	236378	43.710	ng/ul	0.00
11) 2-Chlorophenol-d4	7.175	132	180350	34.140	ng/ul	0.00
15) 4-Methylphenol-d8	8.340	113	120416	19.924	ng/ul	0.00
21) Nitrobenzene-d5	8.798	128	126487	48.370	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	139005	49.176	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.045	165	228355	40.722	ng/ul	0.00
31) 4-Chloroaniline-d4	10.569	131	271425	36.258	ng/ul	0.00
46) Dimethylphthalate-d6	13.733	166	850827	50.891	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	964730	48.414	ng/ul	0.00
54) 4-Nitrophenol-d4	14.592	143	23405m	9.196	ng/ul	0.04
60) Fluorene-d10	15.339	176	733842	49.310	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.492	200	140934	47.093	ng/ul	0.00
73) Anthracene-d10	17.263	188	1167801	50.886	ng/ul	0.00
81) Pyrene-d10	19.663	212	1328822	55.342	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.827	264	1312512	52.688	ng/ul	0.02
Target Compounds						
						Qvalue
22) Nitrobenzene	8.840	77	243319	28.551	ng/ul	99
25) 2-Nitrophenol	9.545	139	3115	1.035	ng/ul#	73
39) 1,2,4,5-Tetrachloroben...	12.463	216	138798m	17.410	ng/ul	
75) 1,2,3,4-Tetrachloroben...	13.086	216	420541	51.783	ng/uL	96
76) Pentachlorobenzene	14.639	250	15992	2.093	ng/uL	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020056.D
Acq On : 21 Apr 2024 00:35
Operator : MA/JU
Sample : P2161-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CORE4

Manual IntegrationsAPPROVED

Quant Time: Apr 22 00:39:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 20 01:32:50 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/30/2024

