




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020061.D
Acq On : 21 Apr 2024 04:11
Operator : MA/JU
Sample : P2104-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Manual IntegrationsAPPROVED

Quant Time: Apr 22 00:30:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 20 01:32:50 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/30/2024

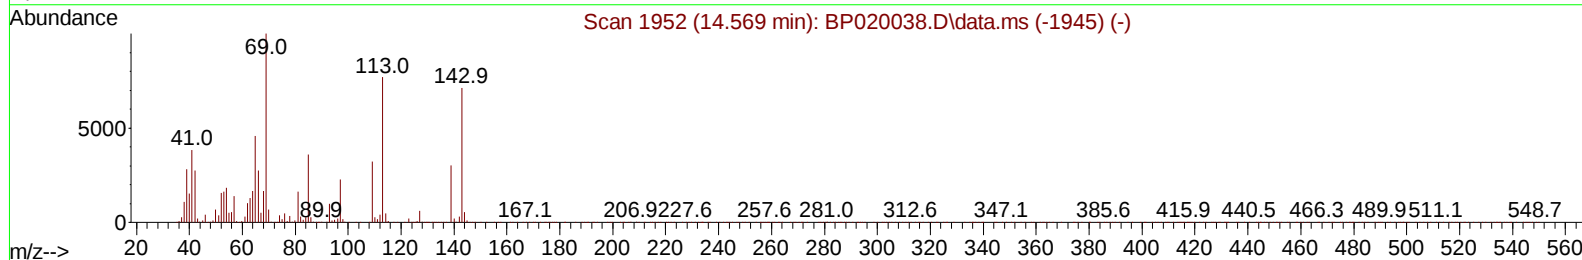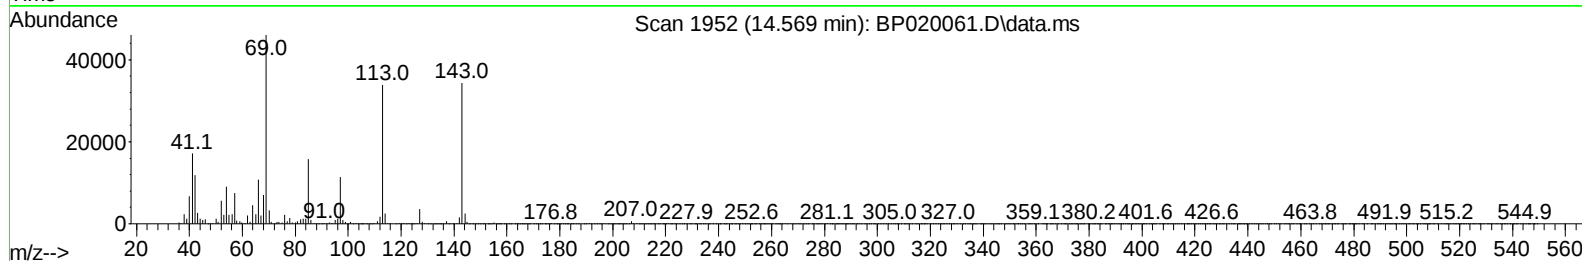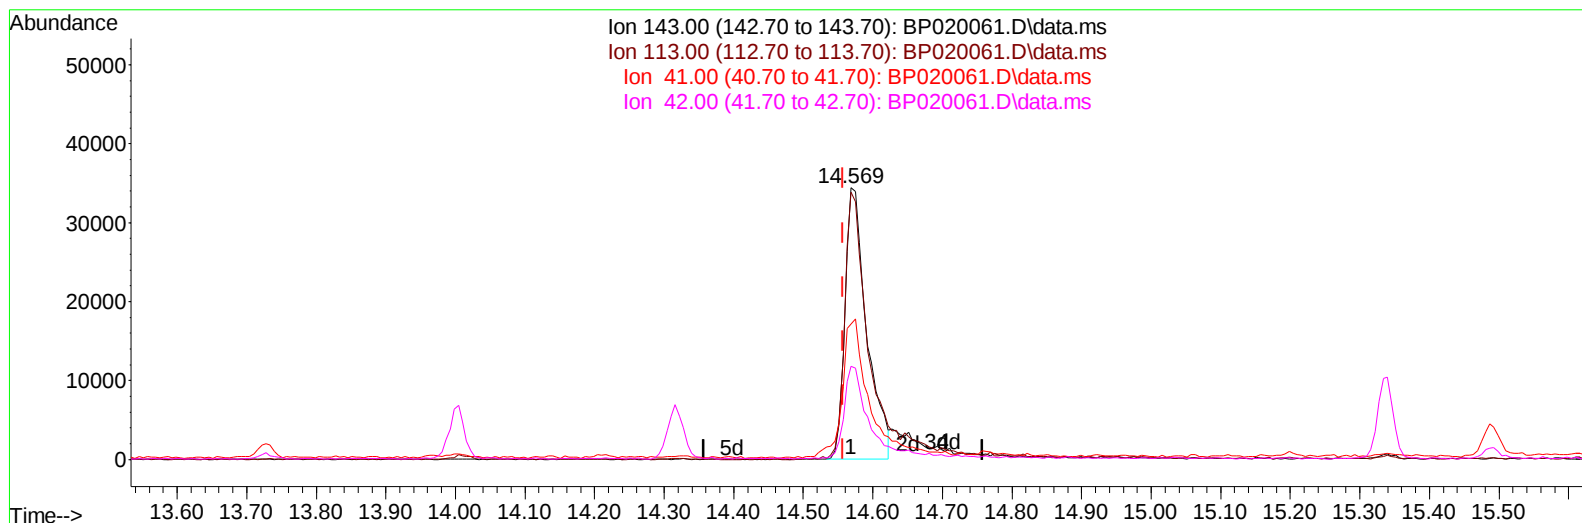

TIC: BP020061.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.569min (+ 0.012) 23.64 ng/u1

response 74540

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.80	98.37
41.00	50.70	49.77
42.00	34.00	34.42

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020061.D
 Acq On : 21 Apr 2024 04:11
 Operator : MA/JU
 Sample : P2104-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/30/2024

Quant Time: Apr 22 01:00:50 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 20 01:32:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	106448	20.000	ng/ul	0.00
20) Naphthalene-d8	10.410	136	454815	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.316	164	303143	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.157	188	593018	20.000	ng/ul	0.00
79) Chrysene-d12	21.663	240	507866	20.000	ng/ul	0.00
88) Perylene-d12	25.063	264	578146	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	11376	4.379	ng/uL	0.00
4) Pyridine-d5	3.634	84	156491	20.465	ng/ul	0.00
7) Phenol-d5	6.828	99	249161	26.857	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67	173923	26.821	ng/ul	0.00
11) 2-Chlorophenol-d4	7.175	132	178672	28.207	ng/ul	0.00
15) 4-Methylphenol-d8	8.346	113	204530	28.223	ng/ul	0.00
21) Nitrobenzene-d5	8.799	128	94896	29.006	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	108040	30.551	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.046	165	188327	26.844	ng/ul	0.00
31) 4-Chloroaniline-d4	10.569	131	264396	28.231	ng/ul	0.00
46) Dimethylphthalate-d6	13.728	166	644250	31.097	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	740016	29.969	ng/ul	0.00
54) 4-Nitrophenol-d4	14.569	143	84207m	26.701	ng/ul	0.01
60) Fluorene-d10	15.339	176	556306	30.165	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.487	200	68711	19.833	ng/ul	0.00
73) Anthracene-d10	17.263	188	809582	30.472	ng/ul	0.00
81) Pyrene-d10	19.663	212	896814	32.858	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.833	264	887027	31.408	ng/ul	0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020061.D
Acq On : 21 Apr 2024 04:11
Operator : MA/JU
Sample : P2104-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:00:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 20 01:32:50 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/30/2024

