




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020064.D
Acq On : 21 Apr 2024 06:19
Operator : MA/JU
Sample : P2104-07MSD
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 00:31:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 20 01:32:50 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/30/2024

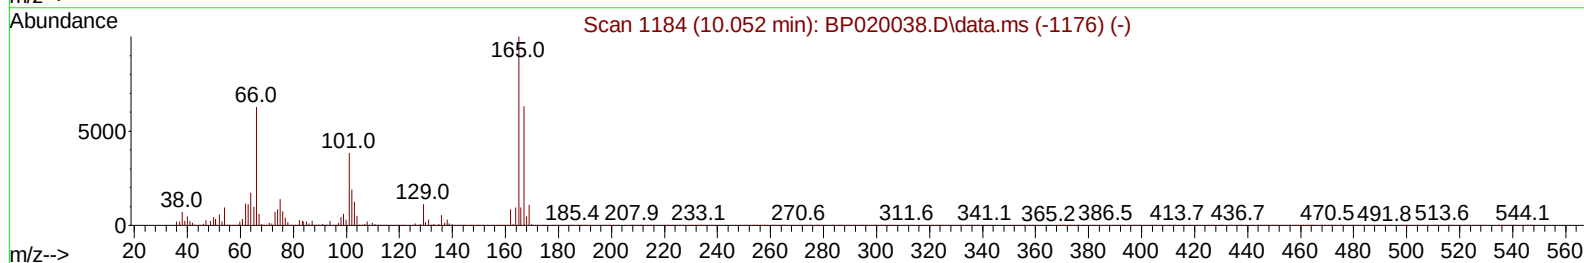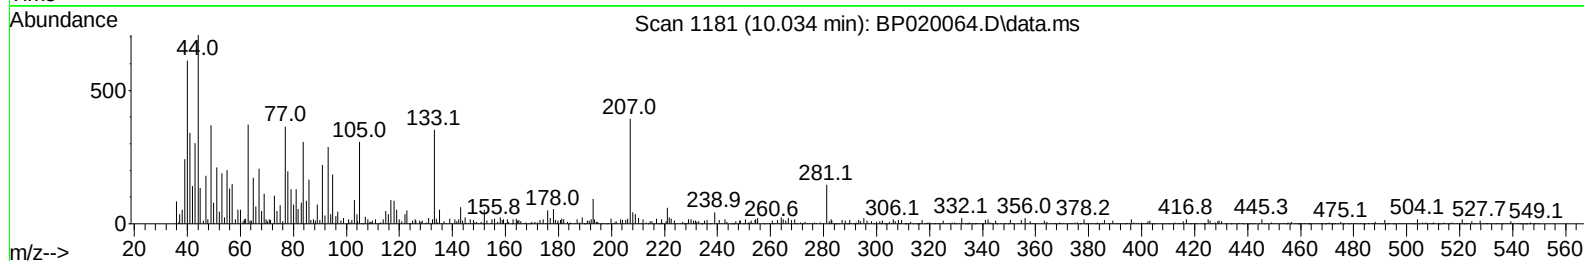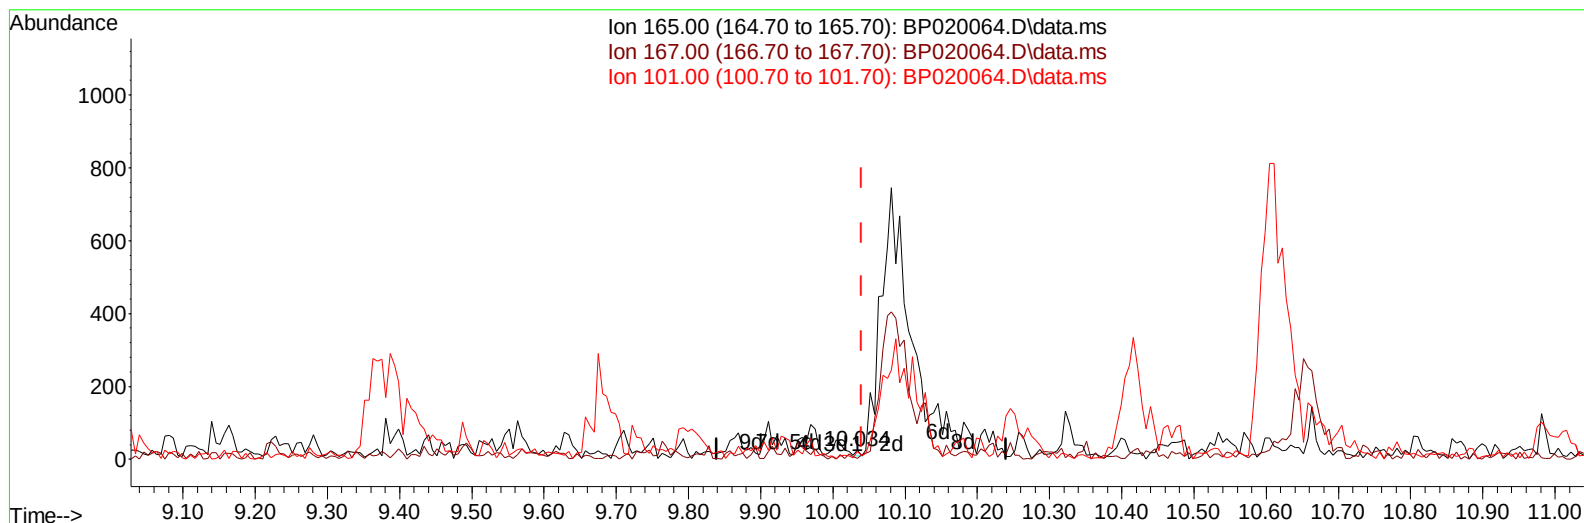

TIC: BP020064.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.034min (-0.006) 0.00 ng/ul

response 6

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.30	5.88#
101.00	40.90	64.71#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020064.D
 Acq On : 21 Apr 2024 06:19
 Operator : MA/JU
 Sample : P2104-07MSD
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 00:31:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 20 01:32:50 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/30/2024

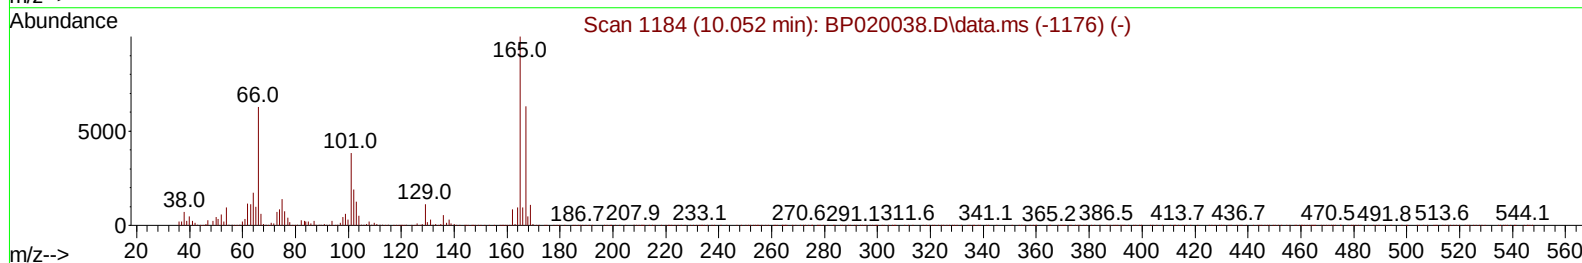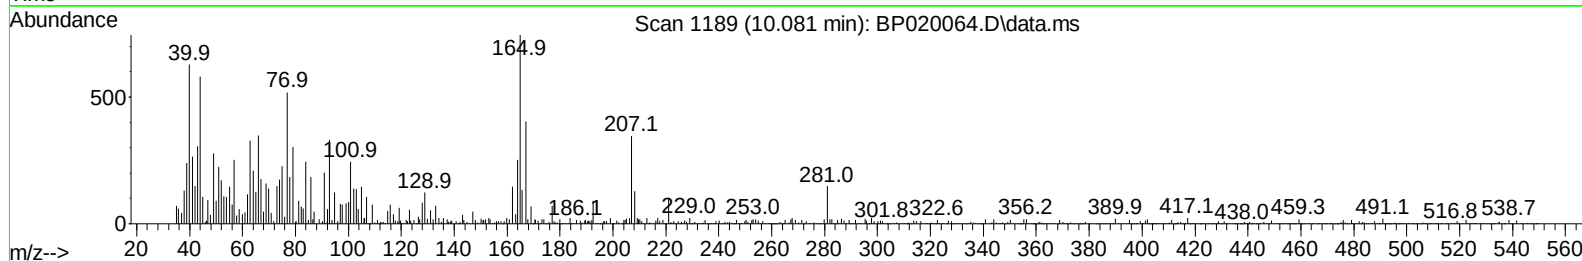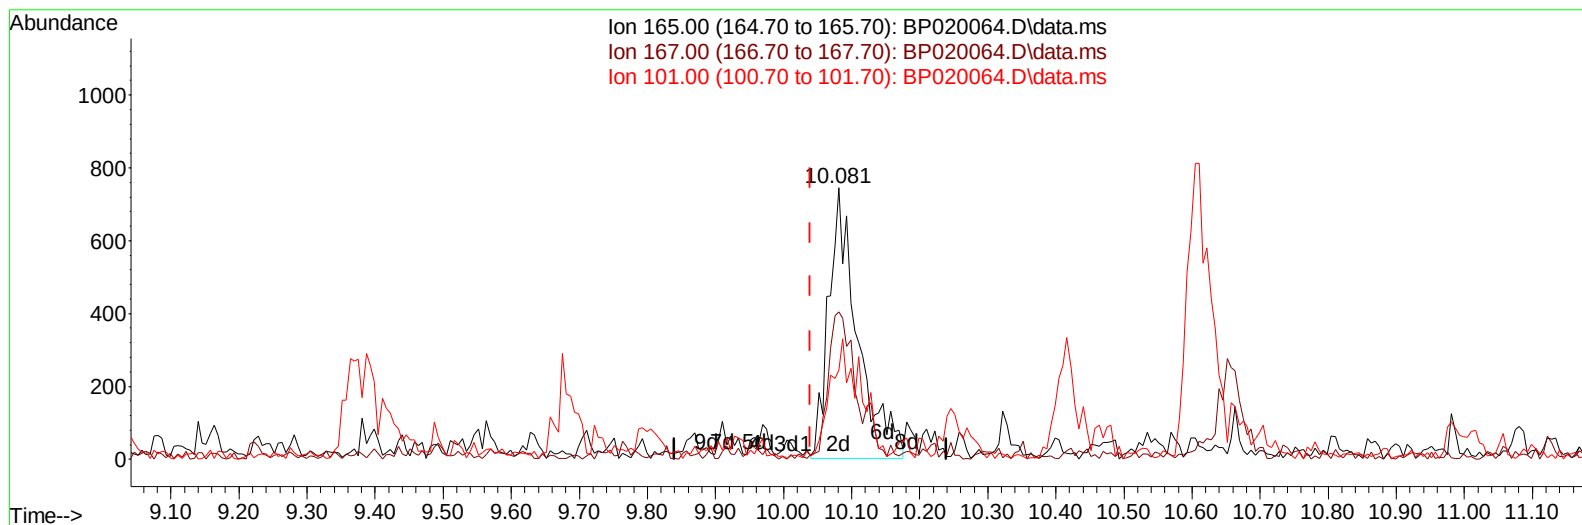

TIC: BP020064.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.081min (+ 0.041) 0.30 ng/ul m

response 2184

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.30	54.23
101.00	40.90	32.75
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020064.D
 Acq On : 21 Apr 2024 06:19
 Operator : MA/JU
 Sample : P2104-07MSD
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:21:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 20 01:32:50 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/30/2024

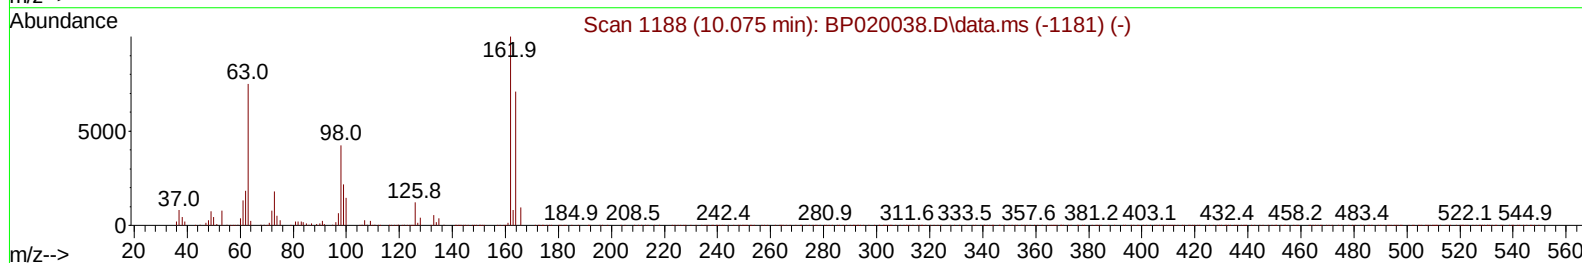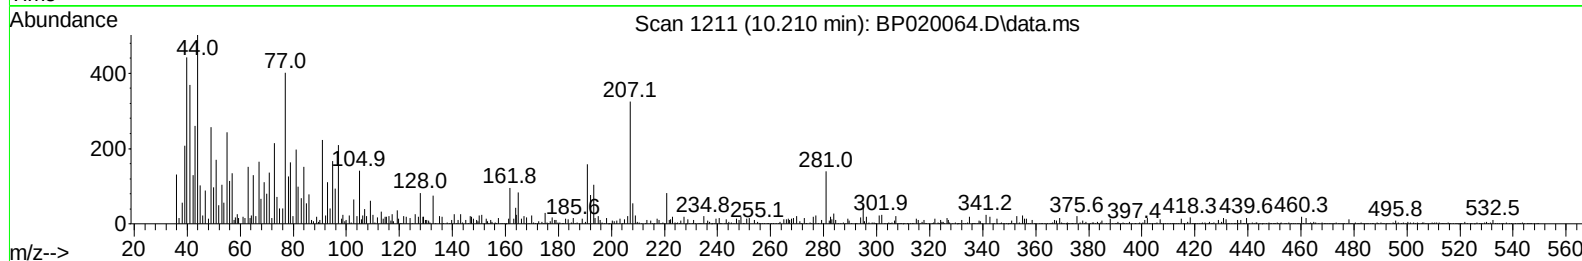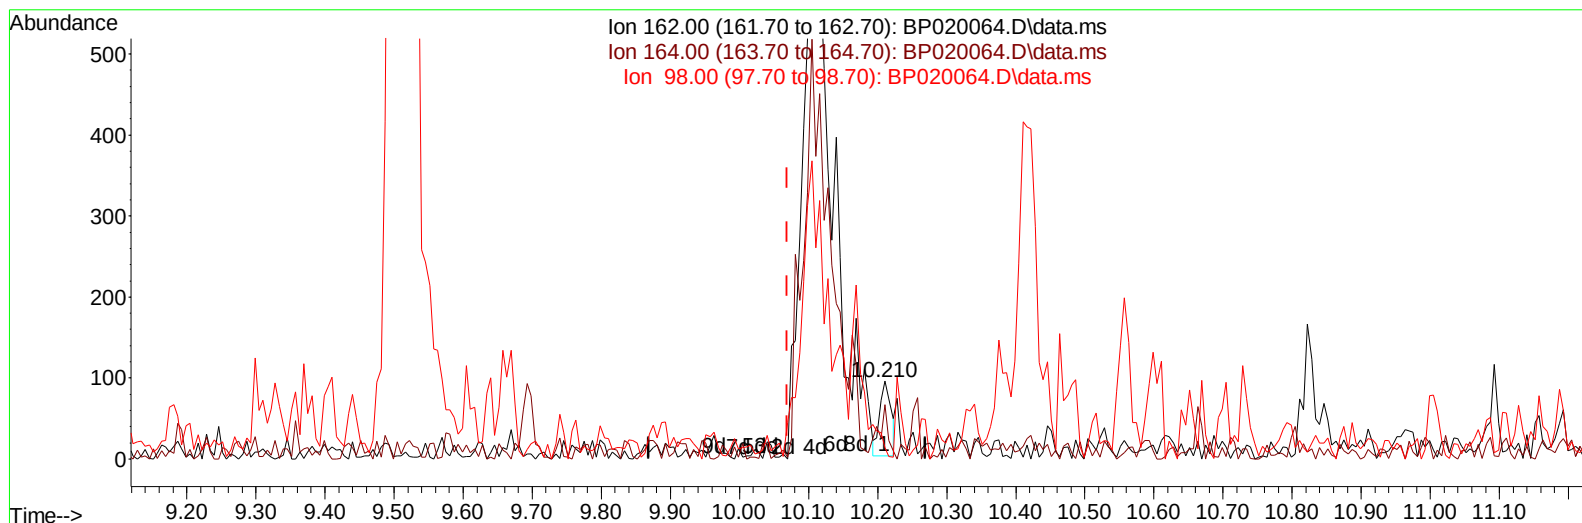

TIC: BP020064.D\data.ms

(29) 2,4-Dichlorophenol (C)

10.210min (+ 0.141) 0.01 ng/ul

response 106

Ion	Exp%	Act%
162.00	100.00	100.00
164.00	64.60	69.79
98.00	41.00	39.58
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020064.D
Acq On : 21 Apr 2024 06:19
Operator : MA/JU
Sample : P2104-07MSD
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:21:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 20 01:32:50 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/30/2024

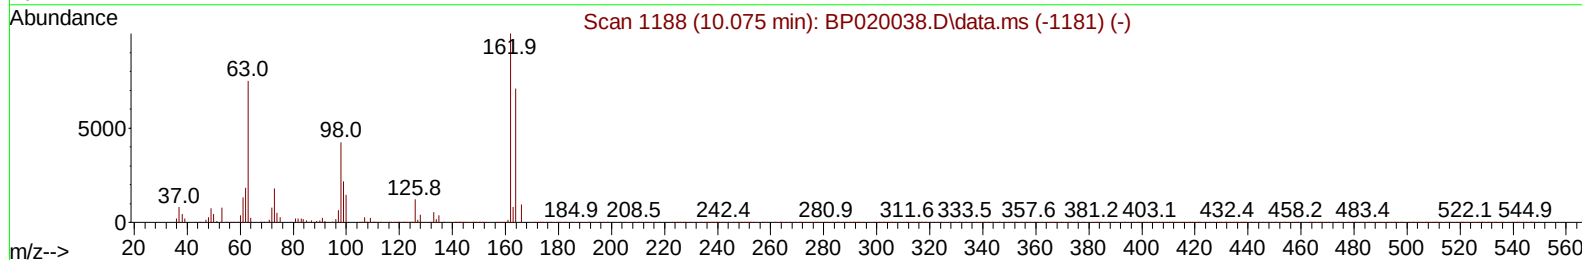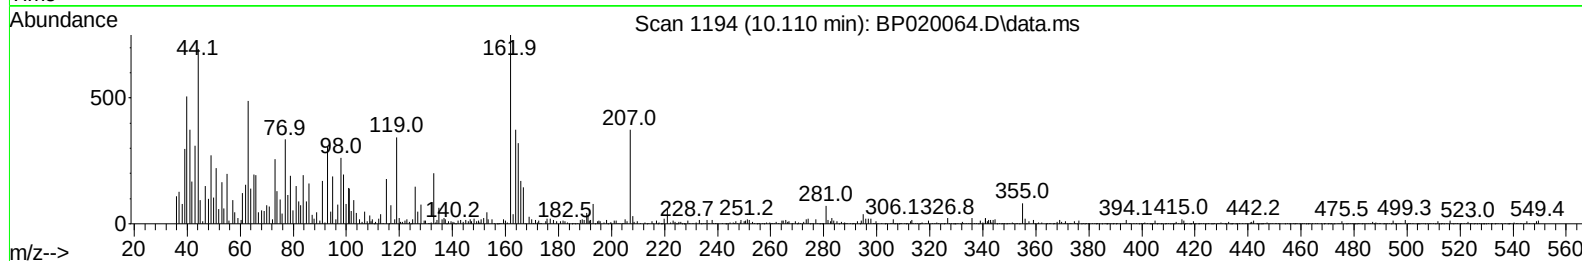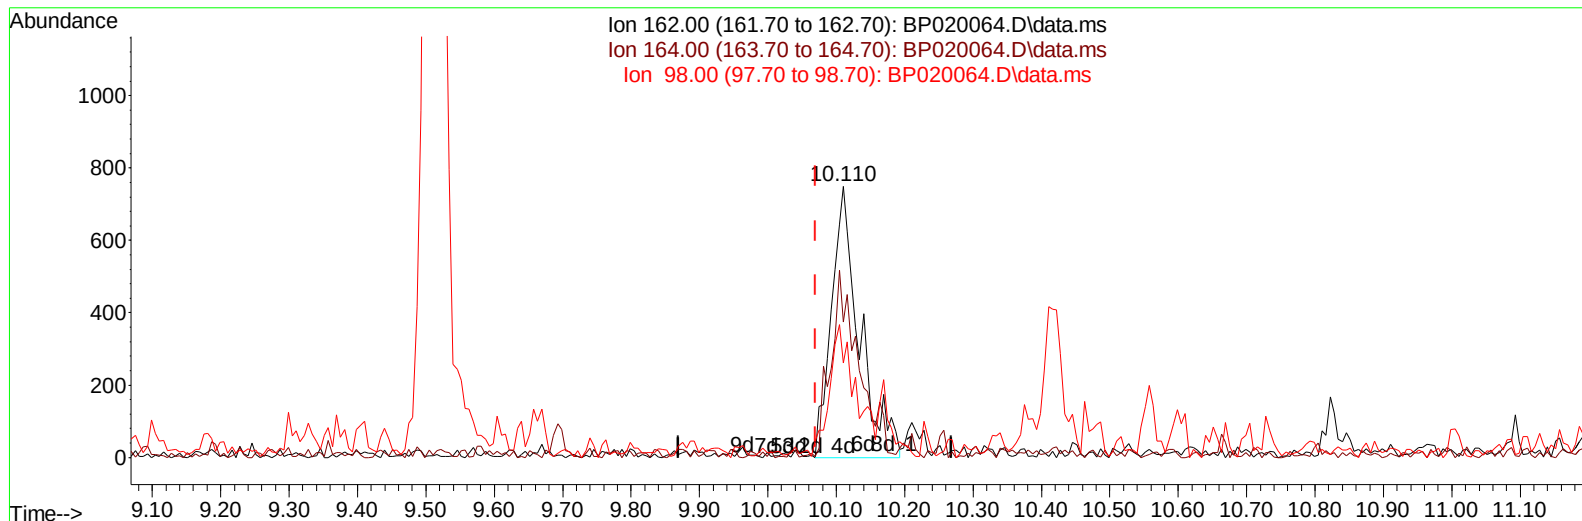

TIC: BP020064.D\data.ms

(29) 2,4-Dichlorophenol (C)

10.110min (+ 0.041) 0.30 ng/ul m

response 2114

Ion	Exp%	Act%
162.00	100.00	100.00
164.00	64.60	49.87#
98.00	41.00	34.80
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020064.D
Acq On : 21 Apr 2024 06:19
Operator : MA/JU
Sample : P2104-07MSD
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:22:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 20 01:32:50 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/30/2024

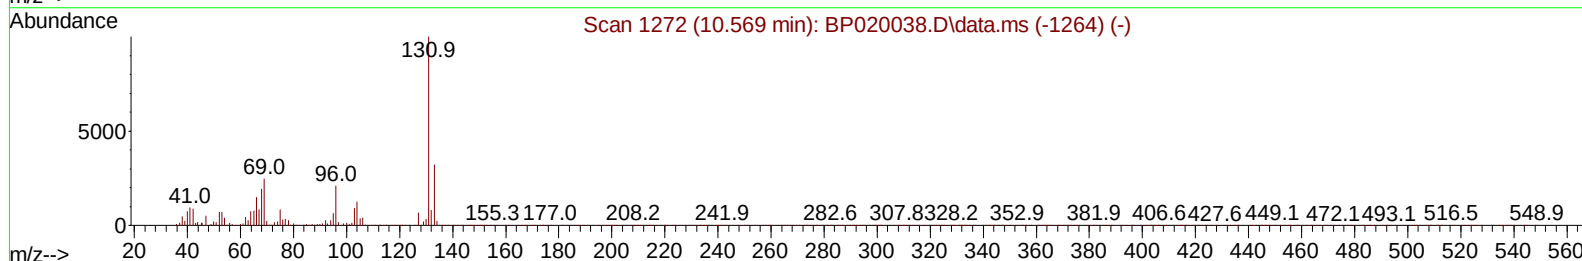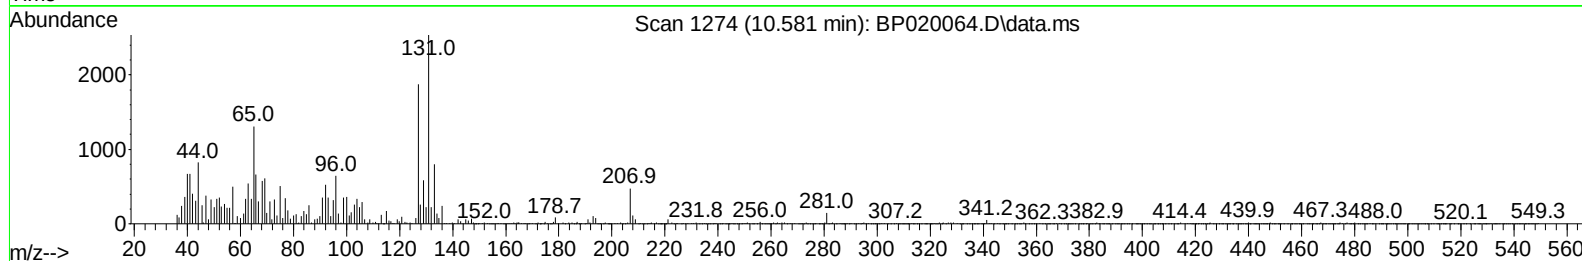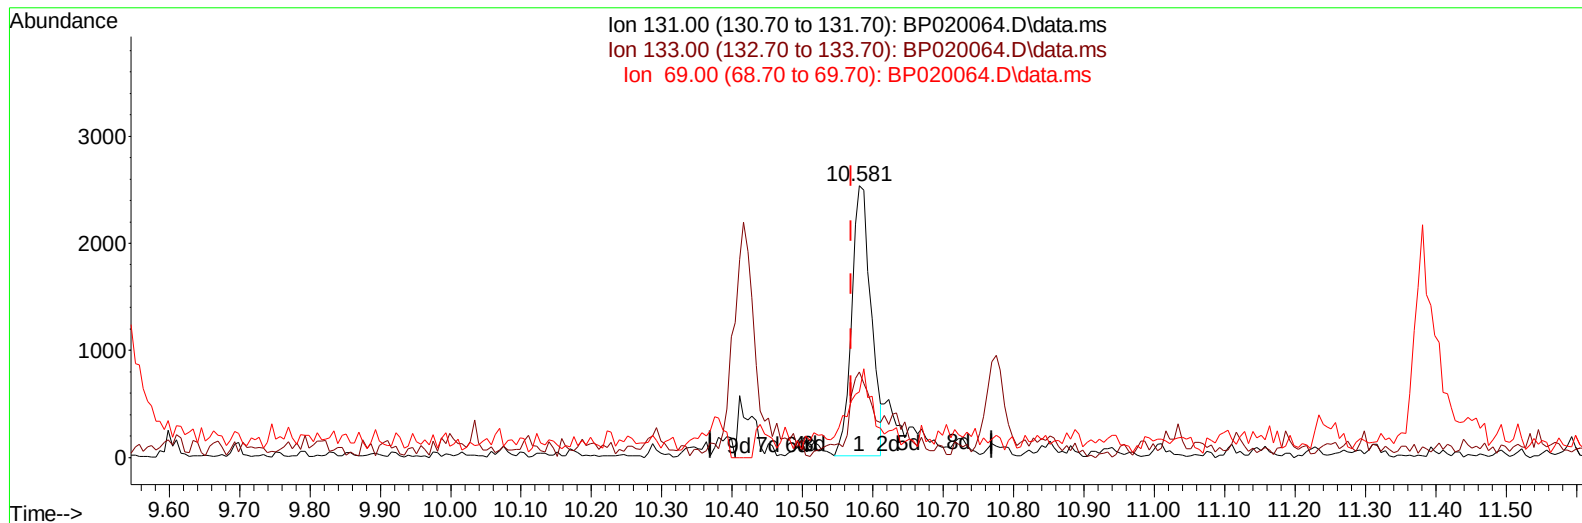

TIC: BP020064.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.581min (+ 0.012) 0.49 ng/u1

response 4787

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.10	31.39
69.00	23.50	24.21
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020064.D
Acq On : 21 Apr 2024 06:19
Operator : MA/JU
Sample : P2104-07MSD
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:22:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 20 01:32:50 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/30/2024

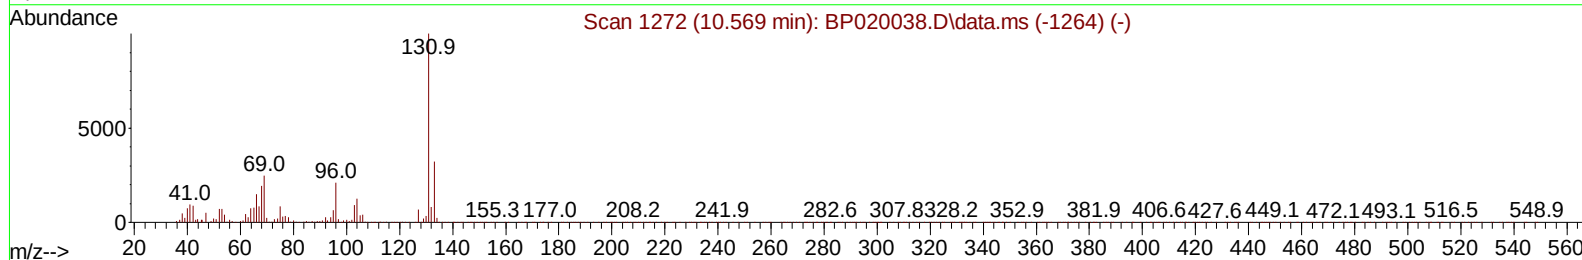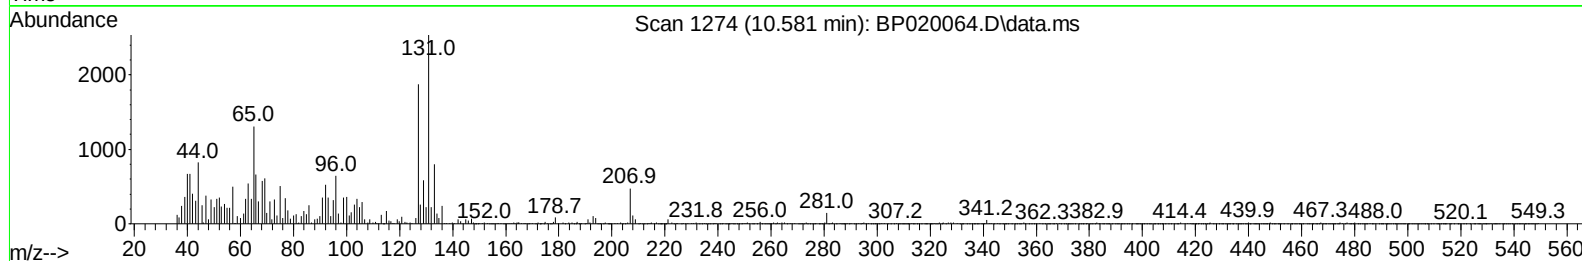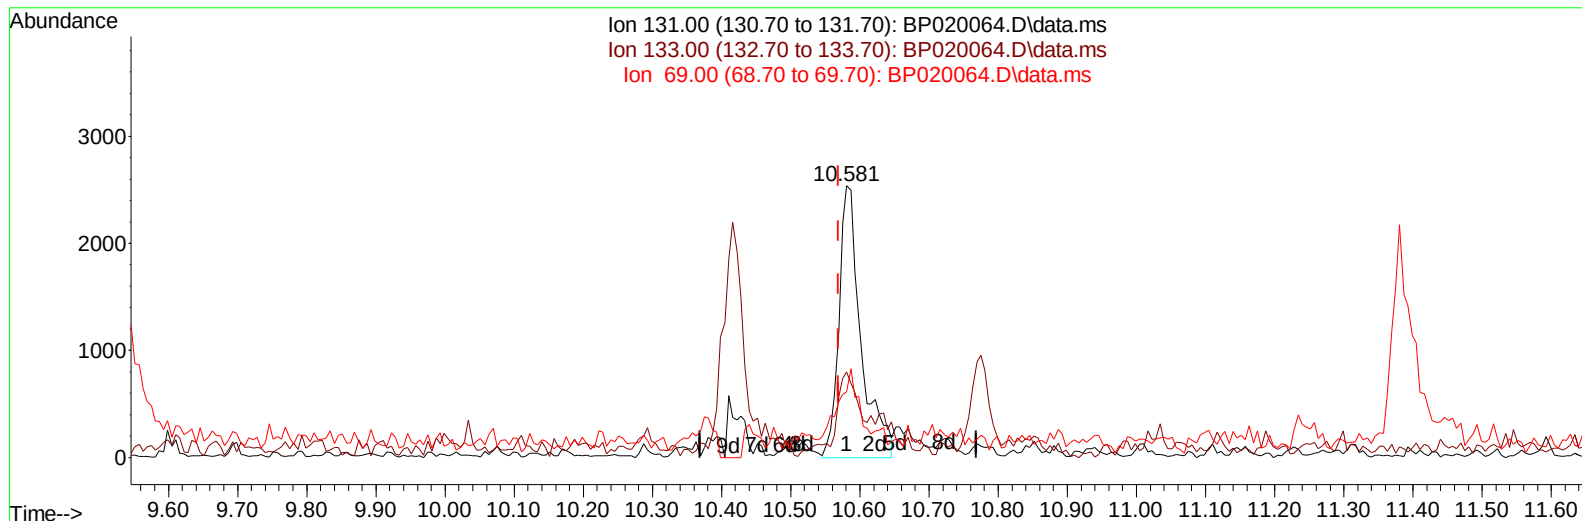

TIC: BP020064.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.581min (+ 0.012) 0.58 ng/ul m

response 5630

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.10	31.39
69.00	23.50	24.21
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020064.D
Acq On : 21 Apr 2024 06:19
Operator : MA/JU
Sample : P2104-07MSD
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:22:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 20 01:32:50 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/30/2024

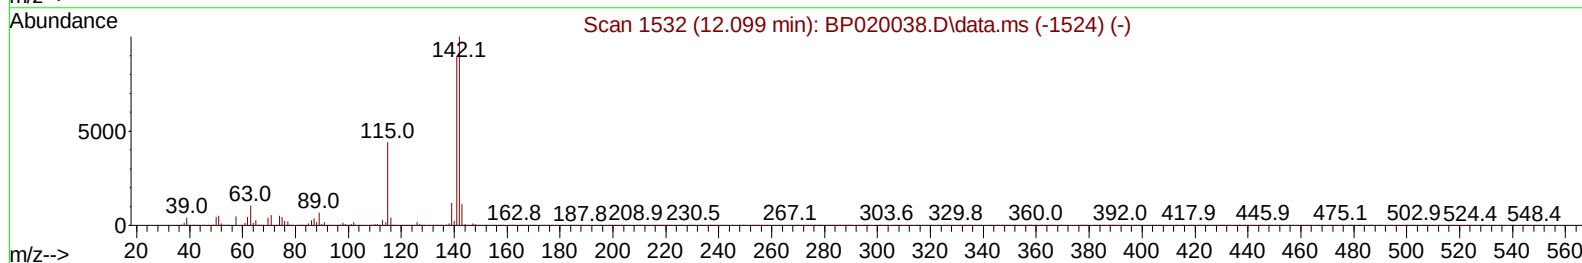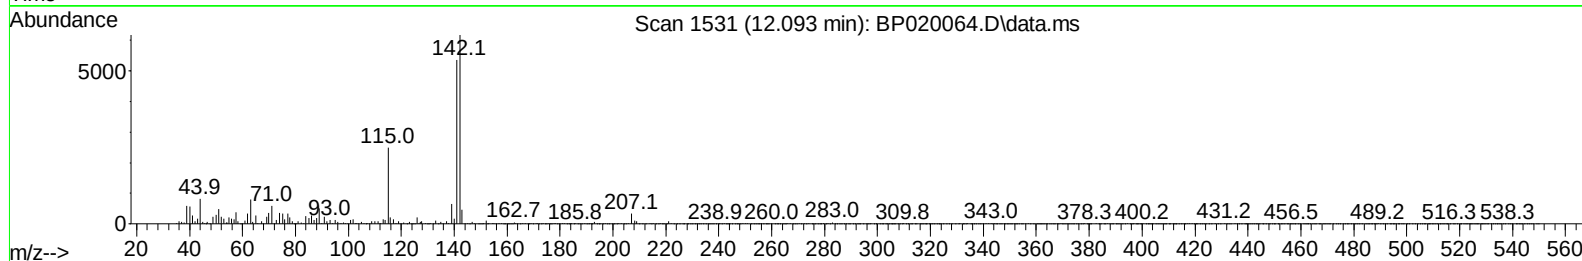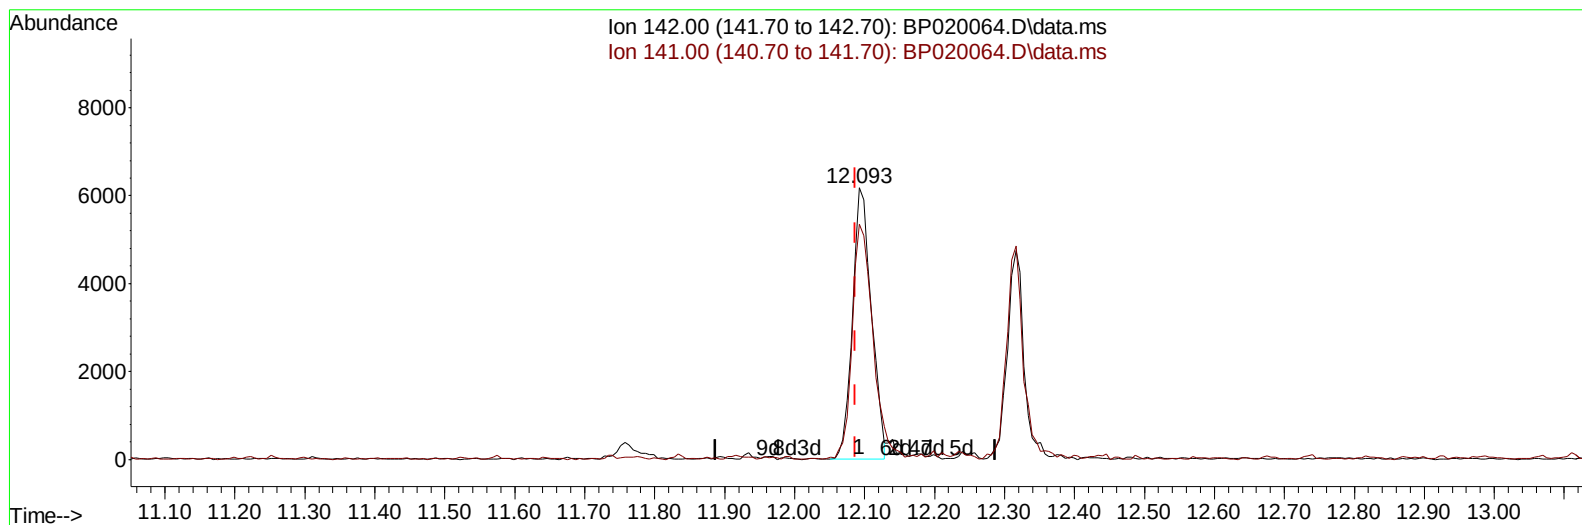

TIC: BP020064.D\data.ms

(36) 2-Methylnaphthalene

12.093min (+ 0.006) 0.68 ng/u1

response 11554

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	90.10	86.63
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020064.D
 Acq On : 21 Apr 2024 06:19
 Operator : MA/JU
 Sample : P2104-07MSD
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:22:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 20 01:32:50 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/30/2024

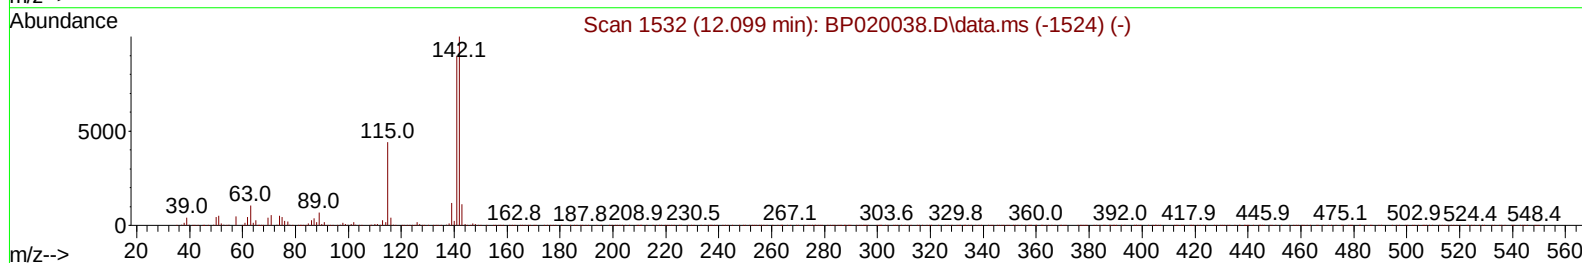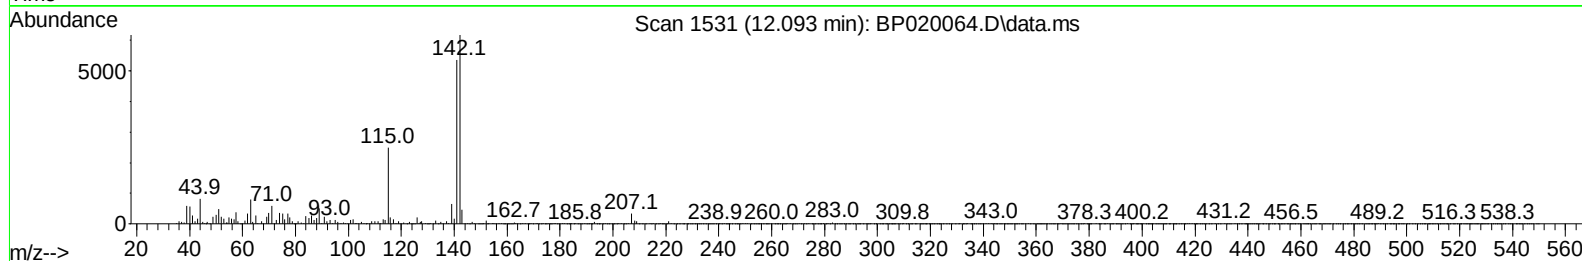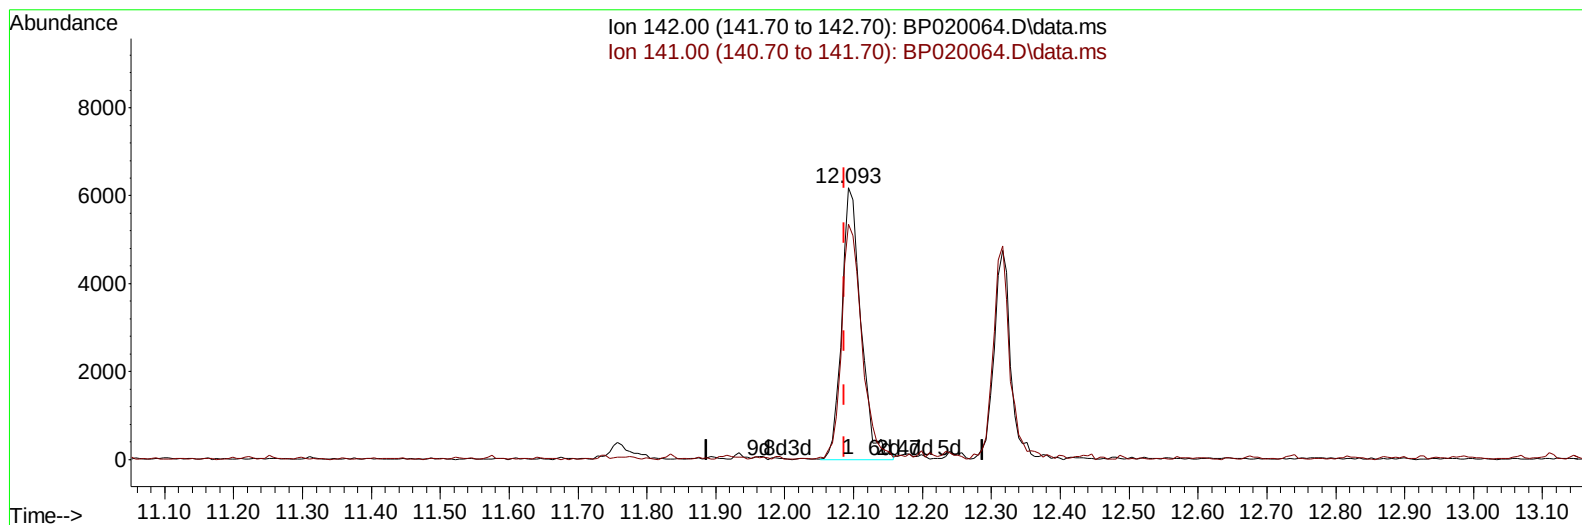

TIC: BP020064.D\data.ms

(36) 2-Methylnaphthalene

12.093min (+ 0.006) 0.71 ng/ul m

response 12042

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	90.10	86.63
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020064.D
Acq On : 21 Apr 2024 06:19
Operator : MA/JU
Sample : P2104-07MSD
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:22:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 20 01:32:50 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/30/2024

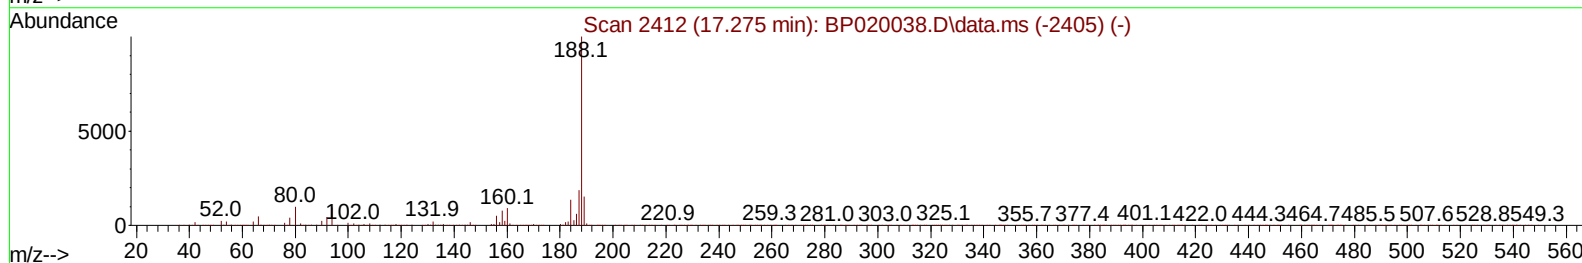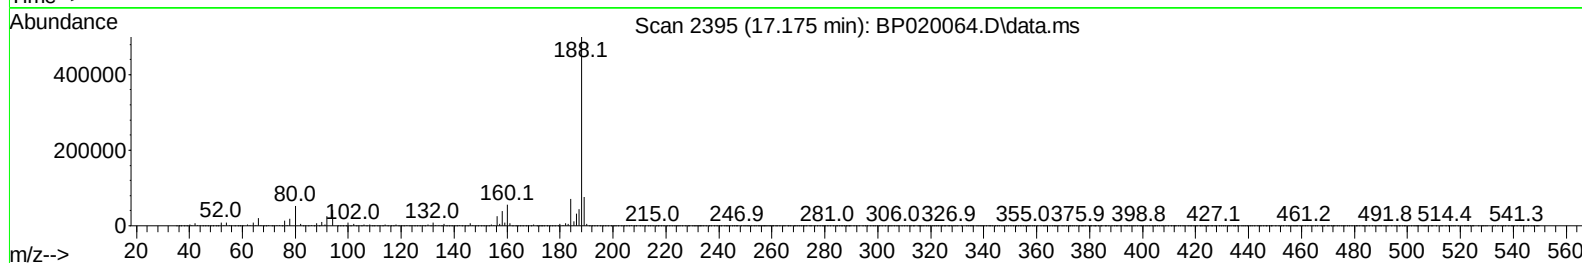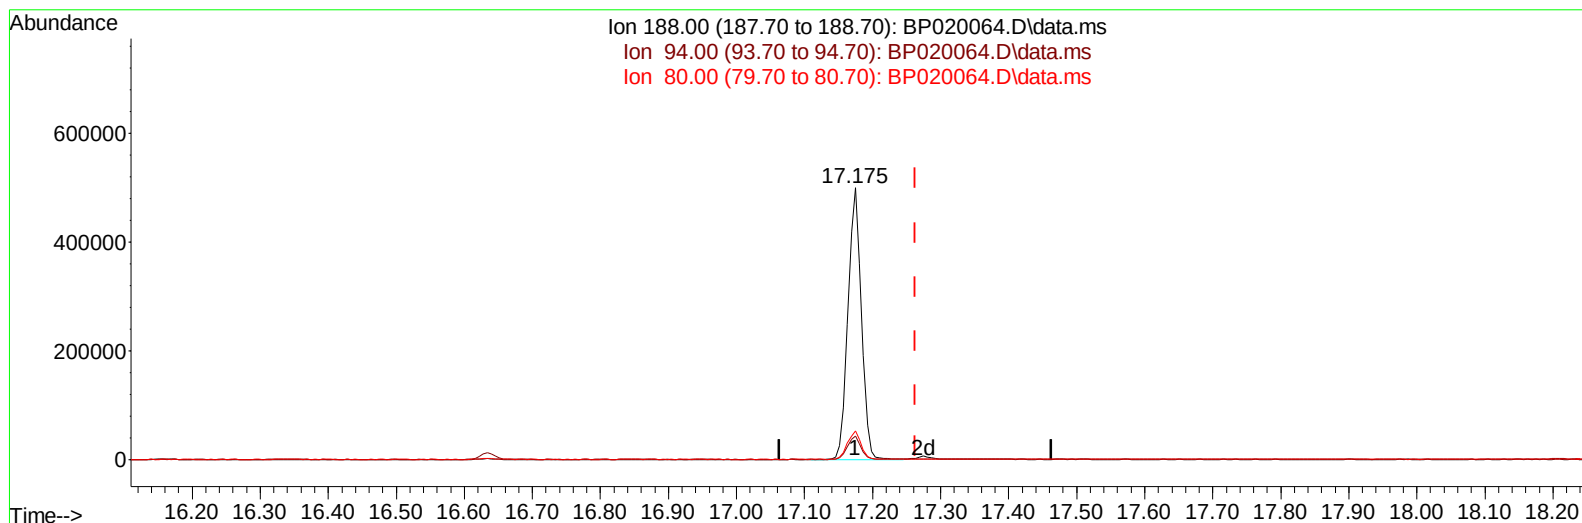

TIC: BP020064.D\data.ms

(73) Anthracene-d10 (S)

17.175min (-0.088) 22.32 ng/u1

response 682744

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.40	8.65
80.00	10.20	10.45
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020064.D
Acq On : 21 Apr 2024 06:19
Operator : MA/JU
Sample : P2104-07MSD
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:22:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 20 01:32:50 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/30/2024

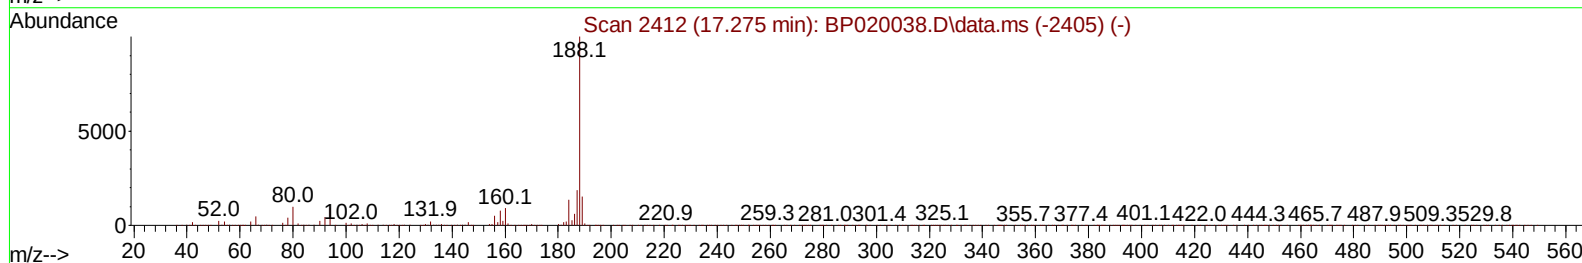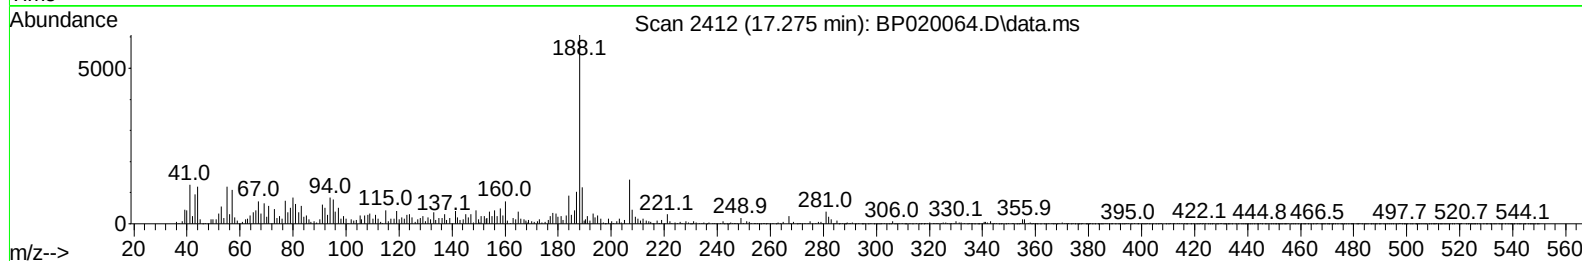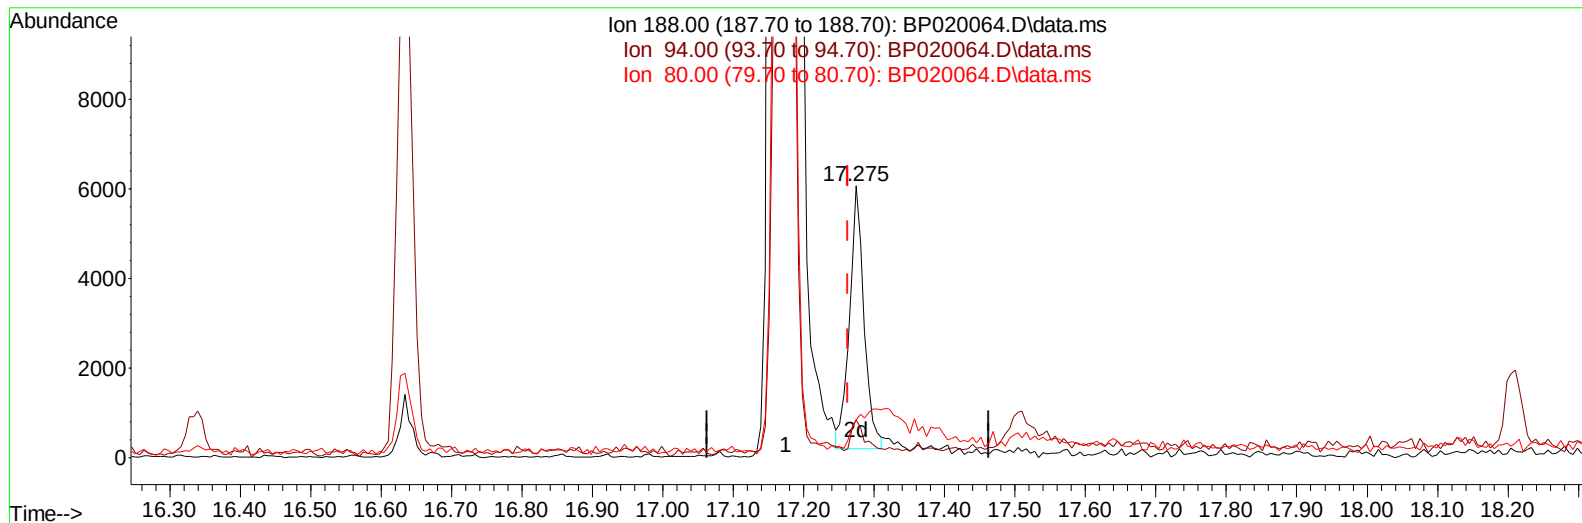

TIC: BP020064.D\data.ms

(73) Anthracene-d10 (S)

17.275min (+ 0.012) 0.27 ng/ul m

response 8403

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.40	13.86#
80.00	10.20	13.79#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020064.D
 Acq On : 21 Apr 2024 06:19
 Operator : MA/JU
 Sample : P2104-07MSD
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:26:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 20 01:32:50 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/30/2024

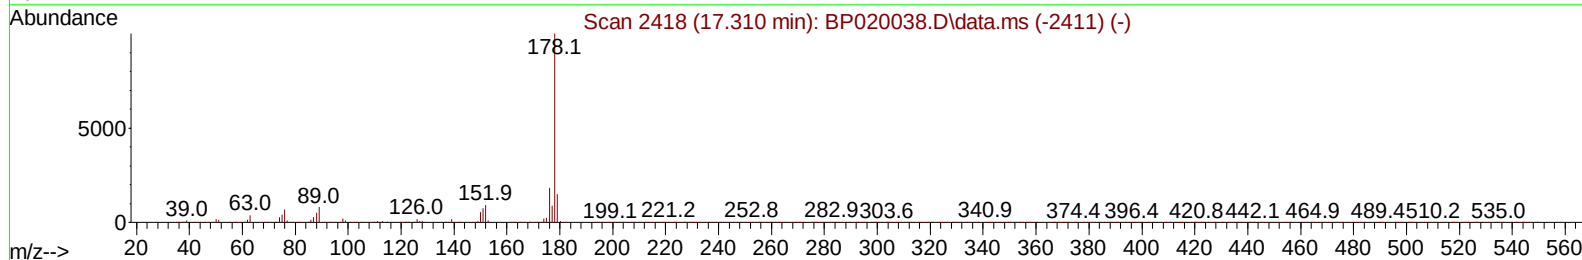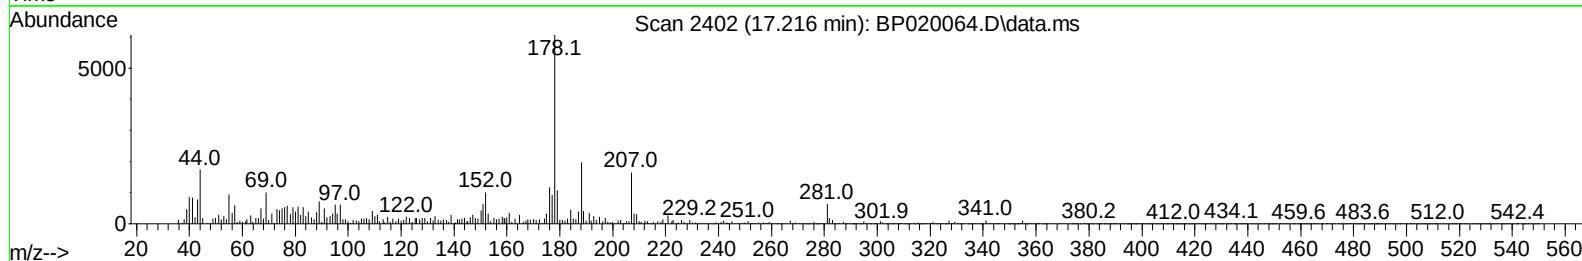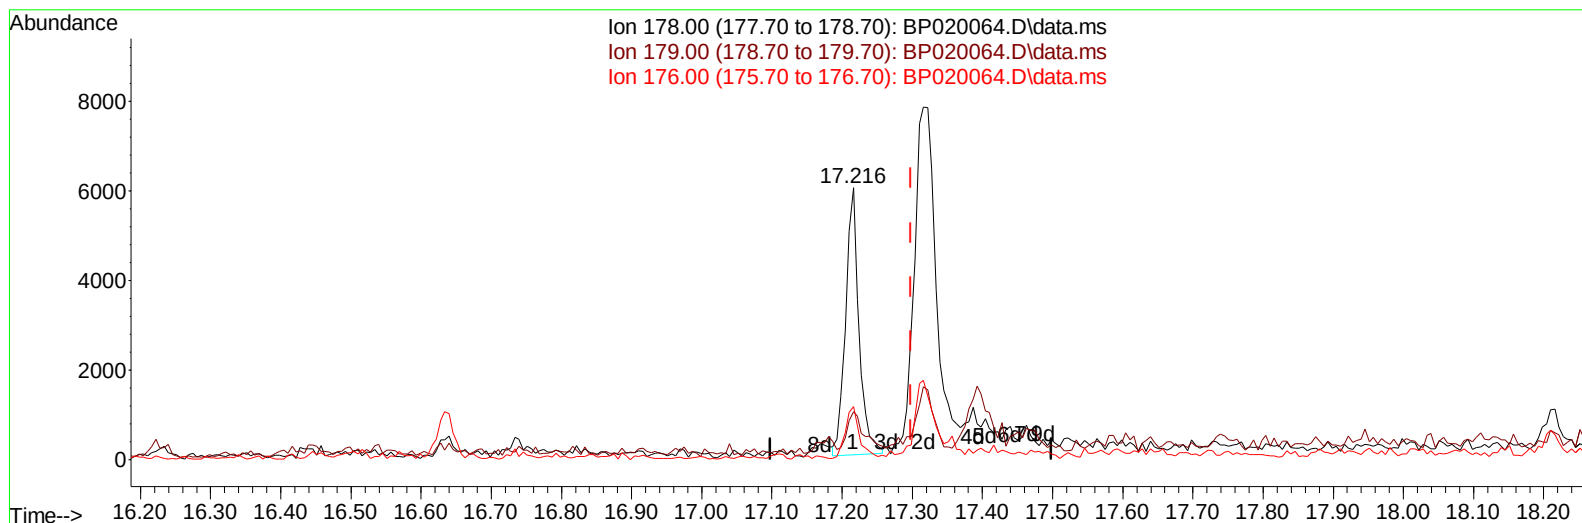

TIC: BP020064.D\data.ms

(74) Anthracene

17.216min (-0.082) 0.22 ng/u1

response 7928

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.30	17.50
176.00	18.20	19.43
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020064.D
 Acq On : 21 Apr 2024 06:19
 Operator : MA/JU
 Sample : P2104-07MSD
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:26:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 20 01:32:50 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/30/2024

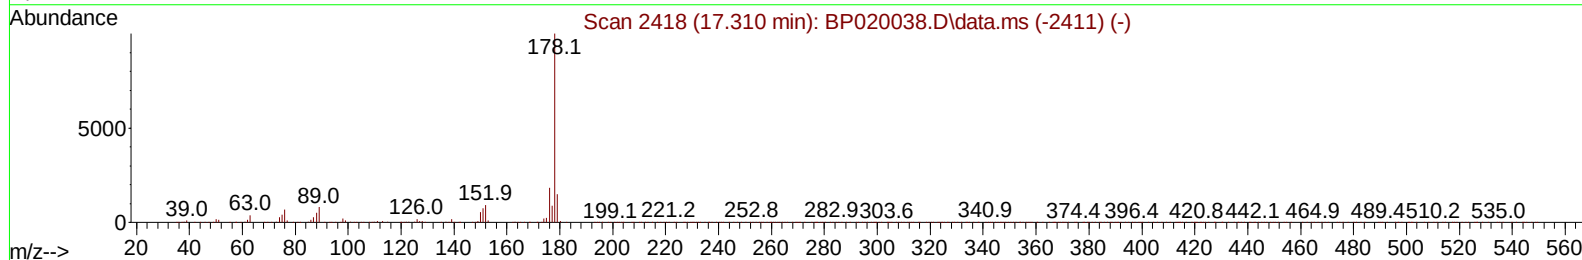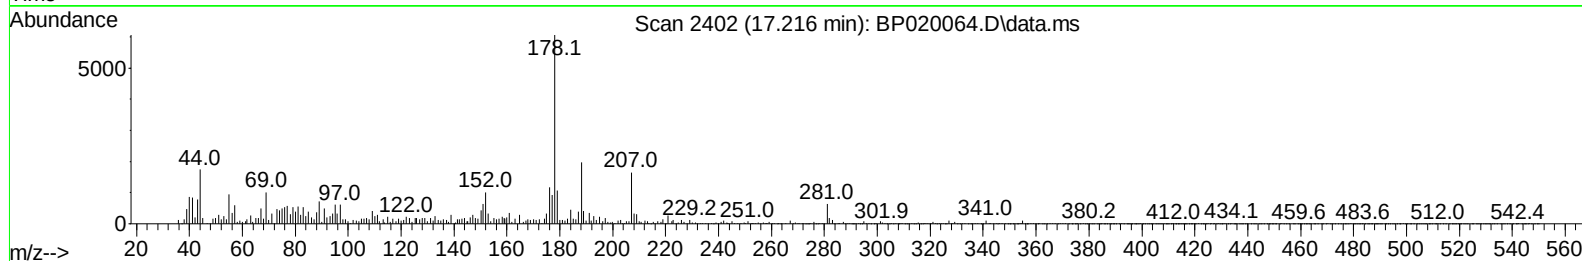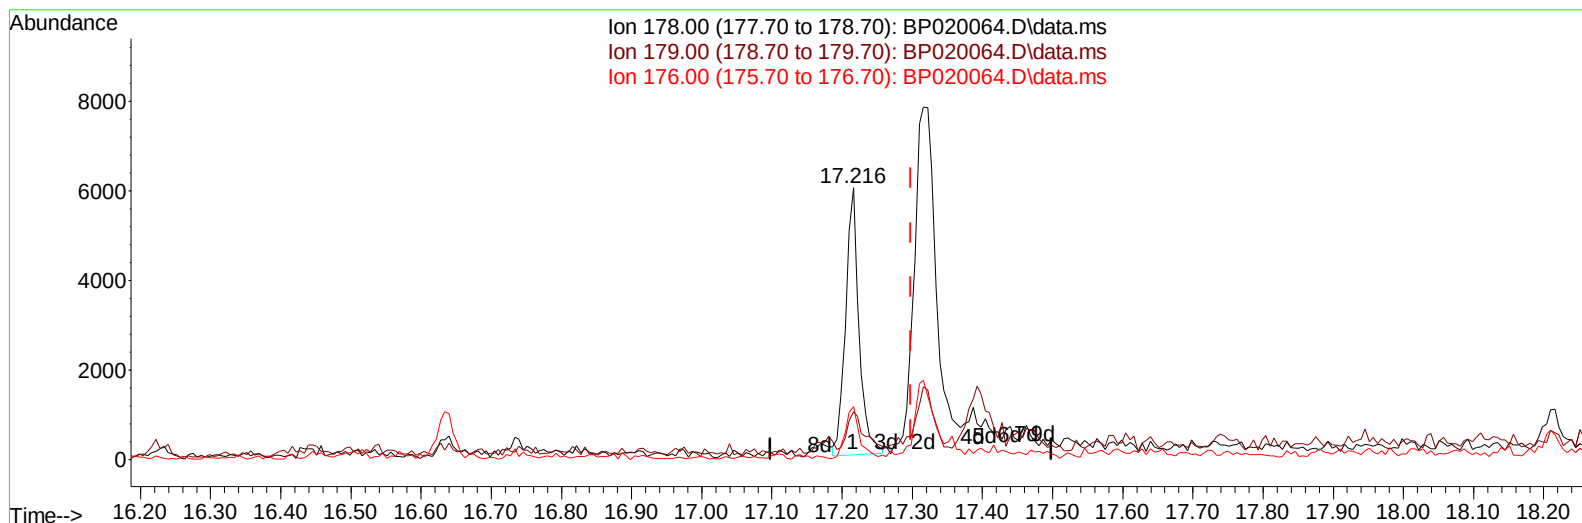

TIC: BP020064.D\data.ms

(74) Anthracene

17.216min (-0.082) 0.22 ng/u1

response 7928

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.30	17.50
176.00	18.20	19.43
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020064.D
 Acq On : 21 Apr 2024 06:19
 Operator : MA/JU
 Sample : P2104-07MSD
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:26:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 20 01:32:50 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/30/2024

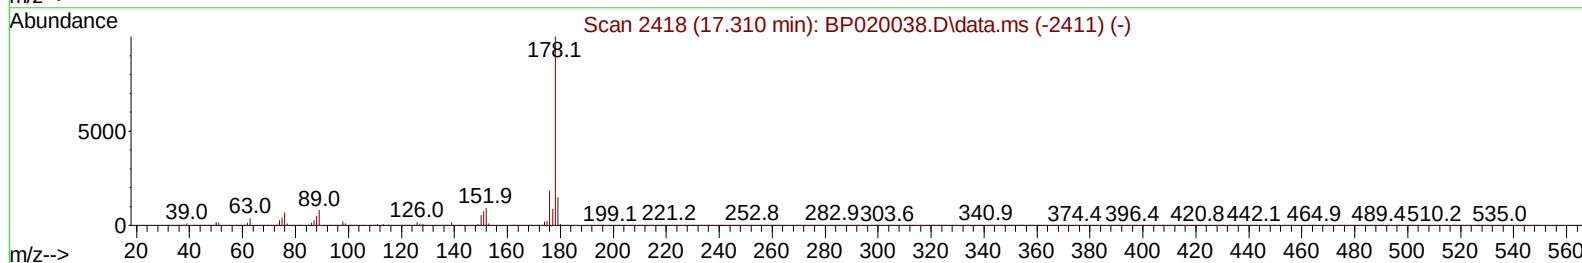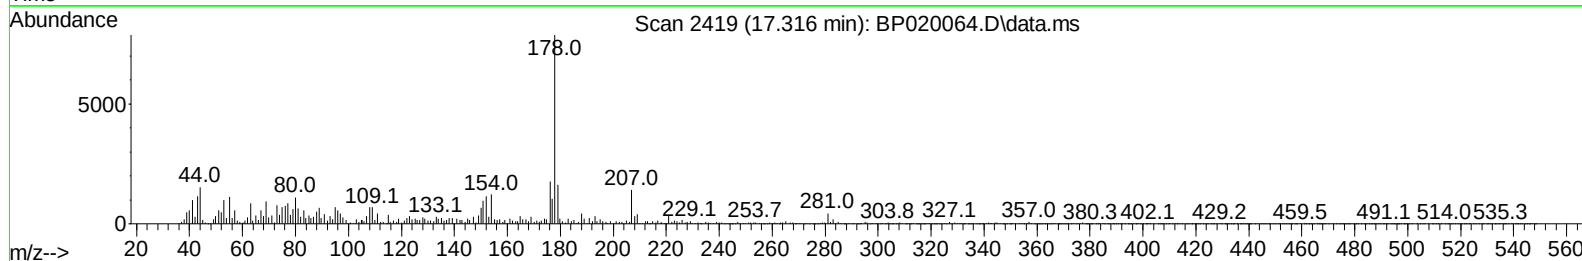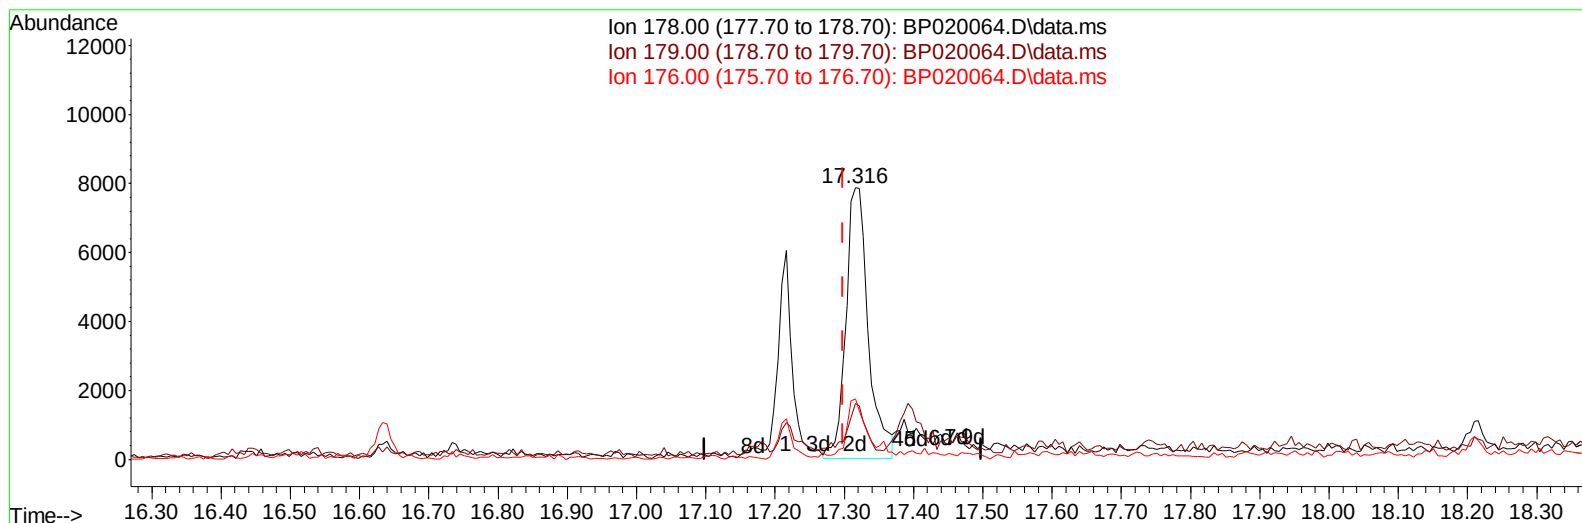

TIC: BP020064.D\data.ms

(74) Anthracene

17.316min (+ 0.018) 0.49 ng/ul m

response 17631

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.30	20.71#
176.00	18.20	22.37#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020064.D
Acq On : 21 Apr 2024 06:19
Operator : MA/JU
Sample : P2104-07MSD
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:26:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 20 01:32:50 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/30/2024

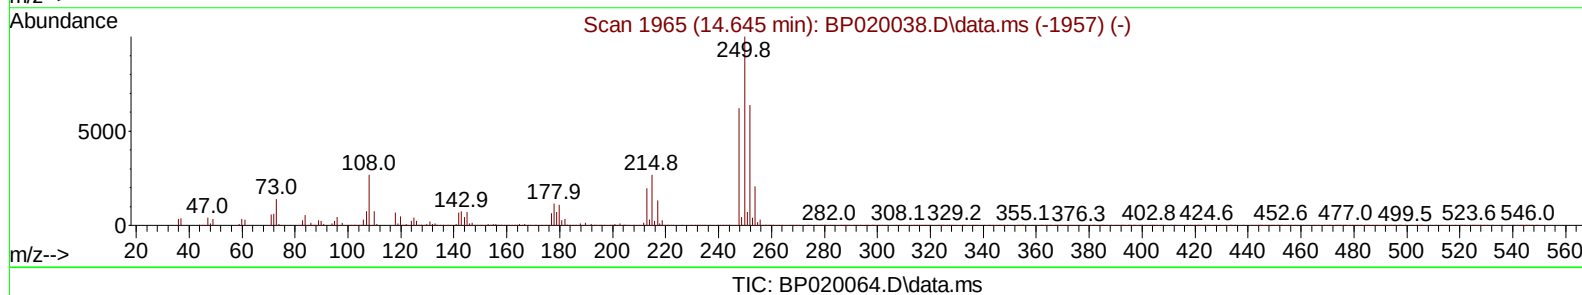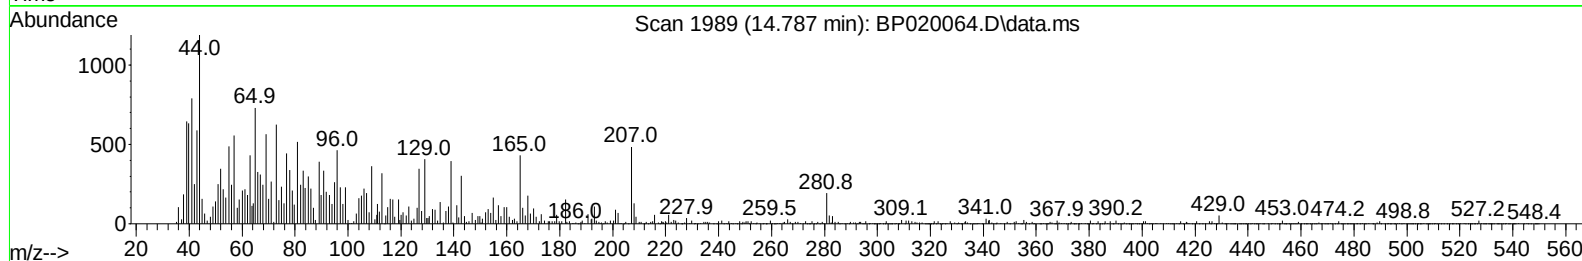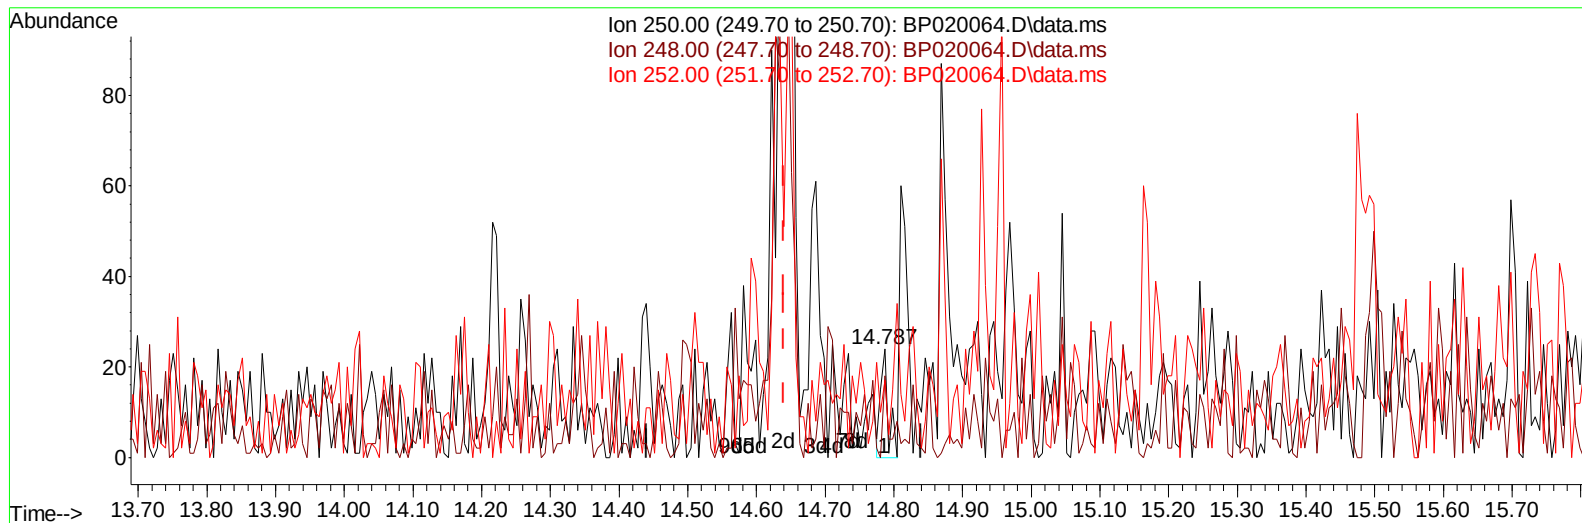

(76) Pentachlorobenzene

14.787min (+ 0.147) 0.00 ng/uL

response 18

Ion	Exp%	Act%
250.00	100.00	100.00
248.00	64.00	75.00
252.00	63.60	70.83
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020064.D
Acq On : 21 Apr 2024 06:19
Operator : MA/JU
Sample : P2104-07MSD
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:26:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 20 01:32:50 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/30/2024

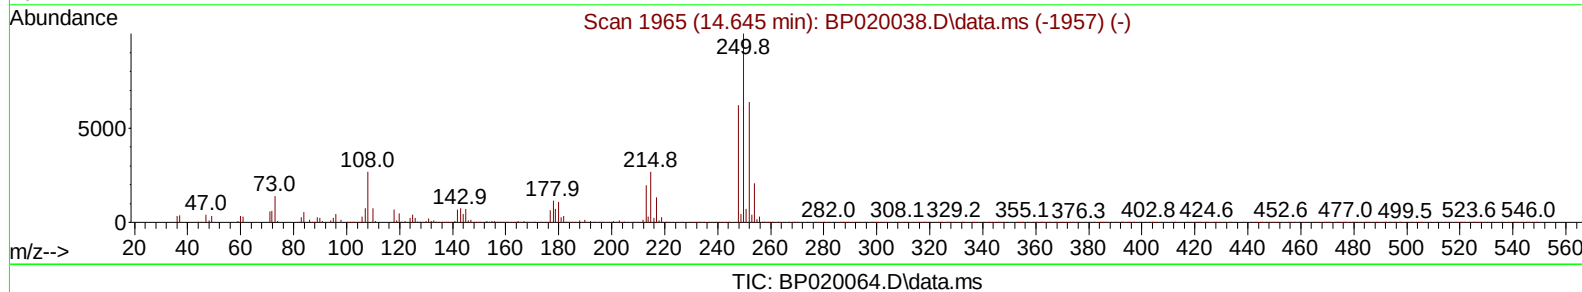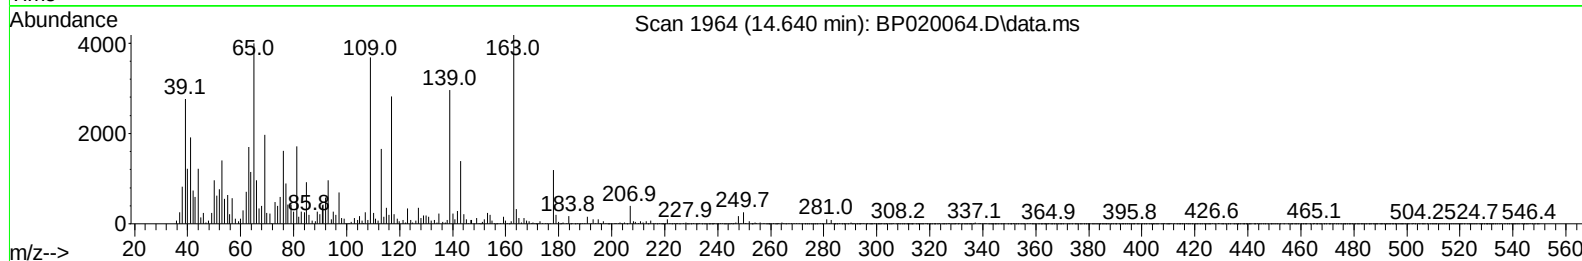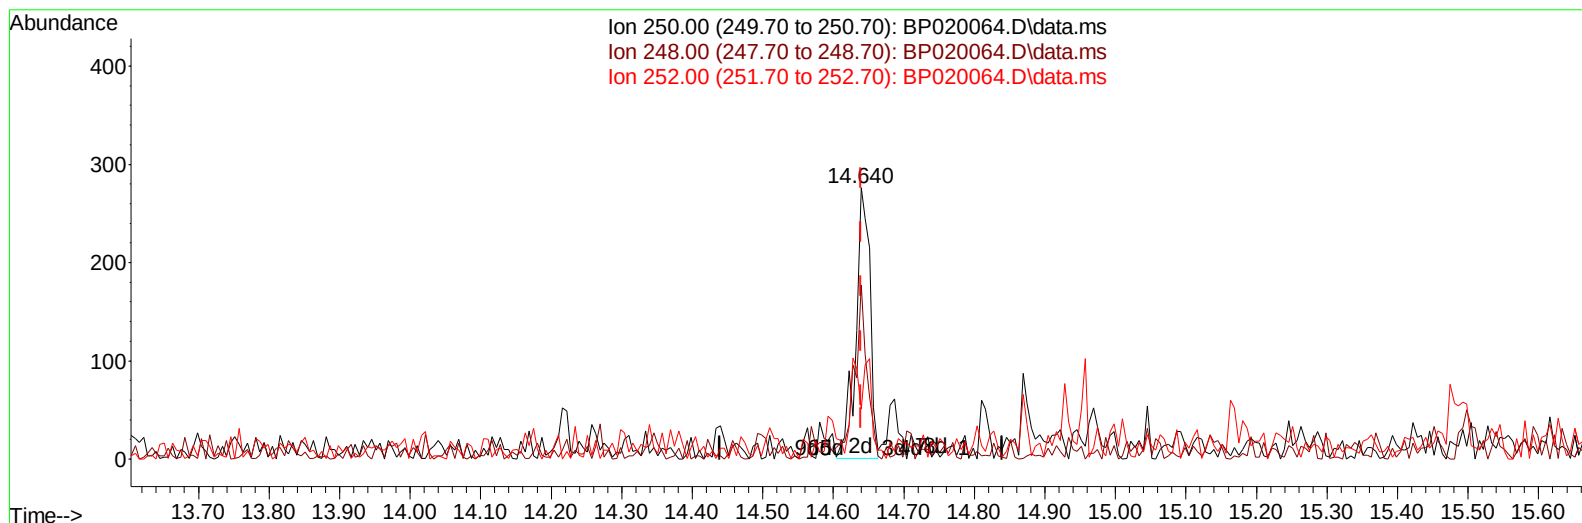

(76) Pentachlorobenzene

14.640min (+ 0.000) 0.04 ng/uL m

response 384

Ion	Exp%	Act%
250.00	100.00	100.00
248.00	64.00	68.87
252.00	63.60	19.84#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020064.D
Acq On : 21 Apr 2024 06:19
Operator : MA/JU
Sample : P2104-07MSD
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:26:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 20 01:32:50 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/30/2024

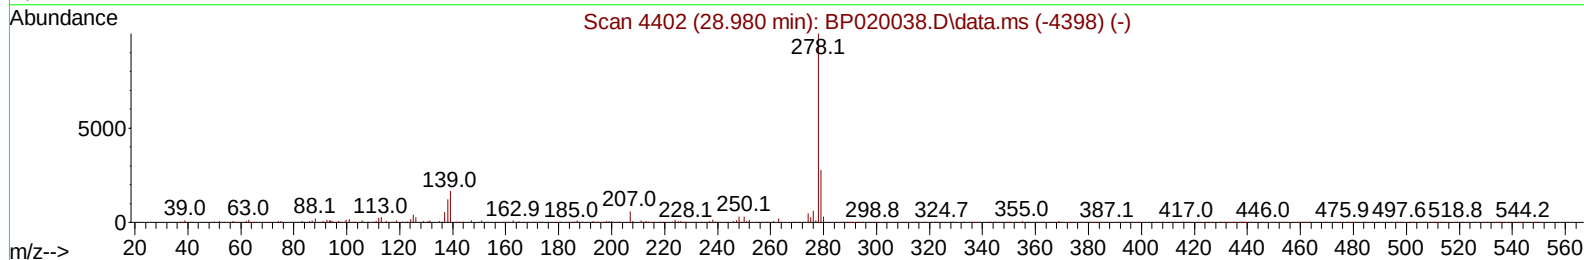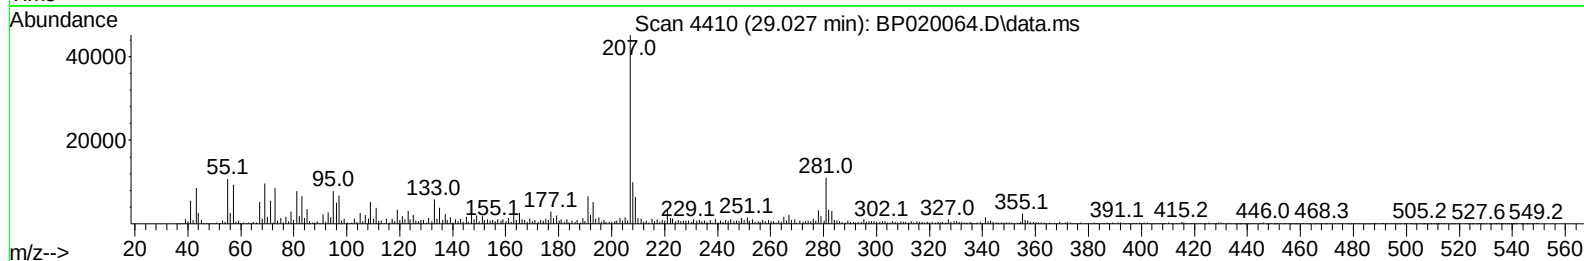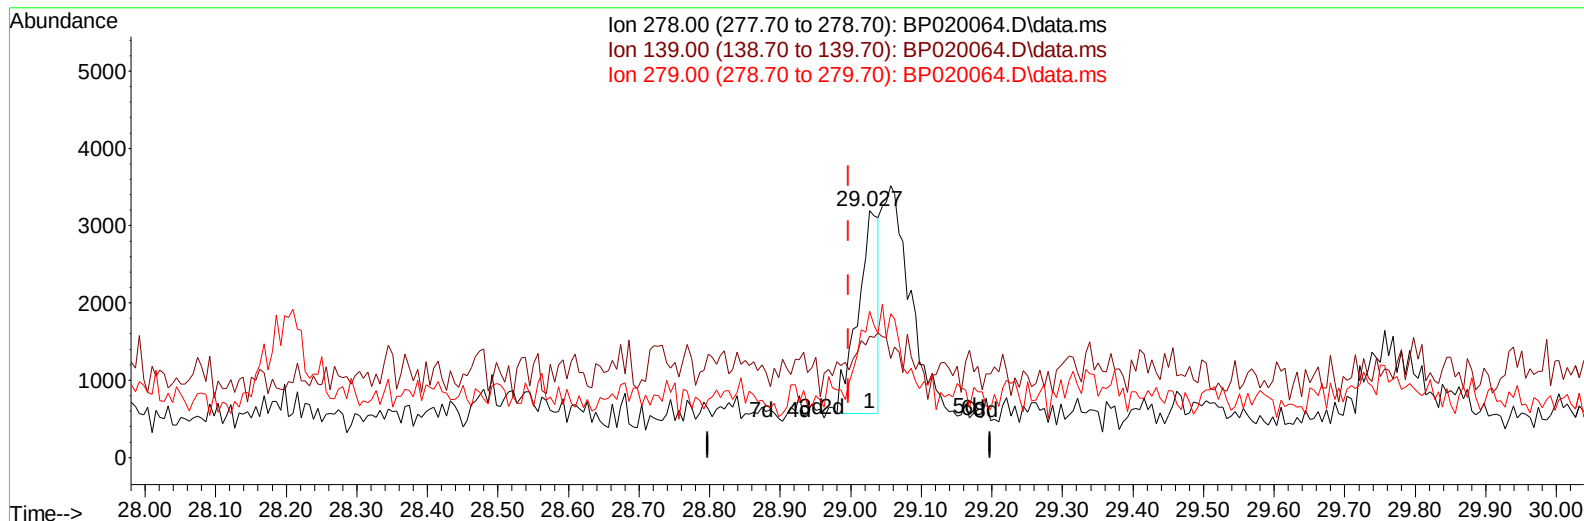

TIC: BP020064.D\data.ms

(95) Dibenzo(a,h)anthracene

29.027min (+ 0.029) 0.14 ng/uI

response 5423

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	11.80	49.09#
279.00	23.80	59.36#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020064.D
Acq On : 21 Apr 2024 06:19
Operator : MA/JU
Sample : P2104-07MSD
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:26:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 20 01:32:50 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/30/2024

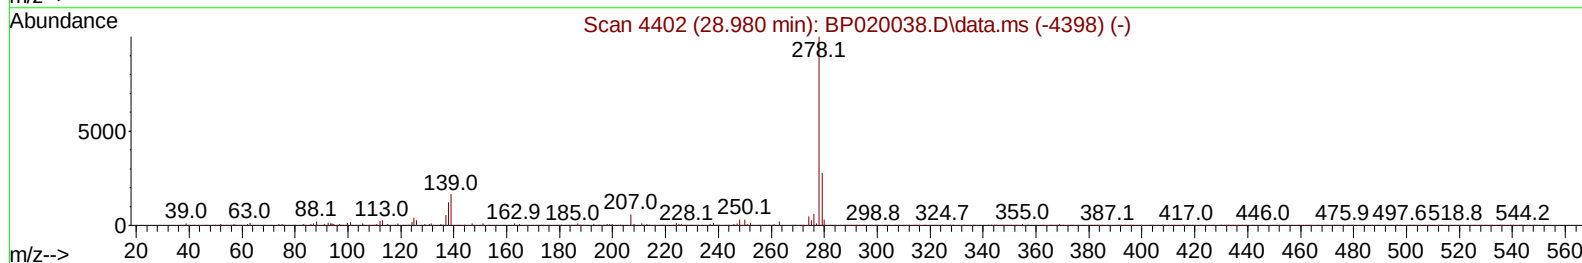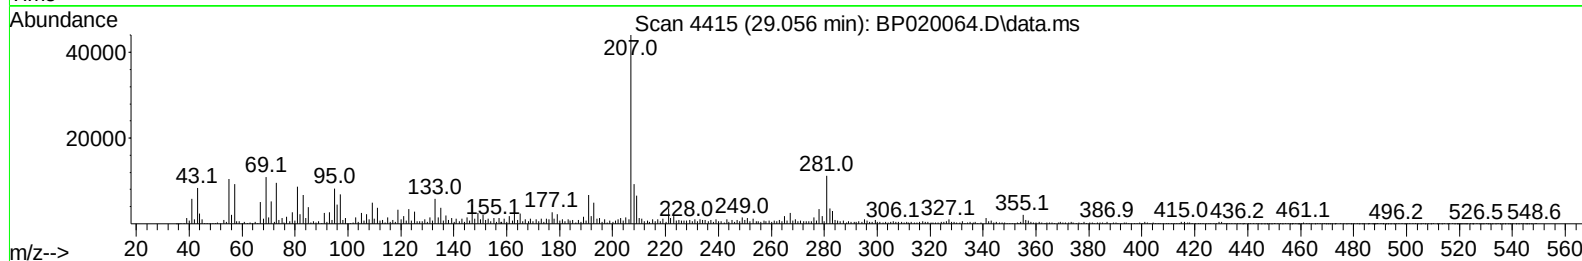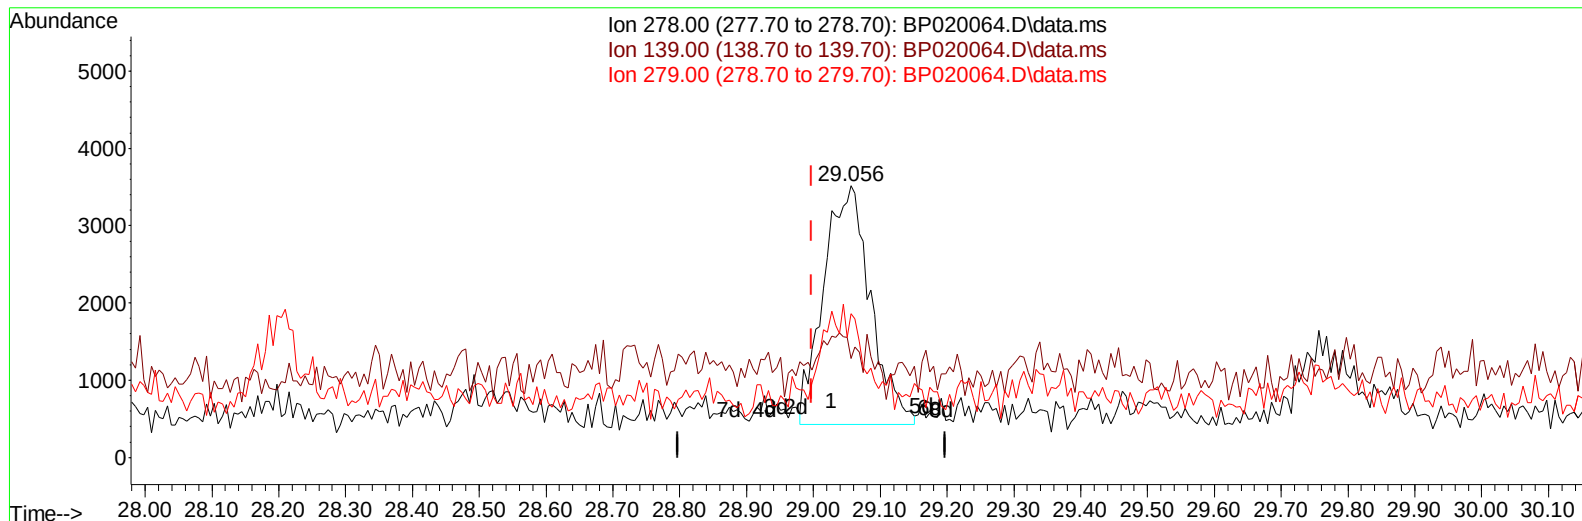

TIC: BP020064.D\data.ms

(95) Dibenzo(a,h)anthracene

29.056min (+ 0.059) 0.40 ng/ul m

response 14977

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	11.80	36.37#
279.00	23.80	52.87#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020064.D
 Acq On : 21 Apr 2024 06:19
 Operator : MA/JU
 Sample : P2104-07MSD
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA7MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:29:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 20 01:32:50 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/30/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	132199	20.000	ng/ul	0.00
20) Naphthalene-d8	10.416	136	472796	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.322	164	314058	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.175	188	682744	20.000	ng/ul	0.02
79) Chrysene-d12	21.680	240	607703	20.000	ng/ul	0.02
88) Perylene-d12	25.080	264	686586	20.000	ng/ul	0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	14661	4.544	ng/uL	0.00
4) Pyridine-d5	3.646	84	39751	4.186	ng/ul	0.01
7) Phenol-d5	6.852	99	1468	0.127	ng/ul	0.03
9) Bis-(2-Chloroethyl)eth...	6.993	67	148483	18.438	ng/ul	0.00
11) 2-Chlorophenol-d4	7.187	132	3102	0.394	ng/ul	0.01
15) 4-Methylphenol-d8	8.358	113	7771	0.863	ng/ul	0.01
21) Nitrobenzene-d5	8.805	128	70533	20.739	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	75231	20.464	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.081	165	2184m	0.299	ng/ul	0.04
31) 4-Chloroaniline-d4	10.581	131	5630m	0.578	ng/ul	0.01
46) Dimethylphthalate-d6	13.728	166	444325	20.702	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	3146	0.123	ng/ul	0.00
54) 4-Nitrophenol-d4	14.575	143	34193	10.465	ng/ul	0.02
60) Fluorene-d10	15.345	176	47855	2.505	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.498	200	47180	11.829	ng/ul	0.01
73) Anthracene-d10	17.275	188	8403m	0.275	ng/ul	0.01
81) Pyrene-d10	19.686	212	3952	0.121	ng/ul	0.02
92) Benzo(a)pyrene-d12	24.845	264	2419	0.072	ng/ul	0.04
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.270	88	28144	7.760	ng/uL	98
5) Pyridine	3.658	79	46976	4.777	ng/ul	97
6) Benzaldehyde	6.811	77	173484	25.188	ng/ul	95
8) Phenol	6.881	94	2033	0.167	ng/ul	96
10) Bis(2-Chloroethyl)ether	7.087	93	219101	22.100	ng/ul	96
12) 2-Chlorophenol	7.222	128	3920	0.473	ng/ul#	85
13) 2-Methylphenol	8.093	108	5360	0.602	ng/ul	95
14) 2,2'-oxybis(1-Chloropr...	8.163	45	310045	21.397	ng/ul	99
16) Acetophenone	8.463	105	321833	20.875	ng/ul	99
17) N-Nitroso-di-n-propyla...	8.446	70	186102	20.665	ng/ul	94
18) 4-Methylphenol	8.428	108	8494	0.897	ng/ul	96
22) Nitrobenzene	8.846	77	250324	22.586	ng/ul	99
23) Isophorone	9.363	82	479845	23.327	ng/ul	99
25) 2-Nitrophenol	9.546	139	90776	23.182	ng/ul	96
26) 2,4-Dimethylphenol	9.616	107	16315	1.742	ng/ul	97
27) Bis(2-Chloroethoxy)met...	9.840	93	263868	22.877	ng/ul	99
29) 2,4-Dichlorophenol	10.110	162	2114m	0.298	ng/ul	
30) Naphthalene	10.463	128	4467	0.182	ng/ul	95
32) 4-Chloroaniline	10.604	127	51284	5.309	ng/ul	97
33) Hexachlorobutadiene	10.734	225	3010	0.515	ng/ul	91
34) Caprolactam	11.381	113	56967	25.596	ng/ul	87
35) 4-Chloro-3-methylphenol	11.763	107	1088	0.128	ng/ul#	96
36) 2-Methylnaphthalene	12.093	142	12042m	0.711	ng/ul	

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020064.D
 Acq On : 21 Apr 2024 06:19
 Operator : MA/JU
 Sample : P2104-07MSD
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA7MSD

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/30/2024

Quant Time: Apr 22 01:29:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 20 01:32:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.316	142	7728	0.460	ng/ul	89
39) 1,2,4,5-Tetrachloroben...	12.457	216	237	0.023	ng/ul#	67
41) 2,4,6-Trichlorophenol	12.734	196	3650	0.595	ng/ul	89
42) 2,4,5-Trichlorophenol	12.816	196	1694	0.266	ng/ul#	89
43) 1,1'-Biphenyl	13.128	154	122666	5.448	ng/ul	99
44) 2-Chloronaphthalene	13.169	162	2369	0.132	ng/ul#	88
45) 2-Nitroaniline	13.398	65	94413	16.156	ng/ul	95
47) Dimethylphthalate	13.781	163	535648	24.304	ng/ul	100
48) 2,6-Dinitrotoluene	13.910	165	111337	26.771	ng/ul	96
50) Acenaphthylene	14.040	152	9960	0.345	ng/ul	98
51) 3-Nitroaniline	14.245	138	82393	20.931	ng/ul	95
52) Acenaphthene	14.381	153	4564	0.240	ng/ul#	84
53) 2,4-Dinitrophenol	14.481	184	30980	12.388	ng/ul	94
55) 4-Nitrophenol	14.587	109	37781	10.149	ng/ul	96
56) Dibenzofuran	14.734	168	18458	0.703	ng/ul#	83
57) 2,4-Dinitrotoluene	14.728	165	170540	28.967	ng/ul#	65
58) 2,3,4,6-Tetrachlorophenol	14.975	232	2313	0.419	ng/ul#	91
59) Diethylphthalate	15.181	149	553056	24.989	ng/ul	98
61) Fluorene	15.404	166	47974	2.212	ng/ul#	97
62) 4-Chlorophenyl-phenyle...	15.404	204	100236	8.508	ng/ul	97
63) 4-Nitroaniline	15.457	138	104725	29.964	ng/ul	92
66) 4,6-Dinitro-2-methylph...	15.510	198	62658	15.114	ng/ul	99
67) N-Nitrosodiphenylamine	15.628	169	223188	11.818	ng/ul	99
68) 4-Bromophenyl-phenylether	16.339	248	48057	6.418	ng/ul	97
70) Atrazine	16.634	200	193457	27.895	ng/ul	97
72) Phenanthrene	17.216	178	7445	0.210	ng/ul	98
74) Anthracene	17.316	178	17631m	0.488	ng/ul	
75) 1,2,3,4-Tetrachloroben...	13.093	216	286	0.026	ng/uL	96
76) Pentachlorobenzene	14.640	250	384m	0.038	ng/uL	
77) Carbazole	17.622	167	5672	0.183	ng/ul	98
78) Di-n-butylphthalate	18.210	149	1082331	28.956	ng/ul	99
80) Fluoranthene	19.333	202	13398	0.349	ng/ul#	94
82) Pyrene	19.710	202	1868	0.047	ng/ul#	85
83) Butylbenzylphthalate	20.686	149	472647	31.031	ng/ul	95
84) 3,3'-Dichlorobenzidine	21.592	252	95842	7.132	ng/ul	99
85) Benzo(a)anthracene	21.657	228	17427	0.415	ng/ul#	71
86) Bis(2-ethylhexyl)phtha...	21.610	149	680613	28.986	ng/ul	98
87) Chrysene	21.722	228	7421	0.187	ng/ul#	76
89) Di-n-octyl phthalate	22.921	149	1168306	27.532	ng/ul	100
90) Benzo(b)fluoranthene	23.998	252	9840	0.238	ng/ul#	44
91) Benzo(k)fluoranthene	24.074	252	8953	0.211	ng/ul#	28
93) Benzo(a)pyrene	24.910	252	206	0.005	ng/ul#	1
94) Indeno(1,2,3-cd)pyrene	28.939	276	346	0.007	ng/ul#	1
95) Dibenzo(a,h)anthracene	29.056	278	14977m	0.398	ng/ul	
96) Benzo(g,h,i)perylene	30.133	276	315	0.009	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020064.D
 Acq On : 21 Apr 2024 06:19
 Operator : MA/JU
 Sample : P2104-07MSD
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :

BNA_P

Client Sample Id :

C0AA7MSD

Manual Integrations APPROVED

Quant Time: Apr 22 01:29:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 20 01:32:50 2024
 Response via : Initial Calibration

Reviewed By : Yogesh Patel 04/24/2024

Supervised By : mohammad ahmed 04/30/2024

