

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020045.D
 Acq On : 20 Apr 2024 15:49
 Operator : MA/JU
 Sample : P2161-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MC0RB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	31	rVB	17799	25362	0.82%	0.095%
2	3.640	91	94	110	rBV	46759	93406	3.02%	0.348%
3	3.928	140	143	147	rVB2	5946	7405	0.24%	0.028%
4	5.017	323	328	335	rBV2	12314	19815	0.64%	0.074%
5	6.828	629	636	654	rVV	66069	154094	4.98%	0.575%
6	6.993	656	664	677	rBV	382963	648484	20.98%	2.418%
7	7.175	688	695	718	rVB	342532	621109	20.09%	2.316%
8	7.540	751	757	765	rVB	1830	4078	0.13%	0.015%
9	7.640	766	774	791	rBV	311335	554426	17.93%	2.067%
10	7.993	828	834	842	rVB5	5948	11090	0.36%	0.041%
11	8.346	887	894	911	rBV	238827	457657	14.80%	1.706%
12	8.799	962	971	984	rBV	477869	895940	28.98%	3.341%
13	9.152	1025	1031	1038	rVB3	6031	10824	0.35%	0.040%
14	9.510	1084	1092	1107	rBV	380604	718506	23.24%	2.679%
15	10.046	1175	1183	1216	rBV	416981	931601	30.13%	3.474%
16	10.287	1220	1224	1226	rVB5	2534	3717	0.12%	0.014%
17	10.416	1238	1246	1258	rBV	419614	722280	23.36%	2.693%
18	10.581	1266	1274	1300	rBV	208268	566027	18.31%	2.111%
19	11.240	1378	1386	1387	rBV8	4070	6011	0.19%	0.022%
20	12.051	1517	1524	1532	rBV2	7677	15705	0.51%	0.059%
21	13.128	1701	1707	1714	rVB9	7244	14689	0.48%	0.055%
22	13.204	1714	1720	1726	rBV2	8460	13755	0.44%	0.051%
23	13.340	1738	1743	1747	rBV4	3344	5896	0.19%	0.022%
24	13.734	1801	1810	1827	rBV	966354	1617844	52.33%	6.033%
25	14.004	1848	1856	1869	rBV2	1124305	1824652	59.02%	6.804%
26	14.087	1869	1870	1876	rVB6	3049	3903	0.13%	0.015%
27	14.316	1902	1909	1923	rBV	581326	956535	30.94%	3.567%
28	14.551	1945	1949	1952	rBV6	2995	4450	0.14%	0.017%
29	14.604	1952	1958	1962	rBV3	19663	43113	1.39%	0.161%
30	15.134	2043	2048	2053	rVB9	1850	4117	0.13%	0.015%
31	15.204	2056	2060	2064	rBV6	2278	3743	0.12%	0.014%
32	15.345	2077	2084	2093	rBV	1504951	2258312	73.04%	8.421%
33	15.422	2095	2097	2103	rVB6	6724	9673	0.31%	0.036%
34	15.492	2103	2109	2123	rBV	466740	825882	26.71%	3.079%
35	15.598	2123	2127	2134	rVB7	9924	19110	0.62%	0.071%
36	15.939	2182	2185	2189	rVB6	2985	4328	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020045.D
 Acq On : 20 Apr 2024 15:49
 Operator : MA/JU
 Sample : P2161-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MC0RB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Title : SVOA CALIBRATION

37	16.163	2219	2223	2230	rVB7	5935	10586	0.34%	0.039%
38	16.757	2321	2324	2327	rBV5	2242	4216	0.14%	0.016%
39	16.834	2334	2337	2342	rVB7	2752	4254	0.14%	0.016%
40	16.945	2347	2356	2357	rBV9	4422	7699	0.25%	0.029%
41	17.163	2386	2393	2404	rBV	773453	1167311	37.76%	4.353%
42	17.263	2404	2410	2427	rVV2	1685384	2591915	83.83%	9.665%
43	17.851	2506	2510	2513	rBV5	5021	8399	0.27%	0.031%
44	17.886	2513	2516	2523	rVB3	10033	15547	0.50%	0.058%
45	18.122	2551	2556	2563	rBV3	44991	84388	2.73%	0.315%
46	18.228	2570	2574	2578	rBV7	9135	16052	0.52%	0.060%
47	19.122	2723	2726	2732	rVB7	14921	21918	0.71%	0.082%
48	19.210	2737	2741	2748	rVB4	21939	33640	1.09%	0.125%
49	19.292	2750	2755	2760	rBV2	15680	30031	0.97%	0.112%
50	19.469	2781	2785	2794	rBV3	37870	68874	2.23%	0.257%
51	19.663	2812	2818	2830	rVB	2257329	3042053	98.39%	11.343%
52	21.663	3152	3158	3172	rVB	740688	1259347	40.73%	4.696%
53	24.821	3685	3695	3713	rVB	1256932	3091689	100.00%	11.528%
54	25.051	3727	3734	3751	rVB2	393732	1283282	41.51%	4.785%




Sum of corrected areas: 26818740

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020045.D
Acq On : 20 Apr 2024 15:49
Operator : MA/JU
Sample : P2161-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MC0RB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

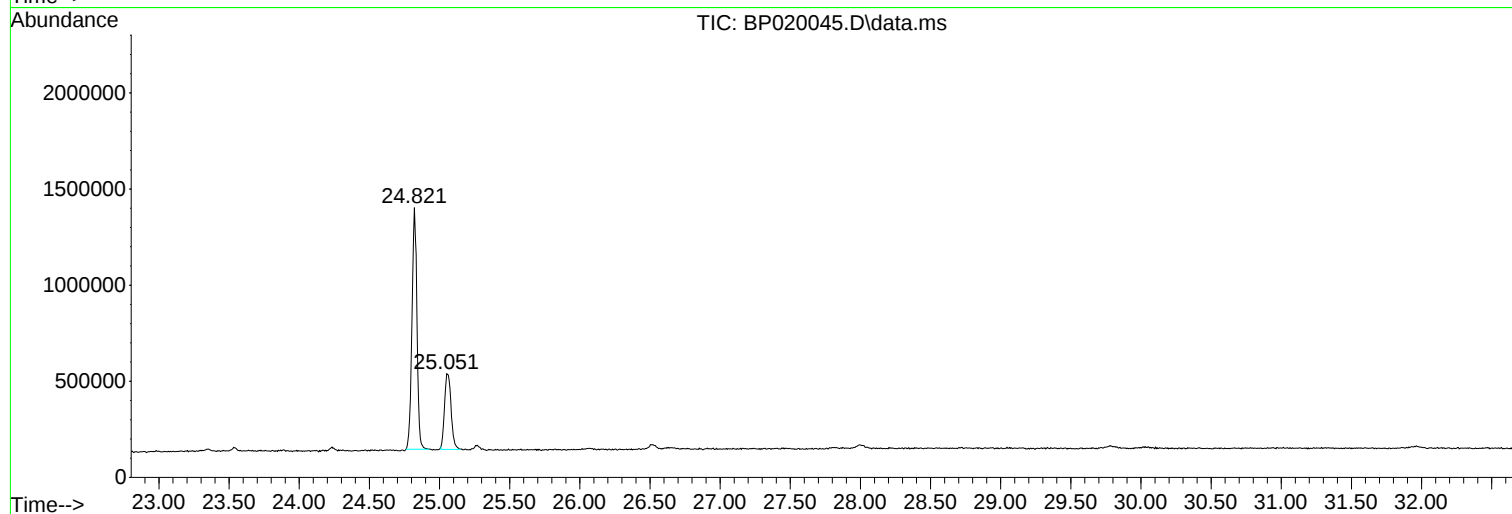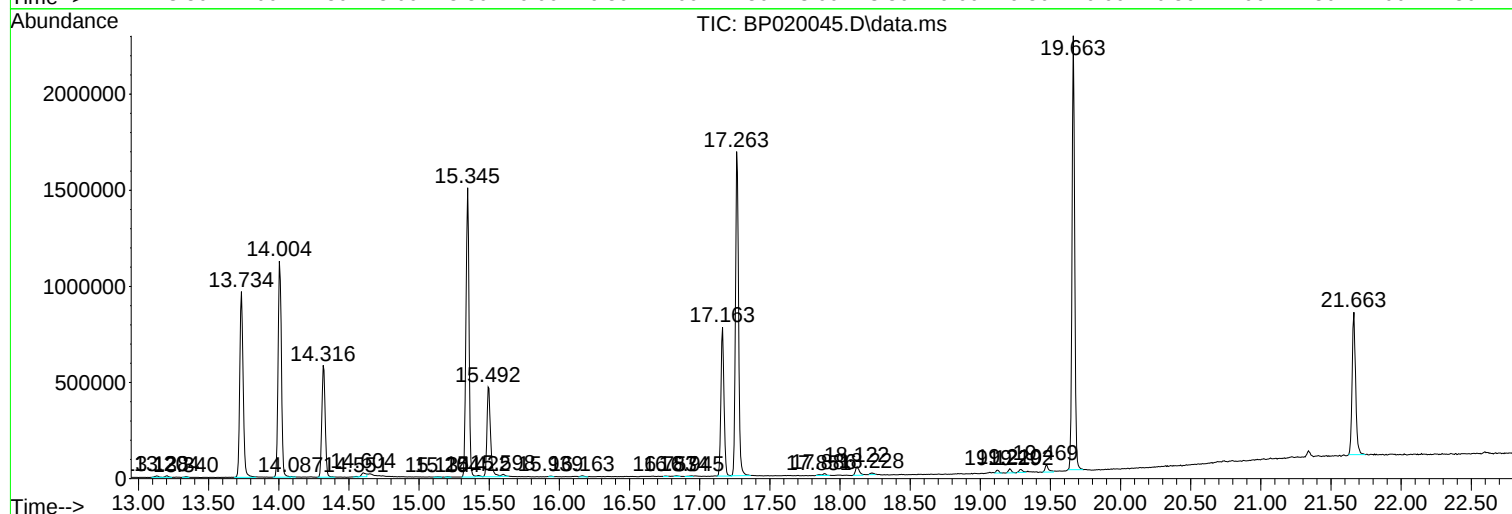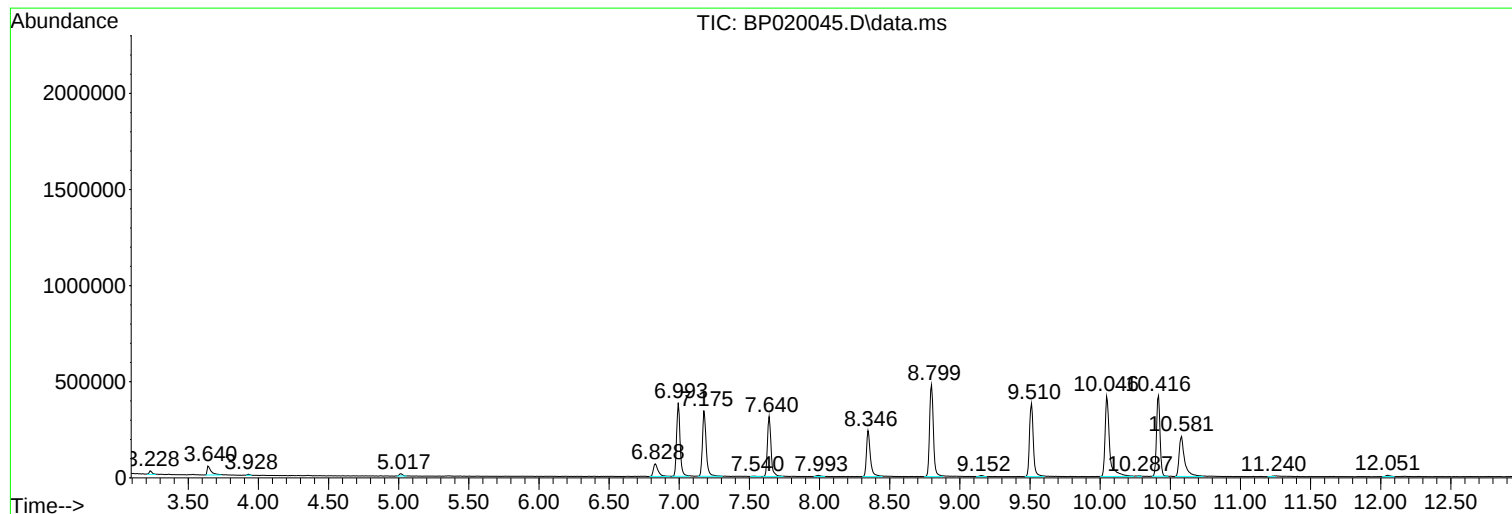

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020045.D
Acq On : 20 Apr 2024 15:49
Operator : MA/JU
Sample : P2161-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MC0RB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020045.D
Acq On : 20 Apr 2024 15:49
Operator : MA/JU
Sample : P2161-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MC0RB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc