

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
 Data File : BP020054.D
 Acq On : 20 Apr 2024 23:09
 Operator : MA/JU
 Sample : PB160221BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK221

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020054.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	29	rBV	30735	37837	1.53%	0.135%
2	3.628	89	92	110	rBV	358124	596911	24.09%	2.130%
3	6.822	628	635	653	rBV	412231	807690	32.59%	2.882%
4	6.987	657	663	679	rVB	359884	607870	24.53%	2.169%
5	7.175	688	695	711	rBV	441774	765402	30.88%	2.732%
6	7.634	766	773	784	rBV	341656	589251	23.78%	2.103%
7	8.340	885	893	907	rBV	487964	954665	38.52%	3.407%
8	8.793	961	970	994	rBV	439452	843468	34.04%	3.010%
9	9.510	1083	1092	1112	rBV	369587	724151	29.22%	2.584%
10	10.046	1172	1183	1210	rBV	453135	994424	40.13%	3.549%
11	10.410	1236	1245	1260	rBV	497117	855704	34.53%	3.054%
12	10.569	1264	1272	1300	rBV	421690	1002792	40.46%	3.579%
13	12.051	1517	1524	1533	rBV3	6295	14366	0.58%	0.051%
14	13.198	1713	1719	1726	rBV4	9176	16124	0.65%	0.058%
15	13.728	1802	1809	1821	rBV	842646	1506938	60.81%	5.378%
16	14.004	1848	1856	1875	rBV	1102446	1719003	69.36%	6.135%
17	14.316	1902	1909	1920	rBV	716072	1158161	46.73%	4.133%
18	14.569	1944	1952	1964	rBV	242807	605263	24.42%	2.160%
19	15.345	2076	2084	2096	rBV2	1204664	2108640	85.09%	7.525%
20	15.498	2103	2110	2122	rBV	402565	708396	28.58%	2.528%
21	15.592	2123	2126	2140	rVB7	10461	25862	1.04%	0.092%
22	16.169	2219	2224	2231	rBV8	4986	8300	0.33%	0.030%
23	16.951	2353	2357	2362	rVB8	2881	5612	0.23%	0.020%
24	17.175	2388	2395	2404	rBV	958442	1348026	54.39%	4.811%
25	17.269	2404	2411	2433	rVV	1430391	2254427	90.97%	8.046%
26	19.216	2739	2742	2747	rBV7	16160	23201	0.94%	0.083%
27	19.292	2753	2755	2763	rVB3	12936	16736	0.68%	0.060%
28	19.675	2814	2820	2834	rBV2	1499823	2478233	100.00%	8.844%
29	21.669	3154	3159	3170	rBV2	793278	1377238	55.57%	4.915%
30	24.827	3686	3696	3711	rBV2	855945	2452040	98.94%	8.751%
31	25.062	3727	3736	3753	rVB	415332	1414123	57.06%	5.047%




Sum of corrected areas: 28020854

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020054.D
Acq On : 20 Apr 2024 23:09
Operator : MA/JU
Sample : PB160221BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK221

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

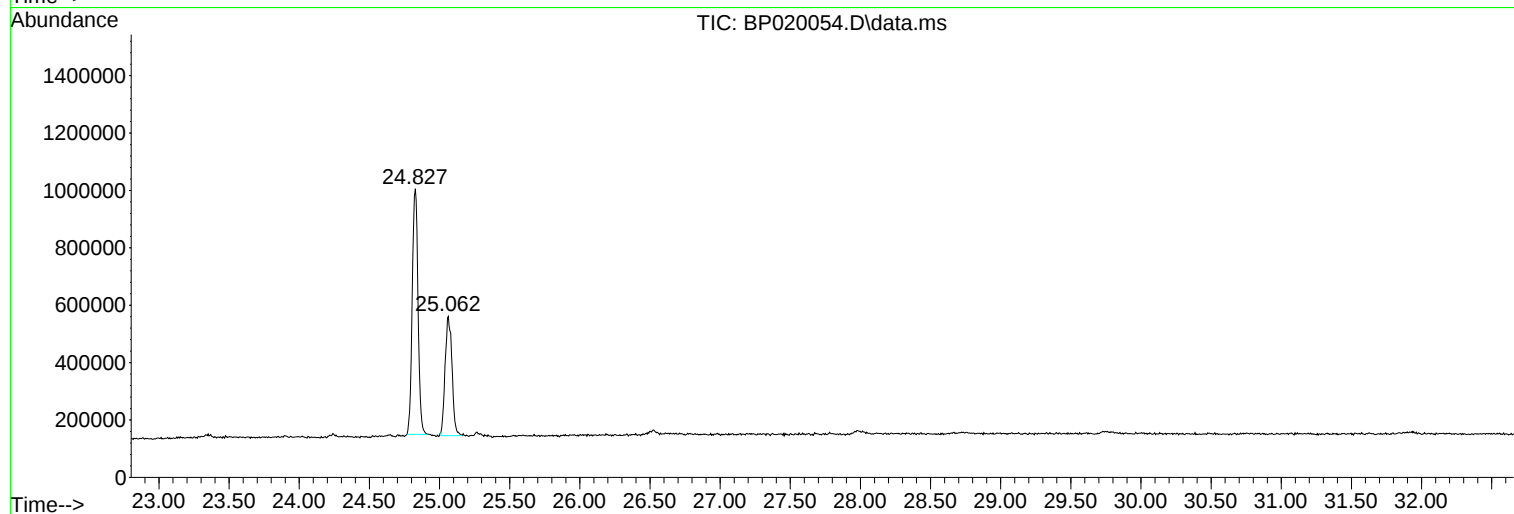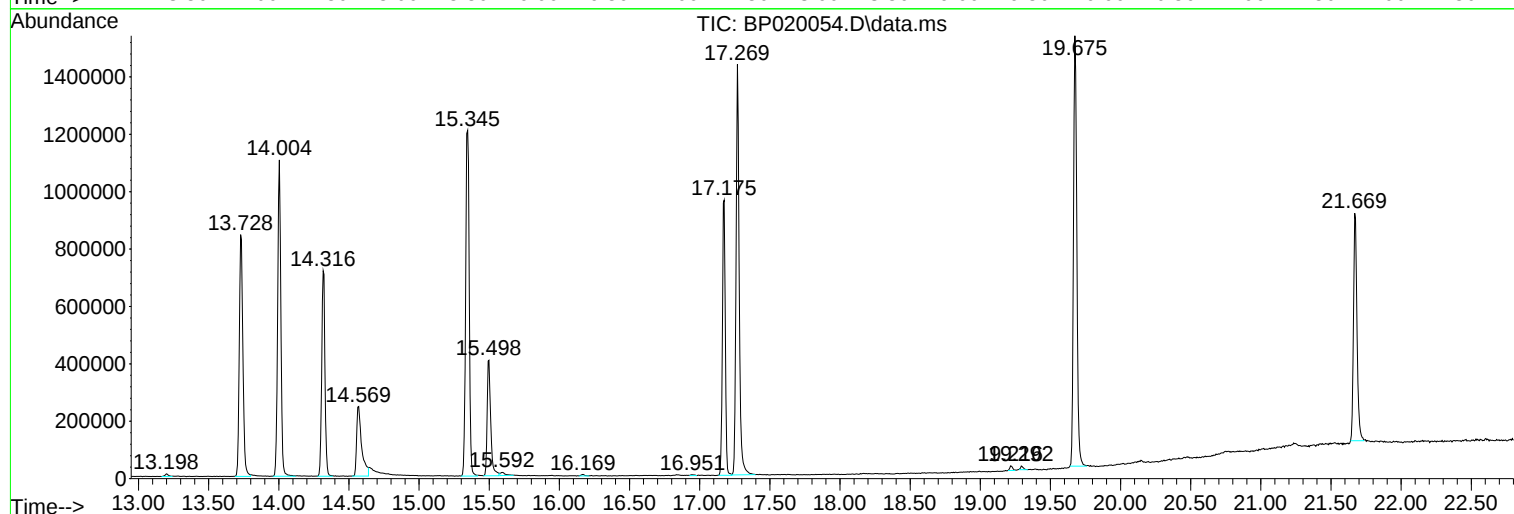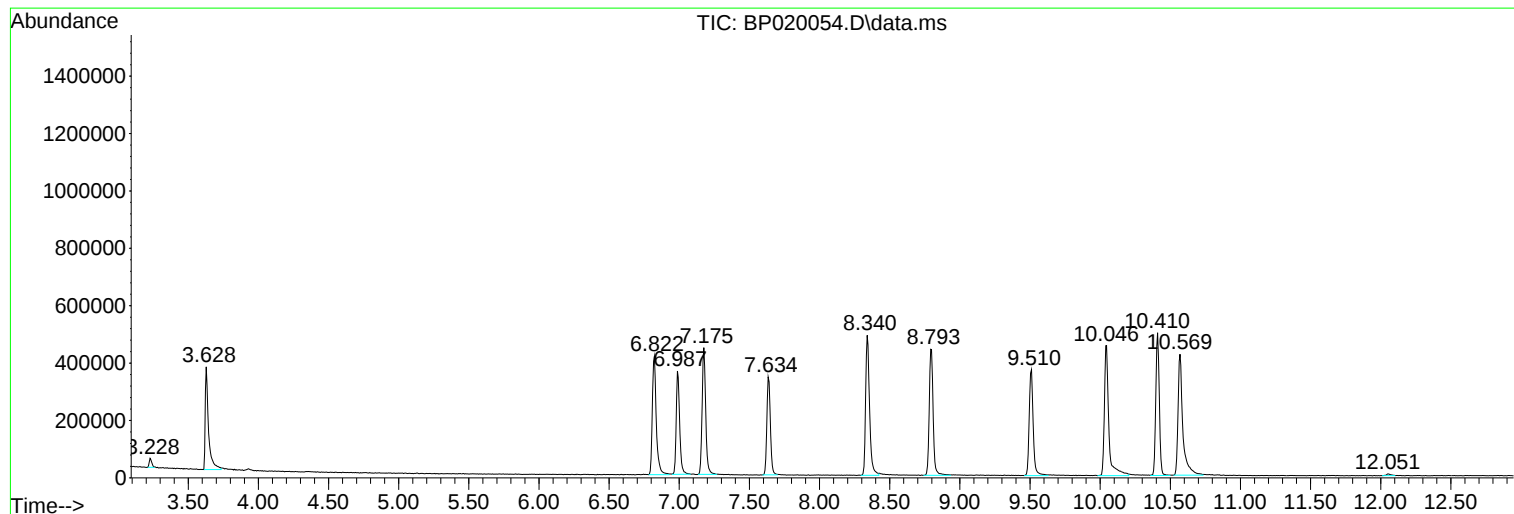

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020054.D
Acq On : 20 Apr 2024 23:09
Operator : MA/JU
Sample : PB160221BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK221

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042024\
Data File : BP020054.D
Acq On : 20 Apr 2024 23:09
Operator : MA/JU
Sample : PB160221BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK221

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------