
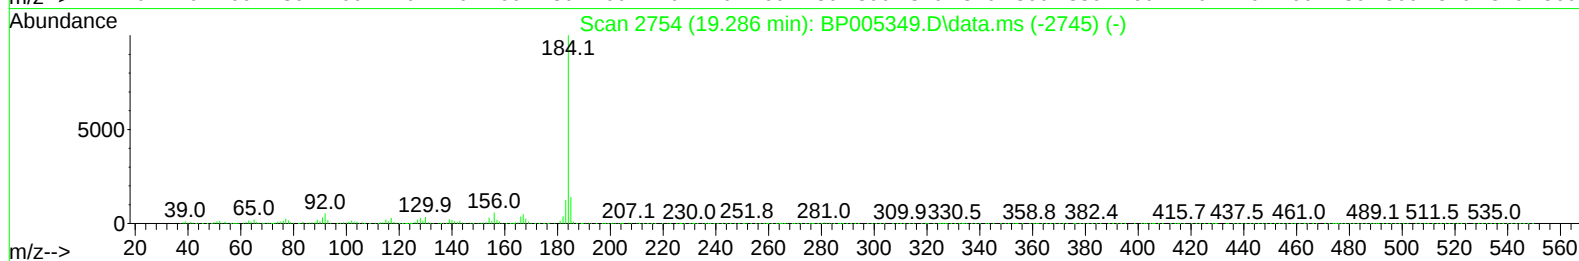
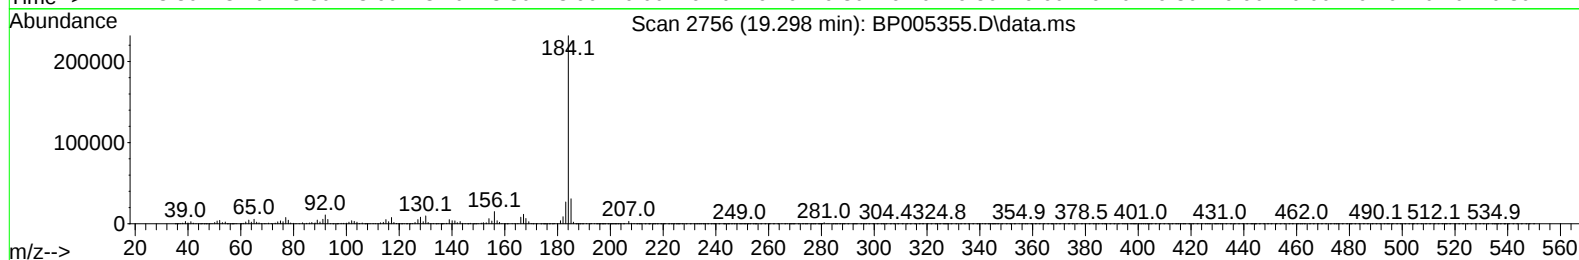


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042121\
Data File : BP005355.D
Acq On : 21 Apr 2021 12:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 13:51:59 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 21 13:46:46 2021
Response via : Initial Calibration

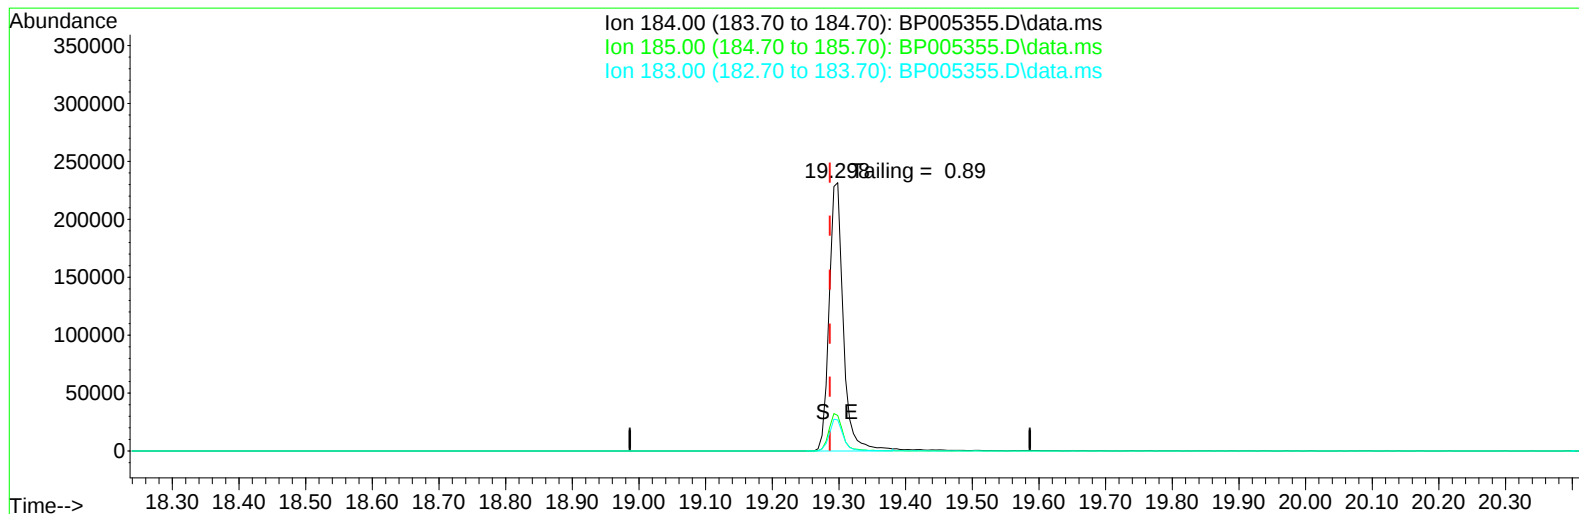




TIC: BP005355.D\data.ms

(77) Benzidine**19.298min (+ 0.012) 1604013.96 ng****response 344928**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.25
183.00	12.30	11.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042121\
 Data File : BP005355.D
 Acq On : 21 Apr 2021 12:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 13:51:59 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 21 13:46:46 2021
 Response via : Initial Calibration

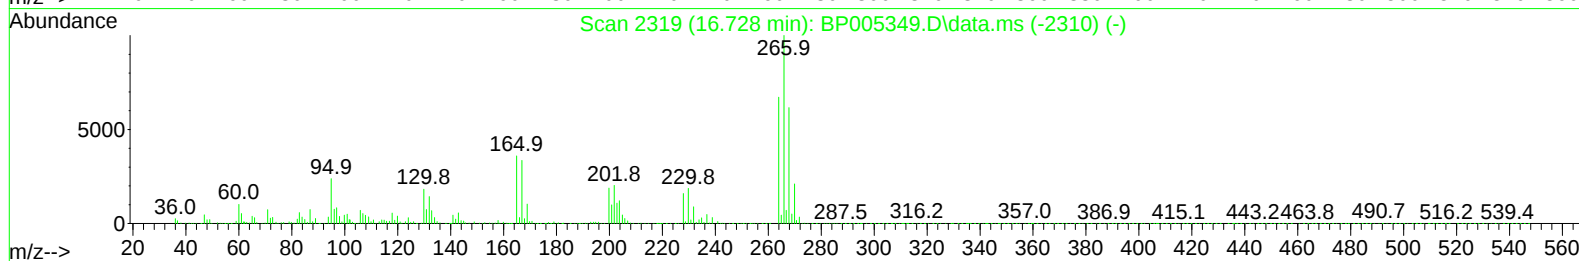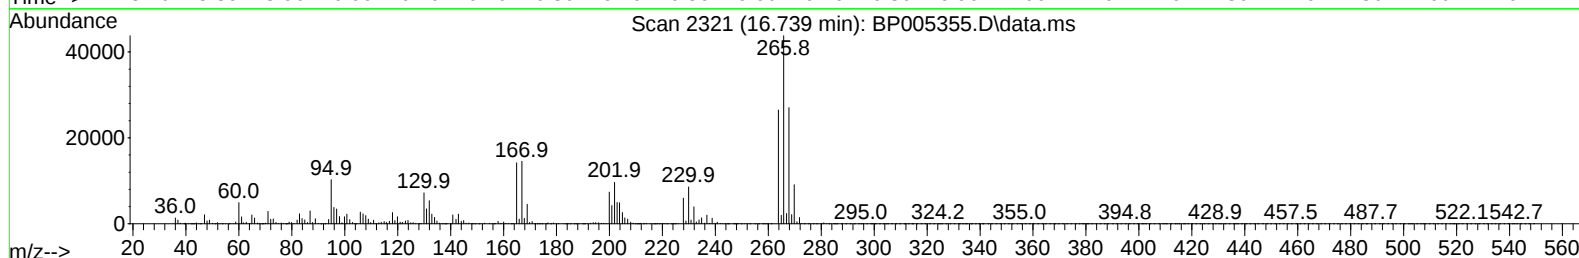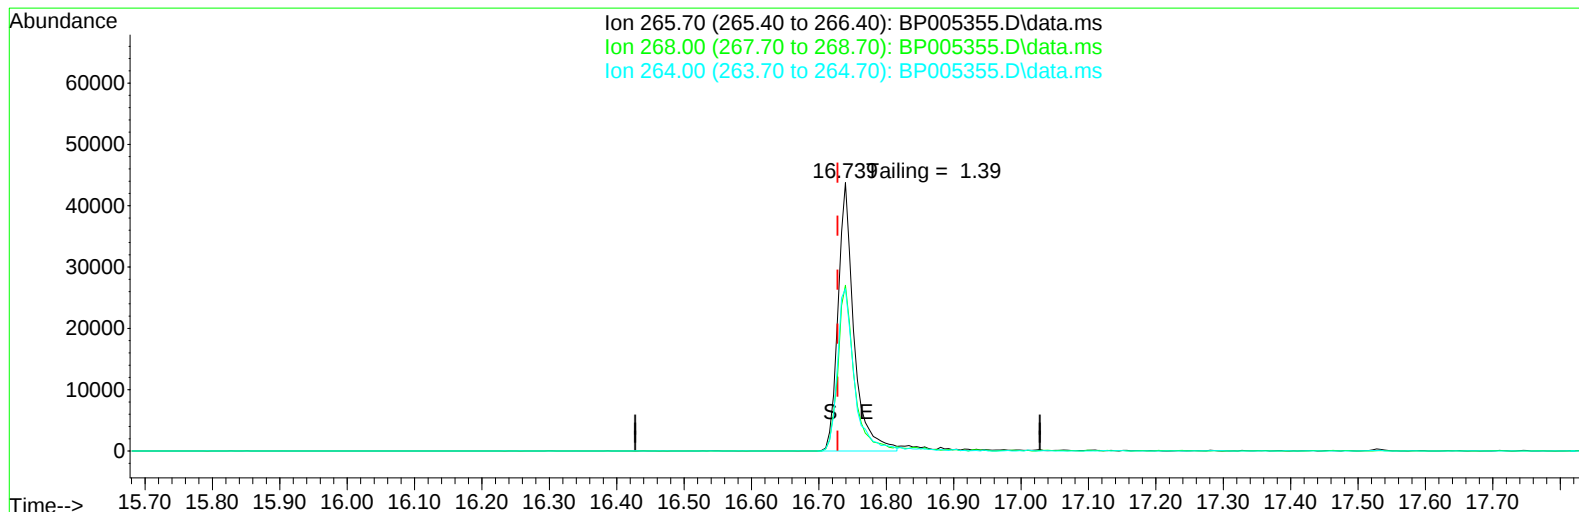

TIC: BP005355.D\data.ms

(70) Pentachlorophenol (C)

16.739min (+ 0.012) 1023054.17 ng

response 72354

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	61.80
264.00	67.10	60.48
0.00	0.00	0.00